

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
 Data File : PL076612.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2022 00:08
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 02:00:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 01:58:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.640	48877195	163.8E6	50.000	50.000
28)	SA Decachlor...	8.908	7.747	40582657	120.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.580	3.621	17962145	44712731	500.000	500.000
24)	Chlordane-2	5.113	4.193	19322306	53605842	500.000	500.000
25)	Chlordane-3	5.824	4.818	71688869	147.0E6	500.000	500.000
26)	Chlordane-4	5.903	4.879	88578595	151.2E6	500.000	500.000
27)	Chlordane-5	6.761	5.543	15977672	41837953	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
Data File : PL076612.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2022 00:08
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 02:00:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 01:58:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

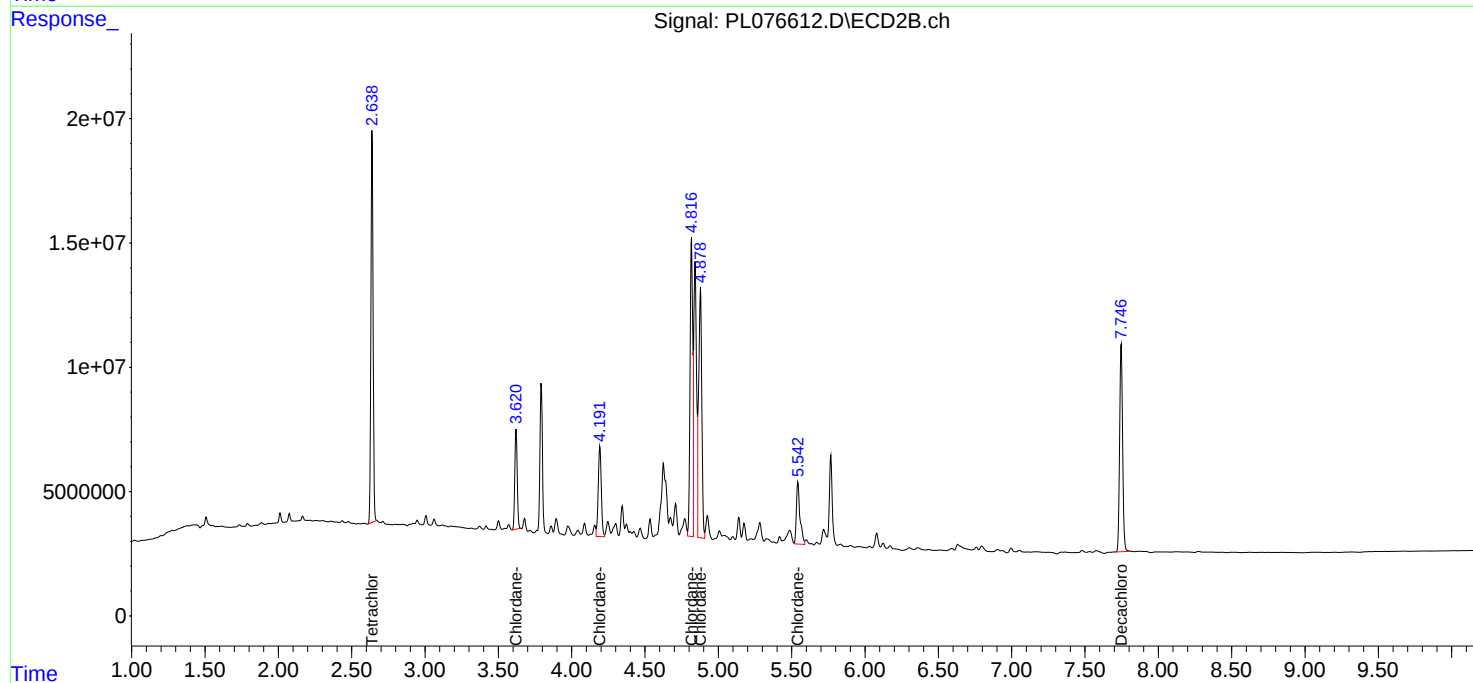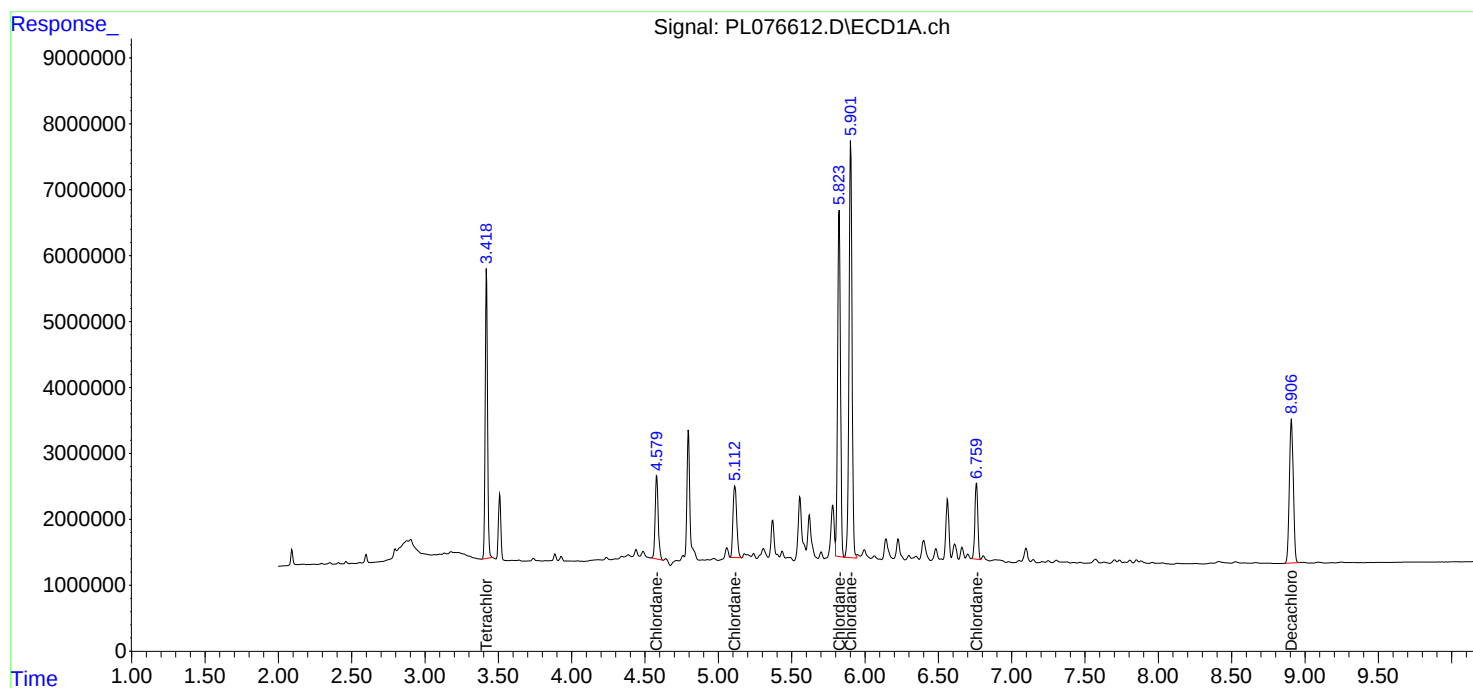


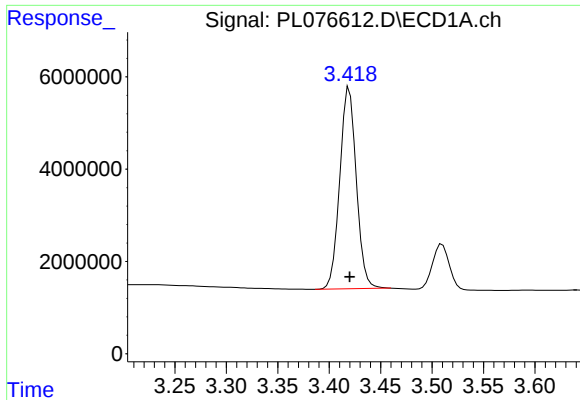

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 48877195
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

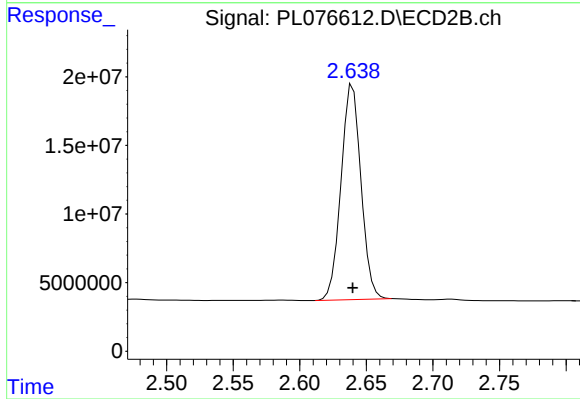


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: 0.000 min
Response: 163829770
Conc: 50.00 ng/ml

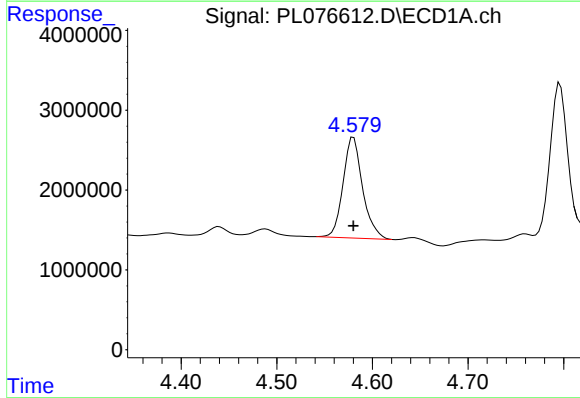


#23 Chlordane-1

R.T.: 4.580 min
Delta R.T.: 0.000 min
Response: 17962145
Conc: 500.00 ng/ml

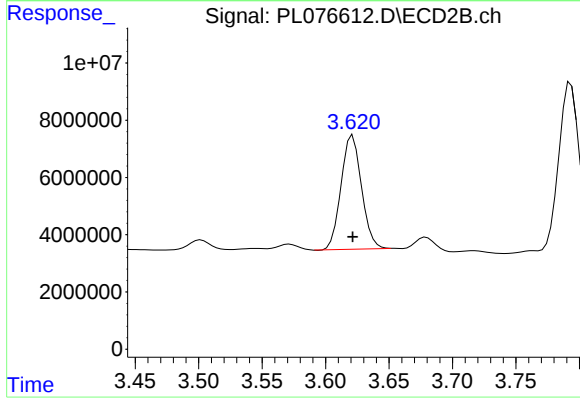

#23 Chlordane-1


R.T.: 3.621 min
Delta R.T.: 0.000 min
Response: 44712731
Conc: 500.00 ng/ml

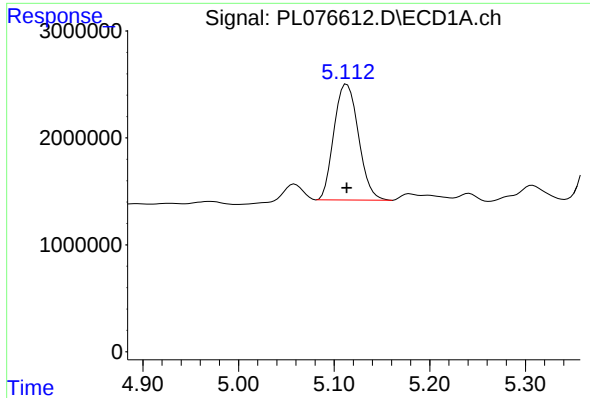

#24 Chlordane-2


R.T.: 5.113 min
Delta R.T.: 0.000 min
Response: 19322306
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

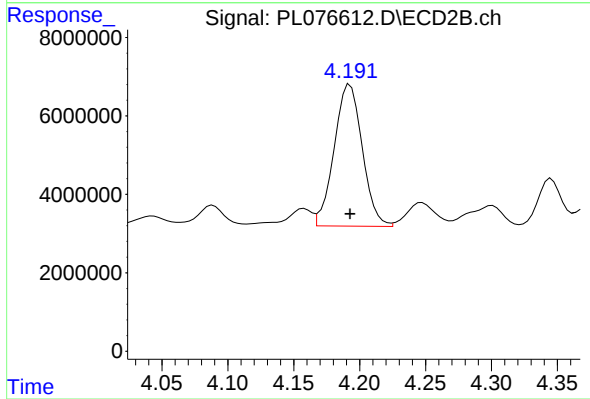


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 53605842
Conc: 500.00 ng/ml

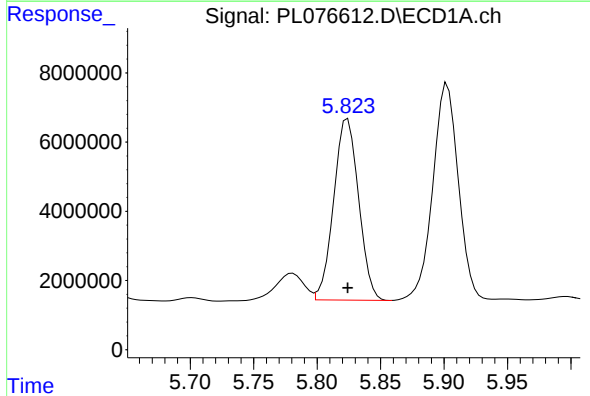


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 71688869
Conc: 500.00 ng/ml

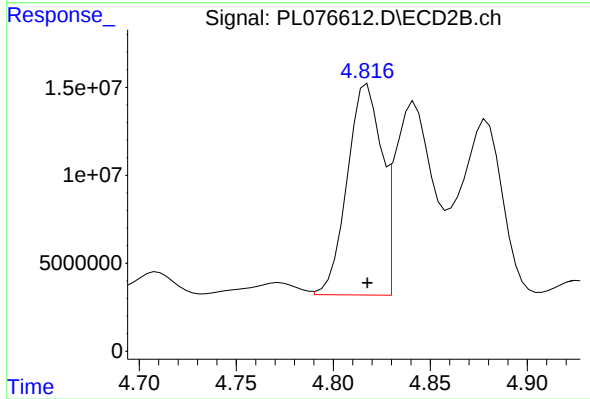

#25 Chlordane-3


R.T.: 4.818 min
Delta R.T.: 0.000 min
Response: 147003257
Conc: 500.00 ng/ml

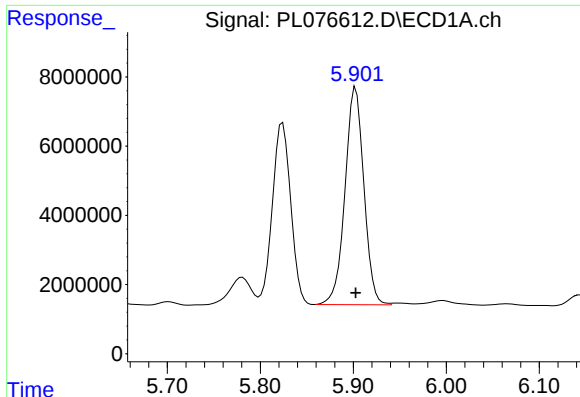

#26 Chlordane-4


R.T.: 5.903 min
Delta R.T.: 0.000 min
Response: 88578595
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

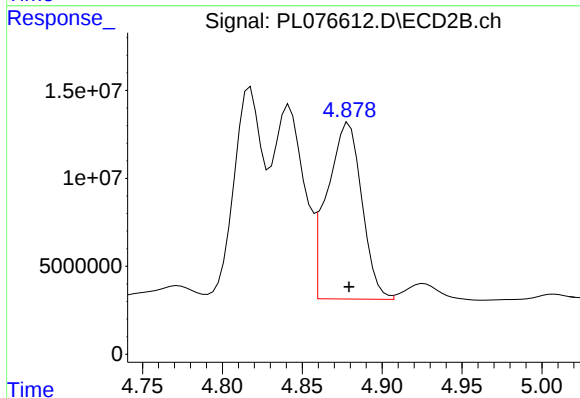


#26 Chlordane-4

R.T.: 4.879 min
Delta R.T.: 0.000 min
Response: 151217023
Conc: 500.00 ng/ml

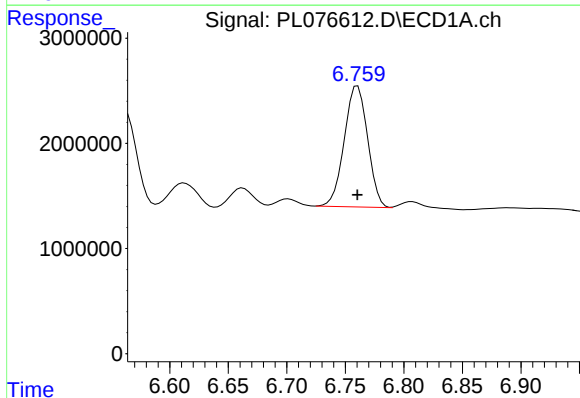


#27 Chlordane-5

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 15977672
Conc: 500.00 ng/ml

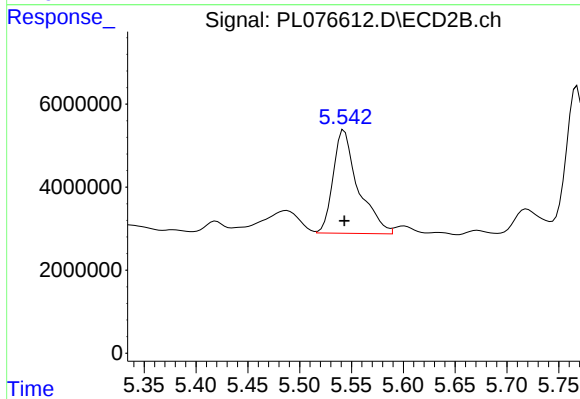

#27 Chlordane-5


R.T.: 5.543 min
Delta R.T.: 0.000 min
Response: 41837953
Conc: 500.00 ng/ml

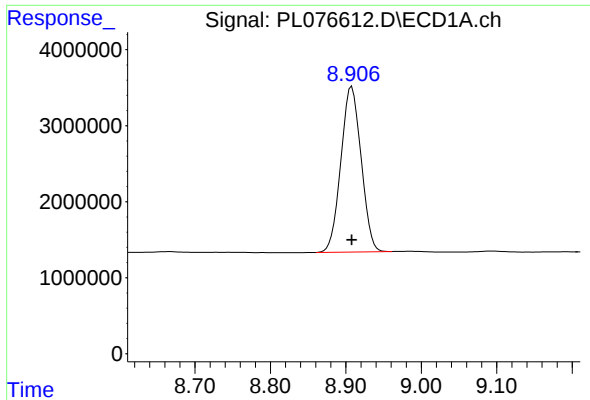

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 40582657
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

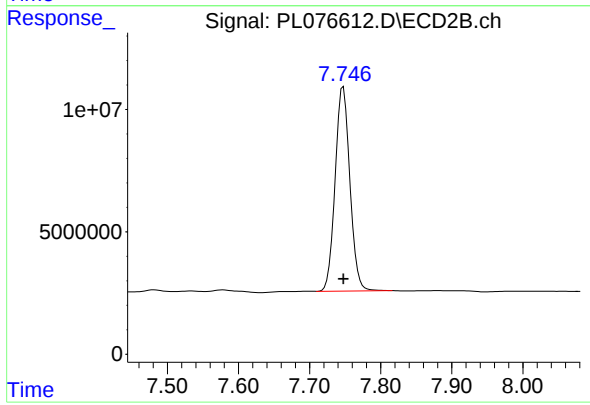

#28 Decachlorobiphenyl

R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 120208192
Conc: 50.00 ng/ml