

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
 Data File : PL076613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2022 00:22
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 02:05:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 02:05:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.640	23184141	78458625	24.325	24.684
28)	SA Decachlor...	8.908	7.747	20809349	60055228	26.558	26.034
Target Compounds							
23)	Chlordane-1	4.580	3.621	8586948	22075722	247.526	253.950
24)	Chlordane-2	5.113	4.193	9539122	26878056	257.201	259.237
25)	Chlordane-3	5.824	4.817	33862706	68625731	241.924	242.651
26)	Chlordane-4	5.903	4.879	42291168	72166352	245.534	245.702
27)	Chlordane-5	6.760	5.543	7635235	19846551	247.536	245.735



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
Data File : PL076613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2022 00:22
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 02:05:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 02:05:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

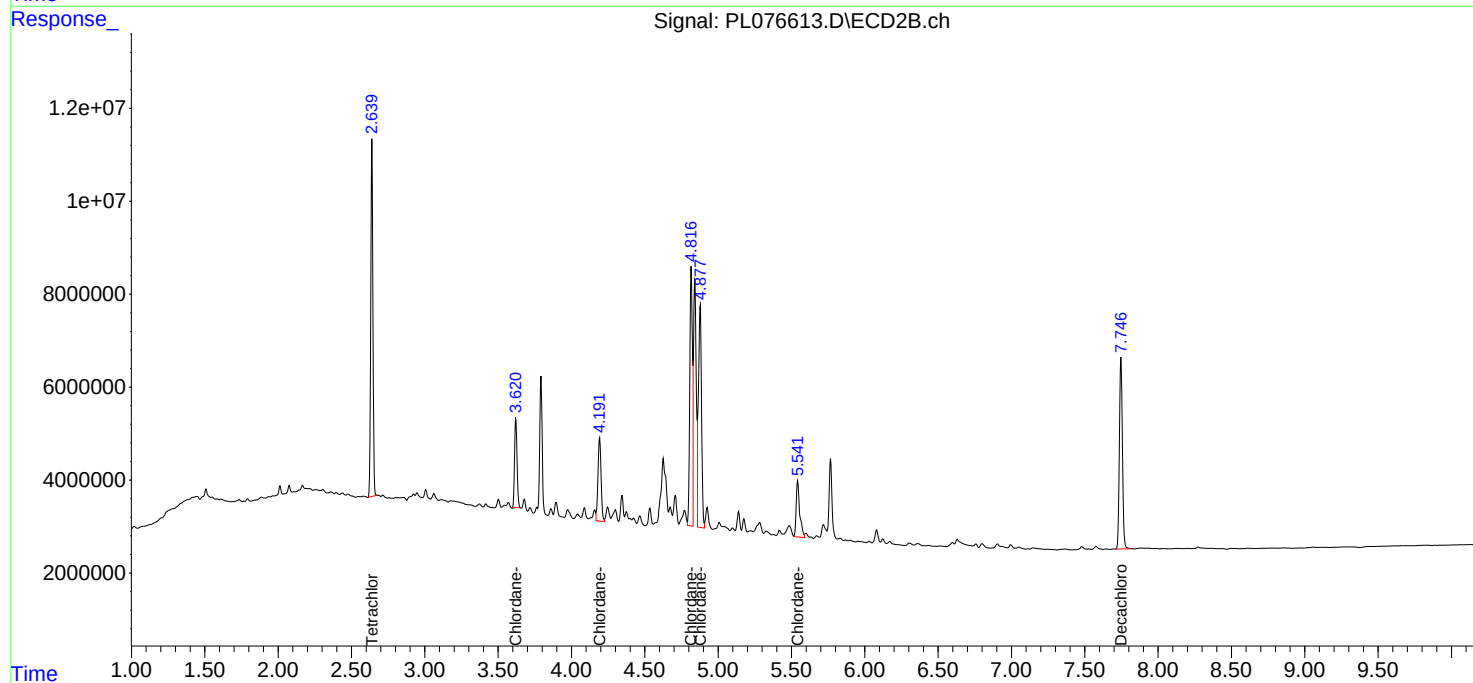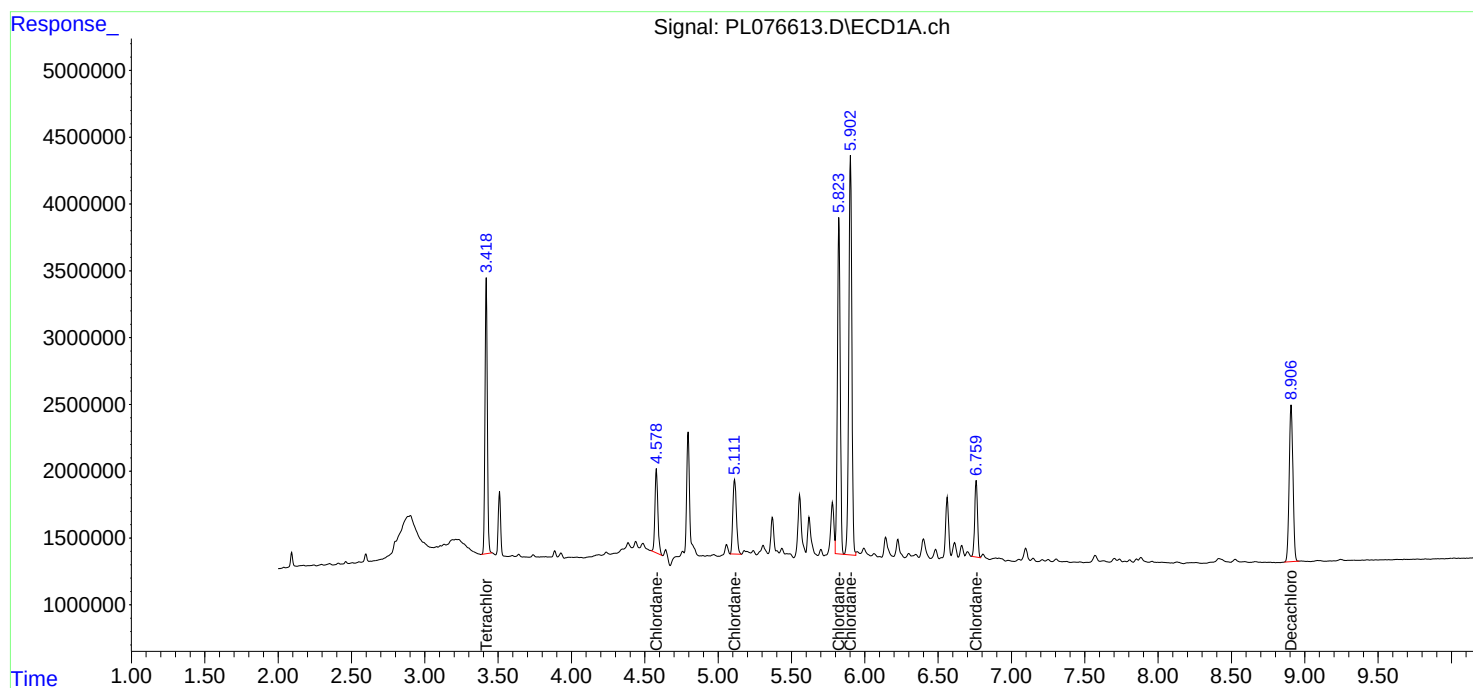


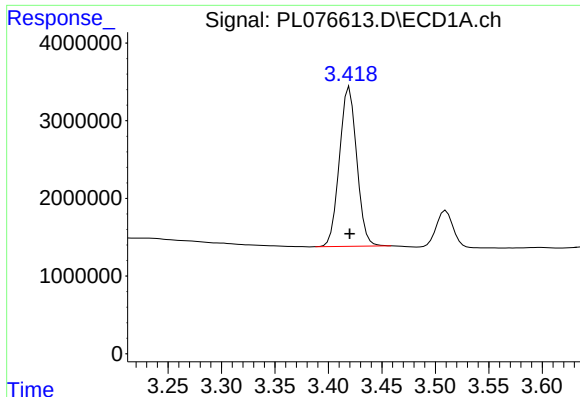

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 23184141
Conc: 24.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

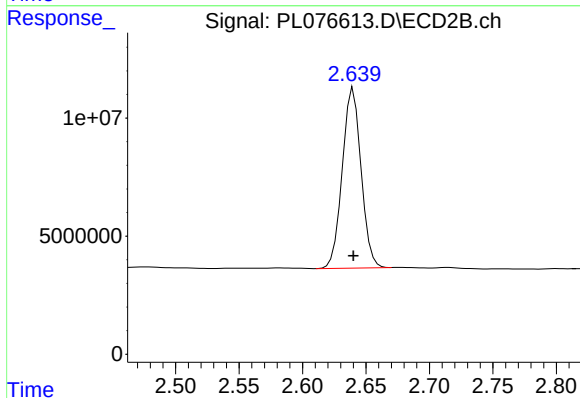


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: 0.000 min
Response: 78458625
Conc: 24.68 ng/ml

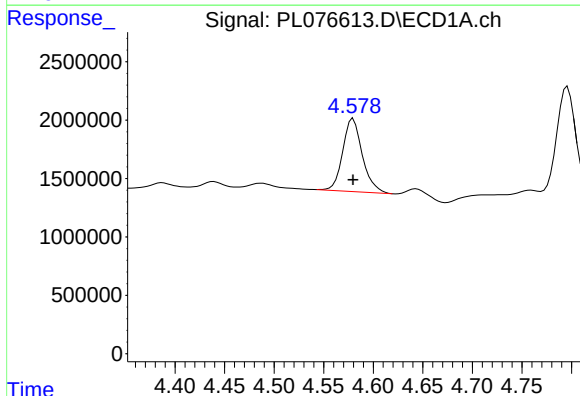


#23 Chlordane-1

R.T.: 4.580 min
Delta R.T.: 0.000 min
Response: 8586948
Conc: 247.53 ng/ml

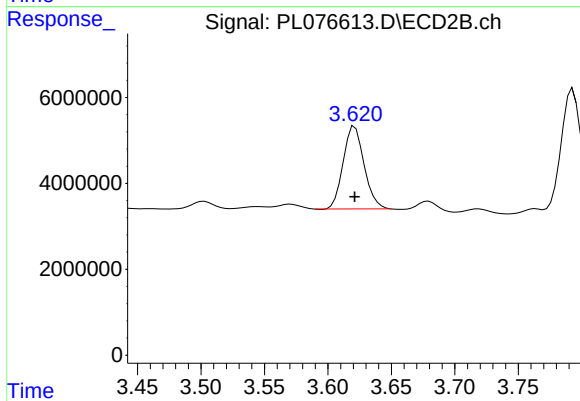

#23 Chlordane-1


R.T.: 3.621 min
Delta R.T.: 0.000 min
Response: 22075722
Conc: 253.95 ng/ml

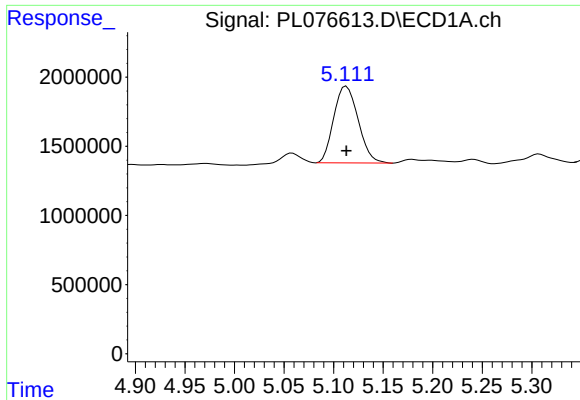

#24 Chlordane-2


R.T.: 5.113 min
Delta R.T.: 0.000 min
Response: 9539122
Conc: 257.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

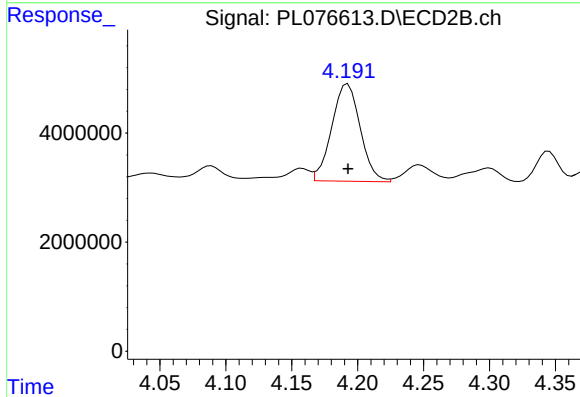


#24 Chlordane-2

R.T.: 4.193 min
Delta R.T.: 0.000 min
Response: 26878056
Conc: 259.24 ng/ml

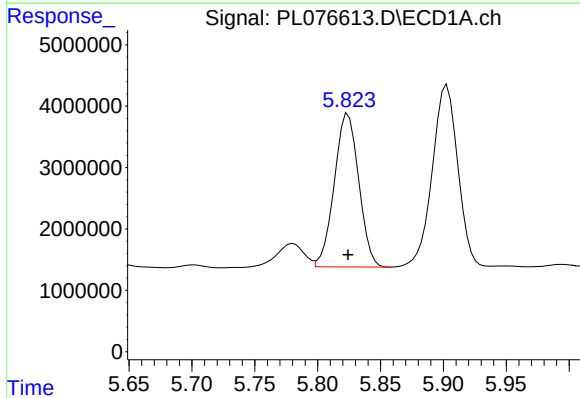


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 33862706
Conc: 241.92 ng/ml

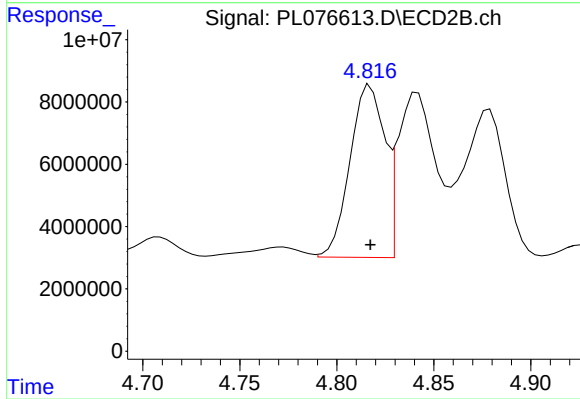

#25 Chlordane-3


R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 68625731
Conc: 242.65 ng/ml

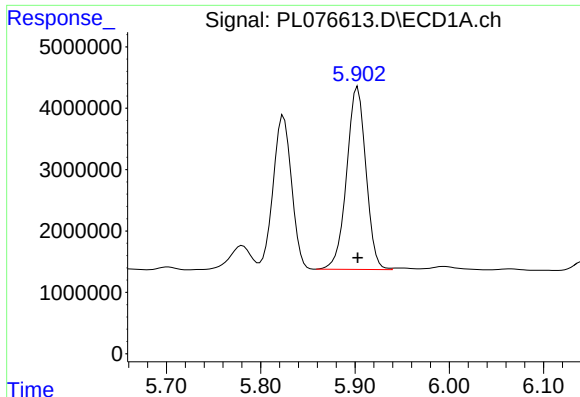

#26 Chlordane-4


R.T.: 5.903 min
Delta R.T.: 0.000 min
Response: 42291168
Conc: 245.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

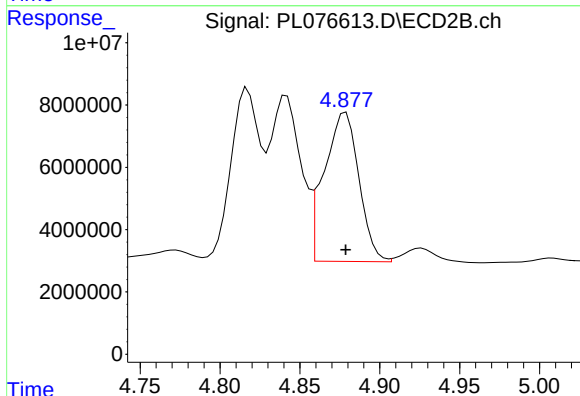


#26 Chlordane-4

R.T.: 4.879 min
Delta R.T.: 0.000 min
Response: 72166352
Conc: 245.70 ng/ml

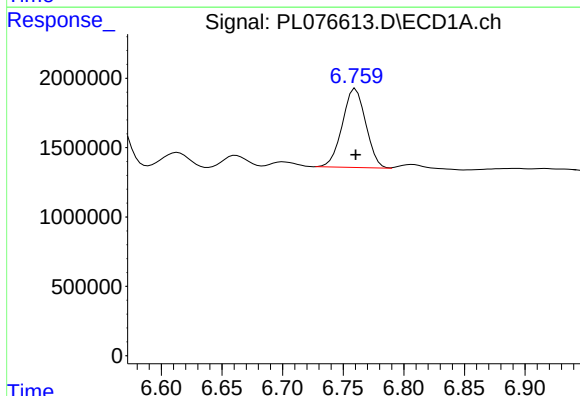


#27 Chlordane-5

R.T.: 6.760 min
Delta R.T.: 0.000 min
Response: 7635235
Conc: 247.54 ng/ml

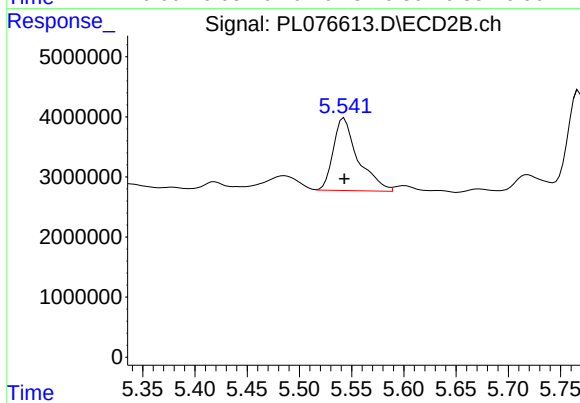

#27 Chlordane-5


R.T.: 5.543 min
Delta R.T.: 0.000 min
Response: 19846551
Conc: 245.73 ng/ml

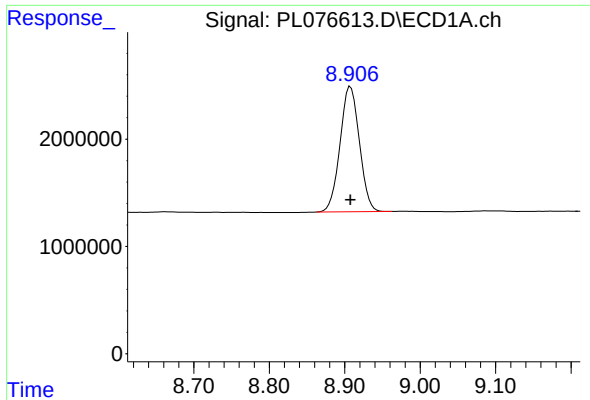

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 20809349
Conc: 26.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

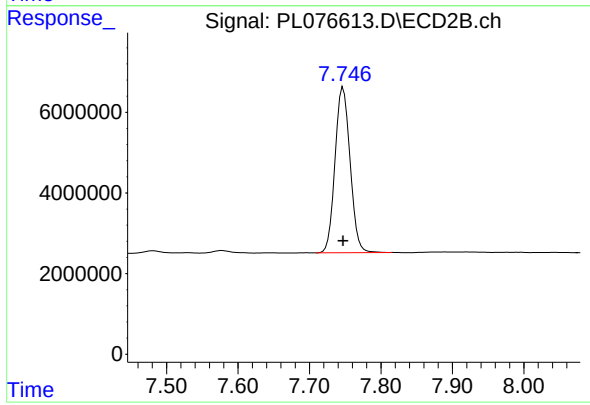

#28 Decachlorobiphenyl

R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 60055228
Conc: 26.03 ng/ml