

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
 Data File : PL076614.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2022 00:36
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/26/2022
 Supervised By : Ankita Jodhani 07/26/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 02:13:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 02:13:36 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.640	4314581	15842957	4.614	4.987
28)	SA Decachlor...	8.908	7.747	4277814	12401484	5.361	5.296
Target Compounds							
23)	Chlordane-1	4.579	3.621	1500345	5201581	44.449	57.572 #
24)	Chlordane-2	5.113	4.191	1736979	5299081	47.434	51.007m
25)	Chlordane-3	5.824	4.817	6642789	14210592	47.945	50.197
26)	Chlordane-4	5.903	4.878	8424597	15473661	49.125	52.123
27)	Chlordane-5	6.761	5.542	1284275	3864335	43.078	47.611m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072622\
Data File : PL076614.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2022 00:36
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/26/2022
Supervised By : Ankita Jodhani 07/26/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 02:13:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 02:13:36 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

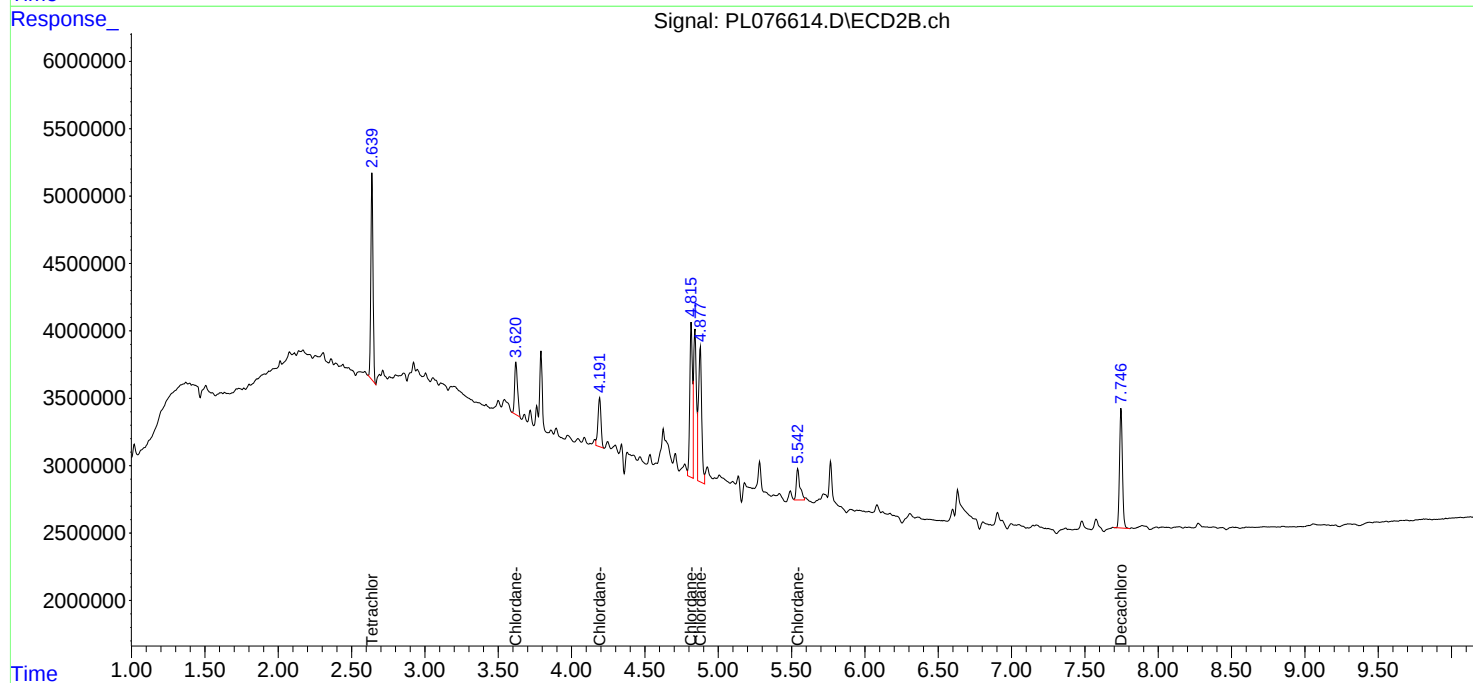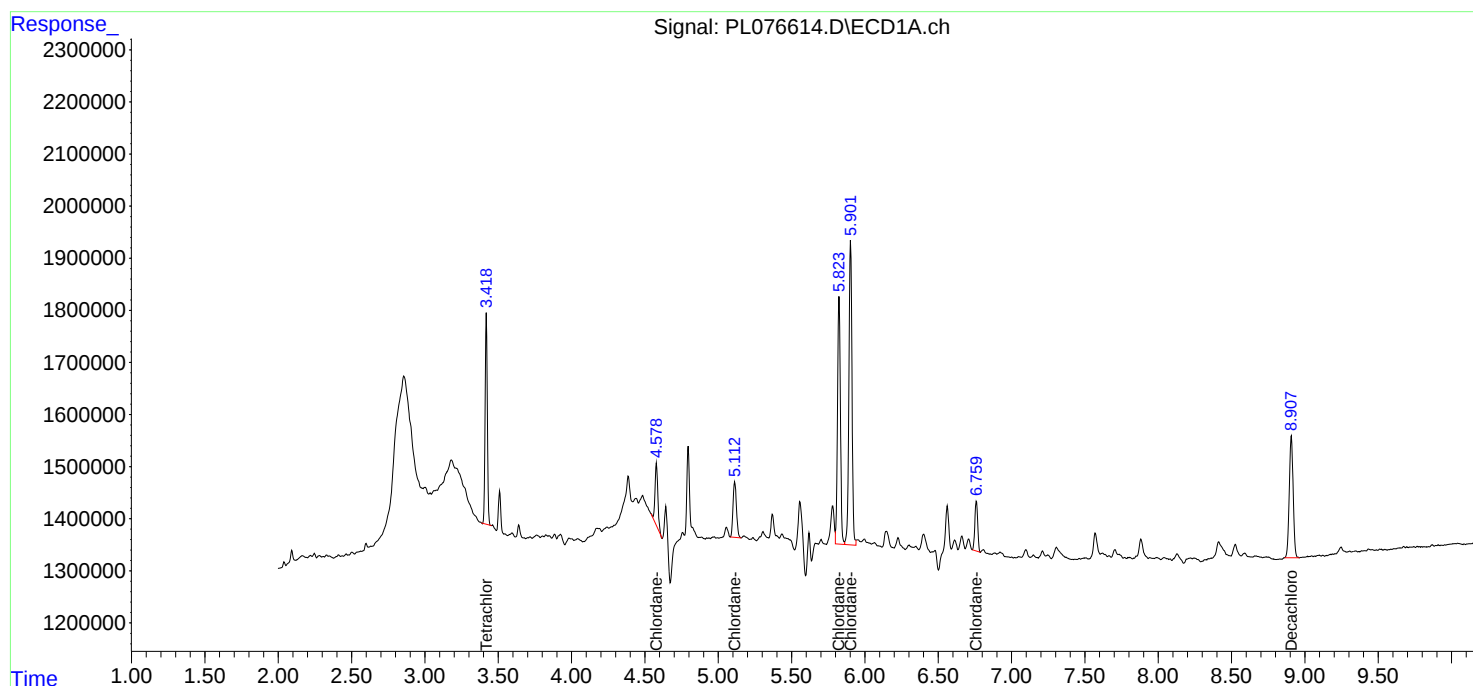

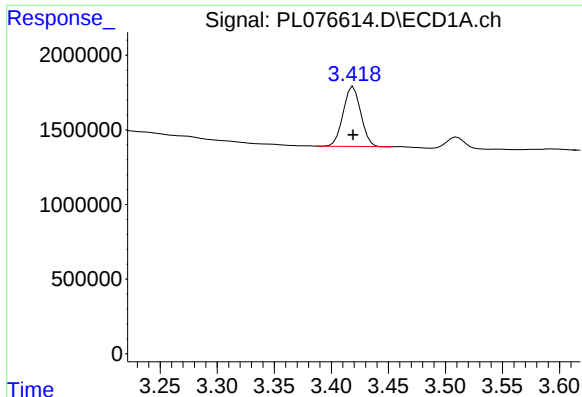


#1 Tetrachloro-m-xylene

R.T.: 3.419 min
Delta R.T.: 0.000 min
Response: 4314581
Conc: 4.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/26/2022
Supervised By :Ankita Jodhani 07/26/2022

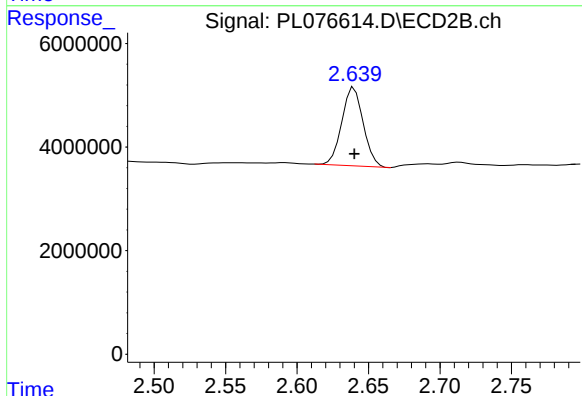


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: 0.000 min
Response: 15842957
Conc: 4.99 ng/ml

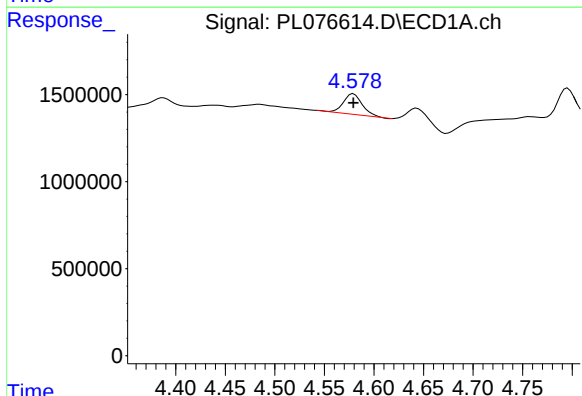


#23 Chlordane-1

R.T.: 4.579 min
Delta R.T.: 0.000 min
Response: 1500345
Conc: 44.45 ng/ml

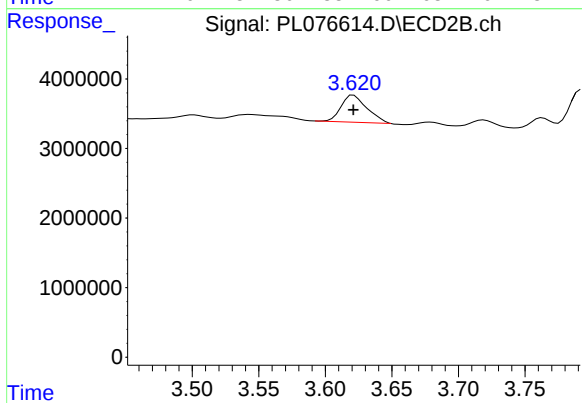

#23 Chlordane-1

R.T.: 3.621 min
Delta R.T.: 0.000 min
Response: 5201581
Conc: 57.57 ng/ml

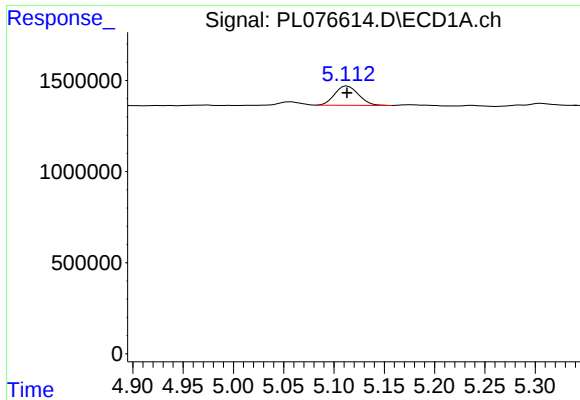


#24 Chlordane-2

R.T.: 5.113 min
Delta R.T.: 0.000 min
Response: 1736979
Conc: 47.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/26/2022
Supervised By :Ankita Jodhani 07/26/2022

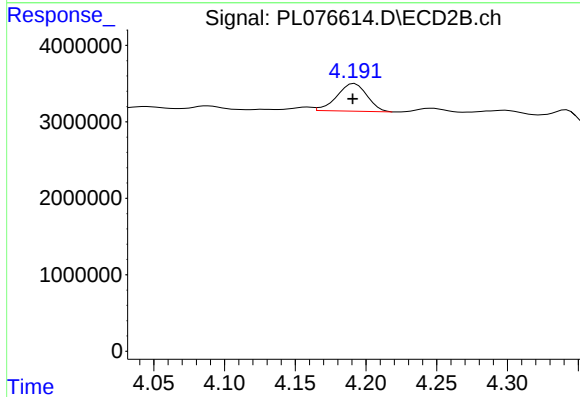


#24 Chlordane-2

R.T.: 4.191 min
Delta R.T.: 0.000 min
Response: 5299081
Conc: 51.01 ng/ml m

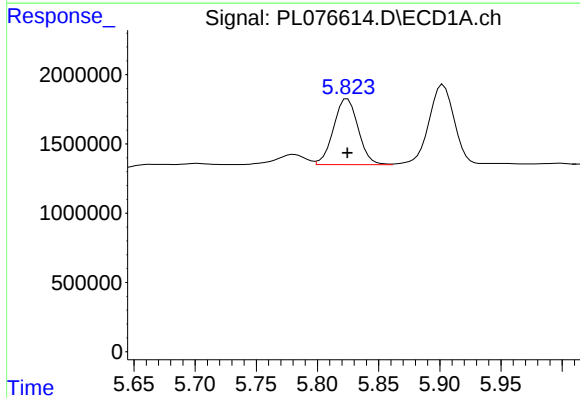


#25 Chlordane-3

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 6642789
Conc: 47.95 ng/ml

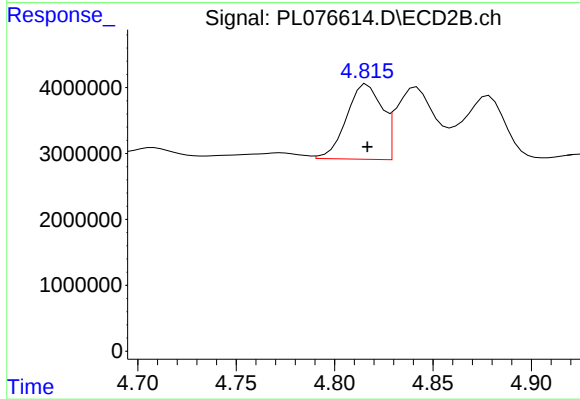

#25 Chlordane-3

R.T.: 4.817 min
Delta R.T.: 0.000 min
Response: 14210592
Conc: 50.20 ng/ml

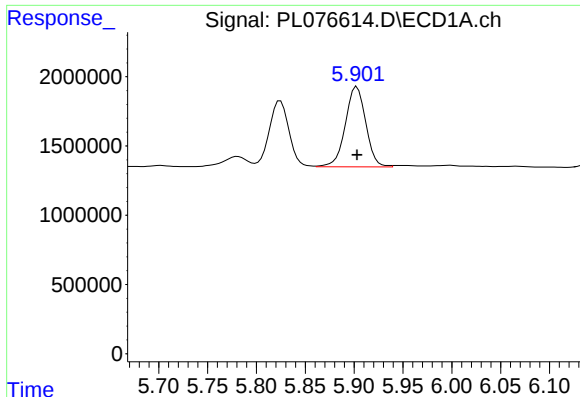


#26 Chlordane-4

R.T.: 5.903 min
Delta R.T.: 0.000 min
Response: 8424597
Conc: 49.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/26/2022
Supervised By :Ankita Jodhani 07/26/2022

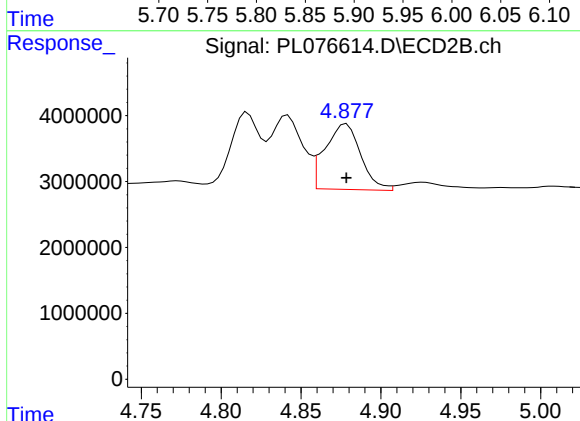


#26 Chlordane-4

R.T.: 4.878 min
Delta R.T.: 0.000 min
Response: 15473661
Conc: 52.12 ng/ml

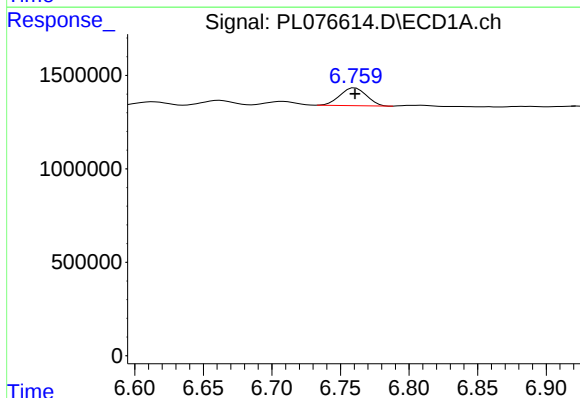


#27 Chlordane-5

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 1284275
Conc: 43.08 ng/ml

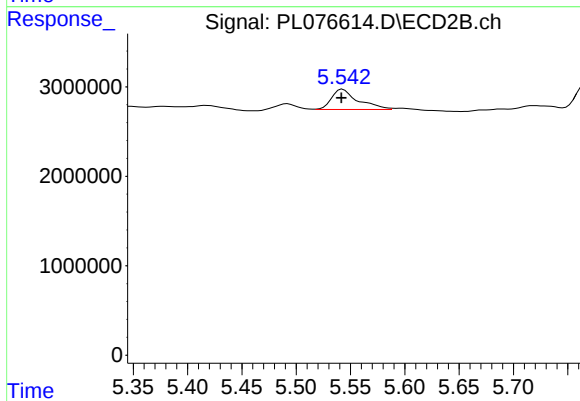

#27 Chlordane-5

R.T.: 5.542 min
Delta R.T.: 0.000 min
Response: 3864335
Conc: 47.61 ng/ml m

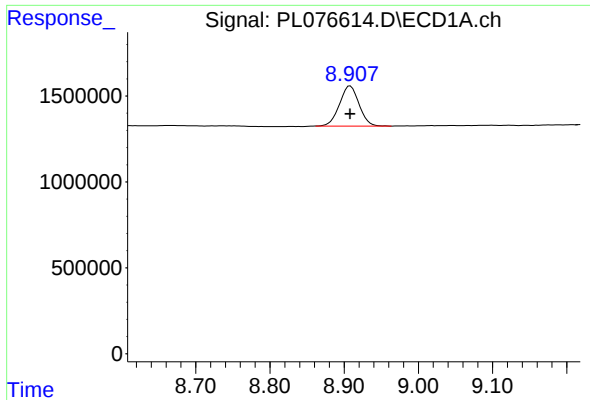


#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.000 min
Response: 4277814
Conc: 5.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/26/2022
Supervised By :Ankita Jodhani 07/26/2022

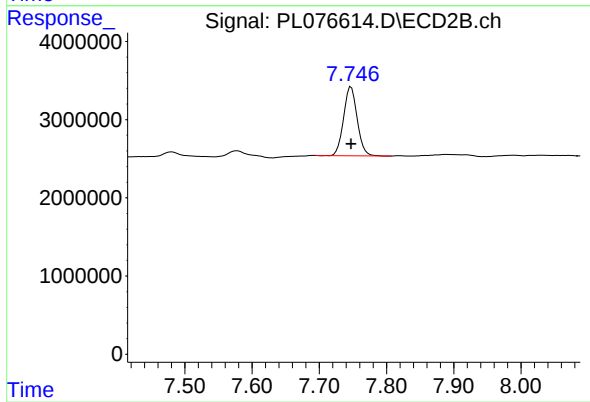

#28 Decachlorobiphenyl

R.T.: 7.747 min
Delta R.T.: 0.000 min
Response: 12401484
Conc: 5.30 ng/ml