

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072623\
 Data File : PL084245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2023 19:38
 Operator : AR\AJ
 Sample : 03770-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HOWE-1-LP

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/27/2023
 Supervised By : Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 21:38:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.474	2.687	17699851	8875783	8.850m	7.992
2) SA Decachlor...	9.023	7.868	17882895	13372485	13.739	12.035

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072623\
Data File : PL084245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2023 19:38
Operator : AR\AJ
Sample : 03770-07
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HOWE-1-LP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/27/2023
Supervised By : Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 21:38:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

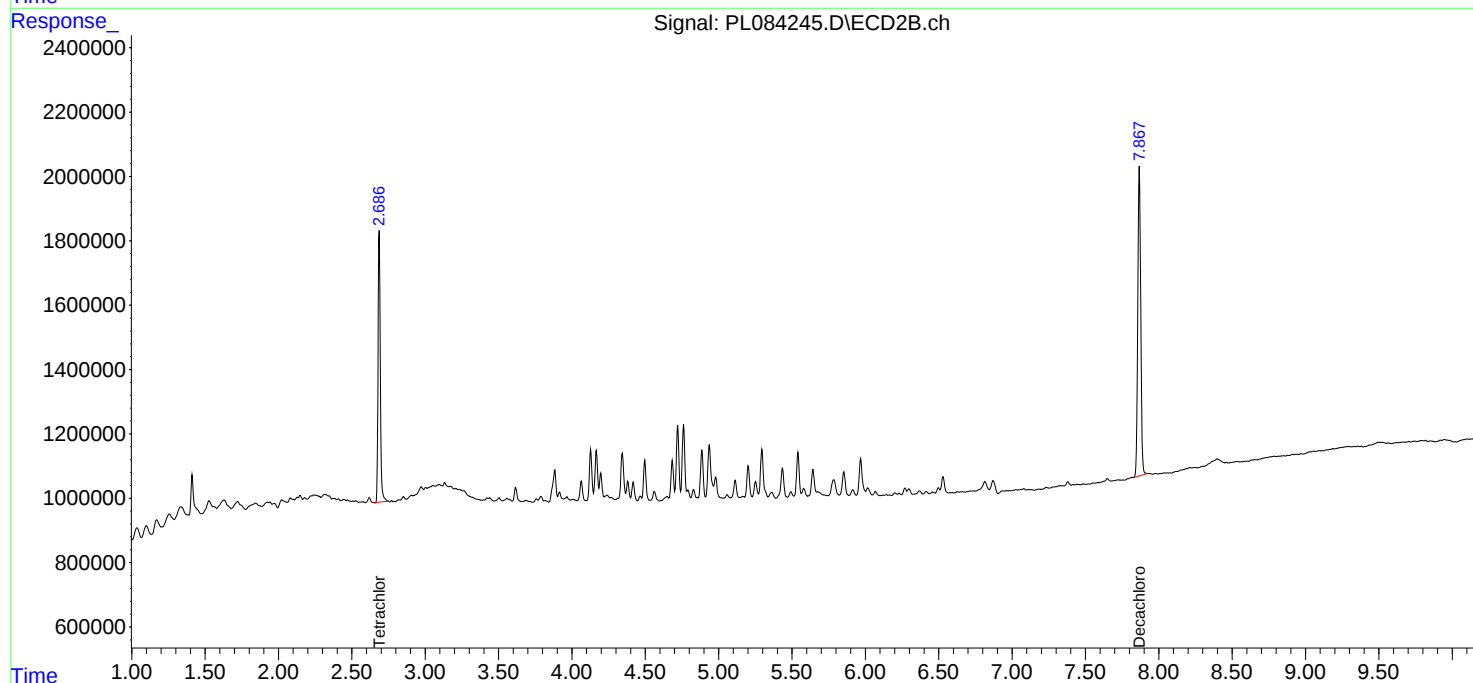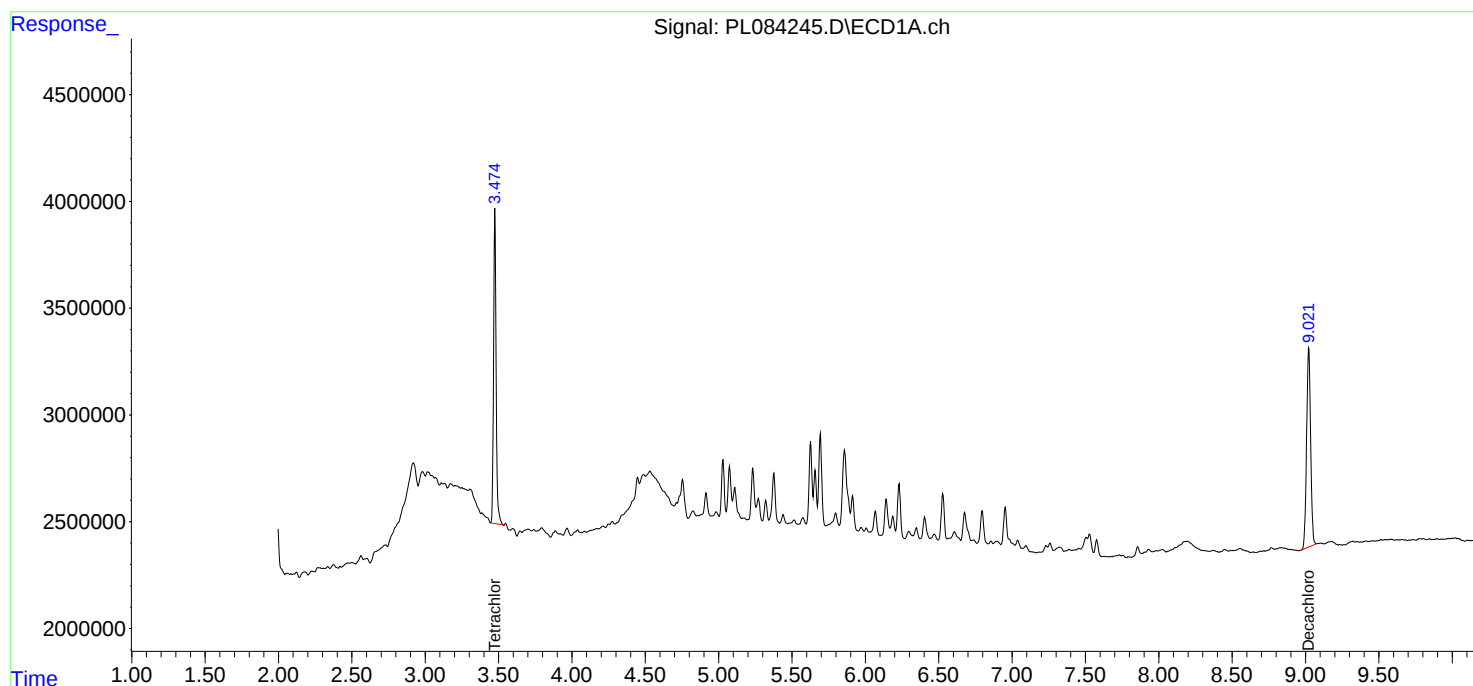

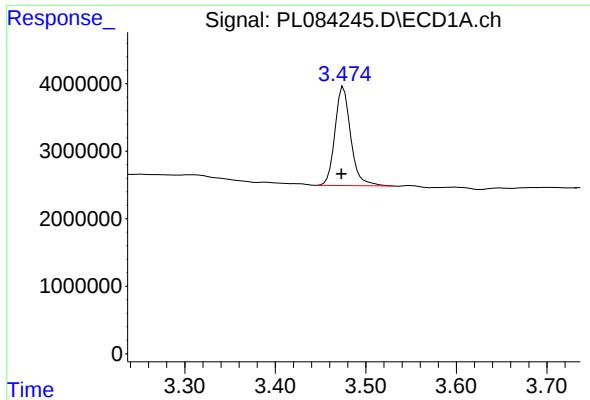


#1 Tetrachloro-m-xylene

R.T.: 3.474 min
Delta R.T.: 0.000 min
Response: 17699851
Conc: 8.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
HOWE-1-LP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

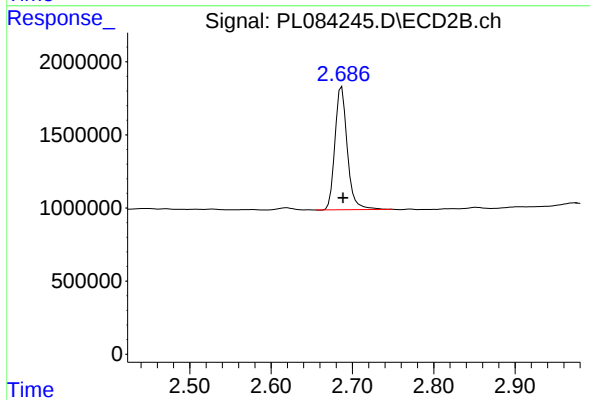


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: -0.001 min
Response: 8875783
Conc: 7.99 ng/ml

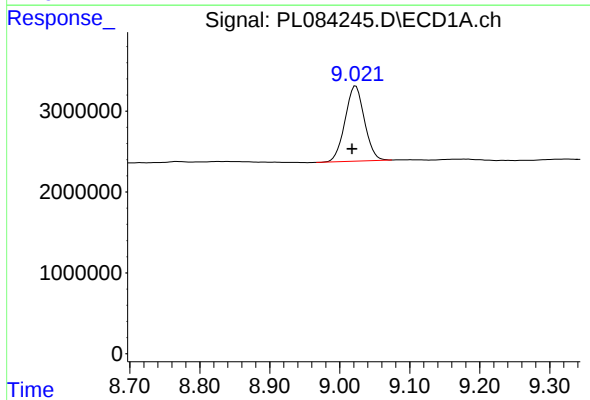

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.005 min
Response: 17882895
Conc: 13.74 ng/ml

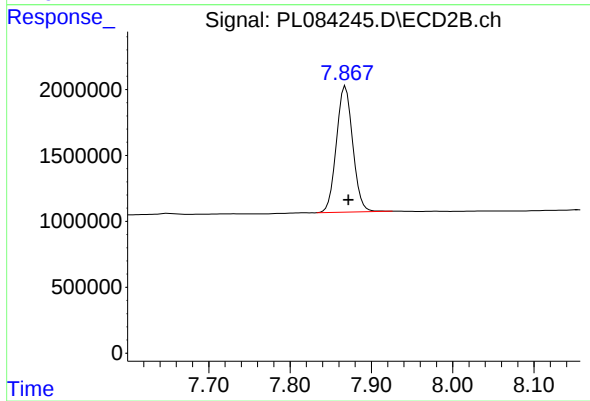

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: -0.003 min
Response: 13372485
Conc: 12.04 ng/ml