

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072623\
 Data File : PL084259.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2023 01:16
 Operator : AR\AJ
 Sample : 03769-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-P40A

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/27/2023
 Supervised By :Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 03:17:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.476	2.688	39811498	20318338	19.907	18.295
28) SA Decachlor...	9.022	7.869	28672650	22583402	22.028	20.325
Target Compounds						
12) B 4,4'-DDE	6.146	5.165	5211703	2576361	2.590m	2.097

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072623\
Data File : PL084259.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2023 01:16
Operator : AR\AJ
Sample : 03769-09
Misc :
ALS Vial : 39 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
B-P40A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/27/2023
Supervised By : Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 03:17:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

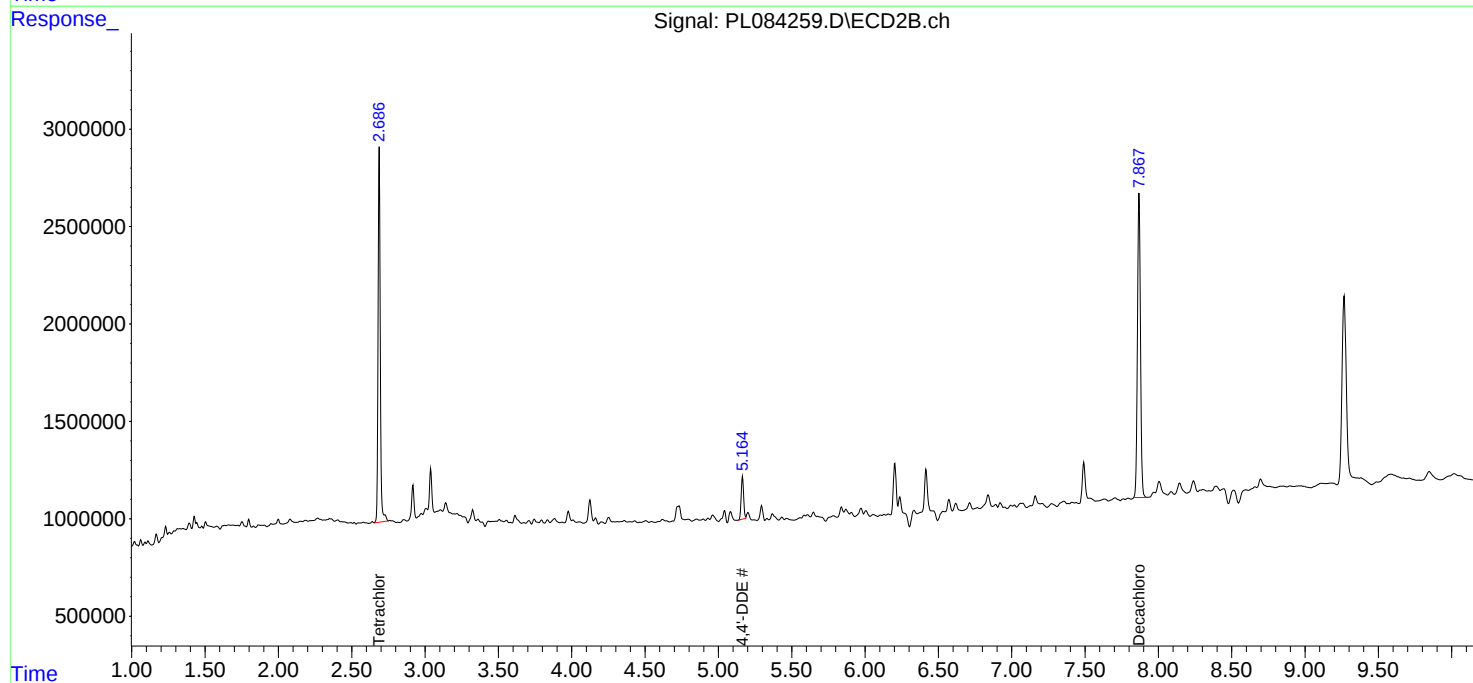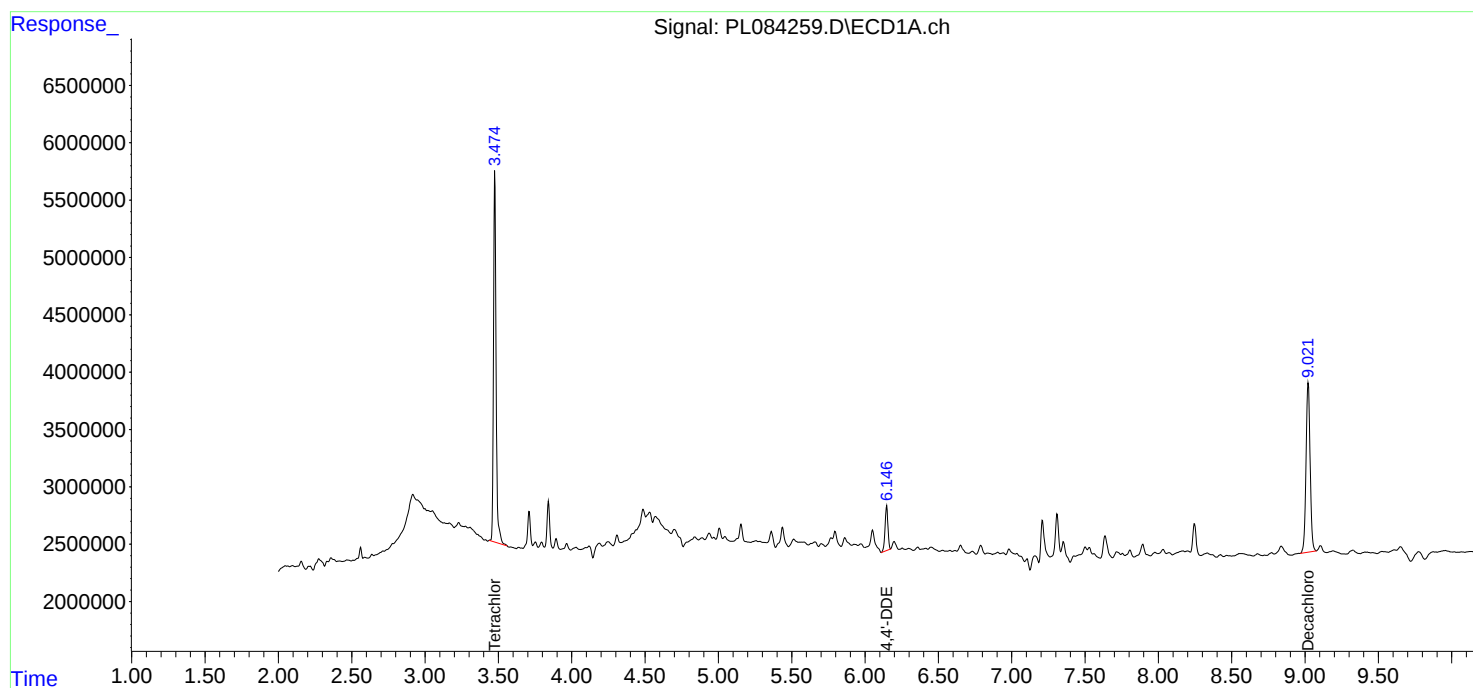

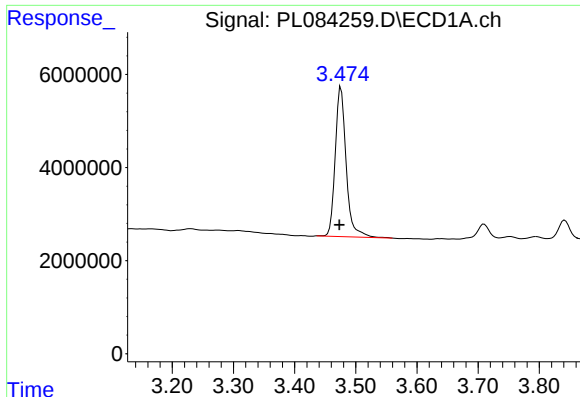


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 39811498
Conc: 19.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-P40A


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

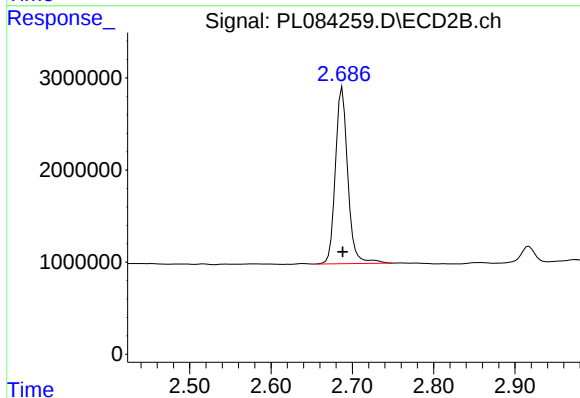


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: 0.000 min
Response: 20318338
Conc: 18.30 ng/ml

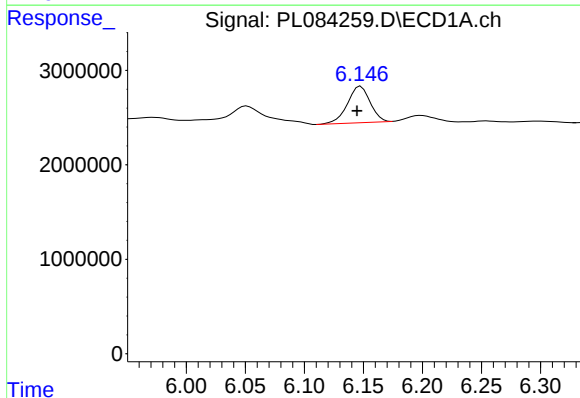


#12 4,4'-DDE

R.T.: 6.146 min
Delta R.T.: 0.002 min
Response: 5211703
Conc: 2.59 ng/ml m

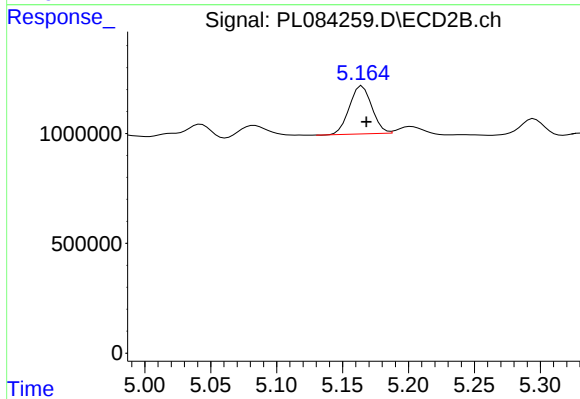

#12 4,4'-DDE

R.T.: 5.165 min
Delta R.T.: -0.003 min
Response: 2576361
Conc: 2.10 ng/ml

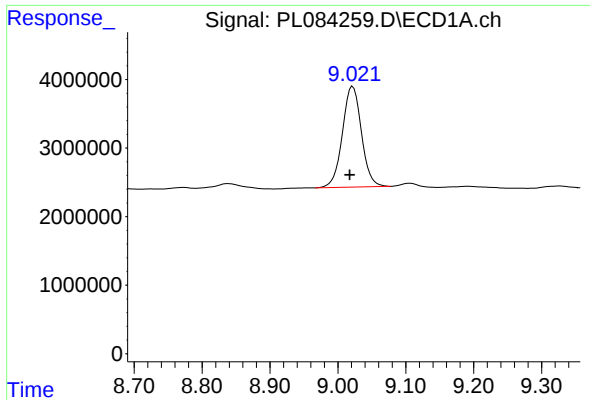


#28 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: 0.004 min
Response: 28672650
Conc: 22.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-P40A

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

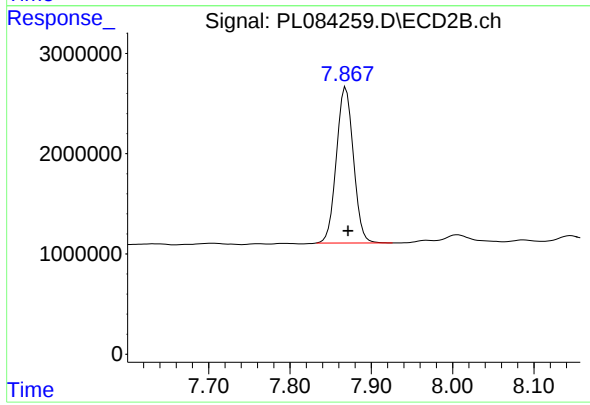

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: -0.003 min
Response: 22583402
Conc: 20.32 ng/ml