

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072623\
 Data File : PL084272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2023 04:59
 Operator : AR\AJ
 Sample : 03756-13
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RRTP-13-CS-13

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/27/2023
 Supervised By : Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 07:02:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.687	15982320	7220244	7.992	6.501
28)	SA Decachlor...	9.023	7.869	15709270	11445941	12.069	10.301
Target Compounds							
12)	B 4,4'-DDE	6.146	5.164	2002605	584639	0.995	0.476m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072623\
Data File : PL084272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2023 04:59
Operator : AR\AJ
Sample : 03756-13
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleID :
RRTP-13-CS-13


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/27/2023
Supervised By : Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 07:02:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

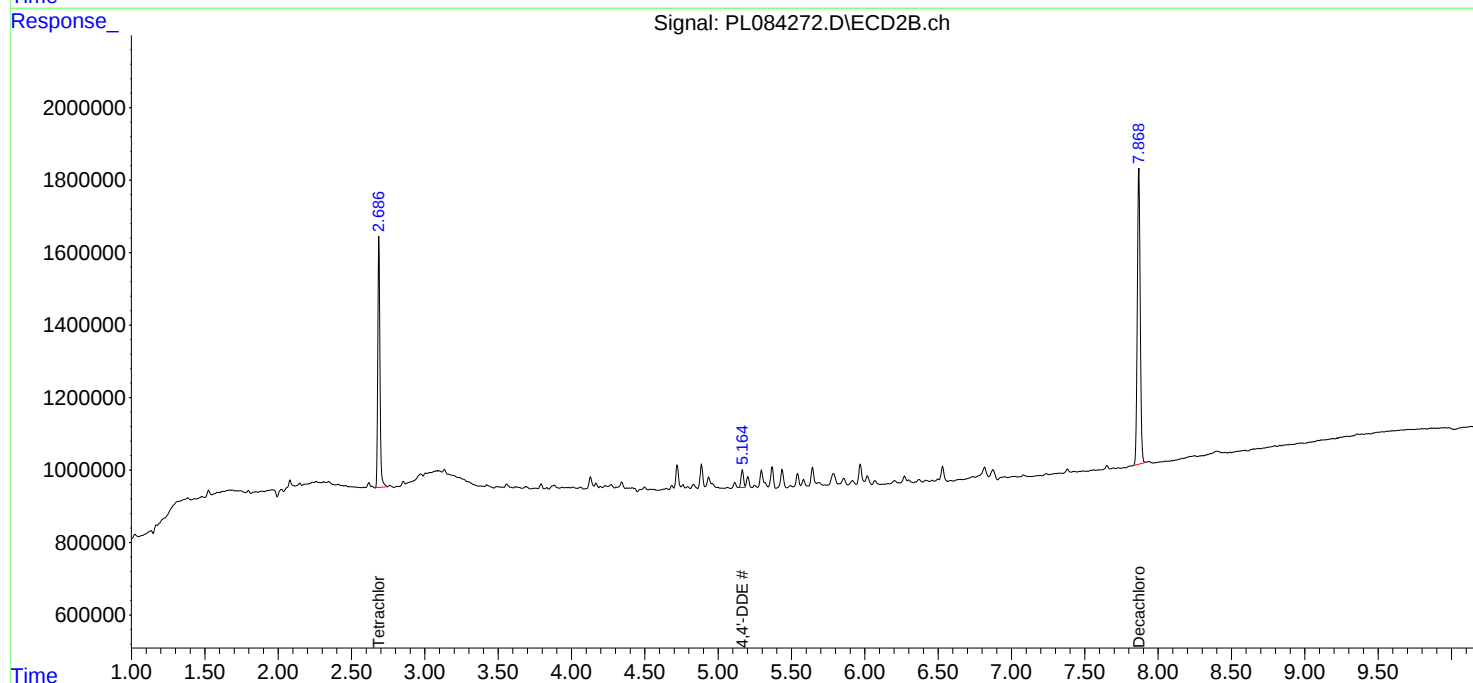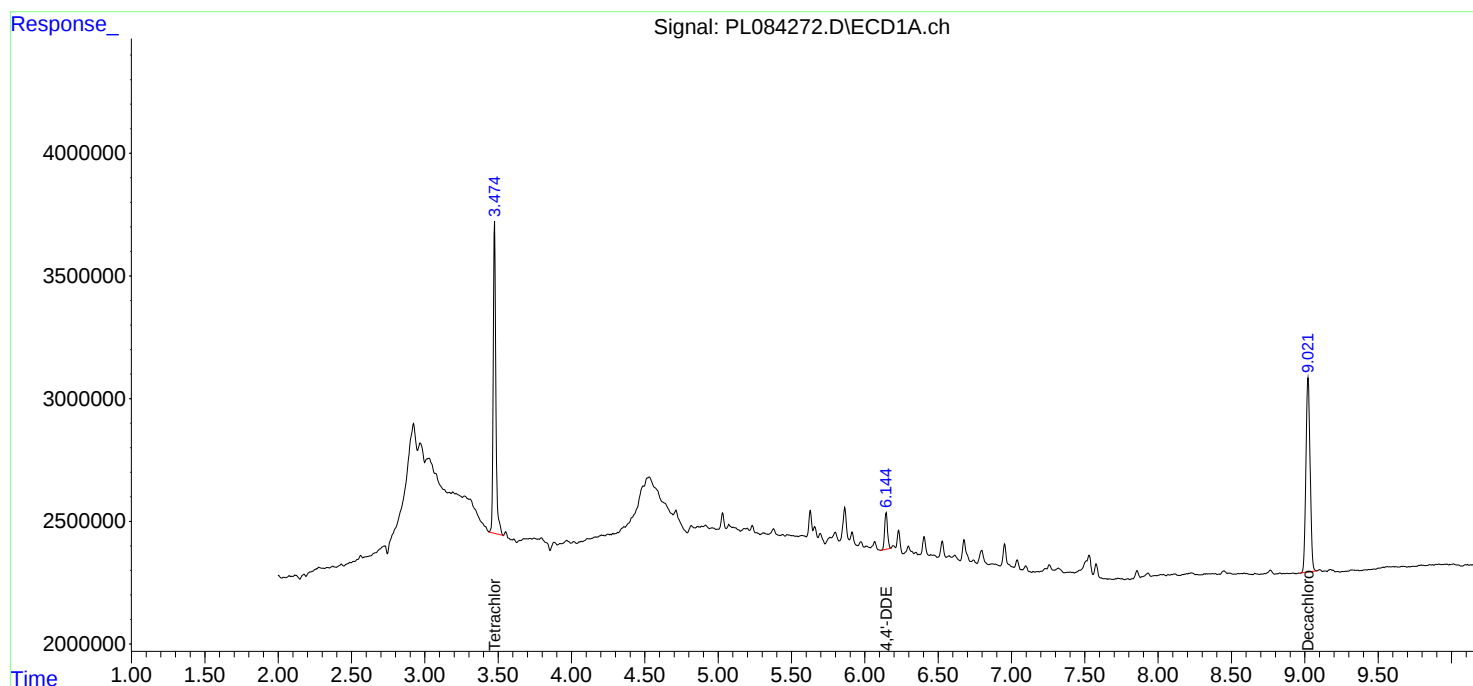

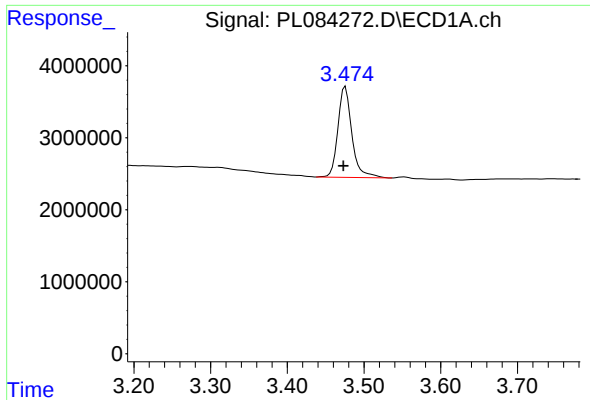


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 15982320
Conc: 7.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
RRTP-13-CS-13


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

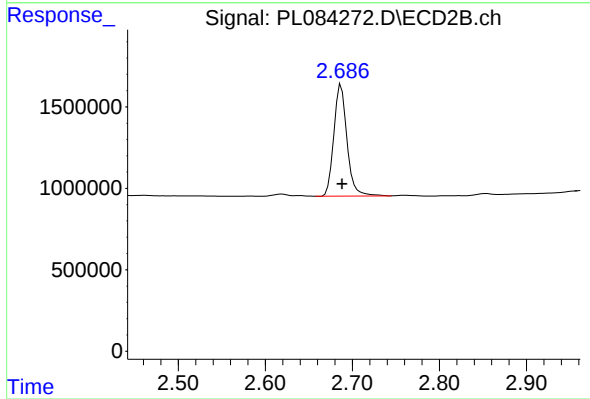


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: -0.001 min
Response: 7220244
Conc: 6.50 ng/ml

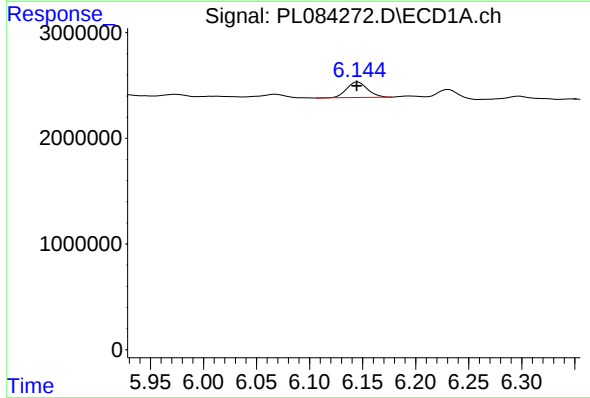


#12 4,4'-DDE

R.T.: 6.146 min
Delta R.T.: 0.001 min
Response: 2002605
Conc: 1.00 ng/ml

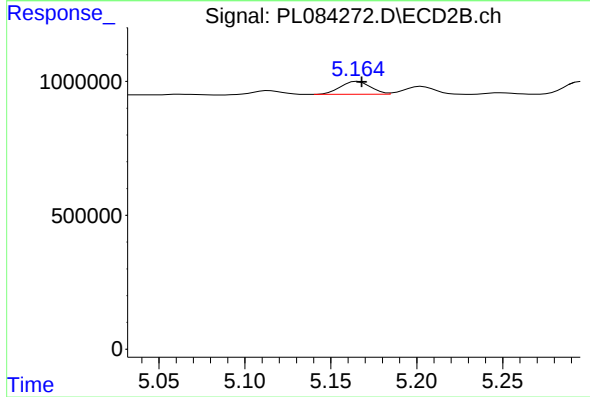

#12 4,4'-DDE

R.T.: 5.164 min
Delta R.T.: -0.004 min
Response: 584639
Conc: 0.48 ng/ml m

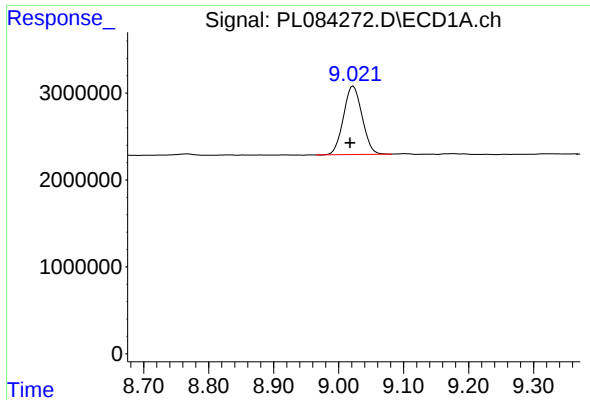


#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.005 min
Response: 15709270
Conc: 12.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
RRTP-13-CS-13

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

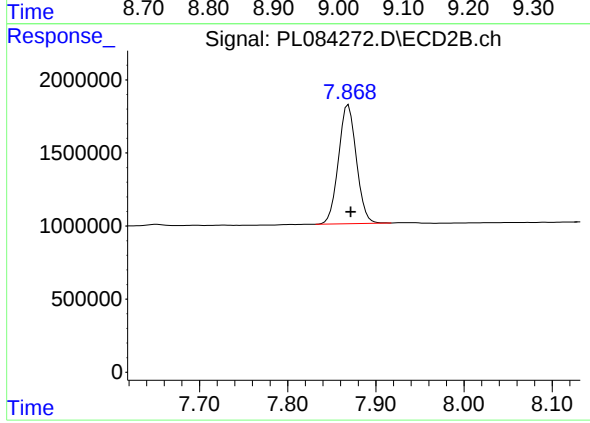

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: -0.003 min
Response: 11445941
Conc: 10.30 ng/ml