

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072623\
 Data File : PL084281.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2023 07:04
 Operator : AR\AJ
 Sample : 03771-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PATERSON-GSMP-COMP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/27/2023
 Supervised By :Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 07:22:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.475	2.686	22137835	11480245	11.070m	10.337m
28) SA Decachlor...	9.024	7.868	13915836	9930269	10.691	8.937m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072623\
Data File : PL084281.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2023 07:04
Operator : AR\AJ
Sample : 03771-01
Misc :
ALS Vial : 58 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PATERSON-GSMP-COMP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/27/2023
Supervised By : Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 07:22:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

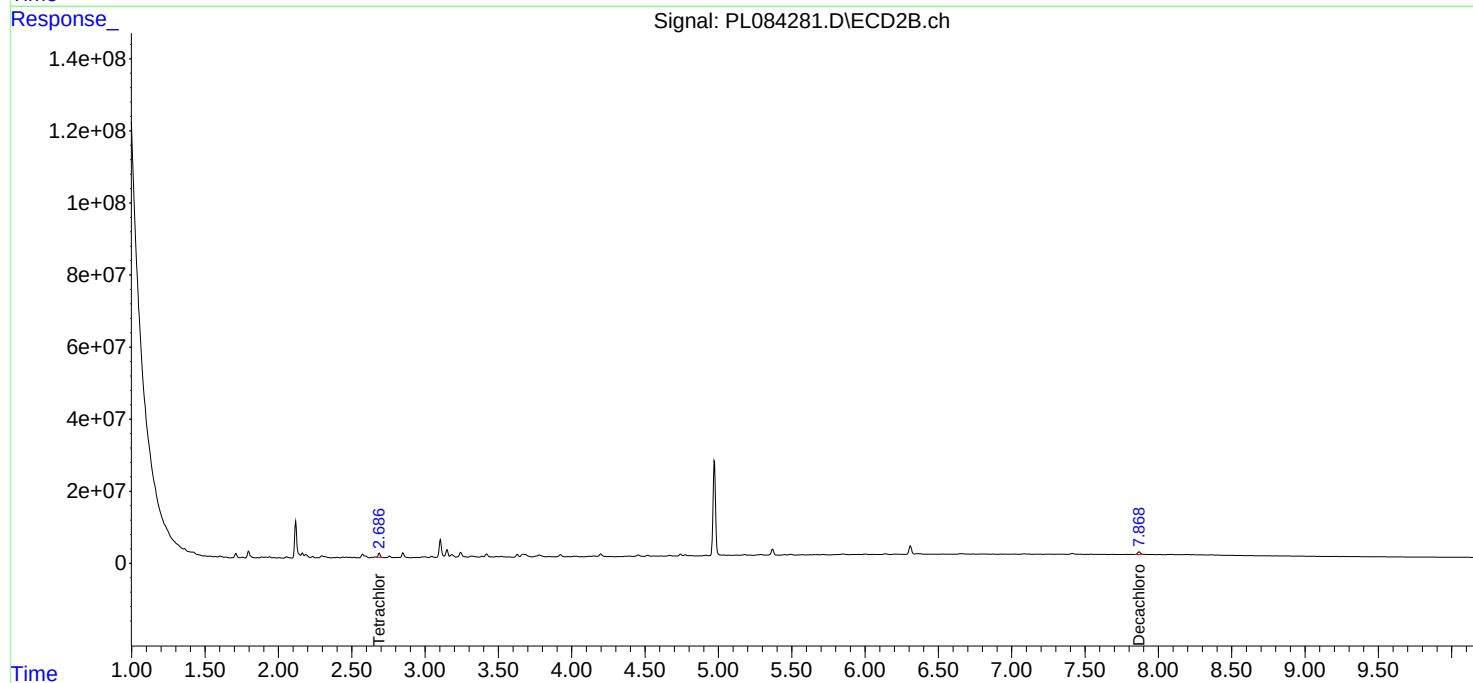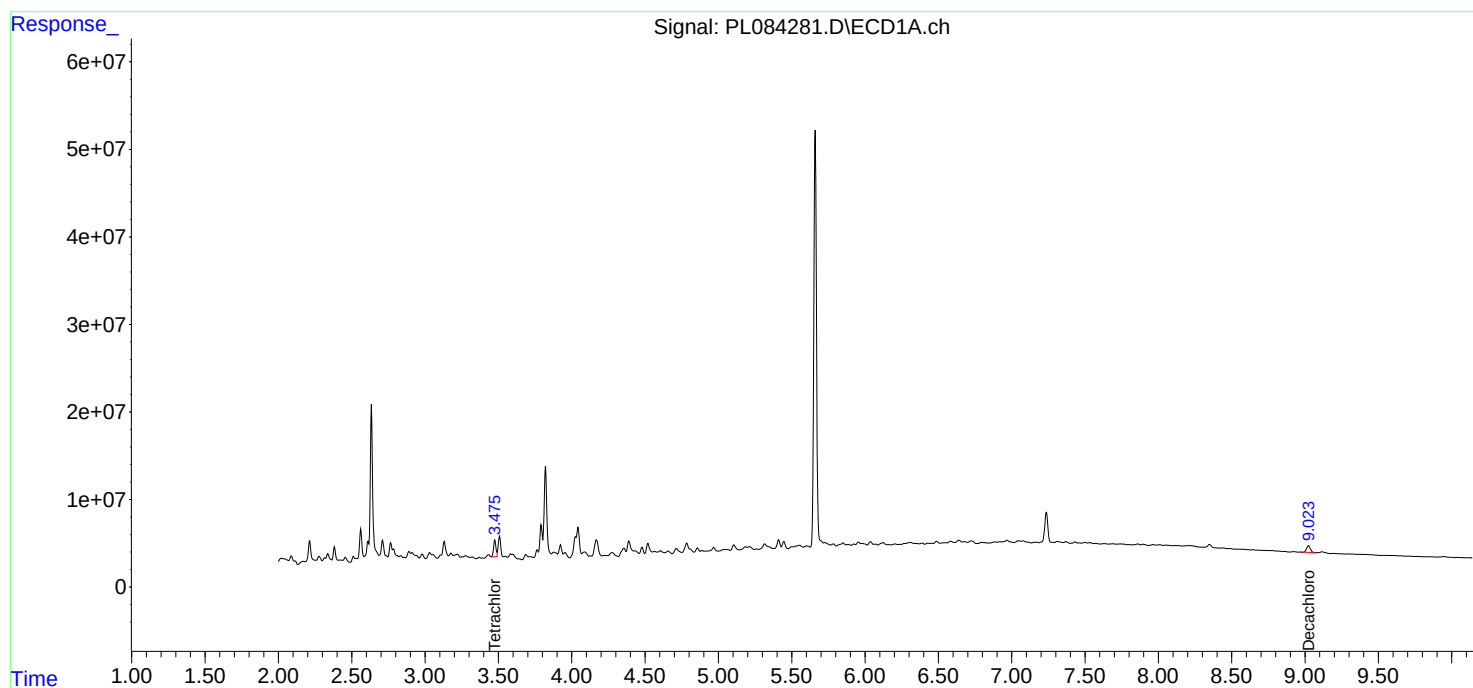

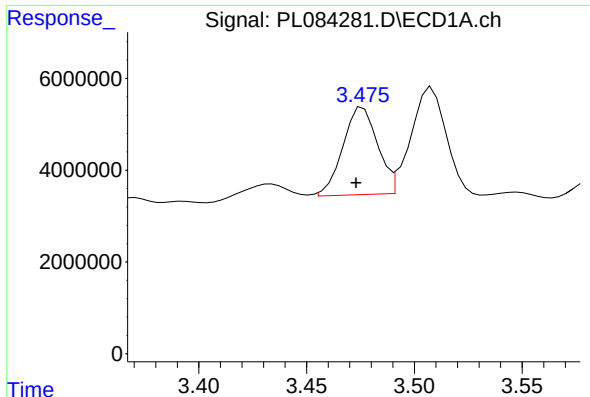


#1 Tetrachloro-m-xylene

R.T.: 3.475 min
Delta R.T.: 0.002 min
Response: 22137835
Conc: 11.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PATERSON-GSMP-COMP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

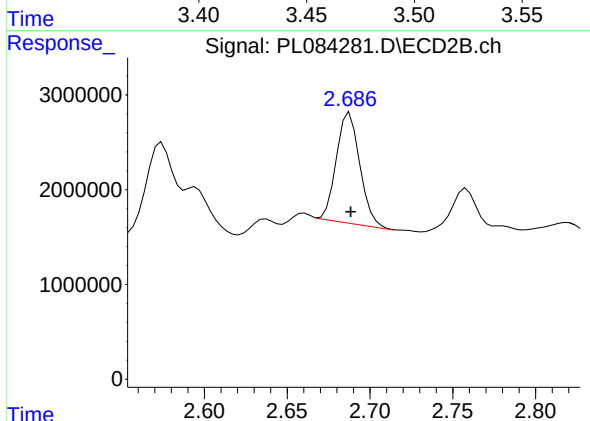


#1 Tetrachloro-m-xylene

R.T.: 2.686 min
Delta R.T.: -0.002 min
Response: 11480245
Conc: 10.34 ng/ml m

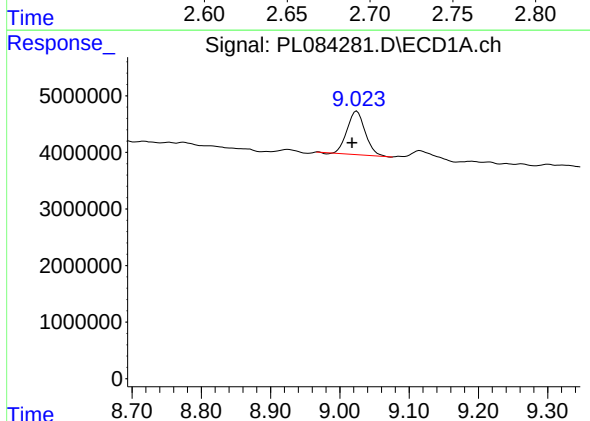

#28 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.007 min
Response: 13915836
Conc: 10.69 ng/ml

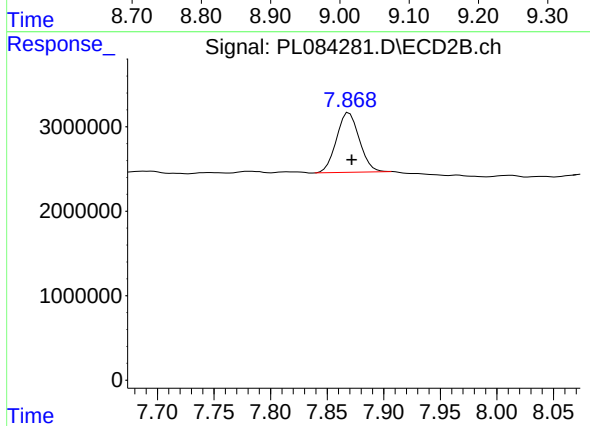

#28 Decachlorobiphenyl

R.T.: 7.868 min
Delta R.T.: -0.004 min
Response: 9930269
Conc: 8.94 ng/ml m