

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL072718\  
 Data File : PL038652.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 27 Jul 2018 13:21  
 Operator : AJ\SJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 27 22:45:50 2018  
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD\_L\methods\PL071318.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Jul 14 00:12:12 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |              |       |        |   |         |               |
|------------------|--------------|-------|--------|---|---------|---------------|
| 2) A             | alpha-BHC    | 0.000 | 4.301  | 0 | 370544  | N.D. 0.096 #  |
| 7) B             | delta-BHC    | 0.000 | 4.957  | 0 | 1769693 | N.D. 0.534 #  |
| 14) MA           | Endrin       | 0.000 | 6.631  | 0 | 458506  | N.D. 0.192 #  |
| 15) B            | Endosulfa... | 0.000 | 6.828  | 0 | 447805  | N.D. 0.186 #  |
| 16) A            | 4,4'-DDD     | 0.000 | 6.675f | 0 | 1597718 | N.D. 0.746 #  |
| 23)              | Chlordane-1  | 0.000 | 4.957  | 0 | 1769693 | N.D. 15.271 # |
| 27)              | Chlordane-5  | 0.000 | 6.828  | 0 | 447805  | N.D. 4.999 #  |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL072718\  
Data File : PL038652.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 27 Jul 2018 13:21  
Operator : AJ\SJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 27 22:45:50 2018  
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD\_L\methods\PL071318.M  
Quant Title : GC Extractables  
QLast Update : Sat Jul 14 00:12:12 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

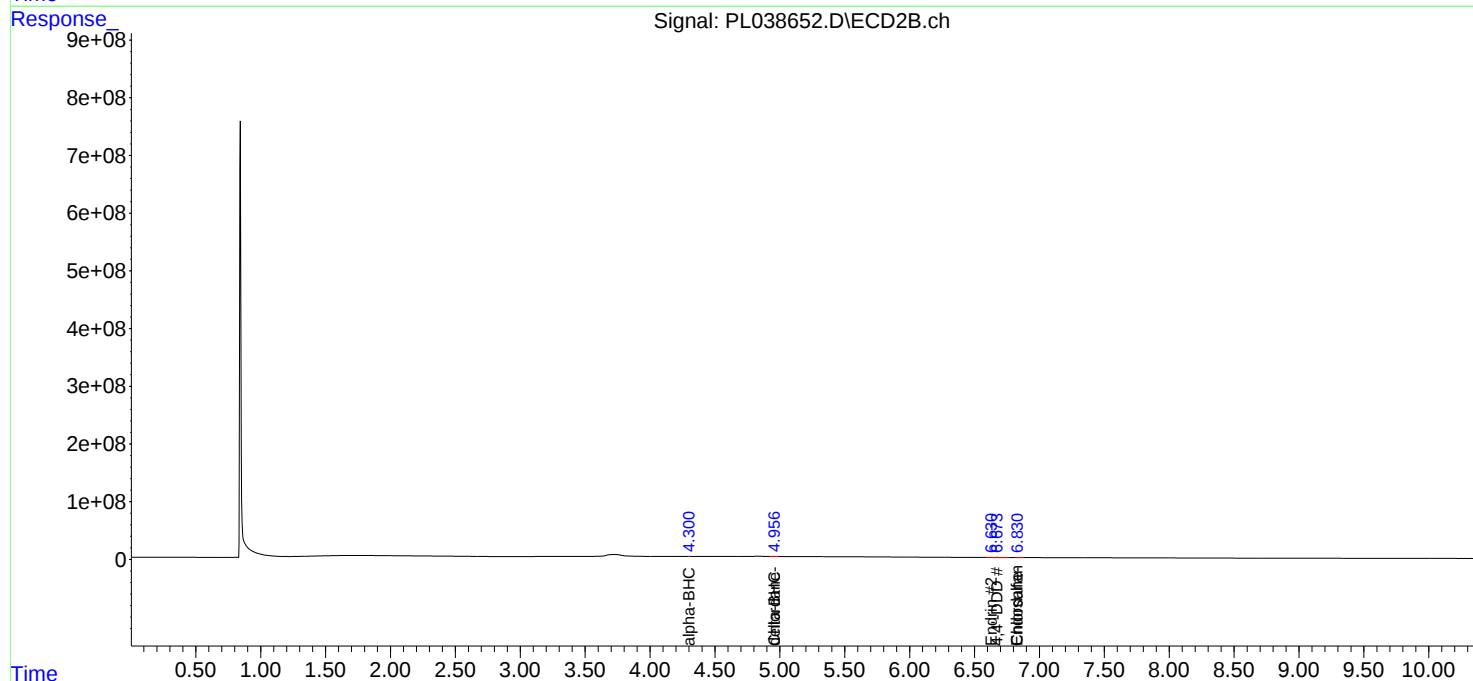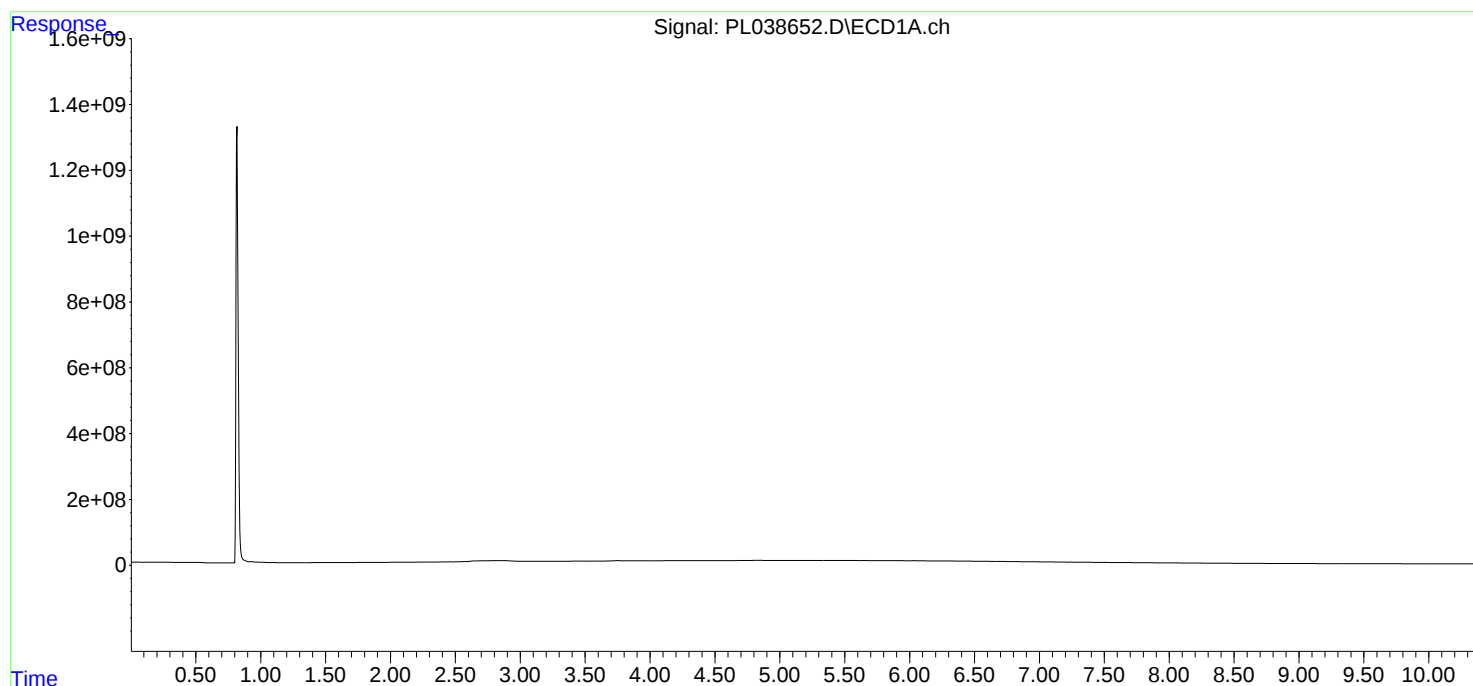


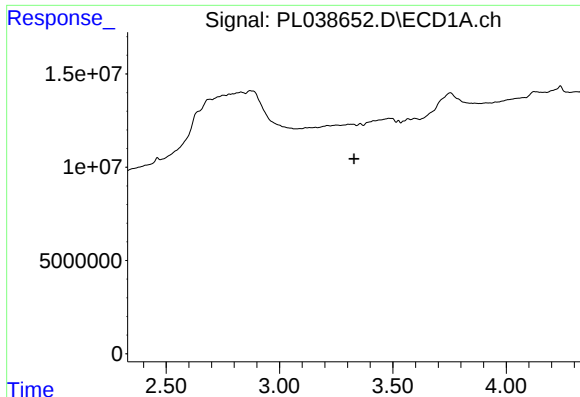

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 3.329 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

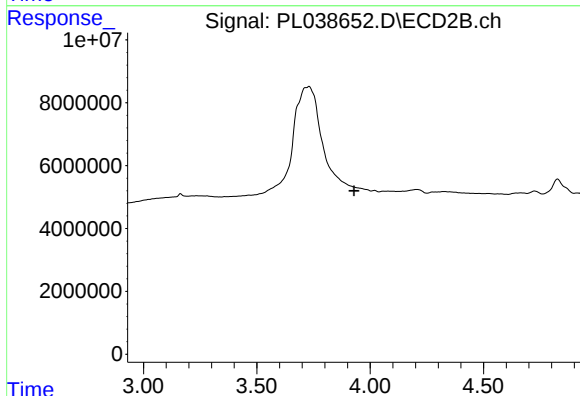


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 3.930 min  
Response: 0  
Conc: N.D.

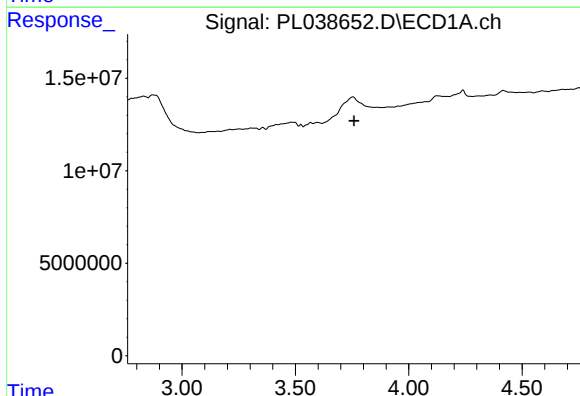


#2 alpha-BHC

R.T.: 0.000 min  
Exp R.T. : 3.758 min  
Response: 0  
Conc: N.D.

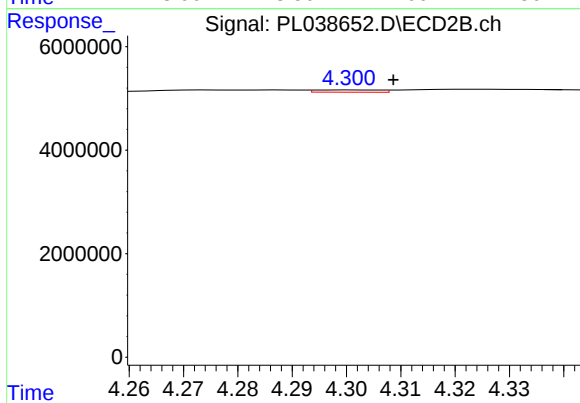

#2 alpha-BHC


R.T.: 4.301 min  
Delta R.T.: -0.007 min  
Response: 370544  
Conc: 0.10 ng/ml

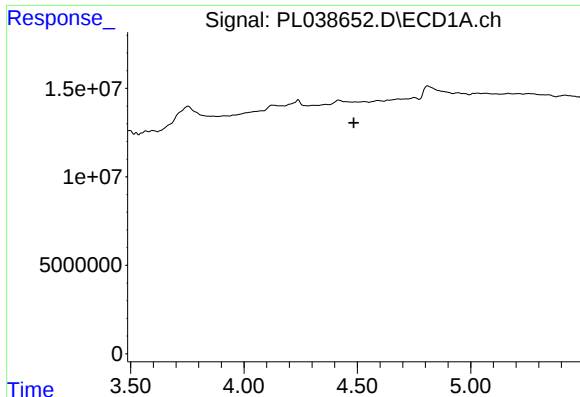

#7 delta-BHC


R.T.: 0.000 min  
Exp R.T. : 4.484 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

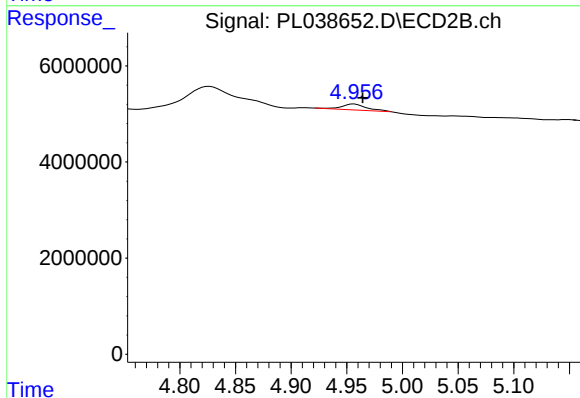


#7 delta-BHC

R.T.: 4.957 min  
Delta R.T.: -0.008 min  
Response: 1769693  
Conc: 0.53 ng/ml

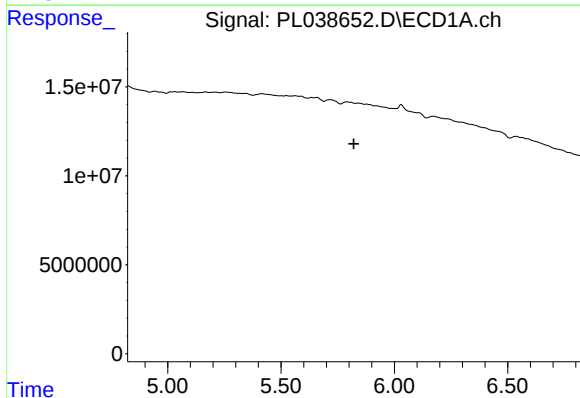


#14 Endrin

R.T.: 0.000 min  
Exp R.T. : 5.821 min  
Response: 0  
Conc: N.D.

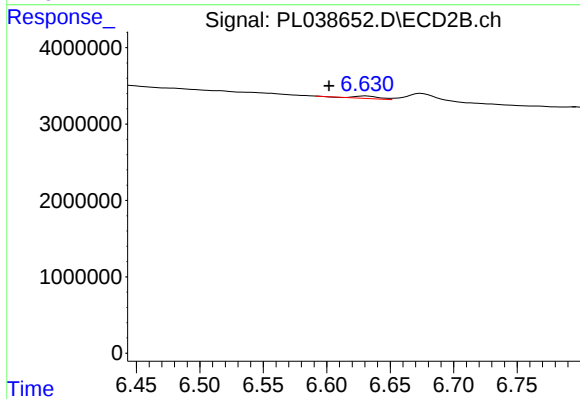

#14 Endrin


R.T.: 6.631 min  
Delta R.T.: 0.029 min  
Response: 458506  
Conc: 0.19 ng/ml

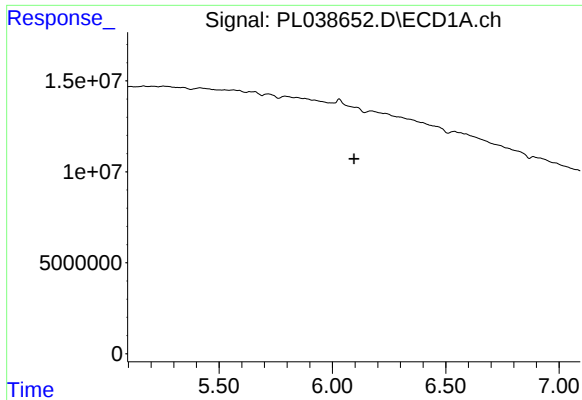

#15 Endosulfan II


R.T.: 0.000 min  
Exp R.T.: 6.096 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

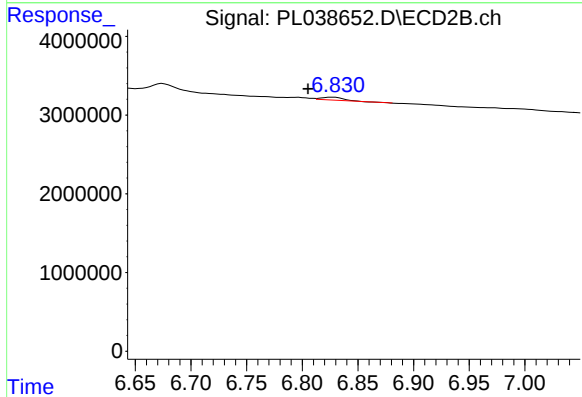


#15 Endosulfan II

R.T.: 6.828 min  
Delta R.T.: 0.022 min  
Response: 447805  
Conc: 0.19 ng/ml

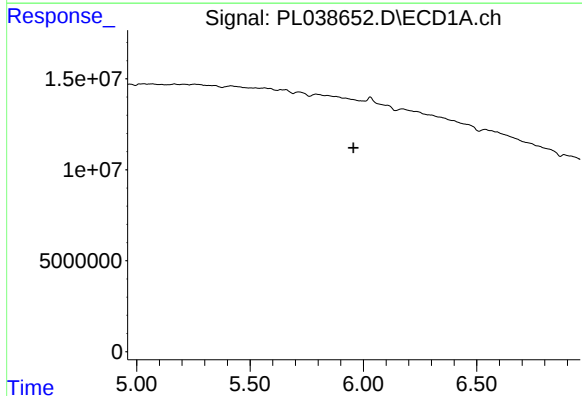


#16 4,4'-DDD

R.T.: 0.000 min  
Exp R.T.: 5.956 min  
Response: 0  
Conc: N.D.

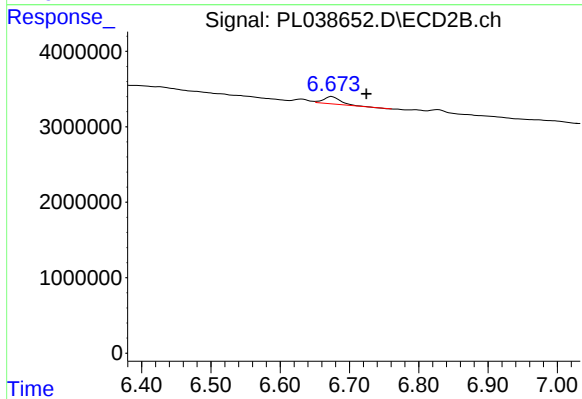

#16 4,4'-DDD


R.T.: 6.675 min  
Delta R.T.: -0.050 min  
Response: 1597718  
Conc: 0.75 ng/ml

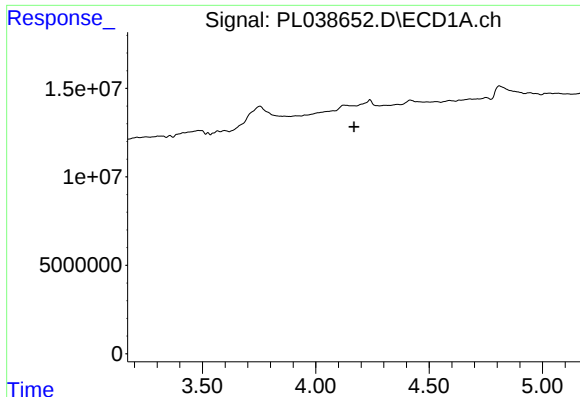

#23 Chlordane-1


R.T.: 0.000 min  
Exp R.T.: 4.169 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

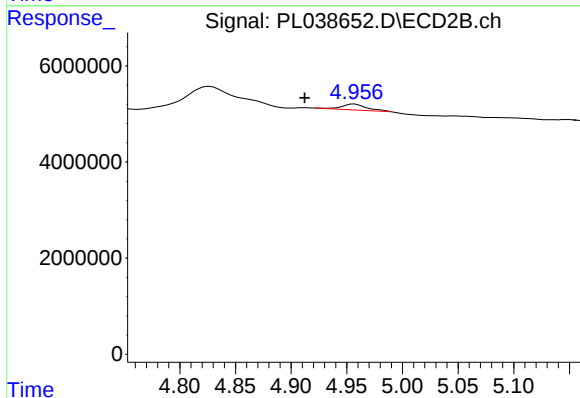


#23 Chlordane-1

R.T.: 4.957 min  
Delta R.T.: 0.044 min  
Response: 1769693  
Conc: 15.27 ng/ml

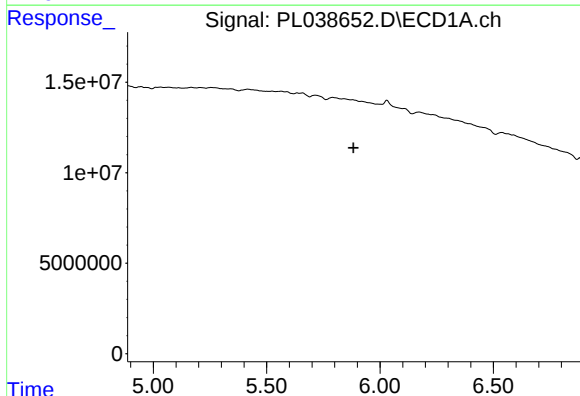


#27 Chlordane-5

R.T.: 0.000 min  
Exp R.T.: 5.883 min  
Response: 0  
Conc: N.D.

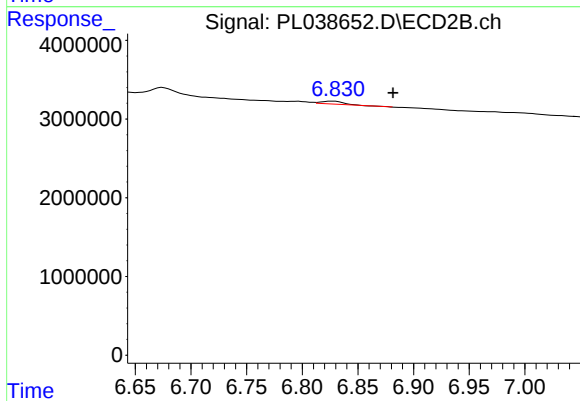

#27 Chlordane-5

R.T.: 6.828 min  
Delta R.T.: -0.054 min  
Response: 447805  
Conc: 5.00 ng/ml

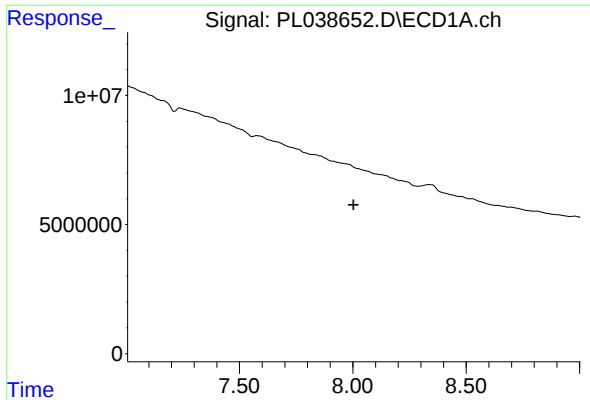

#28 Decachlorobiphenyl


R.T.: 0.000 min

Exp R.T. : 8.004 min

Response: 0

Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

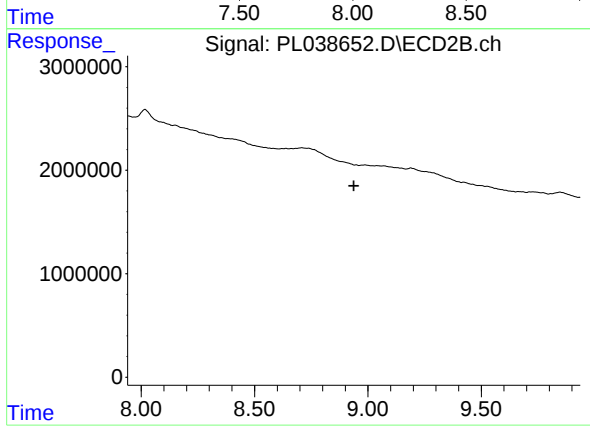

#28 Decachlorobiphenyl

R.T.: 0.000 min

Exp R.T. : 8.937 min

Response: 0

Conc: N.D.