

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072718\
 Data File : PL038657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2018 14:19
 Operator : AJ\SJ
 Sample : PB111522BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB111522BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 22:47:21 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.928	137.7E6	52946218	18.486	20.170
28)	SA Decachlor...	7.997	8.937	132.4E6	49037181	17.455	20.061
Target Compounds							
3)	MA gamma-BHC...	0.000	4.610	0	222543	N.D.	0.062 #
6)	B beta-BHC	4.243f	4.710f	11524982	105628	2.442	0.070 #
7)	B delta-BHC	0.000	4.959	0	2366390	N.D.	0.713 #
8)	B Heptachlo...	0.000	5.799	0	579342	N.D.	0.204 #
15)	B Endosulfa...	6.029f	6.800	7424783	-225353	0.936	N.D. #
16)	A 4,4'-DDD	0.000	6.675f	0	2489188	N.D.	1.163 #
23)	Chlordane-1	4.201	4.959	7183095	2366390	20.745	20.420
27)	Chlordane-5	0.000	6.828	0	696392	N.D.	7.774 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072718\
Data File : PL038657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2018 14:19
Operator : AJ\SJ
Sample : PB111522BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PB111522BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 22:47:21 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

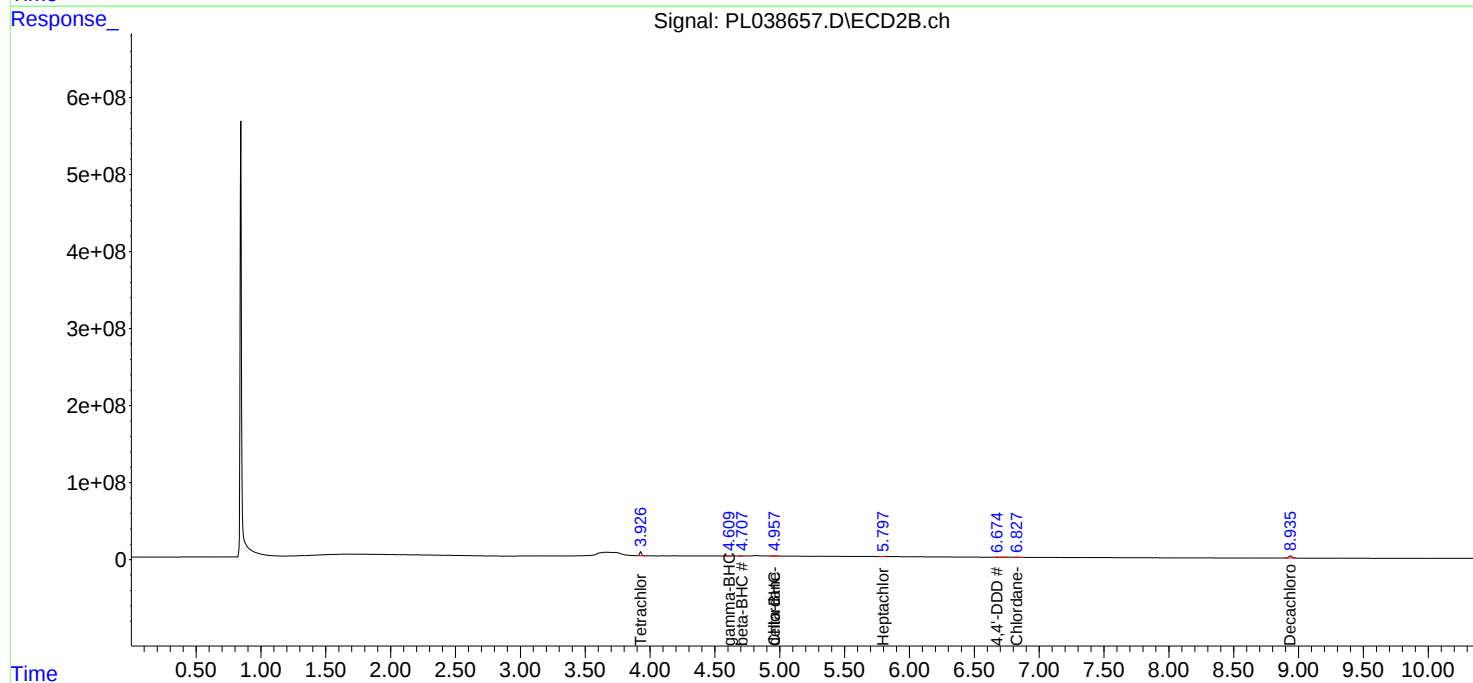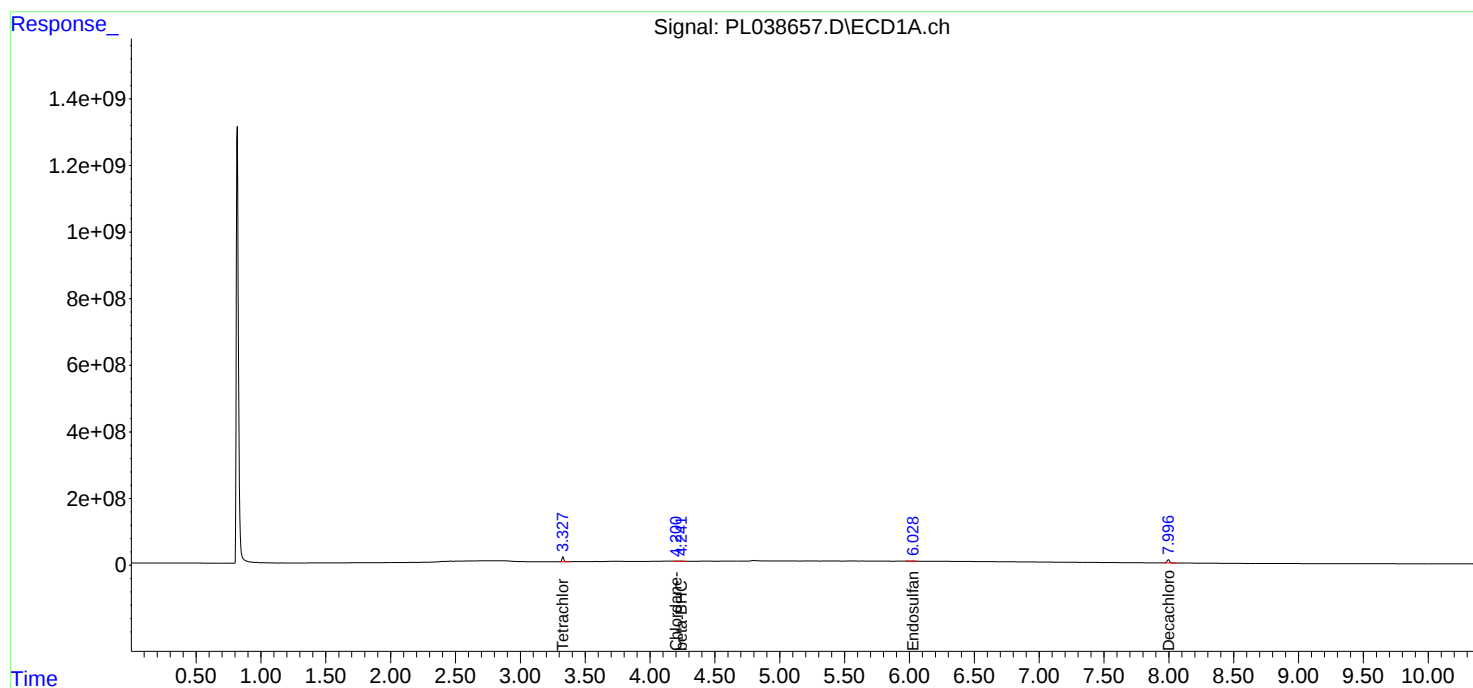


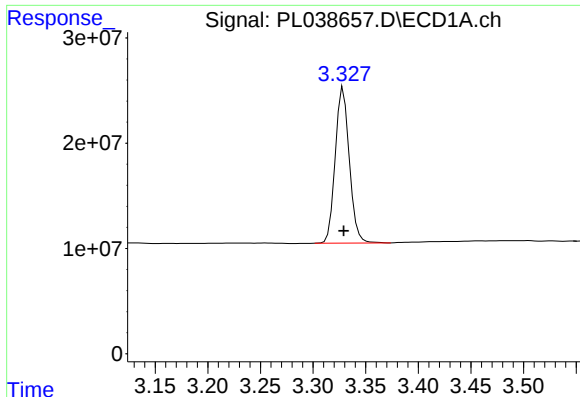

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 137656322
Conc: 18.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB111522BL

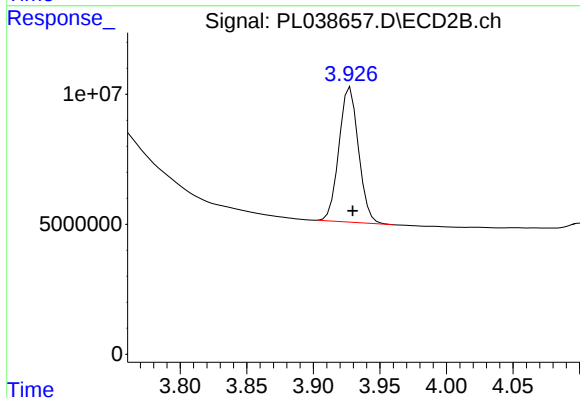


#1 Tetrachloro-m-xylene

R.T.: 3.928 min
Delta R.T.: -0.002 min
Response: 52946218
Conc: 20.17 ng/ml

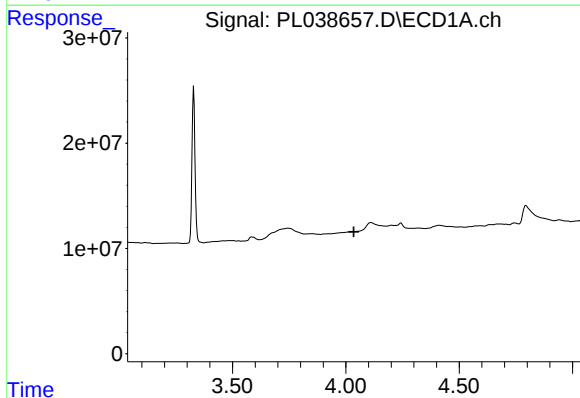


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.035 min
Response: 0
Conc: N.D.

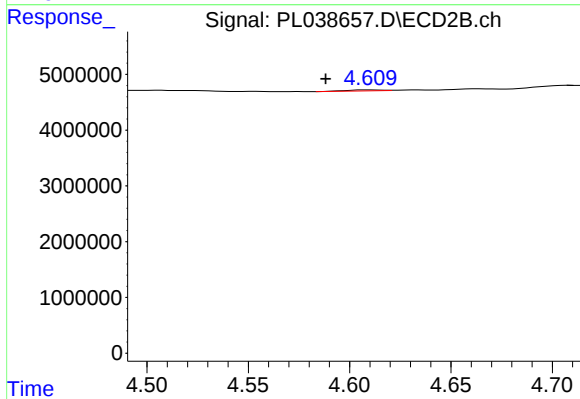

#3 gamma-BHC (Lindane)


R.T.: 4.610 min
Delta R.T.: 0.021 min
Response: 222543
Conc: 0.06 ng/ml

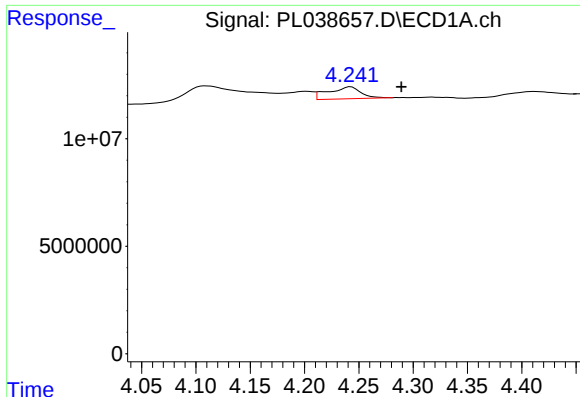

#6 beta-BHC


R.T.: 4.243 min
Delta R.T.: -0.047 min
Response: 11524982
Conc: 2.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB111522BL

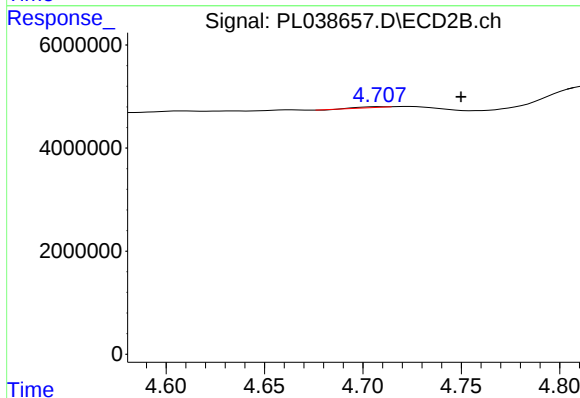


#6 beta-BHC

R.T.: 4.710 min
Delta R.T.: -0.040 min
Response: 105628
Conc: 0.07 ng/ml

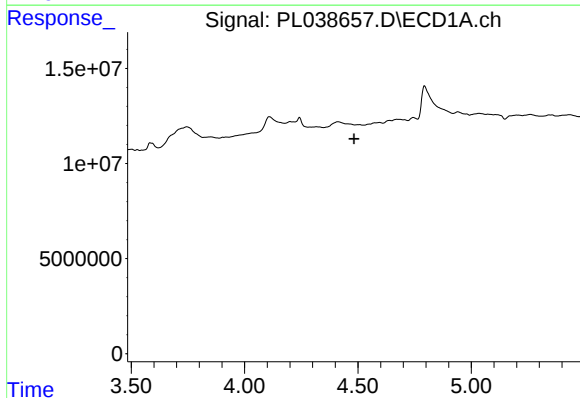


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.484 min
Response: 0
Conc: N.D.

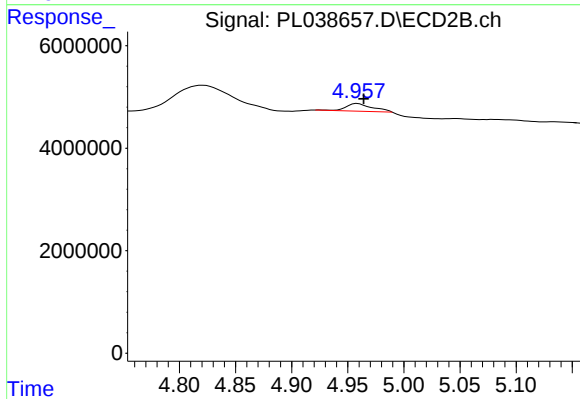

#7 delta-BHC


R.T.: 4.959 min
Delta R.T.: -0.006 min
Response: 2366390
Conc: 0.71 ng/ml

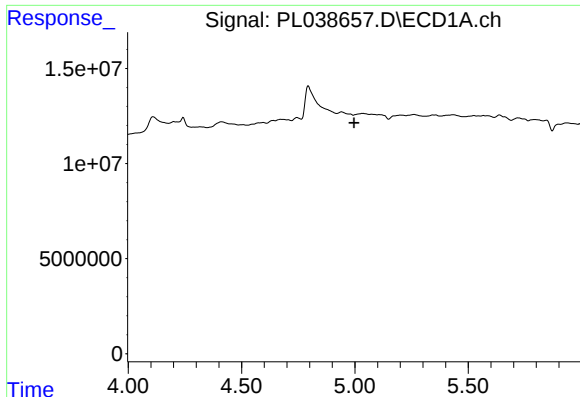

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.997 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB111522BL

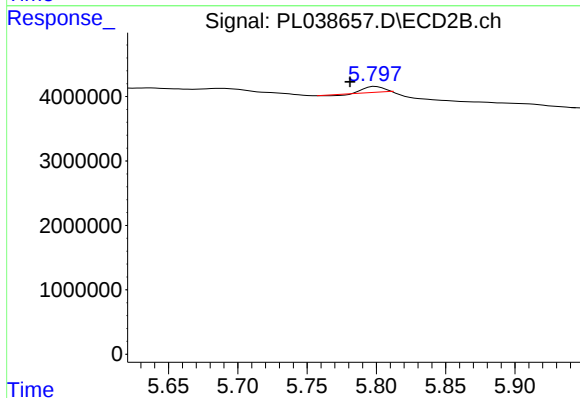


#8 Heptachlor epoxide

R.T.: 5.799 min
Delta R.T.: 0.018 min
Response: 579342
Conc: 0.20 ng/ml

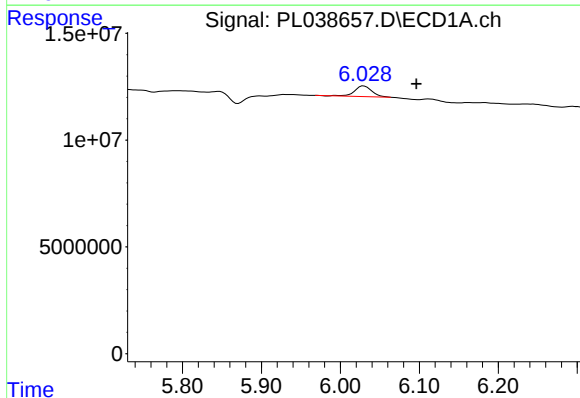


#15 Endosulfan II

R.T.: 6.029 min
Delta R.T.: -0.067 min
Response: 7424783
Conc: 0.94 ng/ml

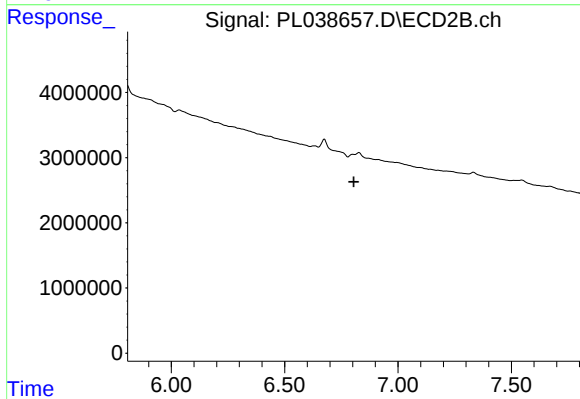

#15 Endosulfan II


R.T.: 6.800 min
Delta R.T.: -0.005 min
Response: -225353
Conc: N.D.

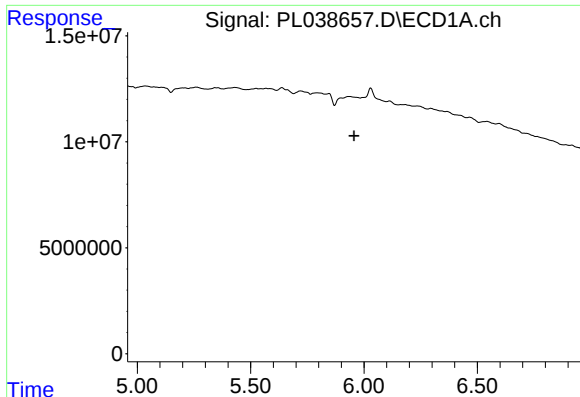

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB111522BL

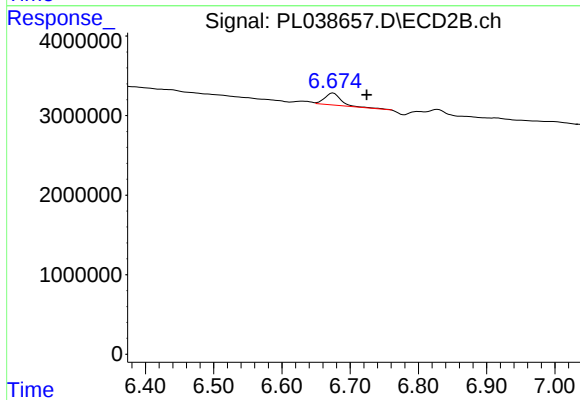


#16 4,4'-DDD

R.T.: 6.675 min
Delta R.T.: -0.049 min
Response: 2489188
Conc: 1.16 ng/ml

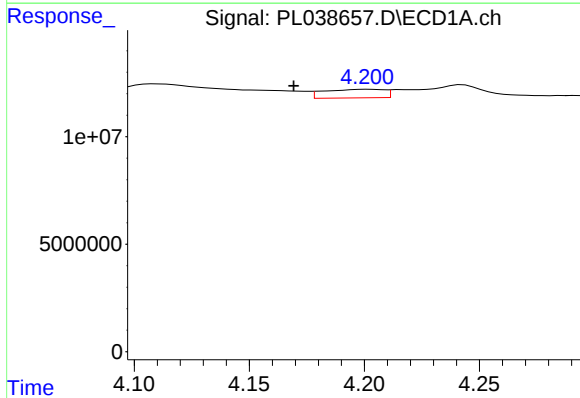


#23 Chlordane-1

R.T.: 4.201 min
Delta R.T.: 0.032 min
Response: 7183095
Conc: 20.75 ng/ml

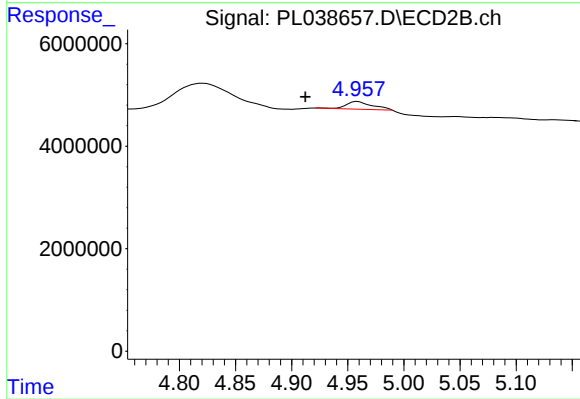

#23 Chlordane-1


R.T.: 4.959 min
Delta R.T.: 0.046 min
Response: 2366390
Conc: 20.42 ng/ml

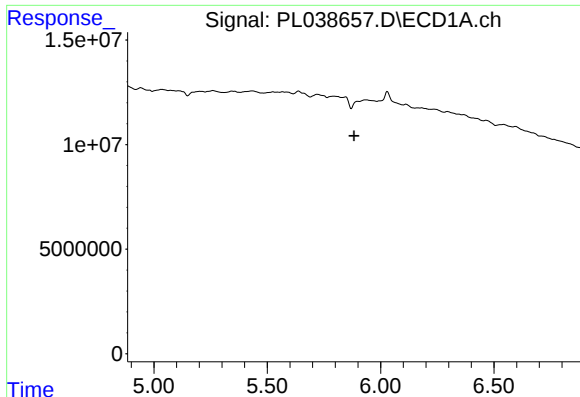

#27 Chlorodane-5


R.T.: 0.000 min
Exp R.T.: 5.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB111522BL

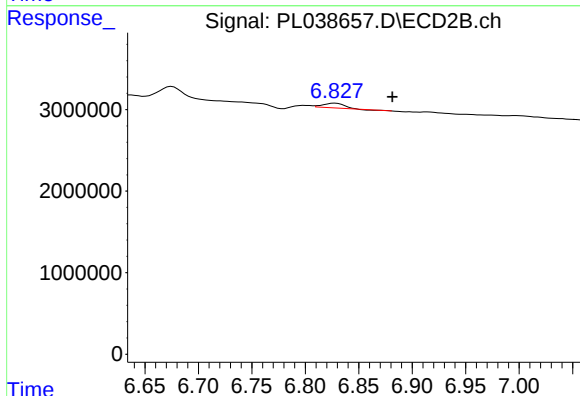


#27 Chlorodane-5

R.T.: 6.828 min
Delta R.T.: -0.054 min
Response: 696392
Conc: 7.77 ng/ml

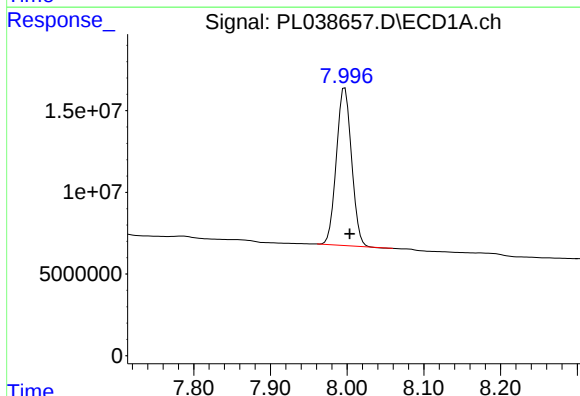

#28 Decachlorobiphenyl

R.T.: 7.997 min
Delta R.T.: -0.007 min
Response: 132411427
Conc: 17.45 ng/ml

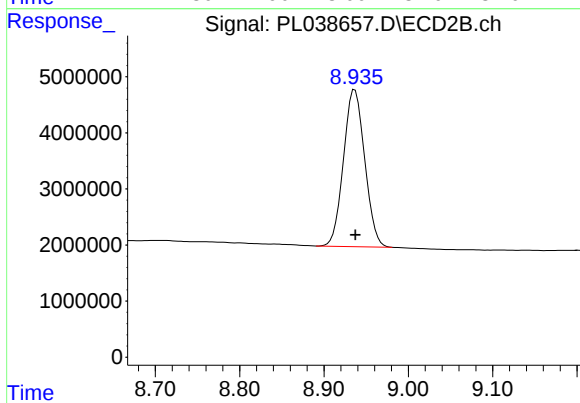

#28 Decachlorobiphenyl

R.T.: 8.937 min
Delta R.T.: 0.000 min
Response: 49037181
Conc: 20.06 ng/ml