

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072718\
 Data File : PL038679.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2018 19:29
 Operator : AJ\SJ
 Sample : J4176-05 (Sig #1); J4177-01 (Sig #2)
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PLASTIC-COAT

Manual Integrations
 APPROVED

Sohil
 7/30/2018 12:37:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 22:54:58 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.332	3.935	181.2E6	57199784	24.329m	21.791m
28)	SA Decachlor...	7.989	8.937	136.5E6	51906784	17.992m	21.235m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072718\
Data File : PL038679.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2018 19:29
Operator : AJ\SJ
Sample : J4176-05 (Sig #1); J4177-01 (Sig #2)
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PLASTIC-COAT


Manual Integrations
APPROVED

Sohil
7/30/2018 12:37:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 22:54:58 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

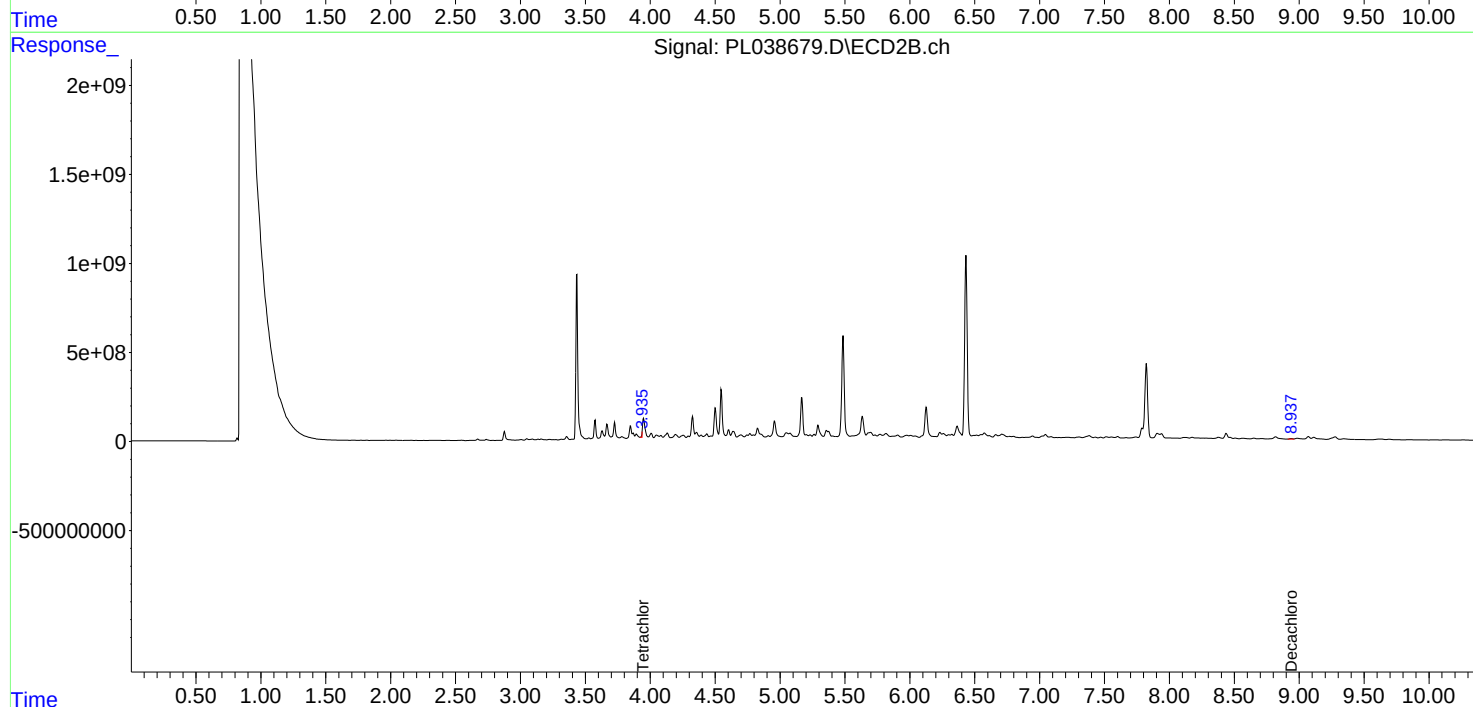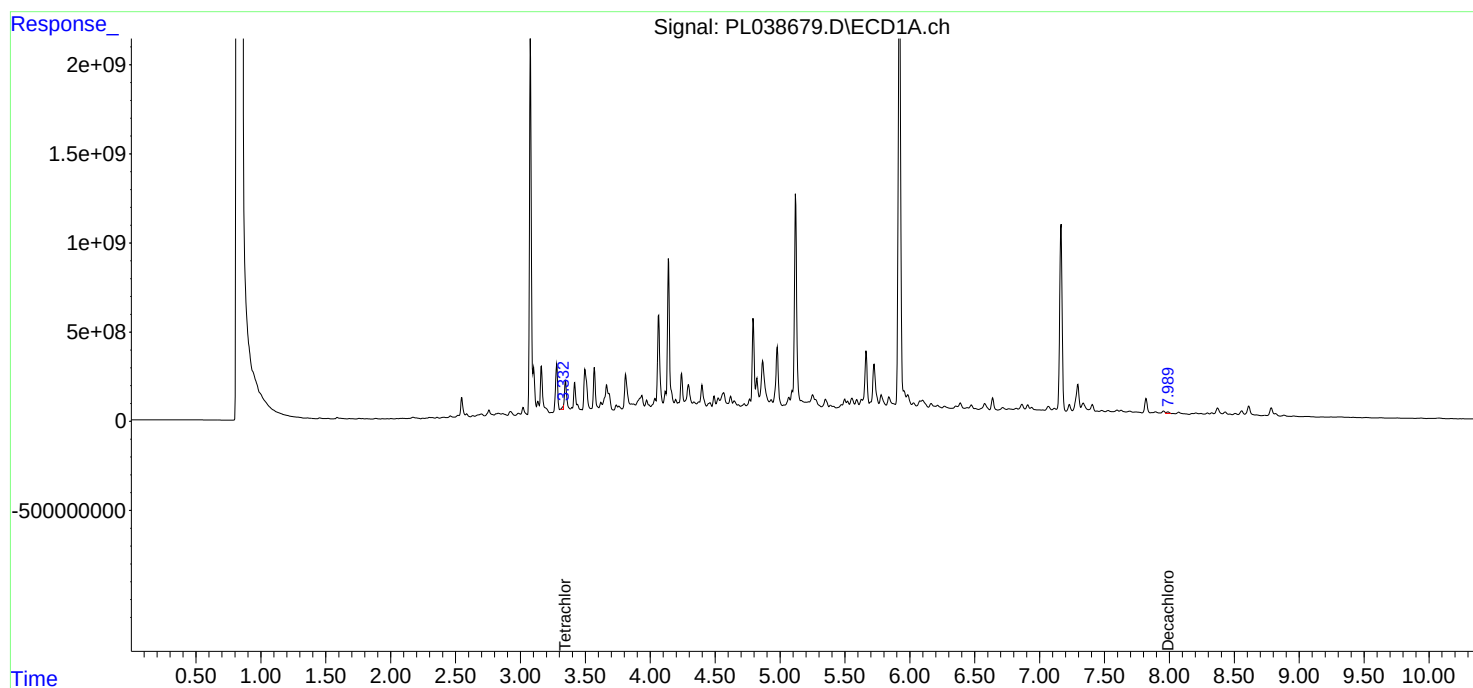

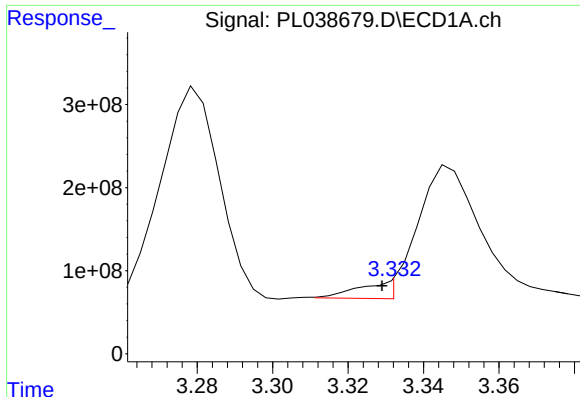


#1 Tetrachloro-m-xylene

R.T.: 3.332 min
Delta R.T.: 0.003 min
Response: 181167247
Conc: 24.33 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PLASTIC-COAT


Manual Integrations
APPROVED

Sohil
7/30/2018 12:37:10 PM

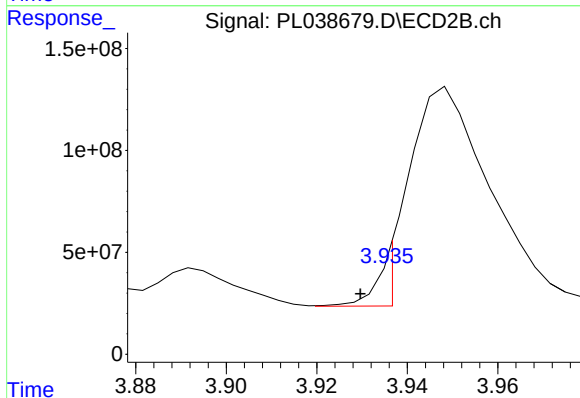


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: 0.005 min
Response: 57199784
Conc: 21.79 ng/ml m

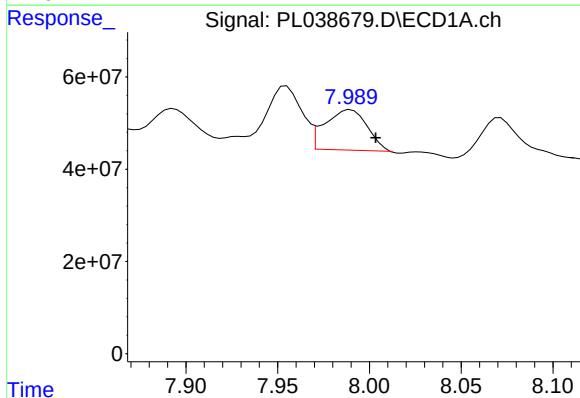

#28 Decachlorobiphenyl

R.T.: 7.989 min
Delta R.T.: -0.015 min
Response: 136484417
Conc: 17.99 ng/ml m

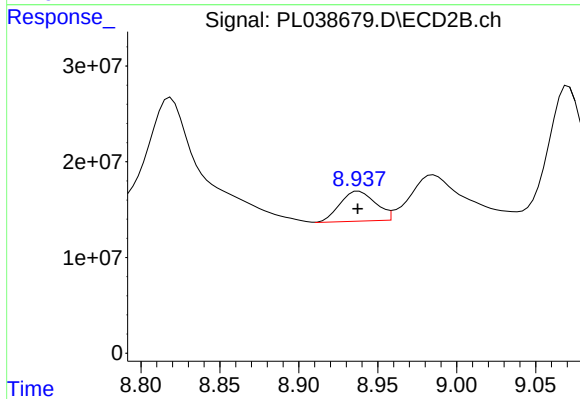

#28 Decachlorobiphenyl

R.T.: 8.937 min
Delta R.T.: 0.000 min
Response: 51906784
Conc: 21.23 ng/ml m