

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072720\
 Data File : PL060221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2020 09:04
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 01:03:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
6) B	beta-BHC	4.445	0.000	849926	0	0.832	N.D. #
8) B	Heptachlo...	5.177	0.000	1348882	0	0.735	N.D. #
17) MA	4,4'-DDT	6.385	0.000	7158047	0	5.505	N.D. #
20) A	Methoxychlor	6.962f	0.000	3176037	0	4.246	N.D. #
23)	Chlordane-1	4.326	0.000	515015	0	8.406	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072720\
Data File : PL060221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2020 09:04
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 01:03:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

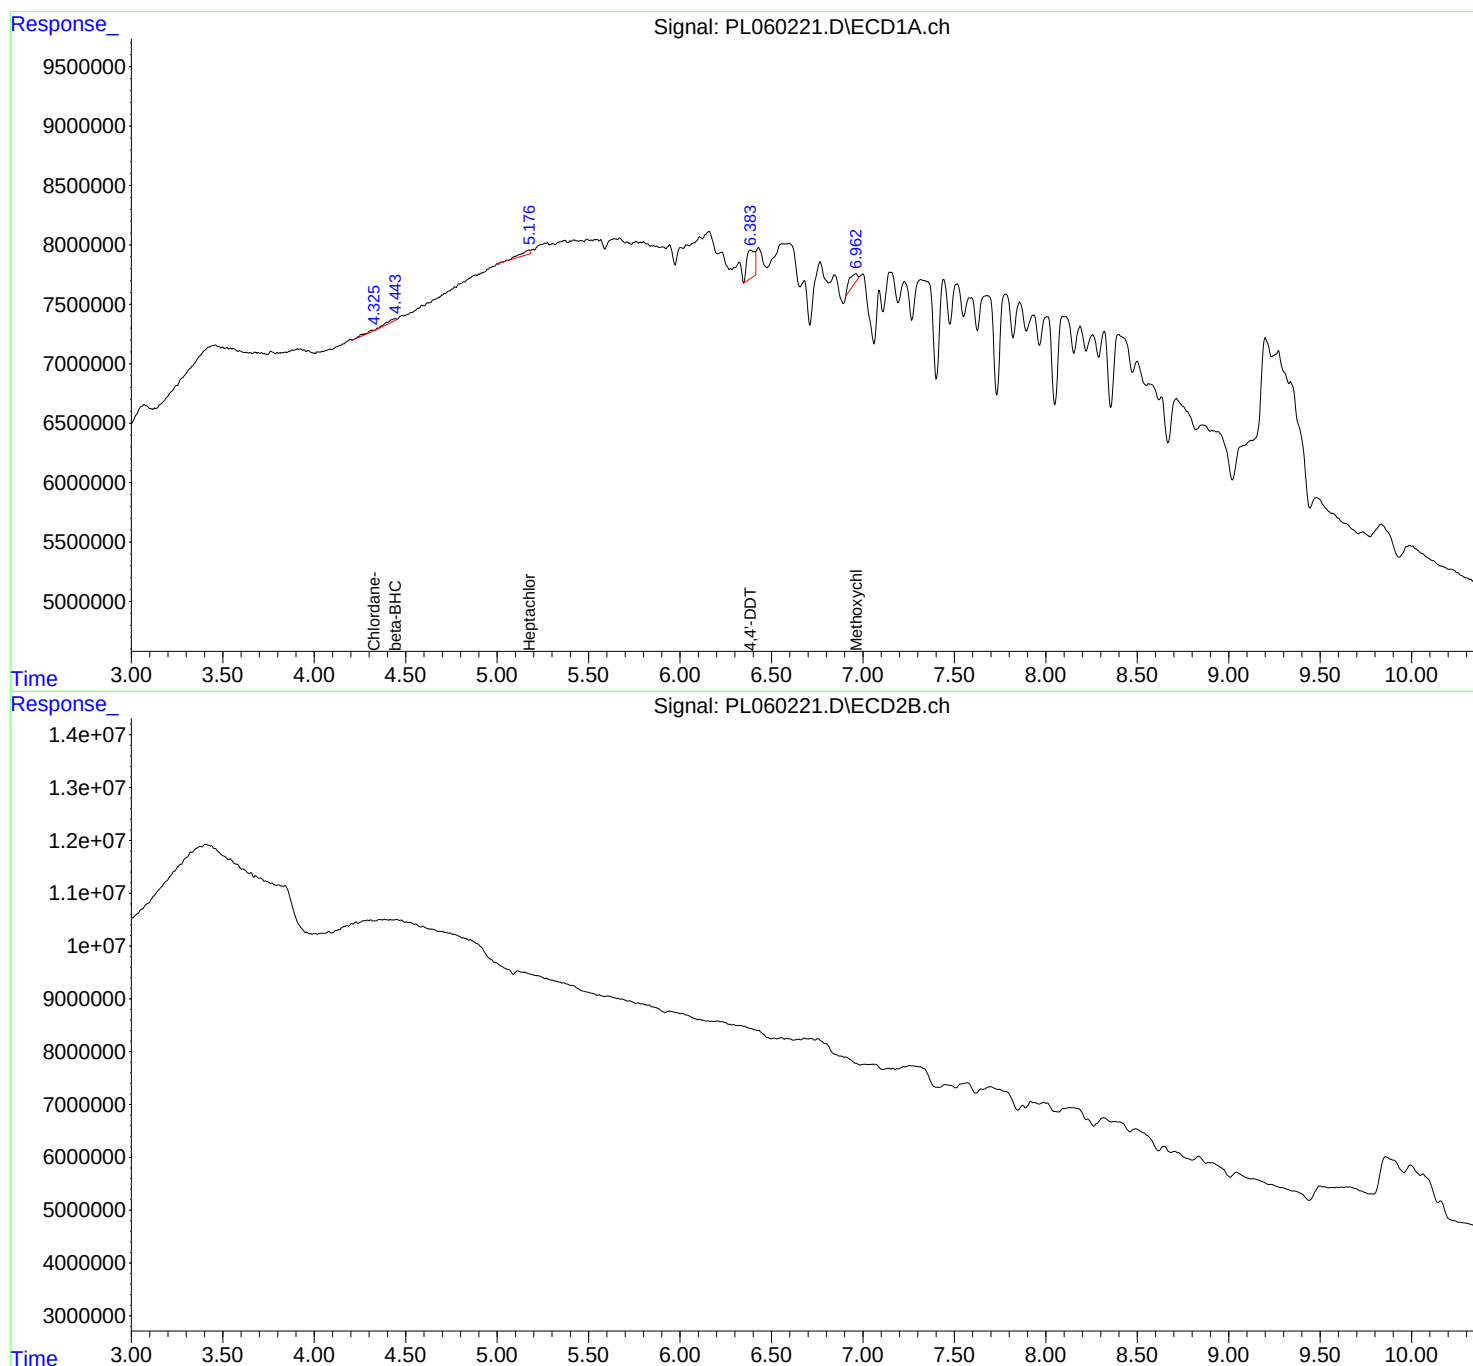


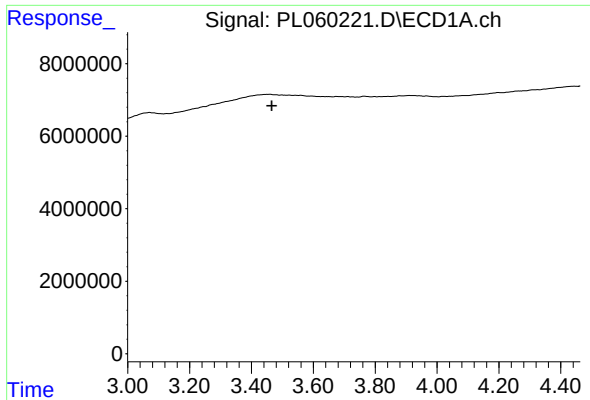

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.466 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

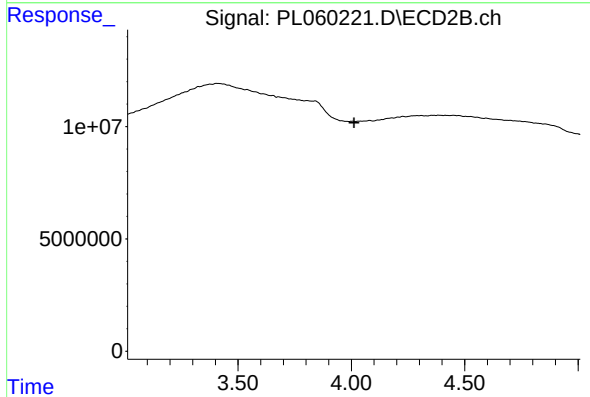


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.012 min
Response: 0
Conc: N.D.

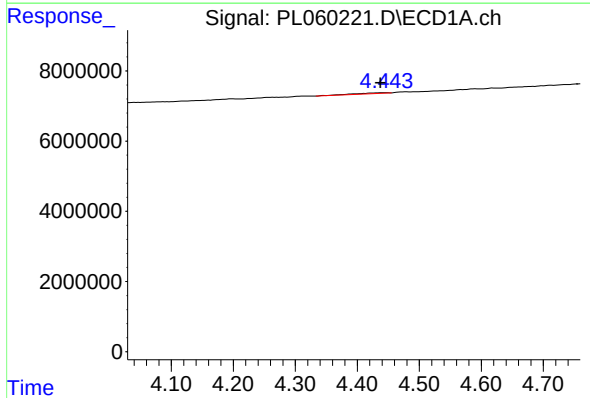


#6 beta-BHC

R.T.: 4.445 min
Delta R.T.: 0.007 min
Response: 849926
Conc: 0.83 ng/ml

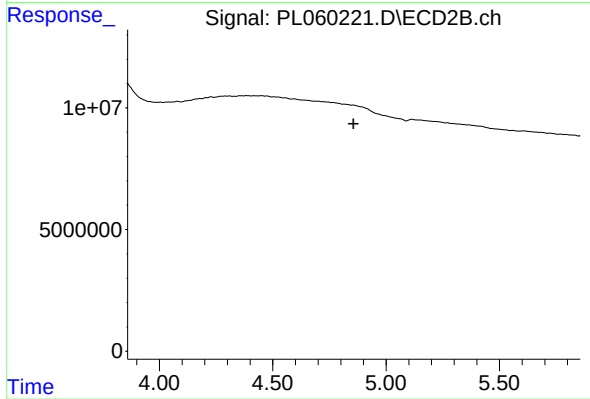

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.857 min
Response: 0
Conc: N.D.

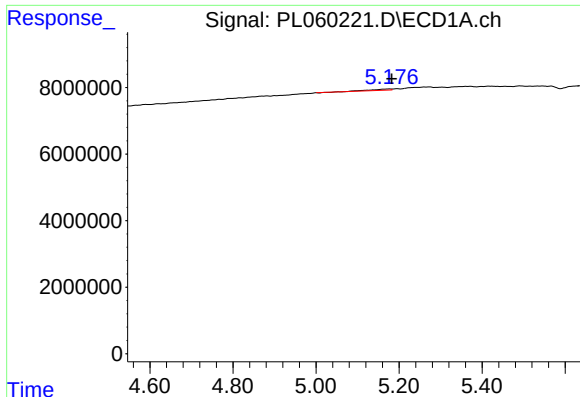

#8 Heptachlor epoxide


R.T.: 5.177 min
Delta R.T.: -0.006 min
Response: 1348882
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

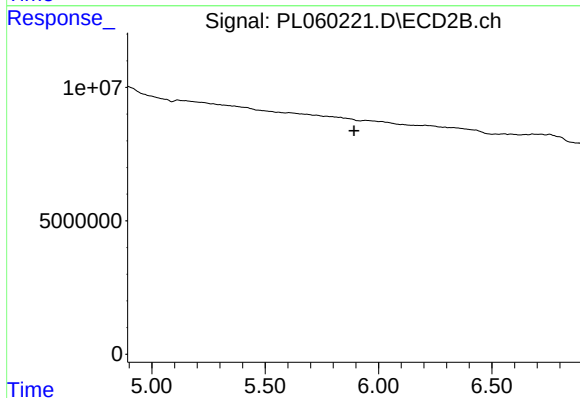


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.892 min
Response: 0
Conc: N.D.

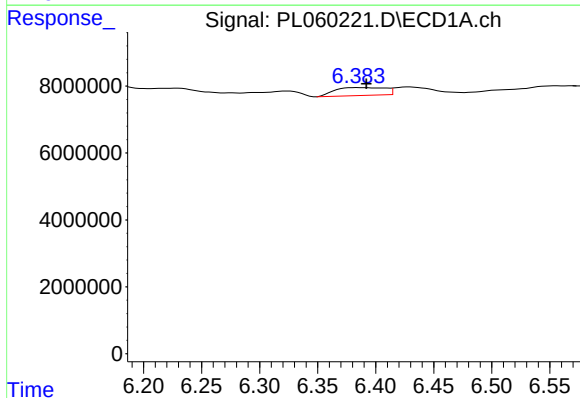


#17 4,4'-DDT

R.T.: 6.385 min
Delta R.T.: -0.007 min
Response: 7158047
Conc: 5.51 ng/ml

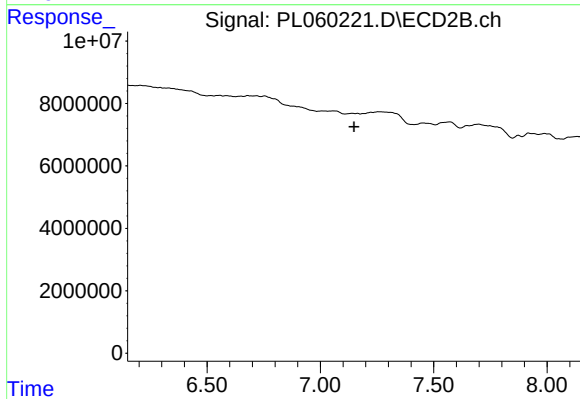

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

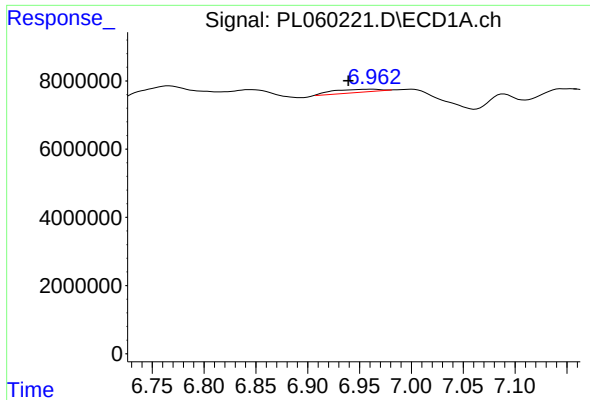

#20 Methoxychlor


R.T.: 6.962 min
Delta R.T.: 0.023 min
Response: 3176037
Conc: 4.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

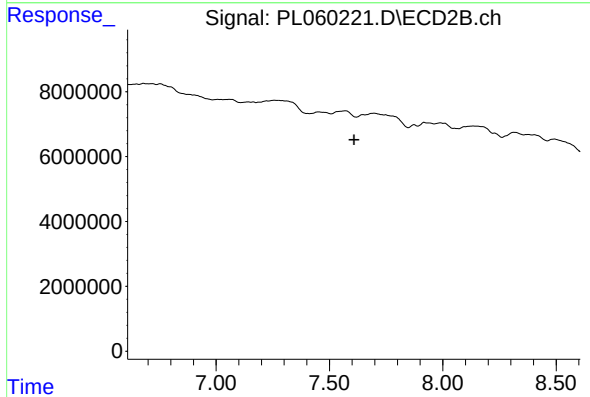


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.609 min
Response: 0
Conc: N.D.

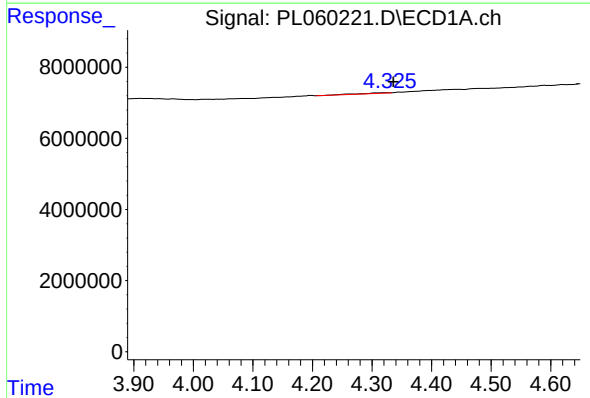


#23 Chlordane-1

R.T.: 4.326 min
Delta R.T.: -0.009 min
Response: 515015
Conc: 8.41 ng/ml

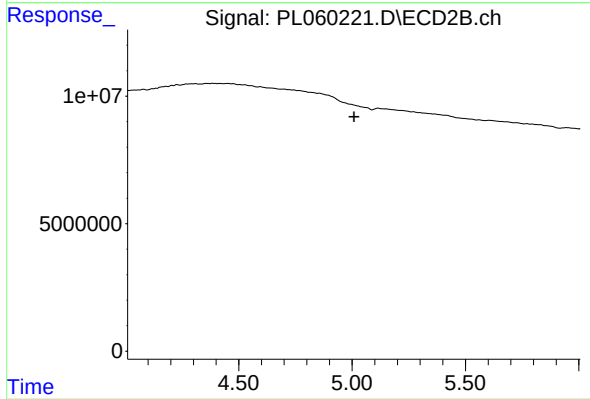

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.009 min
Response: 0
Conc: N.D.

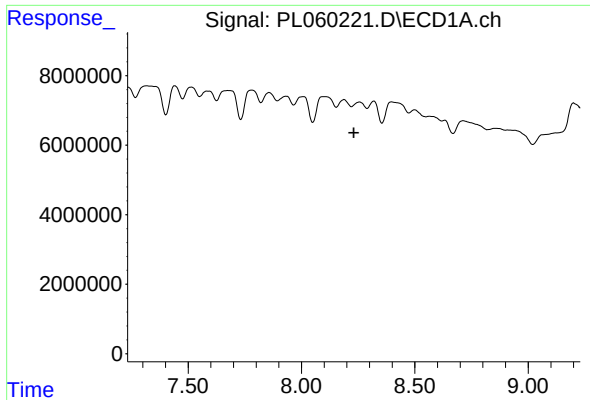

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: 0.025 min
Response: -785817
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

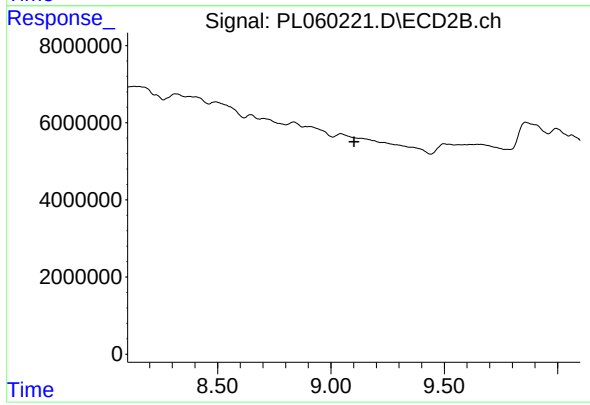

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.103 min
Response: 0
Conc: N.D.