

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072720\
 Data File : PL060238.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2020 15:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 01:07:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.466	4.013	41424403	58107687	21.416	21.926
28)	SA Decachlor...	8.225	9.099	45017520	35690098	27.365	17.065 #
Target Compounds							
4)	MA Heptachlor	0.000	5.202	0	1017145	N.D.	0.302 #
8)	B Heptachlo...	0.000	5.881	0	2865815	N.D.	1.064 #
10)	B gamma-Chl...	0.000	6.132	0	181778	N.D.	0.063 #
25)	Chlordane-3	0.000	6.132	0	181778	N.D.	0.470 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072720\
Data File : PL060238.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2020 15:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 01:07:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

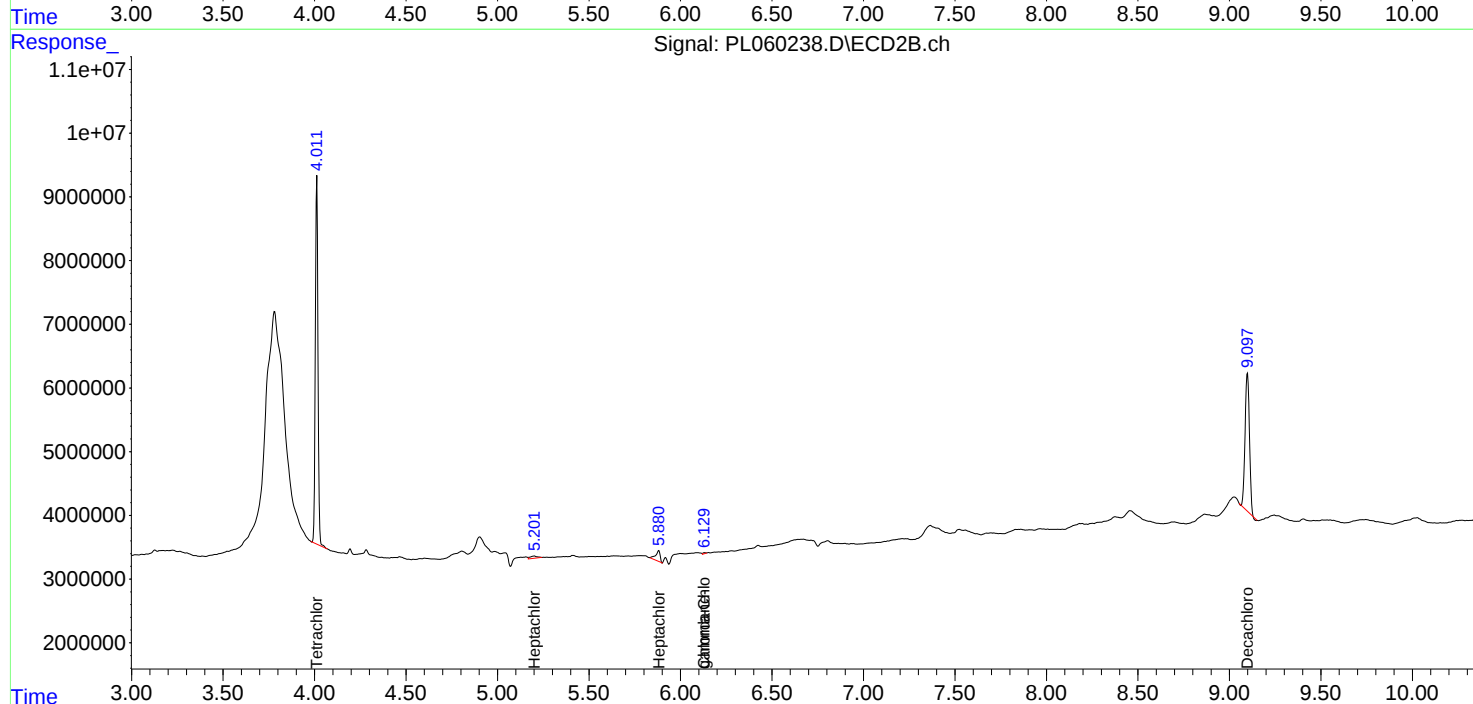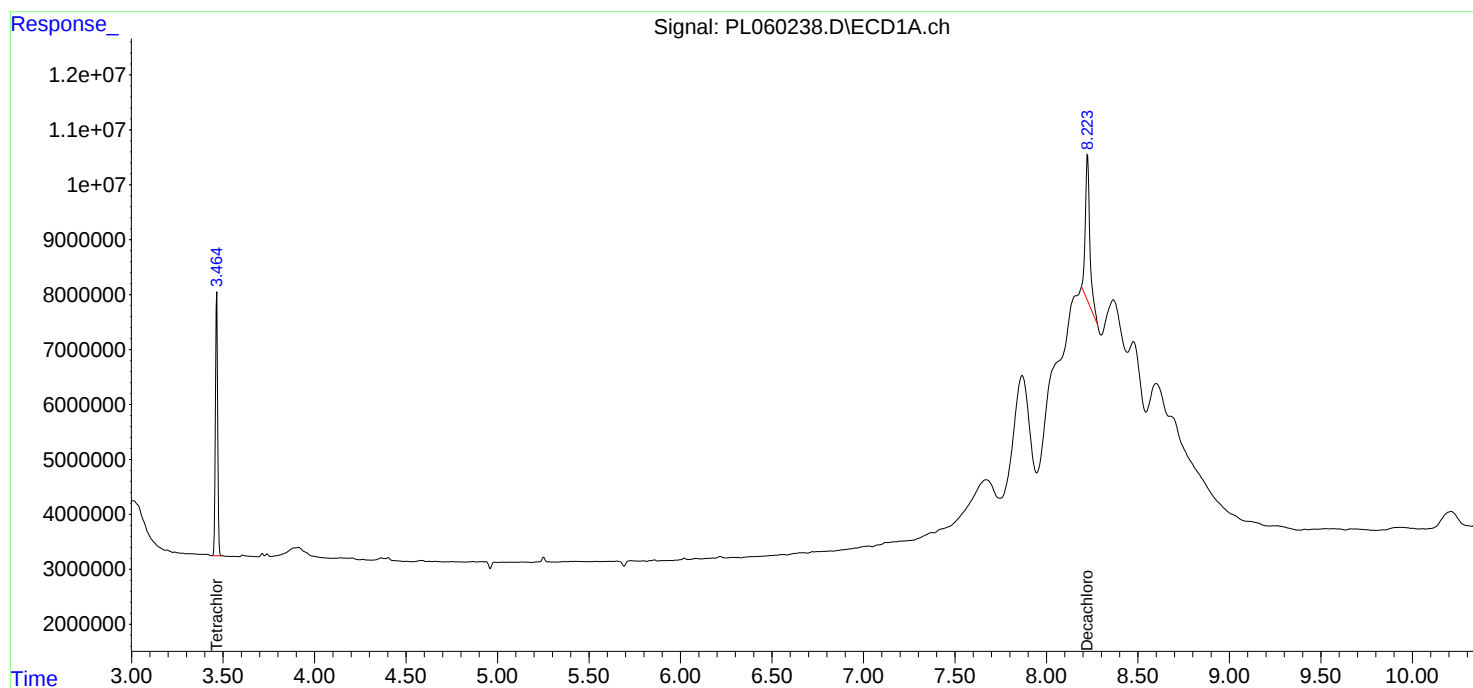


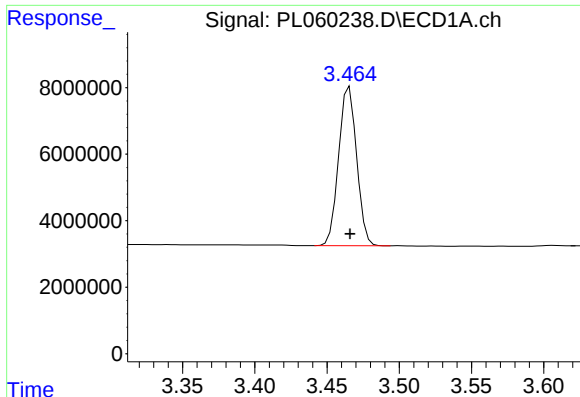

#1 Tetrachloro-m-xylene


R.T.: 3.466 min
Delta R.T.: 0.000 min
Response: 41424403
Conc: 21.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

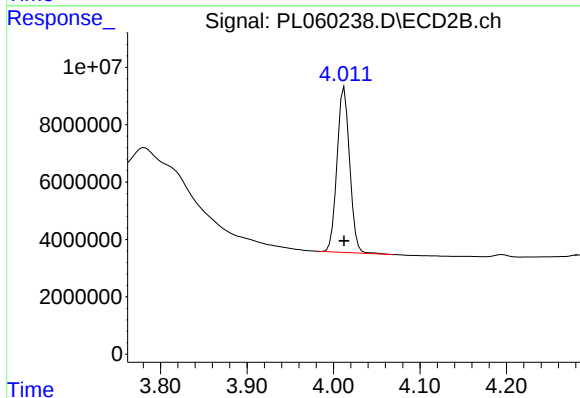


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 58107687
Conc: 21.93 ng/ml

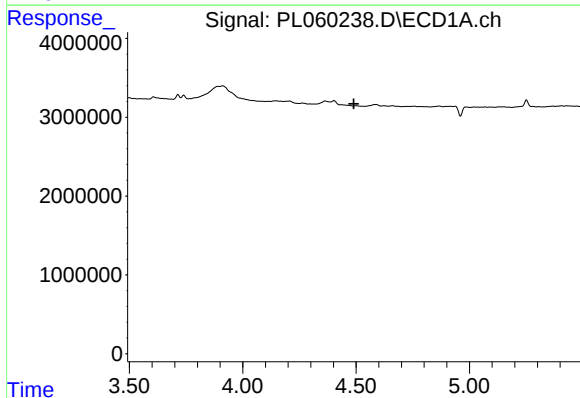


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

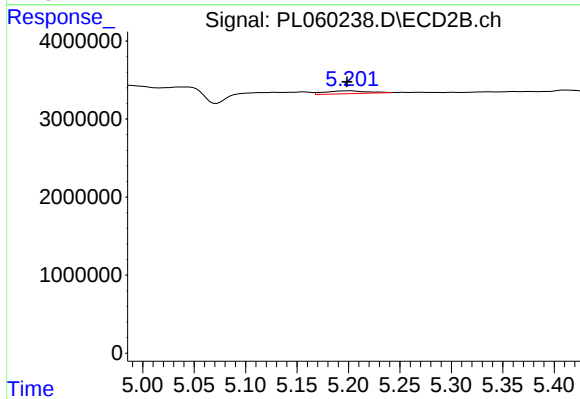

#4 Heptachlor


R.T.: 5.202 min
Delta R.T.: 0.003 min
Response: 1017145
Conc: 0.30 ng/ml

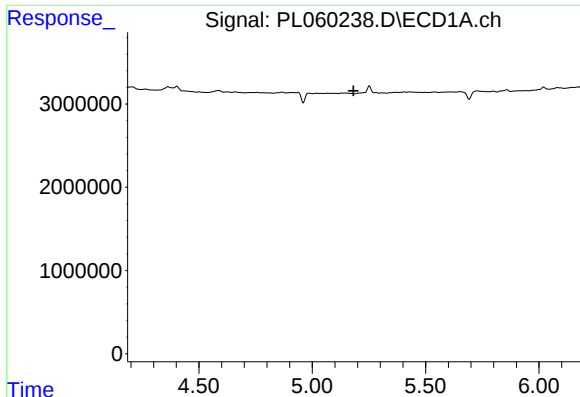

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.183 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

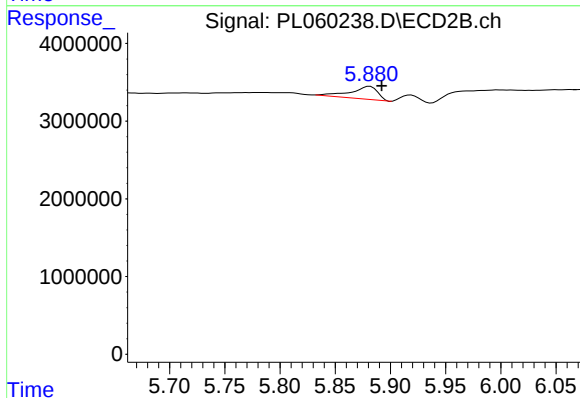


#8 Heptachlor epoxide

R.T.: 5.881 min
Delta R.T.: -0.011 min
Response: 2865815
Conc: 1.06 ng/ml

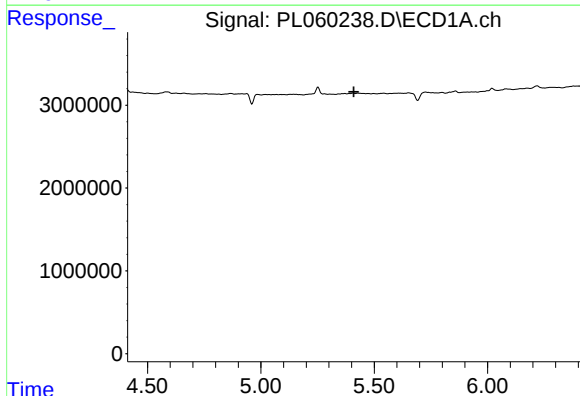


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.410 min
Response: 0
Conc: N.D.

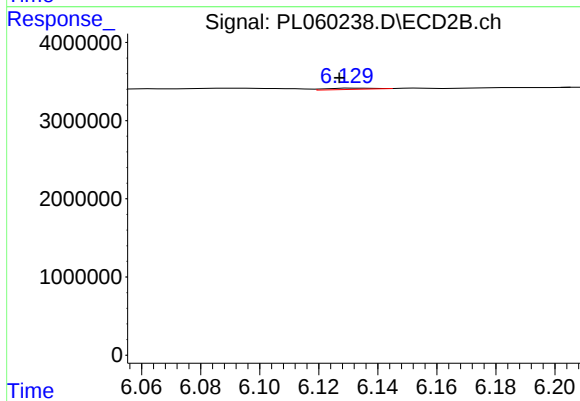

#10 gamma-Chlordane


R.T.: 6.132 min
Delta R.T.: 0.005 min
Response: 181778
Conc: 0.06 ng/ml

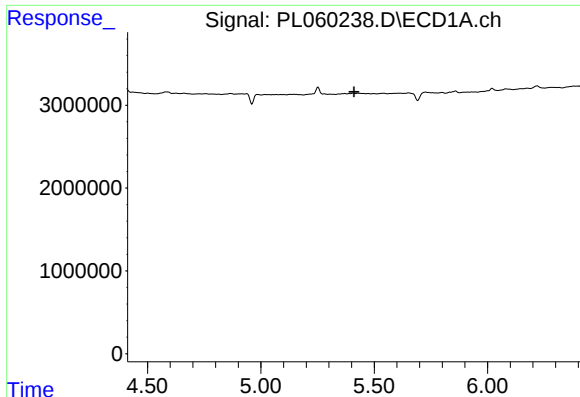

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

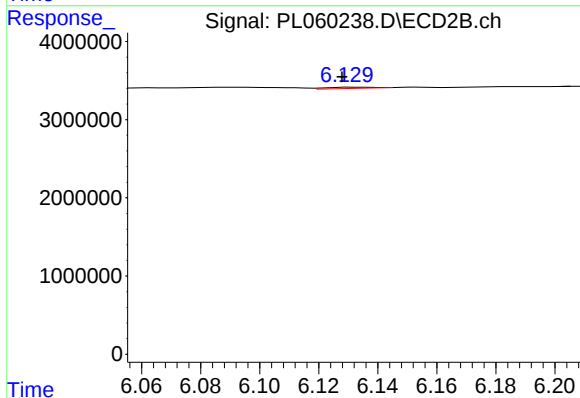


#25 Chlordane-3

R.T.: 6.132 min
Delta R.T.: 0.004 min
Response: 181778
Conc: 0.47 ng/ml

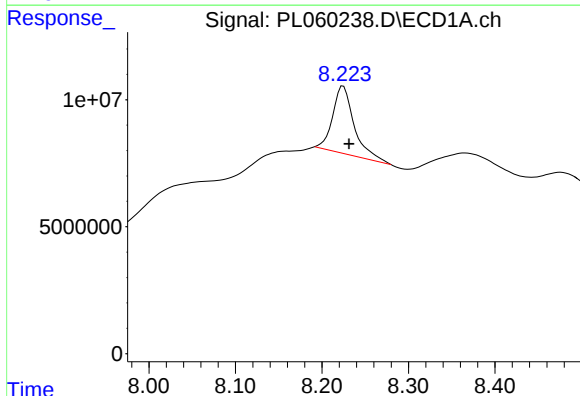

#28 Decachlorobiphenyl

R.T.: 8.225 min
Delta R.T.: -0.006 min
Response: 45017520
Conc: 27.36 ng/ml

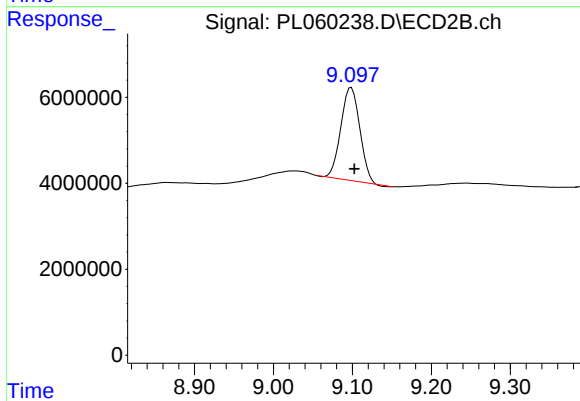

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: -0.004 min
Response: 35690098
Conc: 17.07 ng/ml