

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072720\
 Data File : PL060242.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2020 16:30
 Operator : DD\AJ
 Sample : L3453-01 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 01:08:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.011	6515483	9079331	3.369	3.426
28)	SA Decachlor...	8.223	9.098	5894760	6296915	3.583	3.011
Target Compounds							
8)	B Heptachlo...	0.000	5.872f	0	4778775	N.D.	1.774 #
10)	B gamma-Chl...	5.407	6.126	1082129	5556770	0.596	1.940 #
11)	B alpha-Chl...	5.466	6.201	712528	5596683	0.395	1.957 #
15)	B Endosulfa...	0.000	6.943	0	35959002	N.D.	14.317 #
19)	B Endosulfa...	0.000	7.290	0	19896878	N.D.	8.507 #
20)	A Methoxychlor	0.000	7.625f	0	115.8E6	N.D.	101.997 #
25)	Chlordane-3	5.407	6.126	1082129	5556770	6.399	14.362 #
26)	Chlordane-4	5.466	6.201	712528	5596683	5.107	12.090 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072720\
Data File : PL060242.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2020 16:30
Operator : DD\AJ
Sample : L3453-01 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 01:08:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

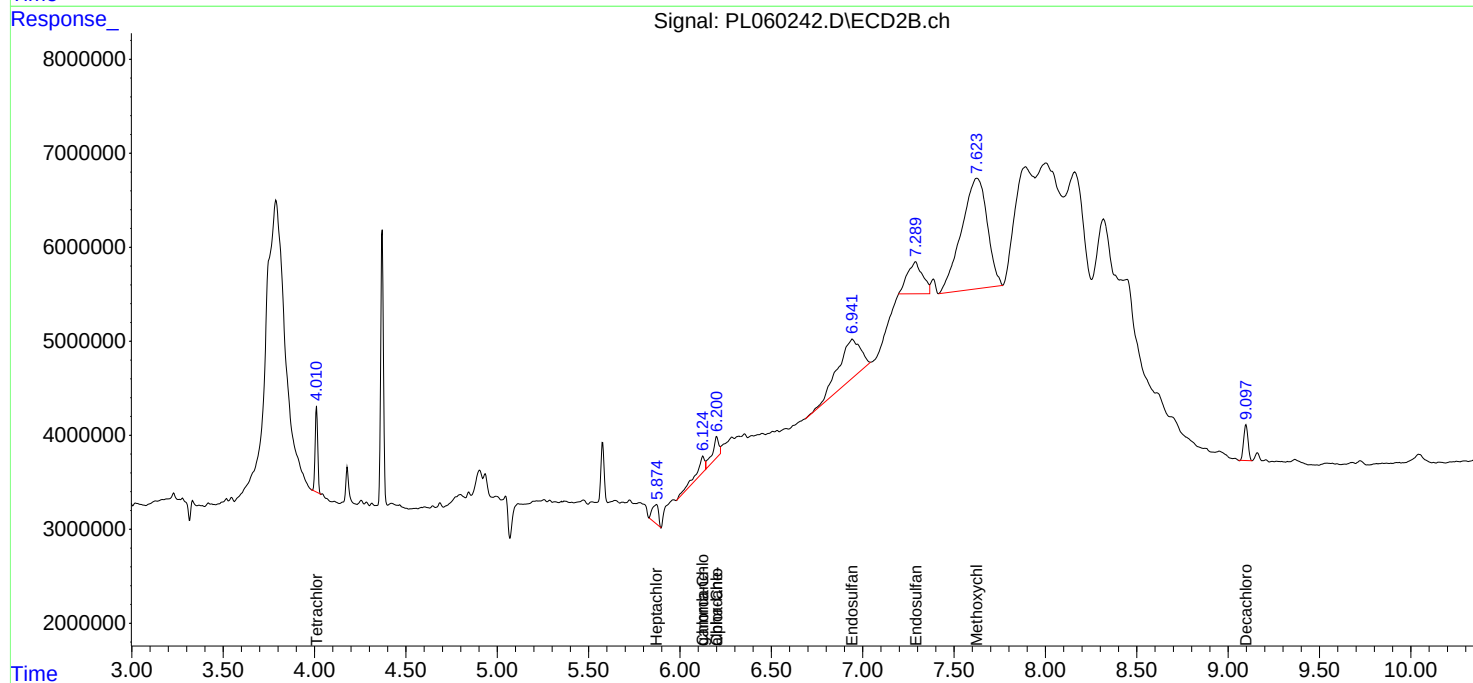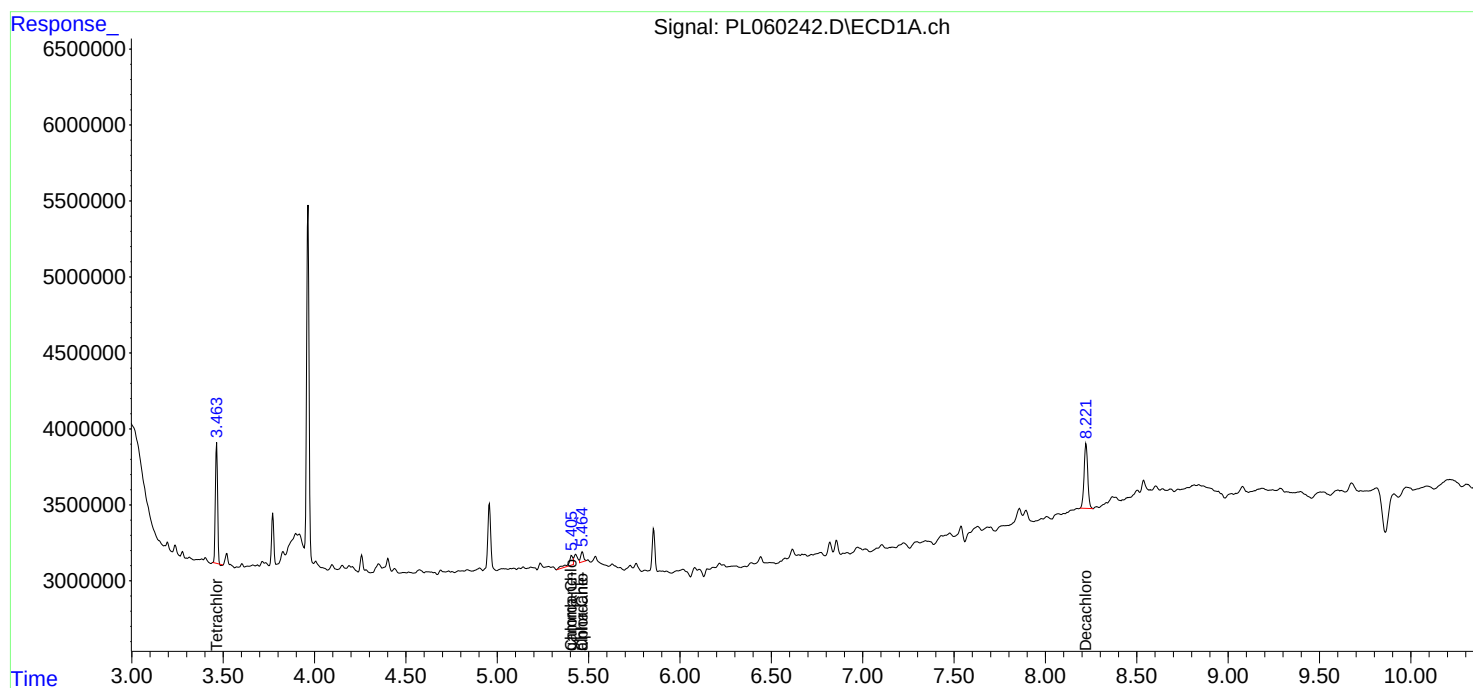


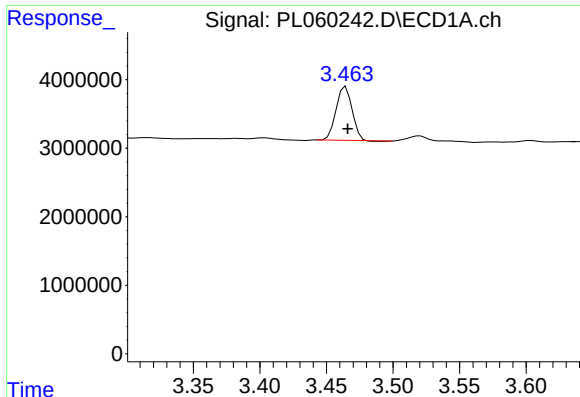

#1 Tetrachloro-m-xylene


R.T.: 3.465 min
Delta R.T.: -0.002 min
Response: 6515483
Conc: 3.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

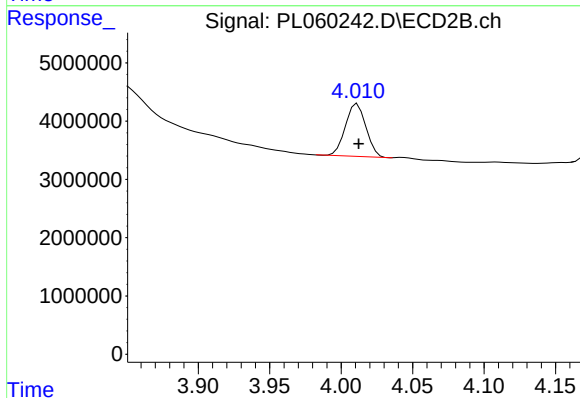


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 9079331
Conc: 3.43 ng/ml

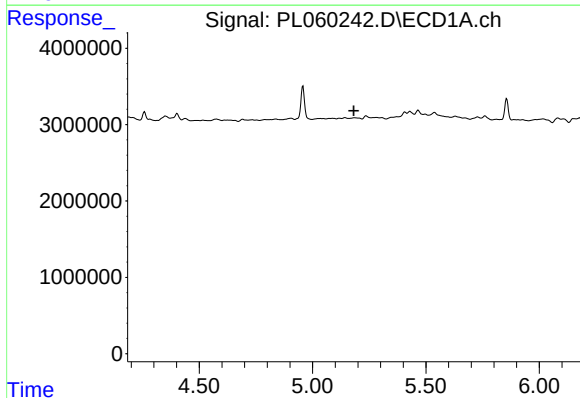


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.183 min
Response: 0
Conc: N.D.

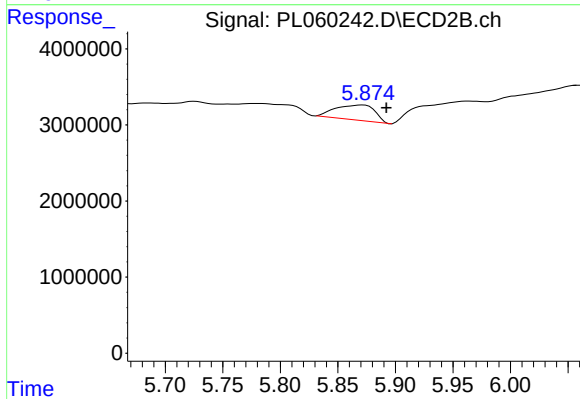

#8 Heptachlor epoxide


R.T.: 5.872 min
Delta R.T.: -0.020 min
Response: 4778775
Conc: 1.77 ng/ml

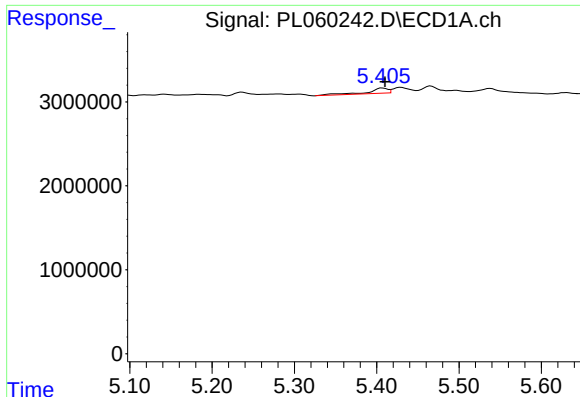

#10 gamma-Chlordane


R.T.: 5.407 min
Delta R.T.: -0.003 min
Response: 1082129
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

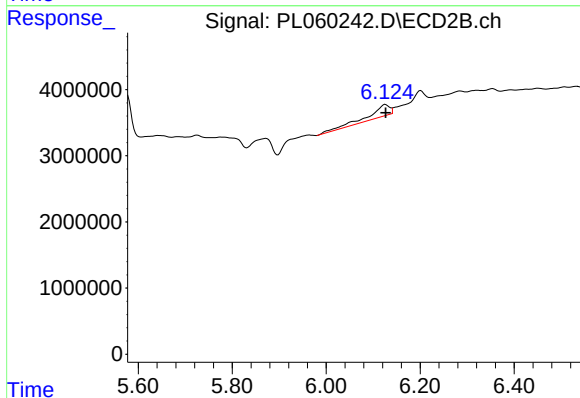


#10 gamma-Chlordane

R.T.: 6.126 min
Delta R.T.: -0.001 min
Response: 5556770
Conc: 1.94 ng/ml

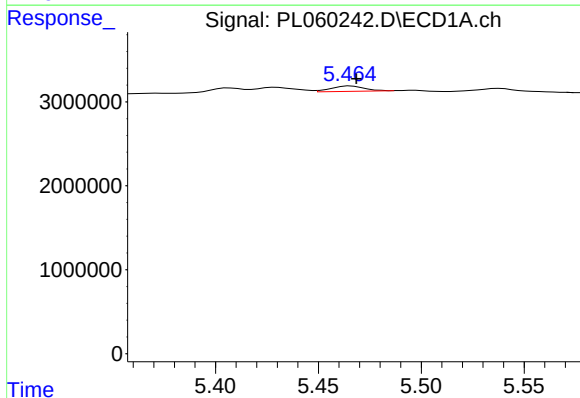


#11 alpha-Chlordane

R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 712528
Conc: 0.40 ng/ml

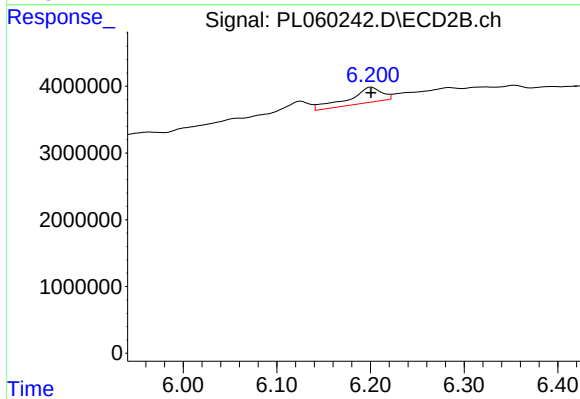

#11 alpha-Chlordane


R.T.: 6.201 min
Delta R.T.: 0.000 min
Response: 5596683
Conc: 1.96 ng/ml

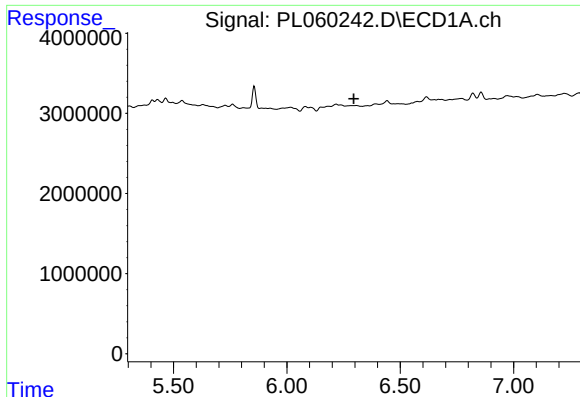

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.296 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

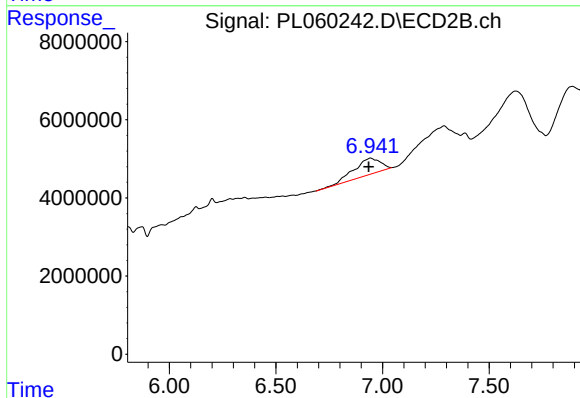


#15 Endosulfan II

R.T.: 6.943 min
Delta R.T.: 0.007 min
Response: 35959002
Conc: 14.32 ng/ml

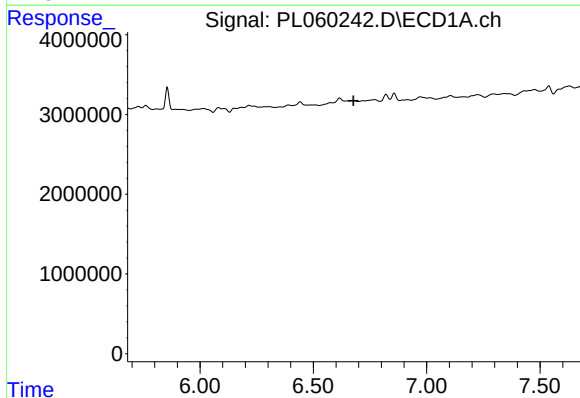


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.678 min
Response: 0
Conc: N.D.

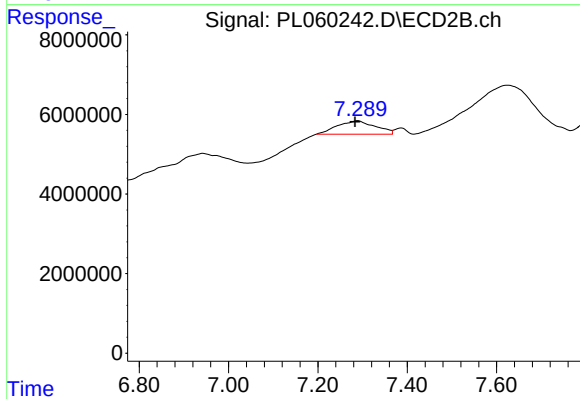

#19 Endosulfan Sulfate


R.T.: 7.290 min
Delta R.T.: 0.007 min
Response: 19896878
Conc: 8.51 ng/ml

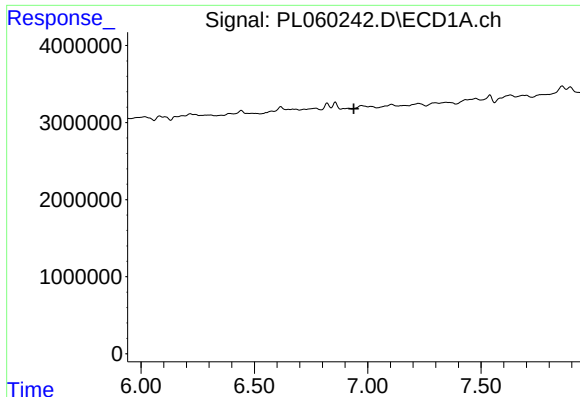

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.939 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

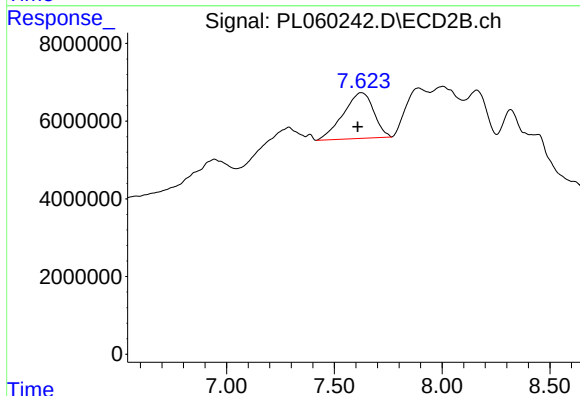


#20 Methoxychlor

R.T.: 7.625 min
Delta R.T.: 0.016 min
Response: 115790481
Conc: 102.00 ng/ml

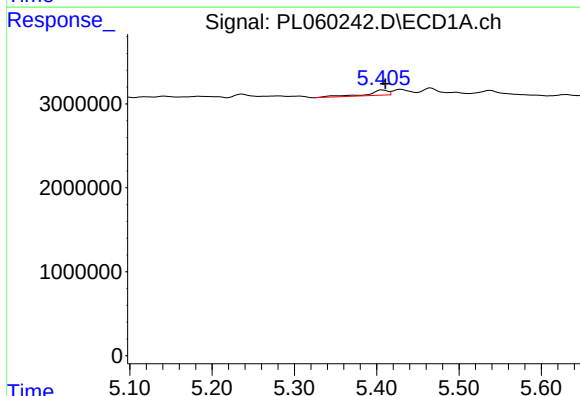


#25 Chlordane-3

R.T.: 5.407 min
Delta R.T.: -0.004 min
Response: 1082129
Conc: 6.40 ng/ml

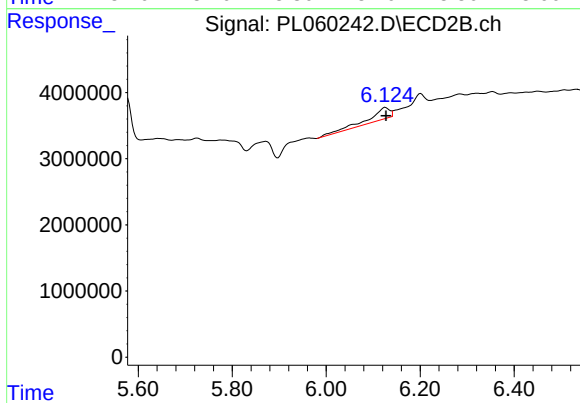

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: -0.002 min
Response: 5556770
Conc: 14.36 ng/ml

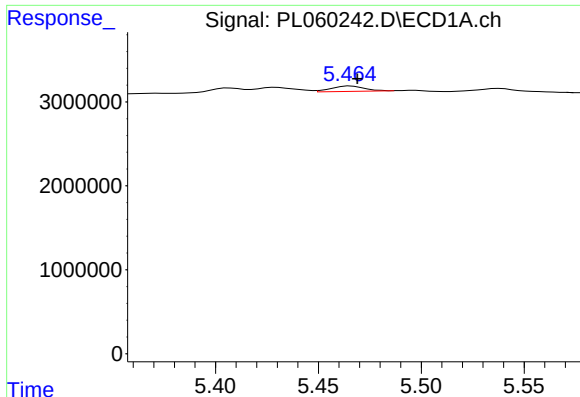

#26 Chlordane-4


R.T.: 5.466 min
Delta R.T.: -0.003 min
Response: 712528
Conc: 5.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

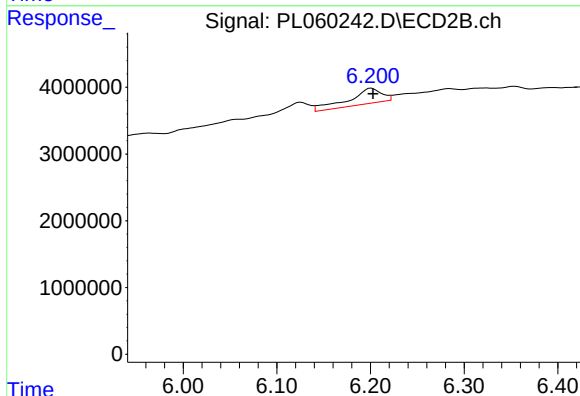


#26 Chlordane-4

R.T.: 6.201 min
Delta R.T.: -0.002 min
Response: 5596683
Conc: 12.09 ng/ml

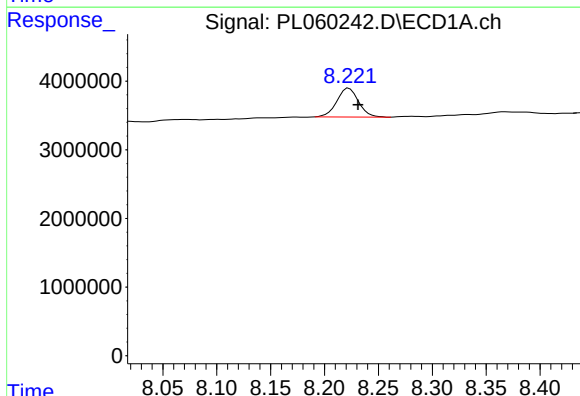

#28 Decachlorobiphenyl

R.T.: 8.223 min
Delta R.T.: -0.008 min
Response: 5894760
Conc: 3.58 ng/ml

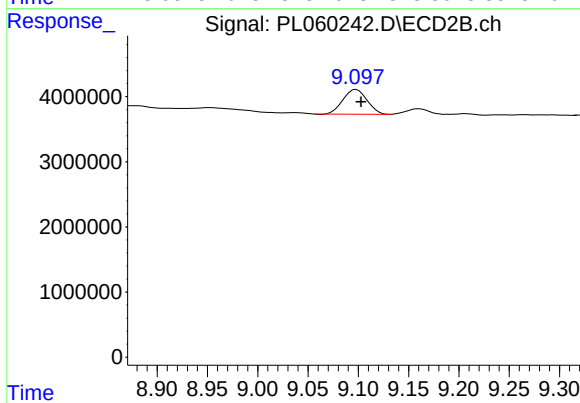

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: -0.005 min
Response: 6296915
Conc: 3.01 ng/ml