

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072720\
 Data File : PL060275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2020 00:22
 Operator : DD\AJ
 Sample : L3430-02 5X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TS2

Manual Integrations
 APPROVED

Ankita
 7/28/2020 12:18:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 01:16:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 10 18:52:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.465	4.014	11049901	8539468	5.713	3.222 #
28)	SA Decachlor...	8.224	9.097	5572483	5719608	3.387	2.735
Target Compounds							
10)	B gamma-Chl...	5.408	6.116	4434569	17729048	2.444m	6.191 #
11)	B alpha-Chl...	5.467	6.202	9844636	8691389	5.459	3.040 #
12)	B 4,4'-DDE	5.631	6.355	2273121	4348797	1.365	1.625

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072720\
Data File : PL060275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2020 00:22
Operator : DD\AJ
Sample : L3430-02 5X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TS2


Manual Integrations
APPROVED

Ankita
7/28/2020 12:18:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 01:16:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071020.M
Quant Title : GC Extractables
QLast Update : Fri Jul 10 18:52:06 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

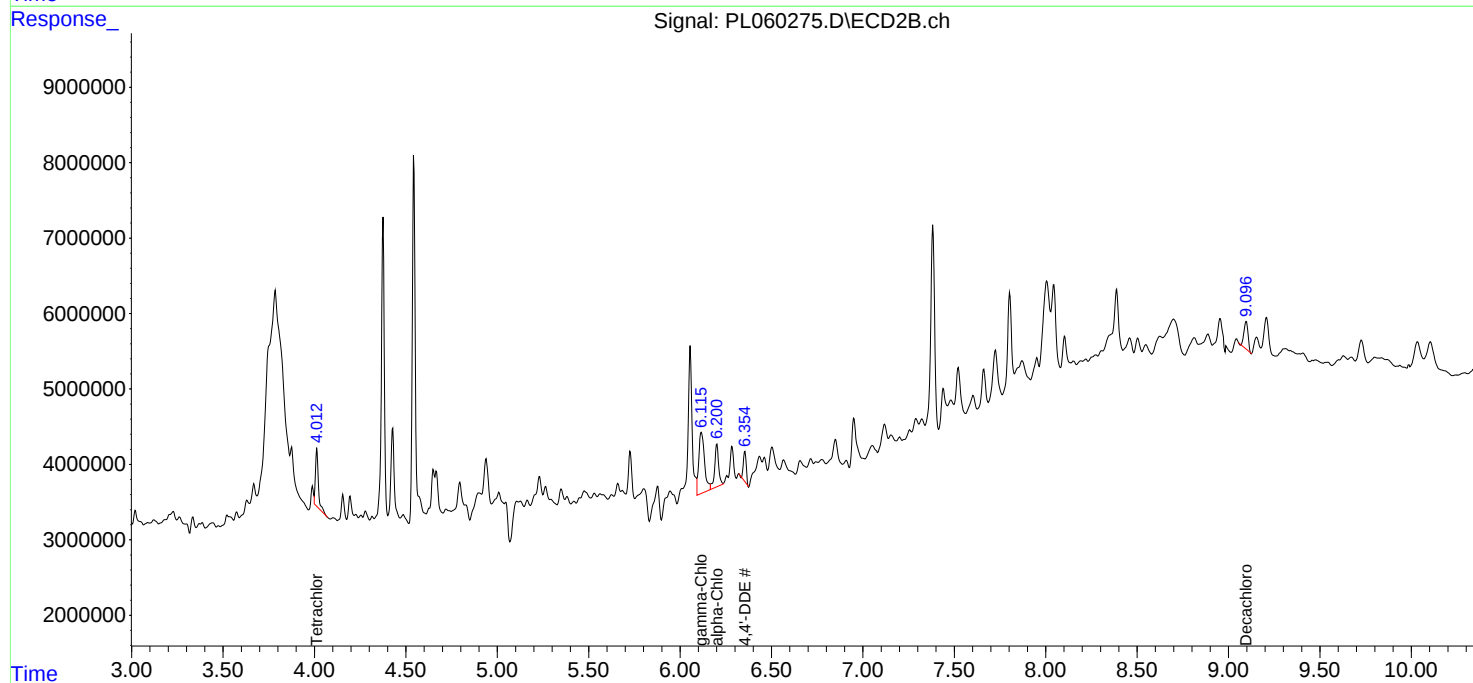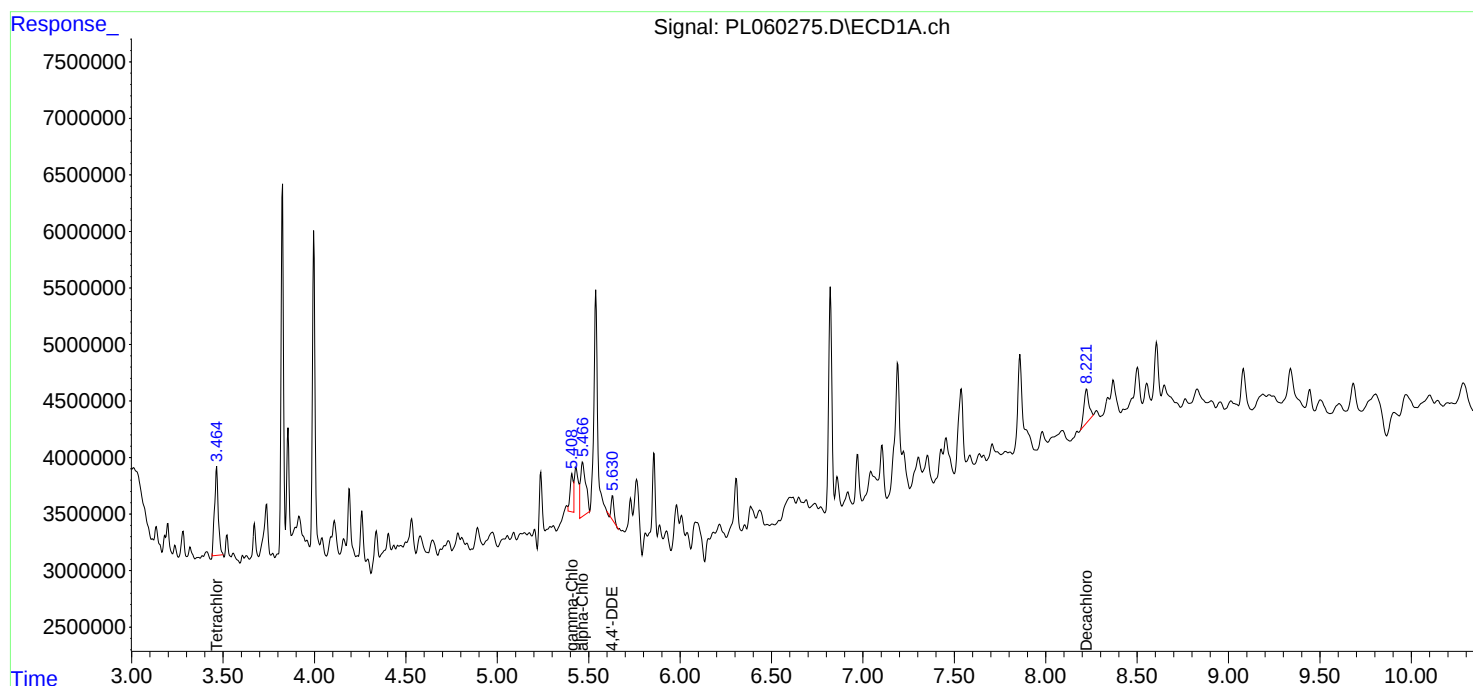

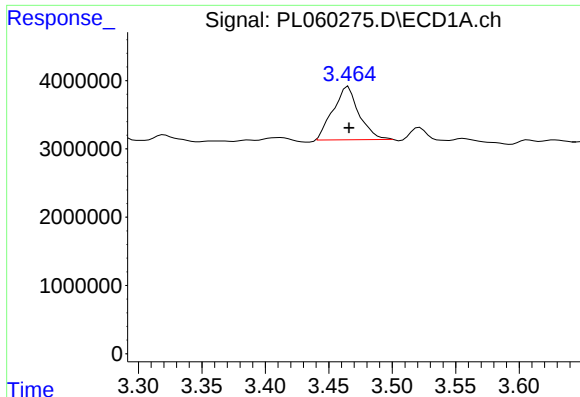


#1 Tetrachloro-m-xylene

R.T.: 3.465 min
Delta R.T.: 0.000 min
Response: 11049901
Conc: 5.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
TS2


Manual Integrations
APPROVED

Ankita
7/28/2020 12:18:00 PM

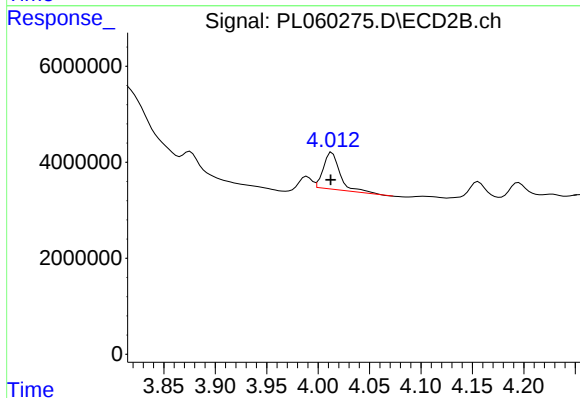


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: 0.001 min
Response: 8539468
Conc: 3.22 ng/ml

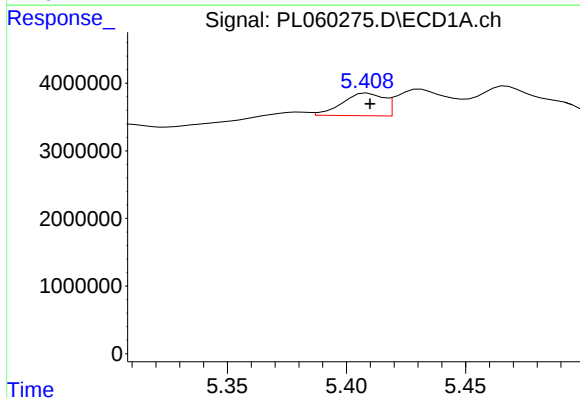


#10 gamma-Chlordane

R.T.: 5.408 min
Delta R.T.: -0.002 min
Response: 4434569
Conc: 2.44 ng/ml m

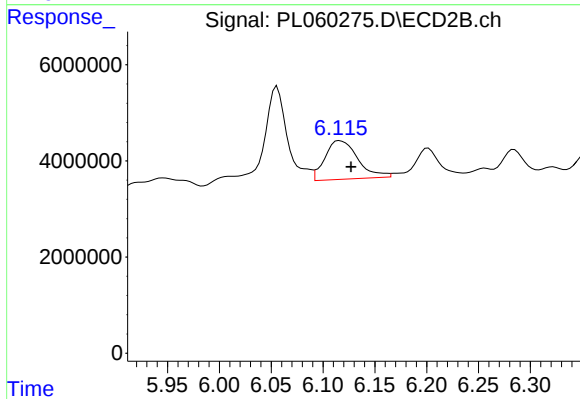

#10 gamma-Chlordane

R.T.: 6.116 min
Delta R.T.: -0.011 min
Response: 17729048
Conc: 6.19 ng/ml

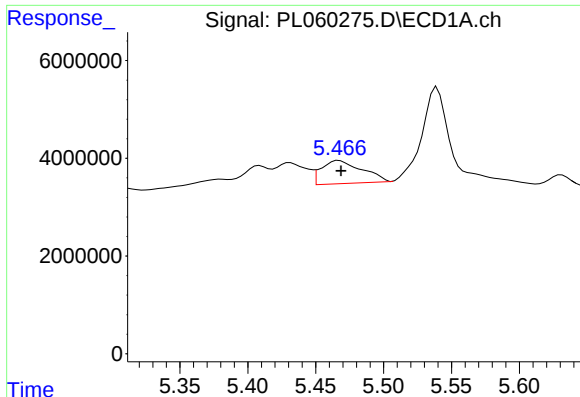


#11 alpha-Chlordane

R.T.: 5.467 min
Delta R.T.: -0.001 min
Response: 9844636
Conc: 5.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
TS2


Manual Integrations
APPROVED

Ankita
7/28/2020 12:18:00 PM

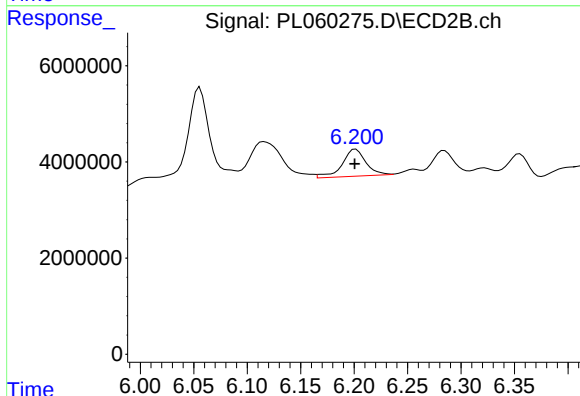


#11 alpha-Chlordane

R.T.: 6.202 min
Delta R.T.: 0.000 min
Response: 8691389
Conc: 3.04 ng/ml

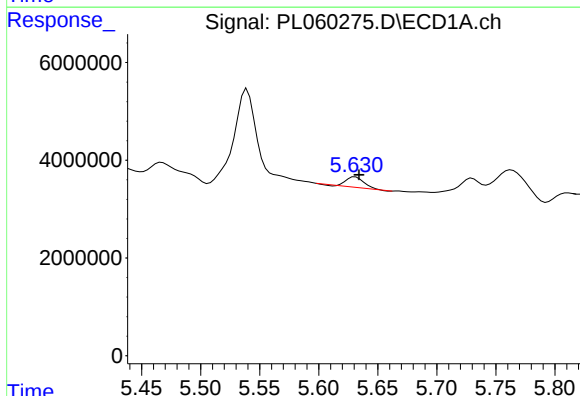


#12 4,4'-DDE

R.T.: 5.631 min
Delta R.T.: -0.003 min
Response: 2273121
Conc: 1.36 ng/ml

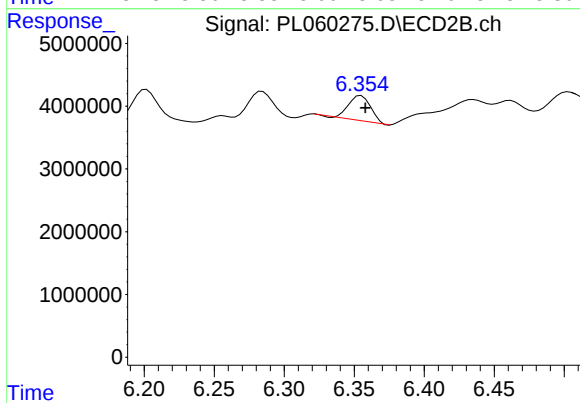

#12 4,4'-DDE

R.T.: 6.355 min
Delta R.T.: -0.003 min
Response: 4348797
Conc: 1.62 ng/ml

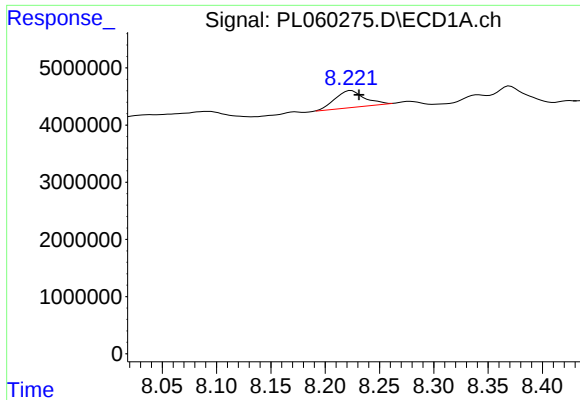


#28 Decachlorobiphenyl

R.T.: 8.224 min
Delta R.T.: -0.007 min
Response: 5572483
Conc: 3.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
TS2

Manual Integrations
APPROVED

Ankita
7/28/2020 12:18:00 PM

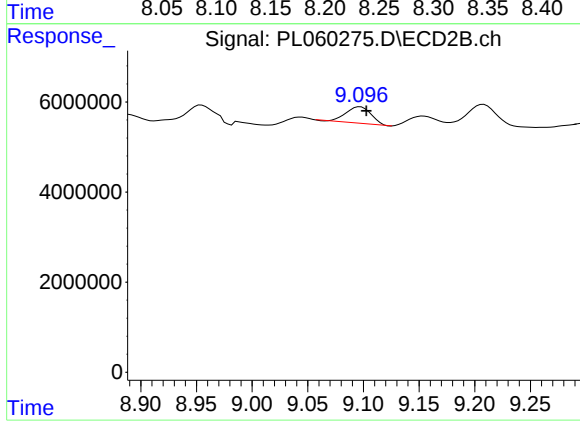

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: -0.006 min
Response: 5719608
Conc: 2.73 ng/ml