

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072721\
 Data File : PL068491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2021 12:26
 Operator : AR\AJ
 Sample : PB137986BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB137986BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 02:32:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.647	5.570	9021441	19578156	21.020	19.186
28)	SA Decachlor...	10.421	11.496	12798018	19092514	22.755	21.404
Target Compounds							
6)	B beta-BHC	0.000	6.826f	0	8946959	N.D.	12.664 #
9)	A Endosulfan I	0.000	8.425	0	43177	N.D.	0.042 #
13)	MA Dieldrin	0.000	8.728	0	84173	N.D.	0.079 #
14)	MA Endrin	0.000	8.948f	0	10422	N.D.	0.012 #
15)	B Endosulfa...	0.000	9.216f	0	188722	N.D.	0.208 #
18)	B Endrin al...	0.000	9.361f	0	16674	N.D.	0.023 #
22)	Mirex	0.000	10.549	0	44228	N.D.	0.057 #
23)	Chlordane-1	0.000	6.971	0	564669	N.D.	13.939 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072721\
Data File : PL068491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2021 12:26
Operator : AR\AJ
Sample : PB137986BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB137986BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 02:32:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

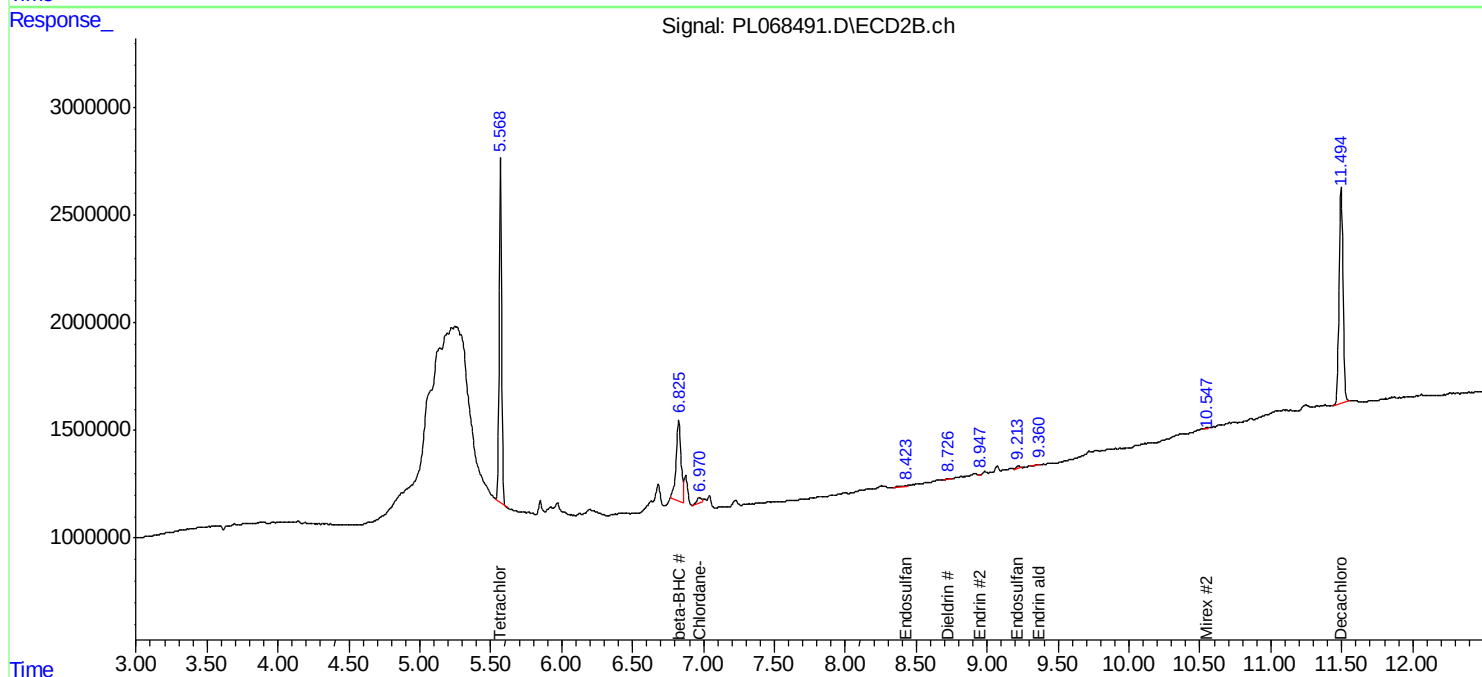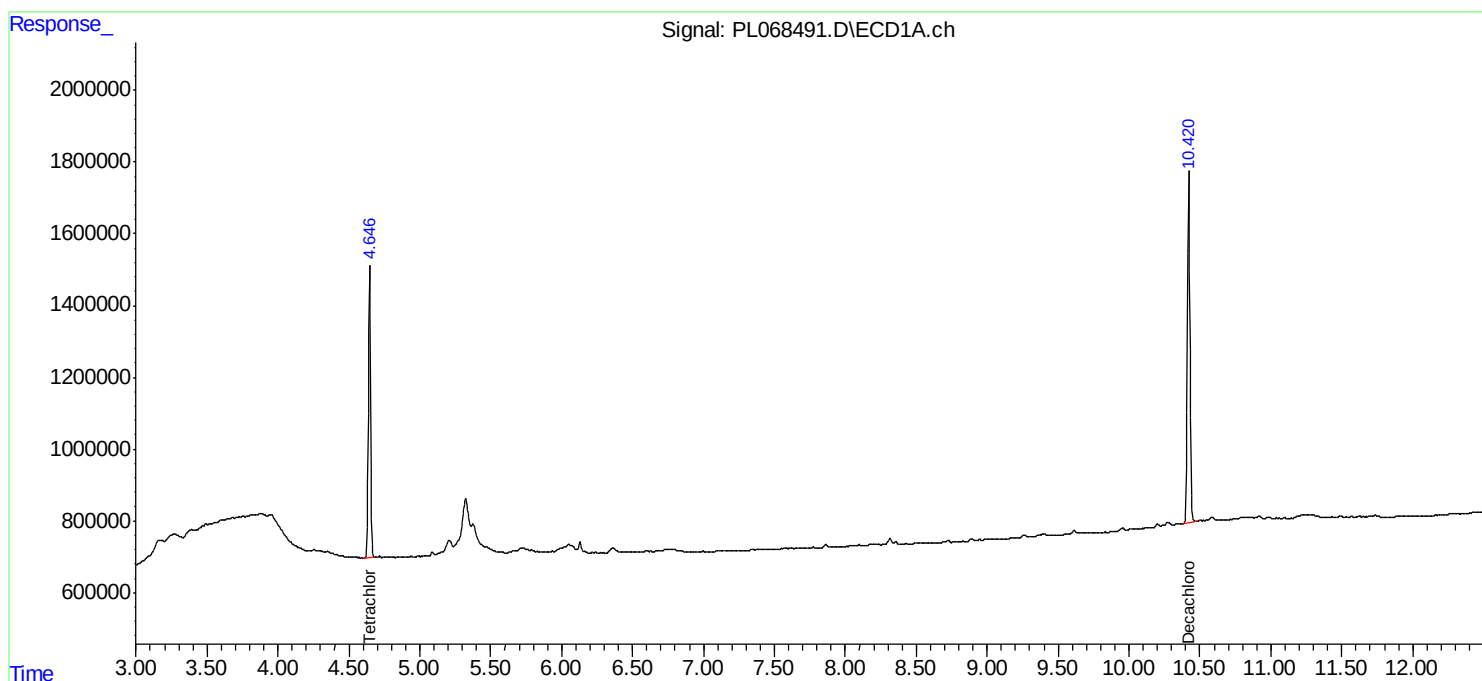


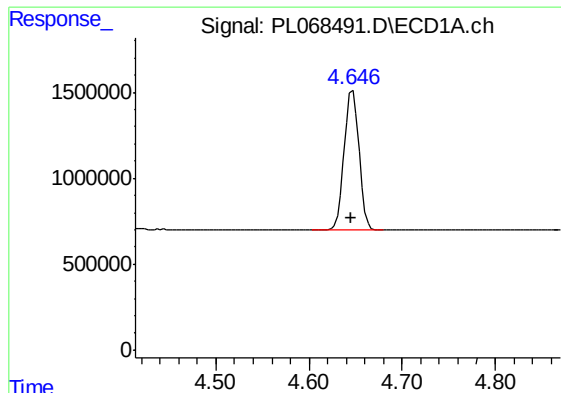

#1 Tetrachloro-m-xylene


R.T.: 4.647 min
Delta R.T.: 0.002 min
Response: 9021441
Conc: 21.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB137986BL

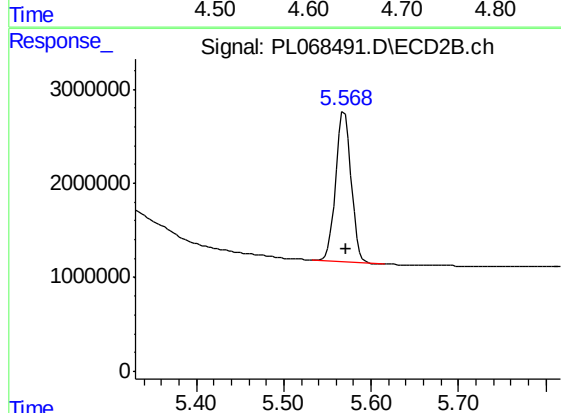


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: -0.001 min
Response: 19578156
Conc: 19.19 ng/ml

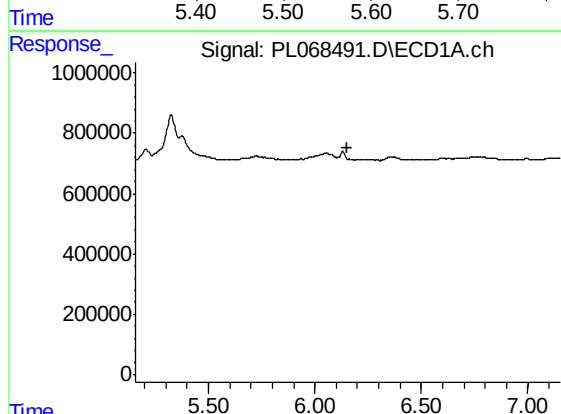


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

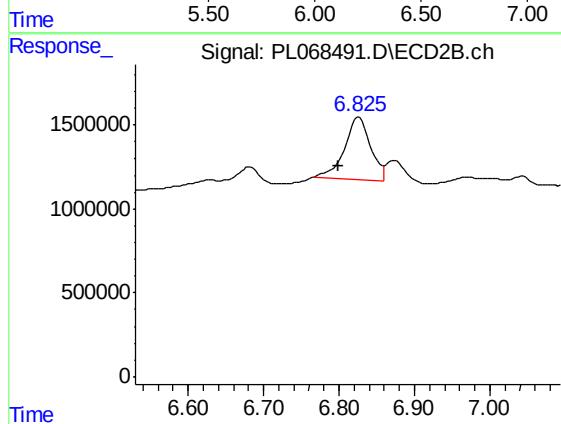

#6 beta-BHC


R.T.: 6.826 min
Delta R.T.: 0.027 min
Response: 8946959
Conc: 12.66 ng/ml

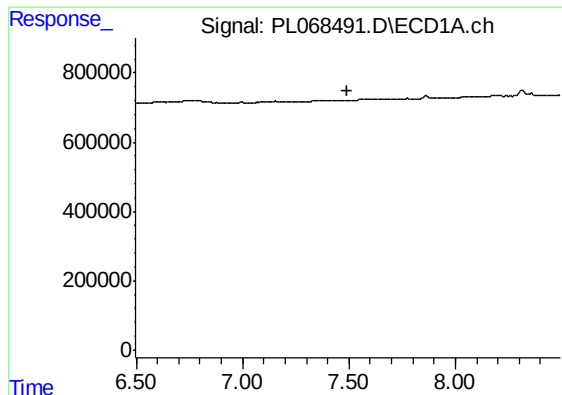

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB137986BL

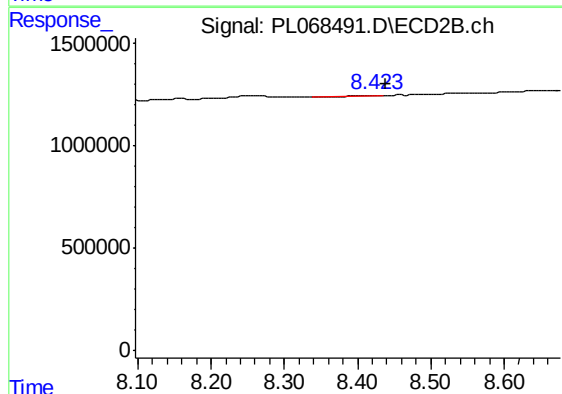


#9 Endosulfan I

R.T.: 8.425 min
Delta R.T.: -0.014 min
Response: 43177
Conc: 0.04 ng/ml

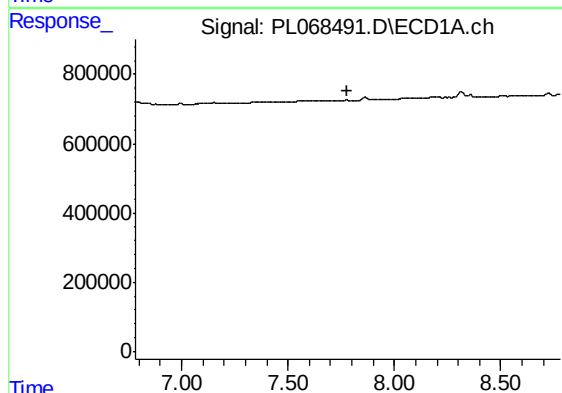


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 7.781 min
Response: 0
Conc: N.D.

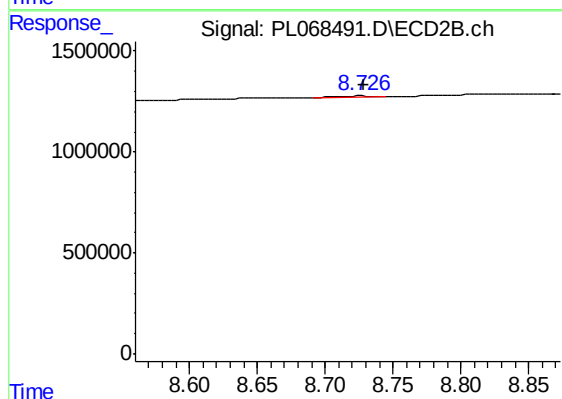

#13 Dieldrin


R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 84173
Conc: 0.08 ng/ml

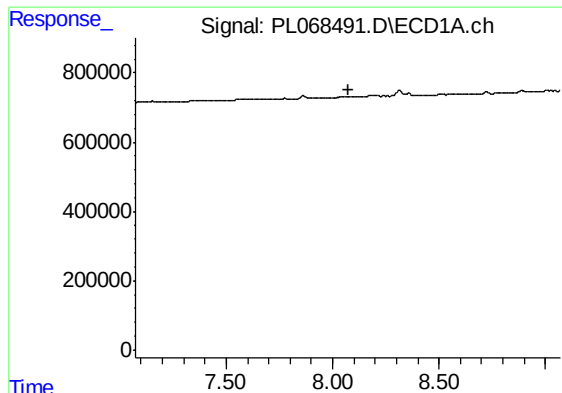

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB137986BL

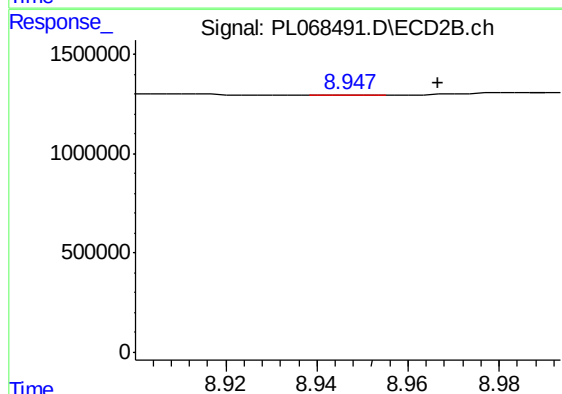


#14 Endrin

R.T.: 8.948 min
Delta R.T.: -0.019 min
Response: 10422
Conc: 0.01 ng/ml

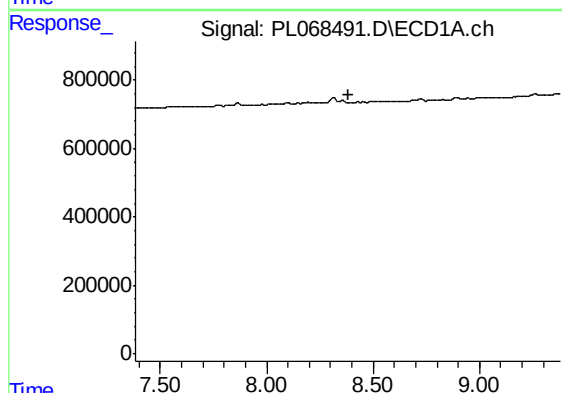


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

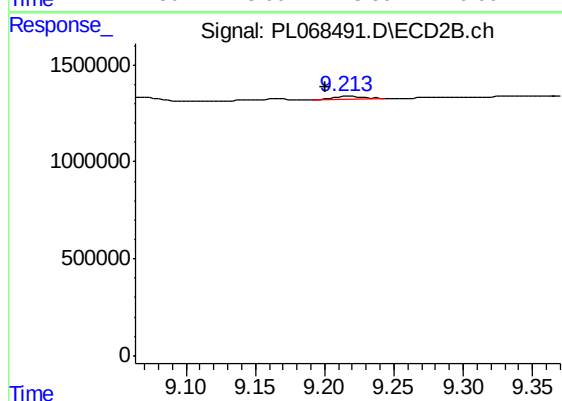

#15 Endosulfan II


R.T.: 9.216 min
Delta R.T.: 0.015 min
Response: 188722
Conc: 0.21 ng/ml

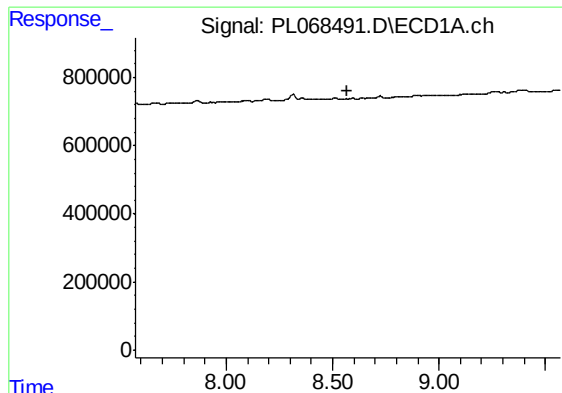

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 8.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB137986BL

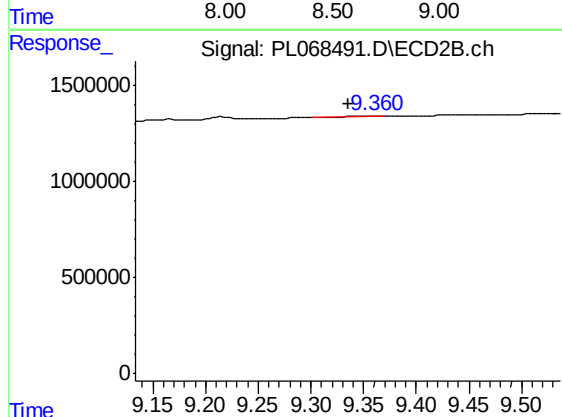


#18 Endrin aldehyde

R.T.: 9.361 min
Delta R.T.: 0.026 min
Response: 16674
Conc: 0.02 ng/ml

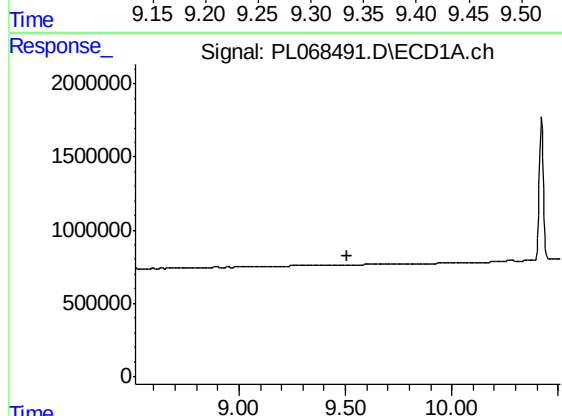


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

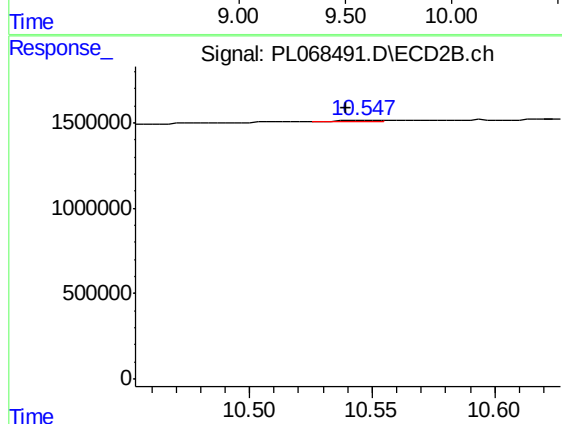

#22 Mirex


R.T.: 10.549 min
Delta R.T.: 0.009 min
Response: 44228
Conc: 0.06 ng/ml

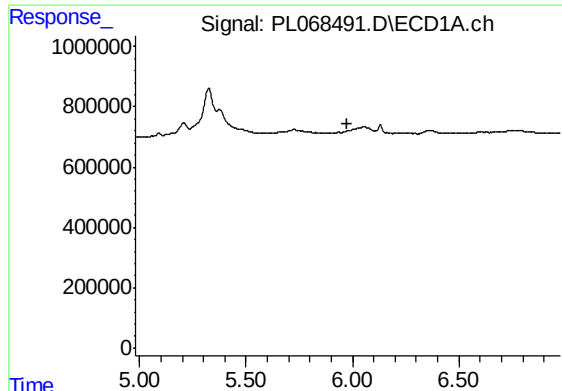

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB137986BL

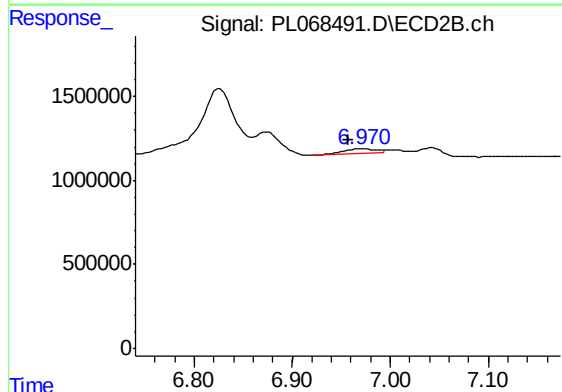


#23 Chlordane-1

R.T.: 6.971 min
Delta R.T.: 0.014 min
Response: 564669
Conc: 13.94 ng/ml

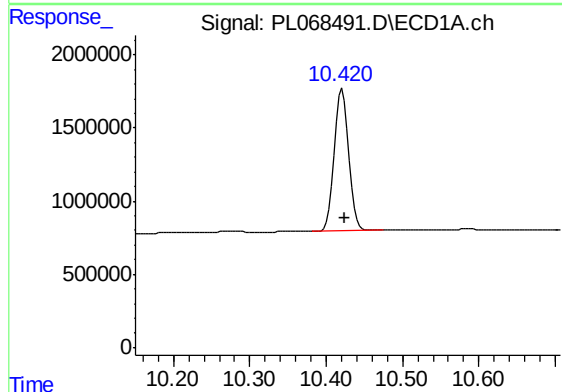

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: -0.003 min
Response: 12798018
Conc: 22.76 ng/ml

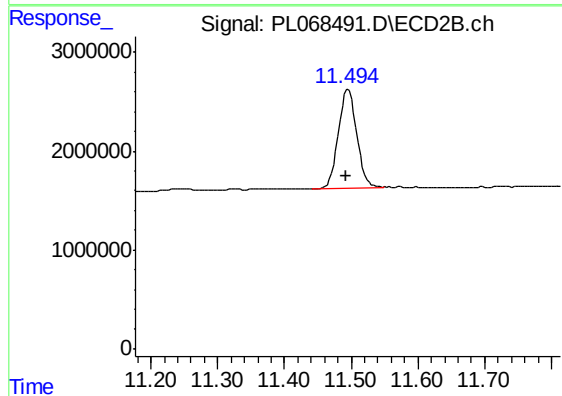

#28 Decachlorobiphenyl

R.T.: 11.496 min
Delta R.T.: 0.003 min
Response: 19092514
Conc: 21.40 ng/ml