

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072721\
 Data File : PL068494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2021 13:16
 Operator : AR\AJ
 Sample : M3184-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210564-COM-37

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 02:33:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.570	5444902	11825101	12.687	11.588
28)	SA Decachlor...	10.416	11.491	6072555	9529819	10.797	10.684
Target Compounds							
8)	B Heptachlo...	0.000	8.033	0	201443	N.D.	0.178 #
12)	B 4,4'-DDE	0.000	8.570	0	101047	N.D.	0.098 #
13)	MA Dieldrin	0.000	8.727	0	53444	N.D.	0.050 #
14)	MA Endrin	0.000	8.964	0	106162	N.D.	0.119 #
15)	B Endosulfa...	0.000	9.216	0	105772	N.D.	0.117 #
19)	B Endosulfa...	0.000	9.573	0	35451	N.D.	0.039 #
21)	B Endrin ke...	0.000	10.097f	0	59405	N.D.	0.060 #
22)	Mirex	0.000	10.559f	0	183275	N.D.	0.237 #
23)	Chlordane-1	0.000	6.977f	0	474135	N.D.	11.704 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072721\
Data File : PL068494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2021 13:16
Operator : AR\AJ
Sample : M3184-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20210564-COM-37

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 02:33:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

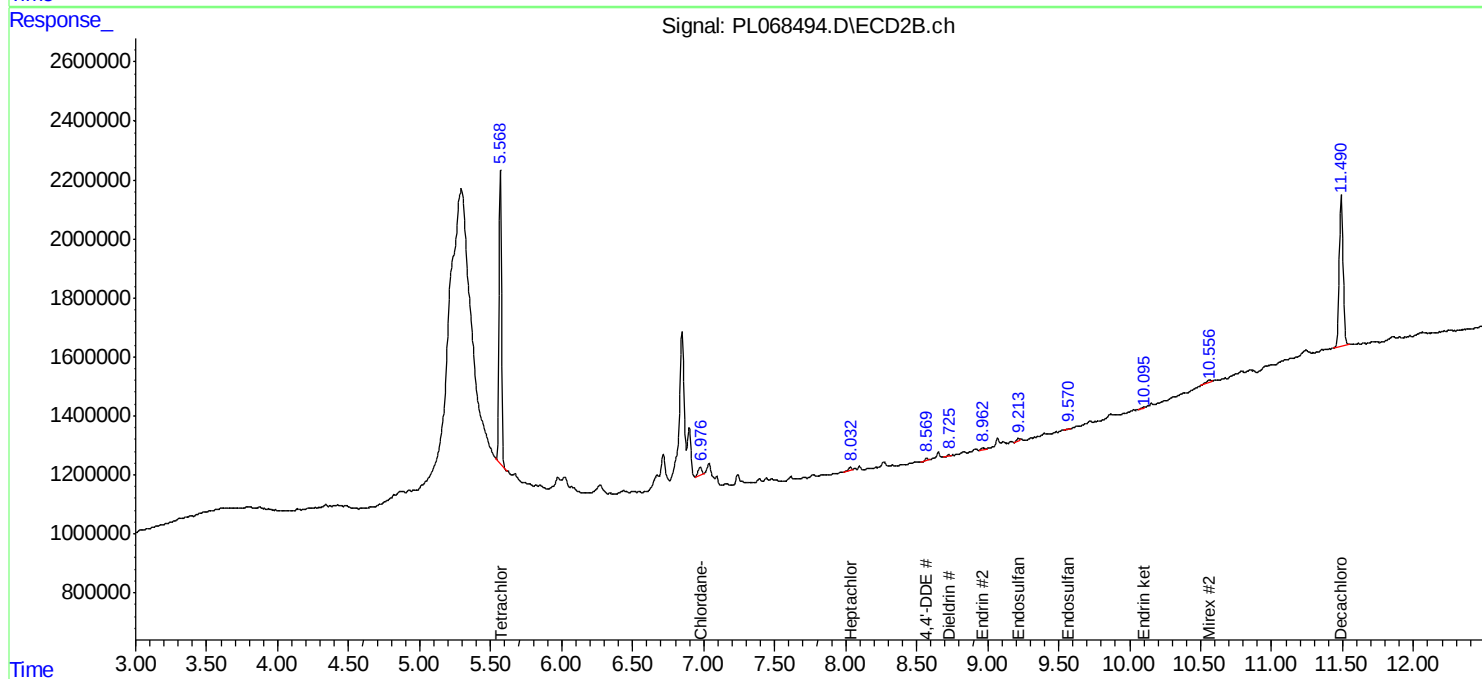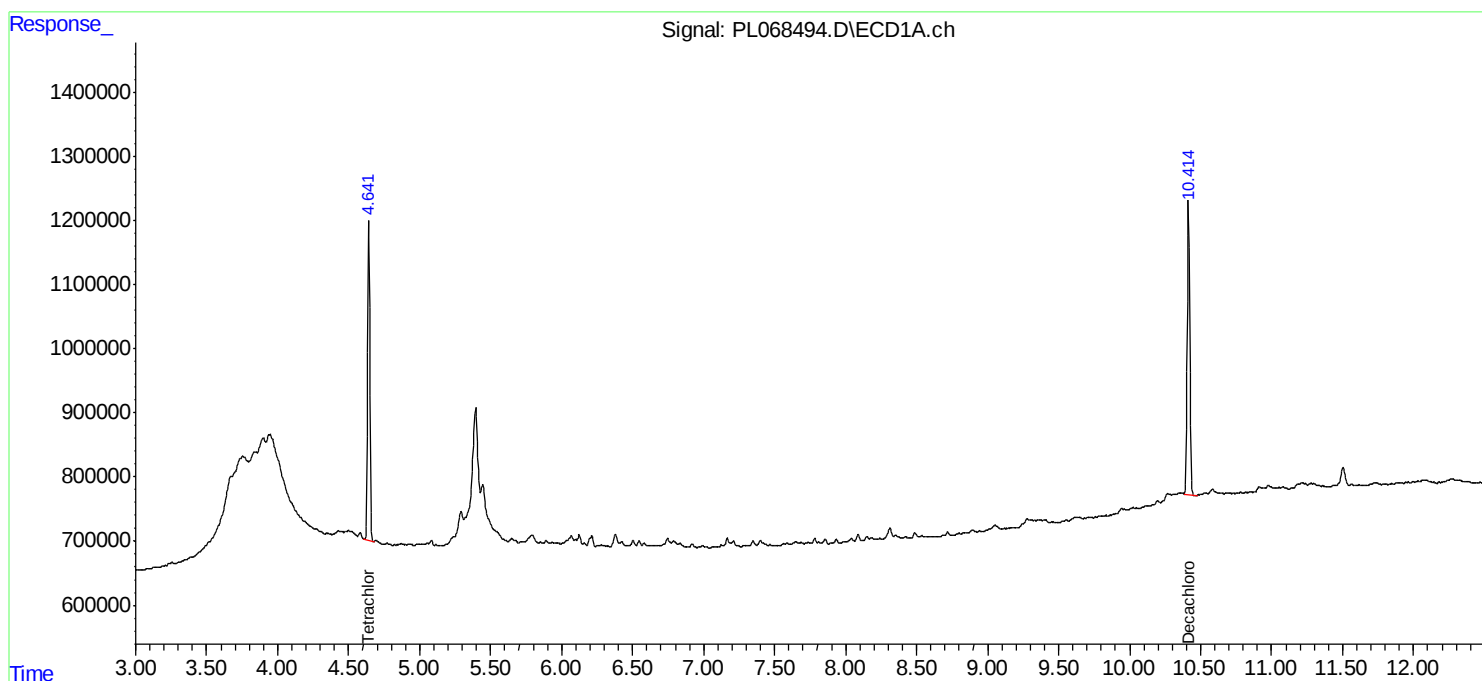


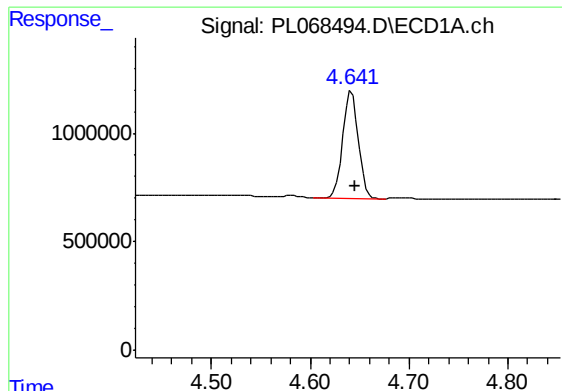

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 5444902
Conc: 12.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210564-COM-37

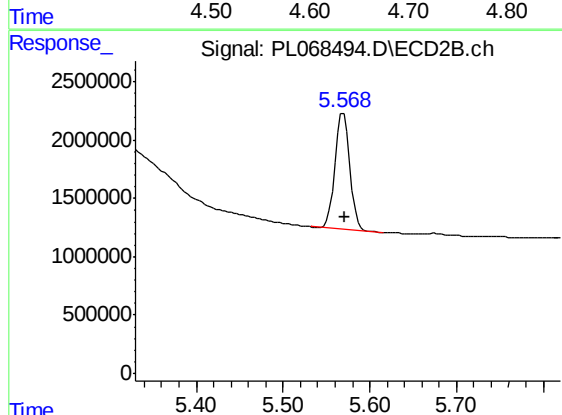


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: -0.001 min
Response: 11825101
Conc: 11.59 ng/ml

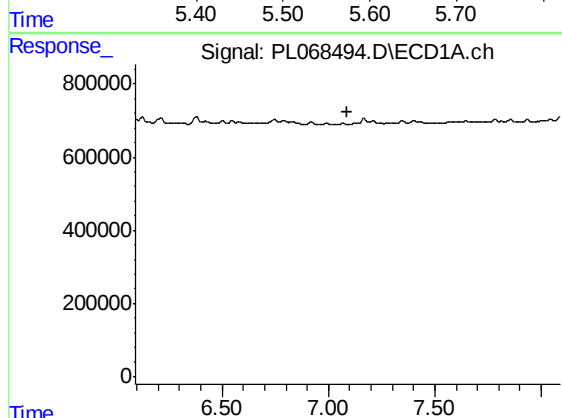


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

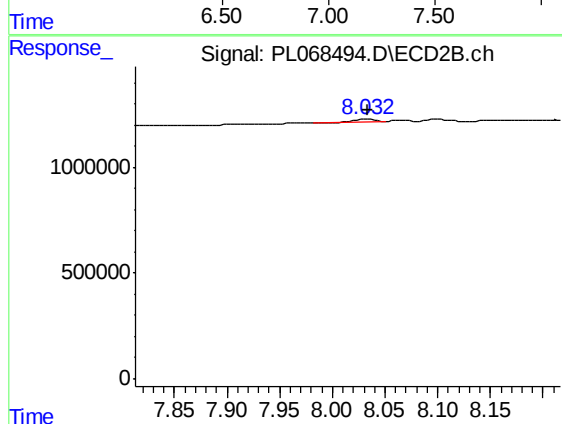

#8 Heptachlor epoxide


R.T.: 8.033 min
Delta R.T.: 0.000 min
Response: 201443
Conc: 0.18 ng/ml

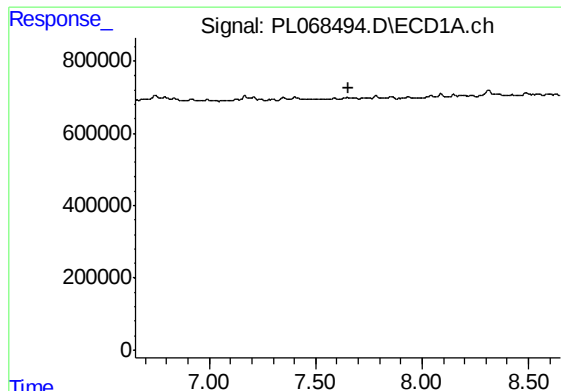

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.653 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210564-COM-37

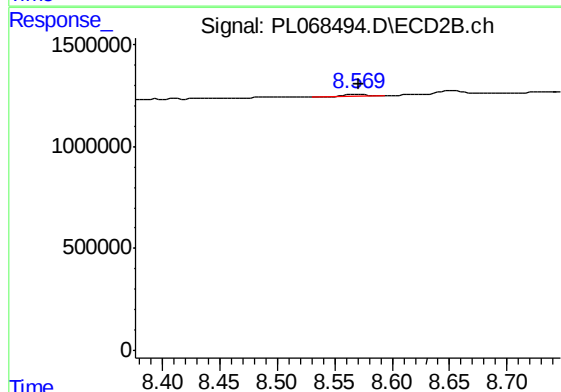


#12 4,4'-DDE

R.T.: 8.570 min
Delta R.T.: 0.000 min
Response: 101047
Conc: 0.10 ng/ml

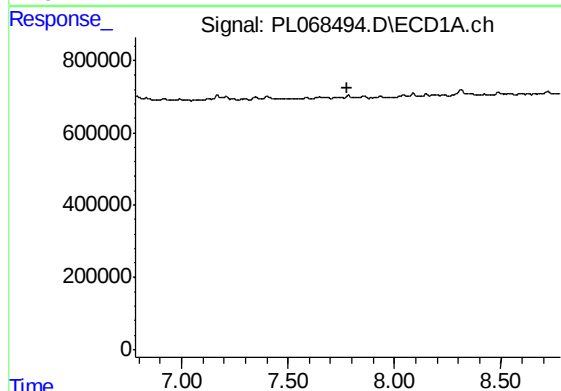


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.781 min
Response: 0
Conc: N.D.

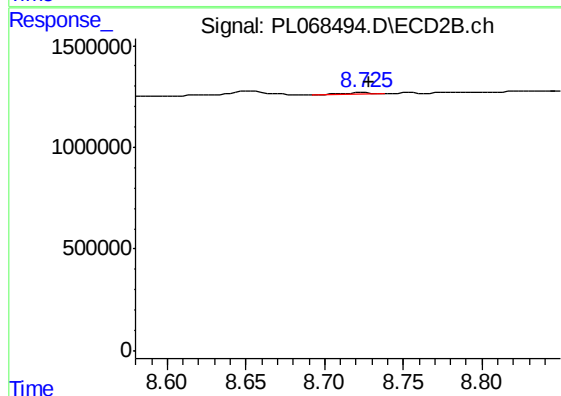

#13 Dieldrin


R.T.: 8.727 min
Delta R.T.: -0.002 min
Response: 53444
Conc: 0.05 ng/ml

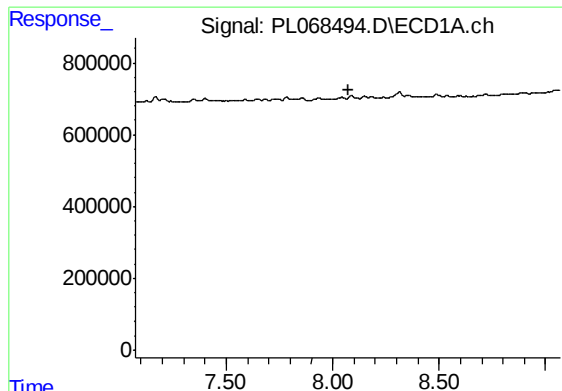

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210564-COM-37

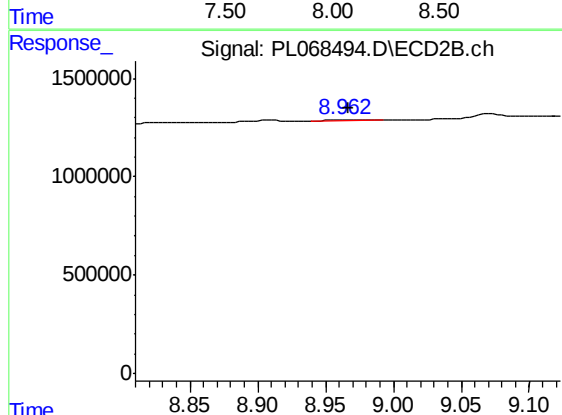


#14 Endrin

R.T.: 8.964 min
Delta R.T.: -0.003 min
Response: 106162
Conc: 0.12 ng/ml

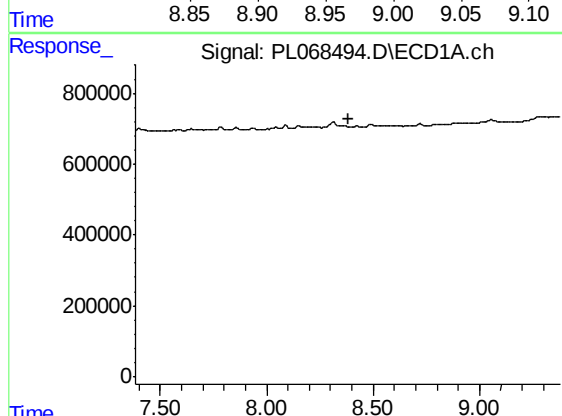


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

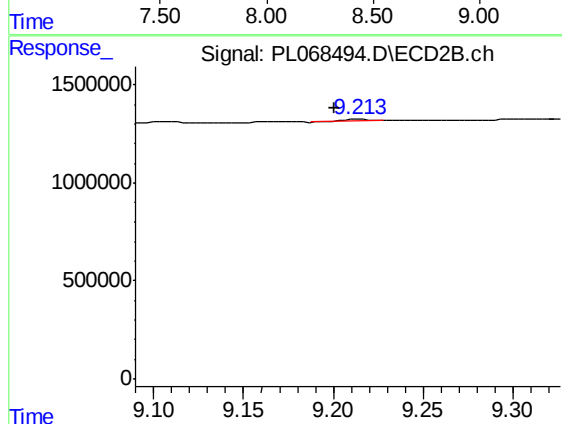

#15 Endosulfan II


R.T.: 9.216 min
Delta R.T.: 0.015 min
Response: 105772
Conc: 0.12 ng/ml

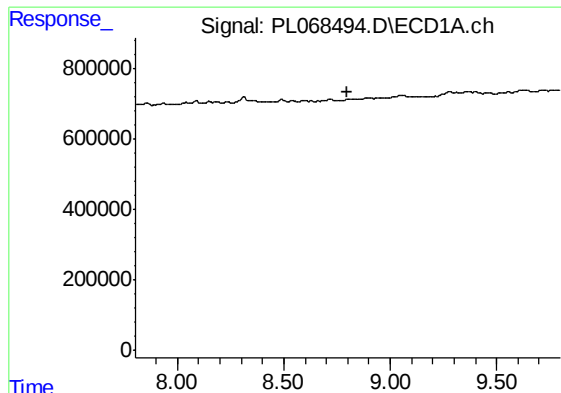

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 8.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210564-COM-37

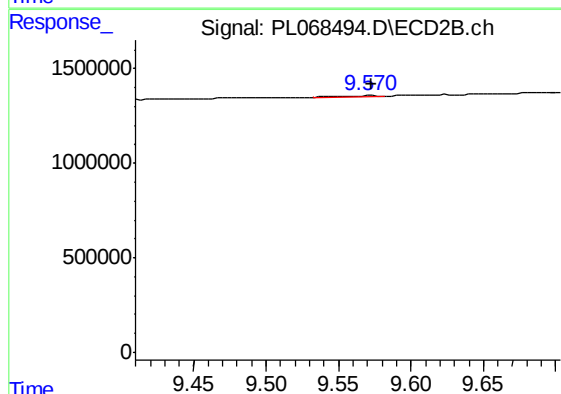


#19 Endosulfan Sulfate

R.T.: 9.573 min
Delta R.T.: 0.000 min
Response: 35451
Conc: 0.04 ng/ml

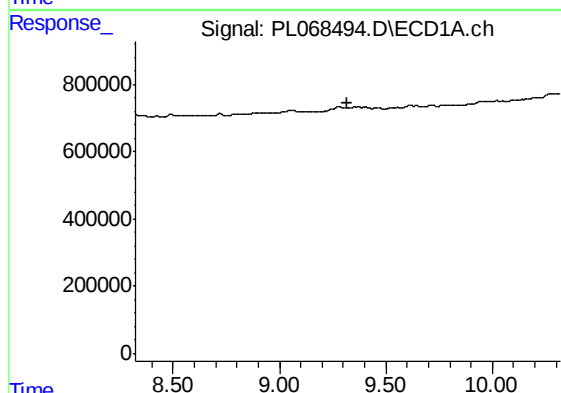


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.320 min
Response: 0
Conc: N.D.

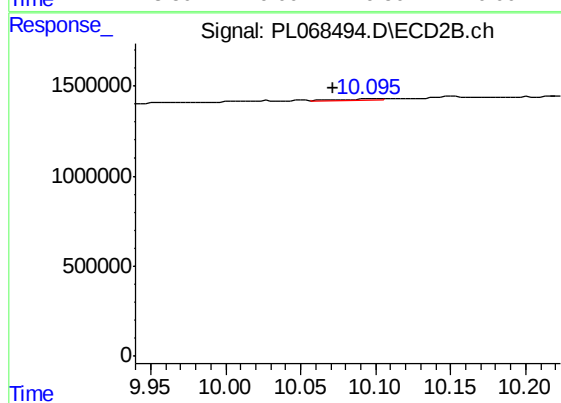

#21 Endrin ketone


R.T.: 10.097 min
Delta R.T.: 0.025 min
Response: 59405
Conc: 0.06 ng/ml

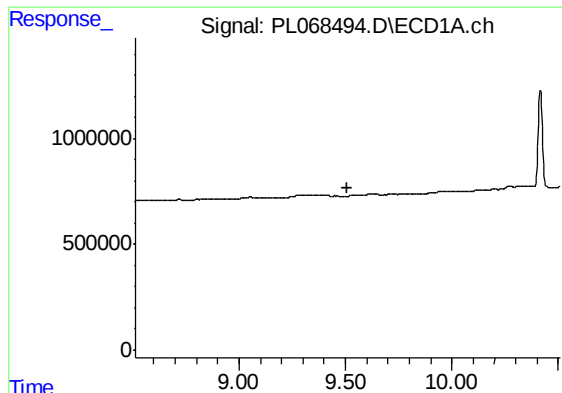

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210564-COM-37

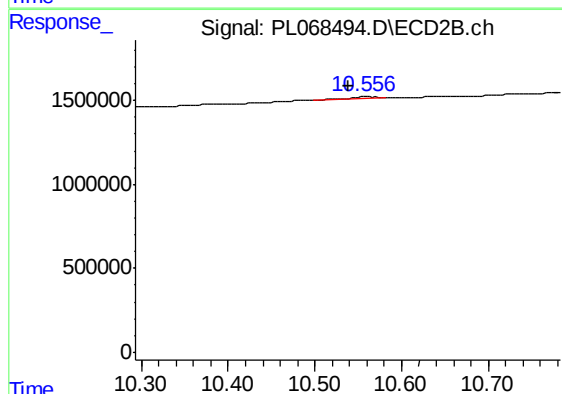


#22 Mirex

R.T.: 10.559 min
Delta R.T.: 0.020 min
Response: 183275
Conc: 0.24 ng/ml

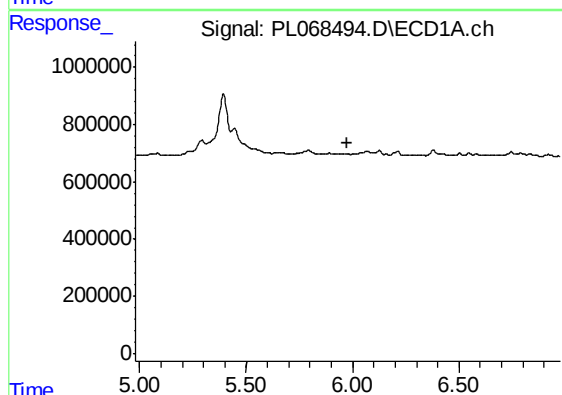


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.978 min
Response: 0
Conc: N.D.

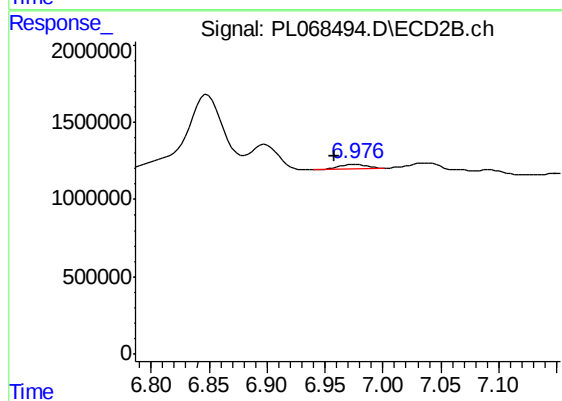

#23 Chlordane-1


R.T.: 6.977 min
Delta R.T.: 0.019 min
Response: 474135
Conc: 11.70 ng/ml

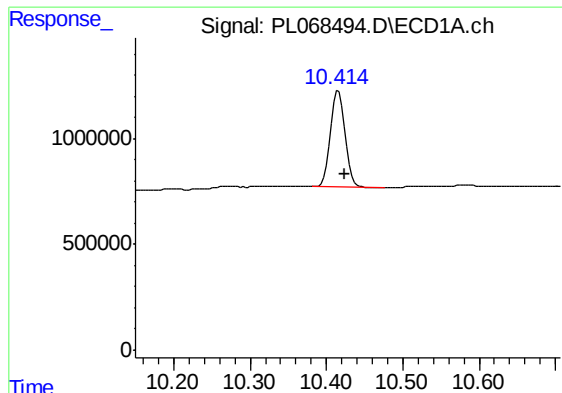

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.009 min
Response: 6072555
Conc: 10.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210564-COM-37

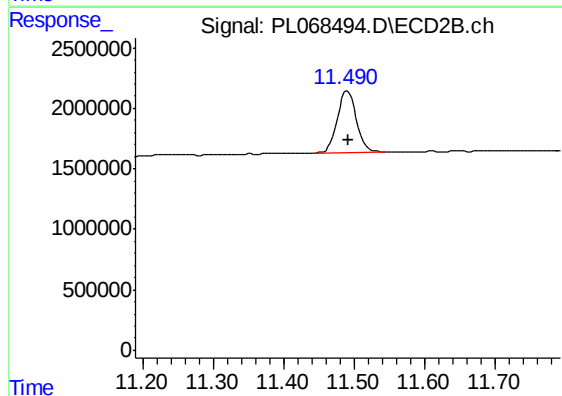

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: -0.001 min
Response: 9529819
Conc: 10.68 ng/ml