

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072722\
 Data File : PL076675.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2022 16:25
 Operator : AR\AJ
 Sample : N3888-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 03:26:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	2.644	11816541	29702614	11.450	10.014
28)	SA Decachlor...	8.916	7.754	10523741	26405433	11.932	10.287
Target Compounds							
3)	MA gamma-BHC...	4.245f	0.000	49575	0	0.037	N.D. #
4)	MA Heptachlor	0.000	3.818f	0	4139615	N.D.	1.096 #
5)	MB Aldrin	0.000	4.059	0	833282	N.D.	0.237 #
6)	B beta-BHC	4.433	0.000	329400	0	0.552	N.D. #
9)	A Endosulfan I	0.000	4.955f	0	1106650	N.D.	0.382 #
12)	B 4,4'-DDE	0.000	5.077	0	303833	N.D.	0.102 #
14)	MA Endrin	0.000	5.495f	0	38277	N.D.	0.015 #
17)	MA 4,4'-DDT	0.000	5.868	0	149448	N.D.	0.062 #
23)	Chlordane-1	0.000	3.622	0	767778	N.D.	8.498 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072722\
Data File : PL076675.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2022 16:25
Operator : AR\AJ
Sample : N3888-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 03:26:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

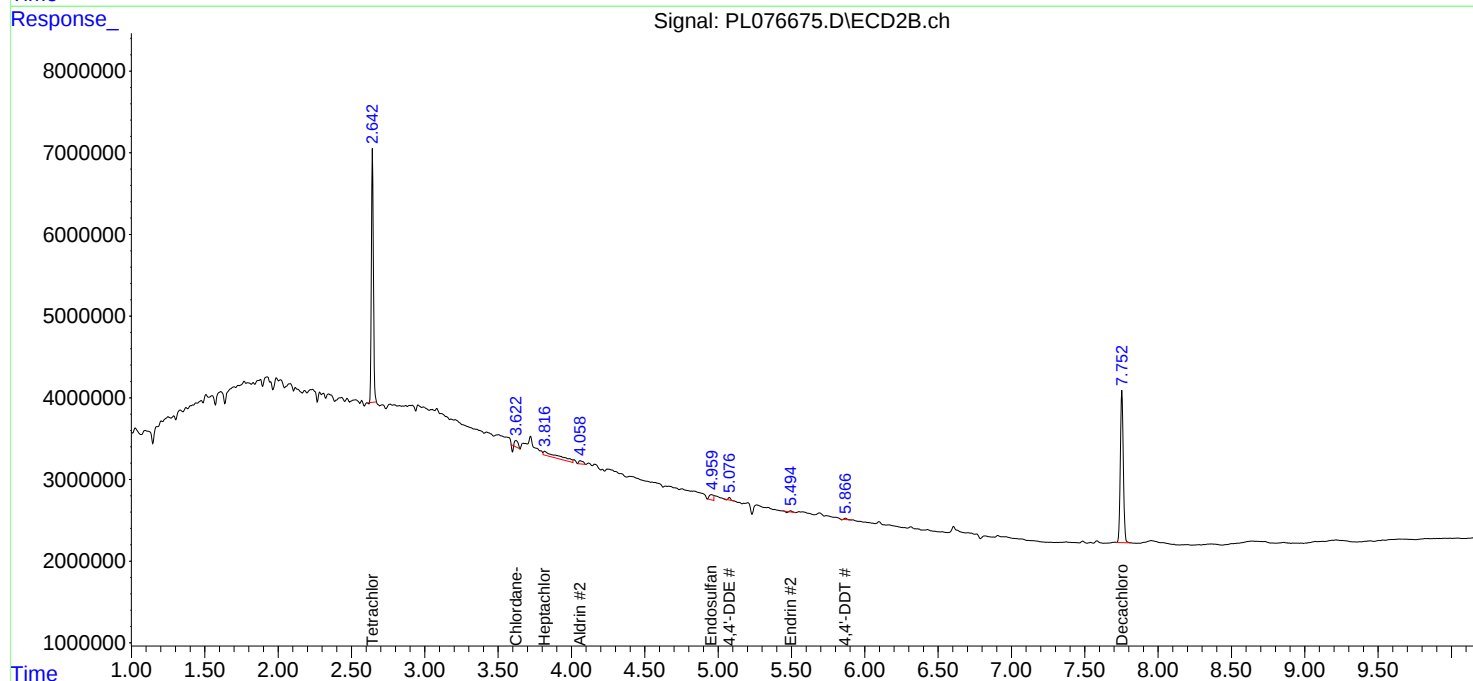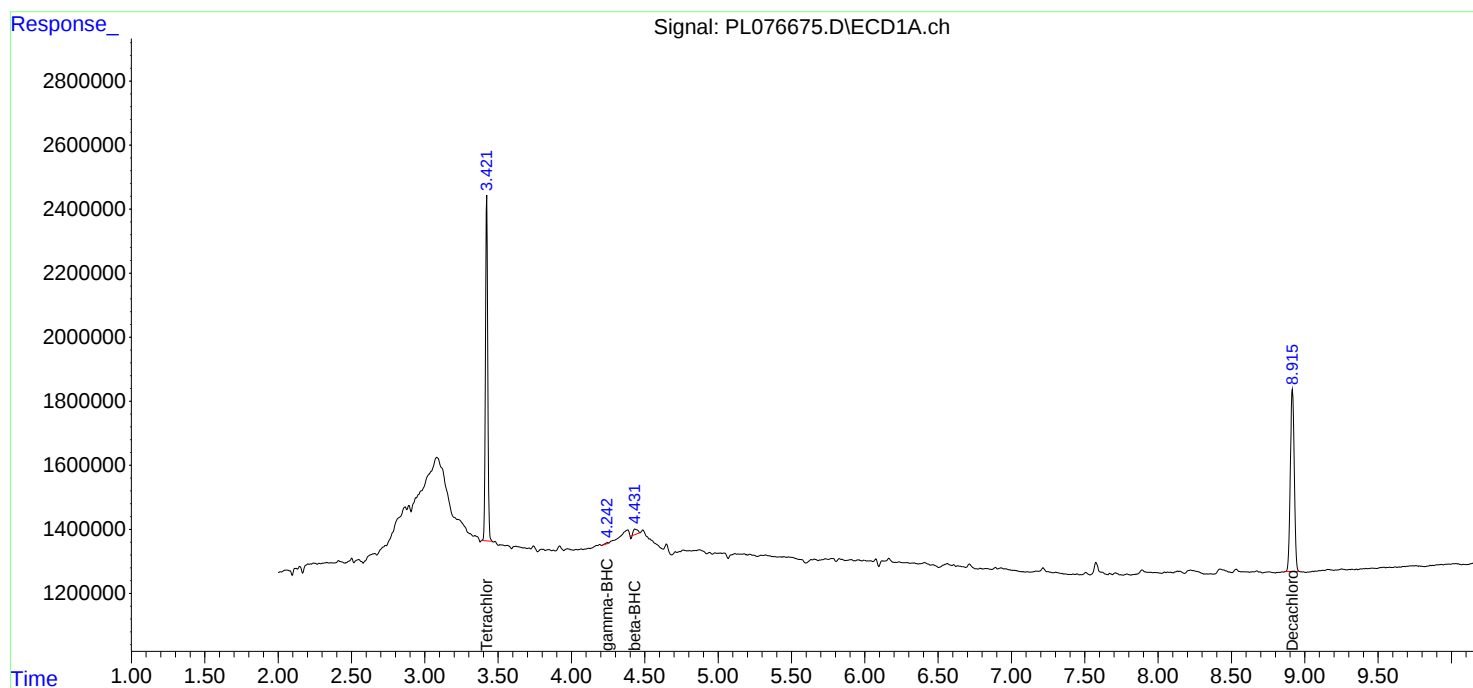


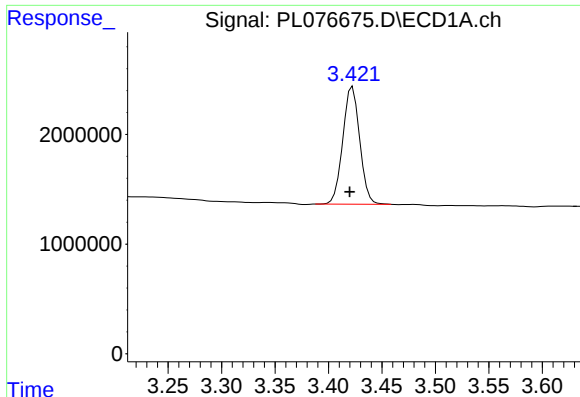

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: 0.003 min
Response: 11816541
Conc: 11.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

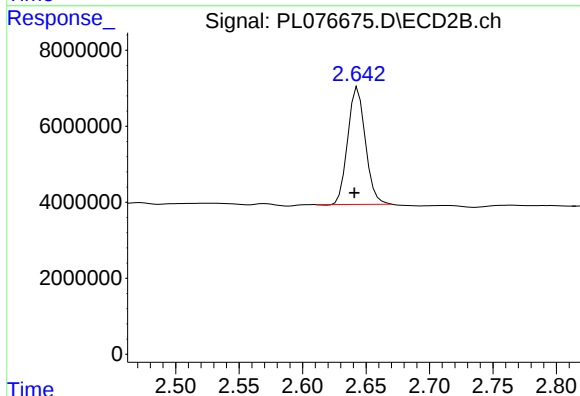


#1 Tetrachloro-m-xylene

R.T.: 2.644 min
Delta R.T.: 0.003 min
Response: 29702614
Conc: 10.01 ng/ml

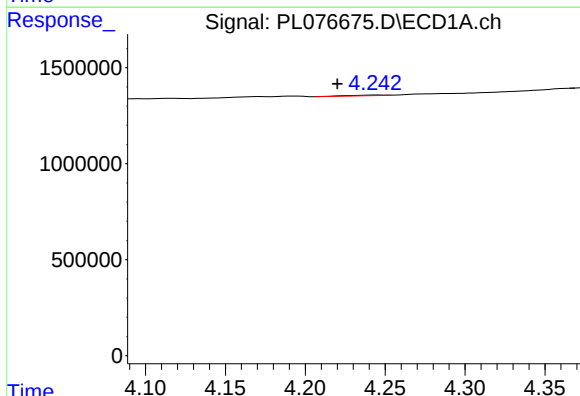


#3 gamma-BHC (Lindane)

R.T.: 4.245 min
Delta R.T.: 0.025 min
Response: 49575
Conc: 0.04 ng/ml

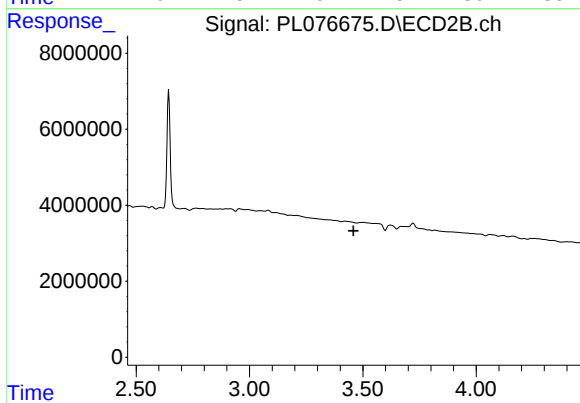

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.459 min
Response: 0
Conc: N.D.

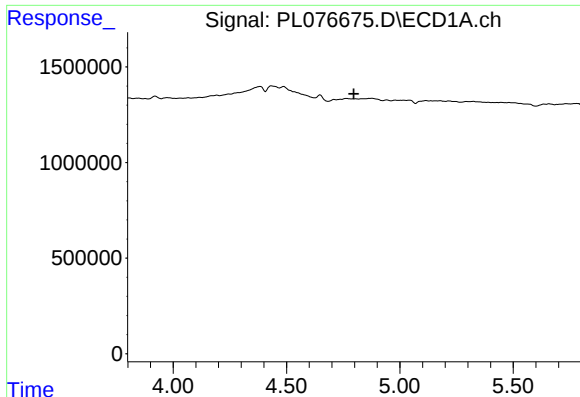

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.796 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

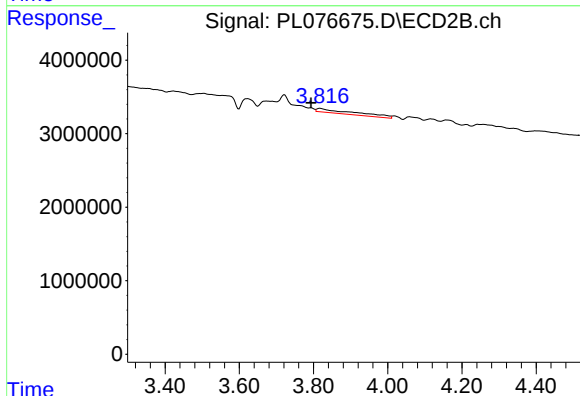


#4 Heptachlor

R.T.: 3.818 min
Delta R.T.: 0.025 min
Response: 4139615
Conc: 1.10 ng/ml

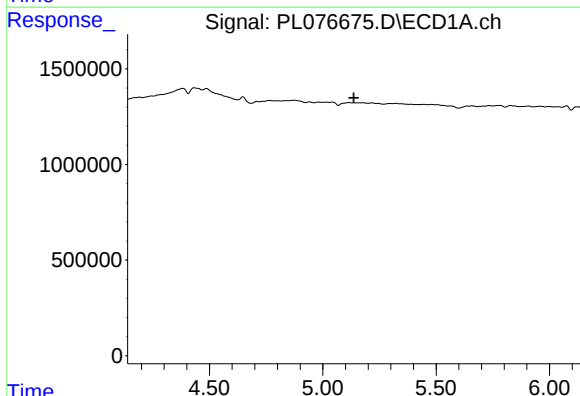


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.137 min
Response: 0
Conc: N.D.

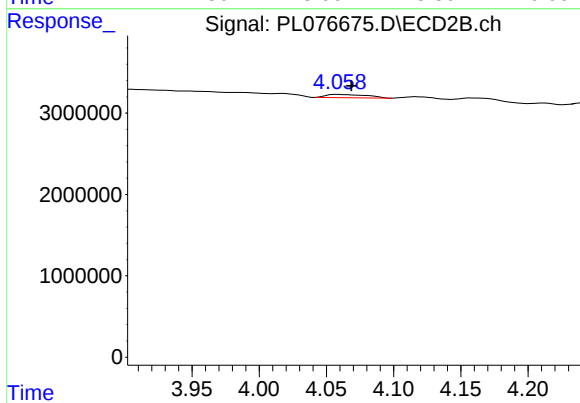

#5 Aldrin


R.T.: 4.059 min
Delta R.T.: -0.009 min
Response: 833282
Conc: 0.24 ng/ml

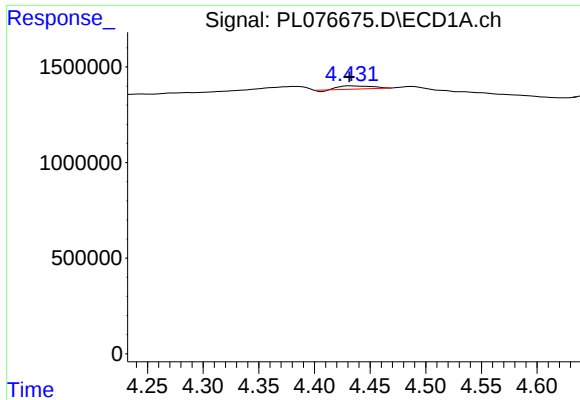

#6 beta-BHC


R.T.: 4.433 min
Delta R.T.: 0.001 min
Response: 329400
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

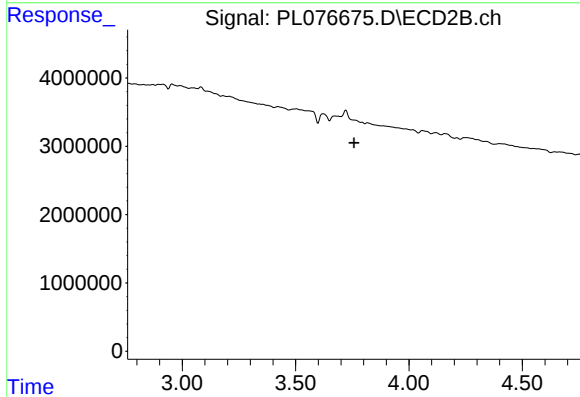


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.758 min
Response: 0
Conc: N.D.

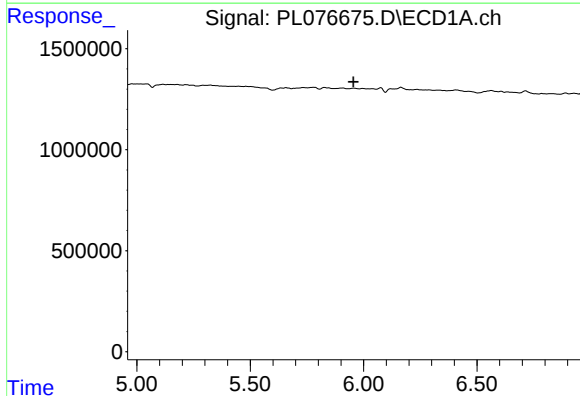


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.956 min
Response: 0
Conc: N.D.

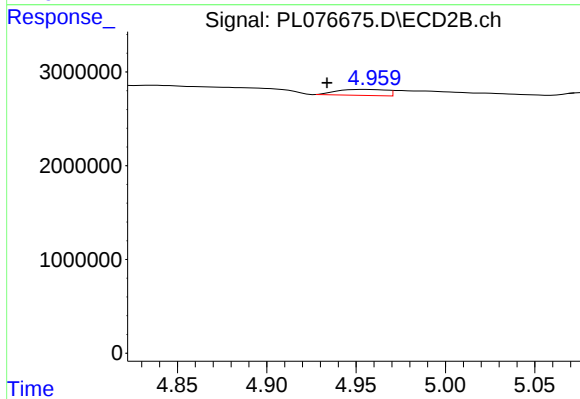

#9 Endosulfan I


R.T.: 4.955 min
Delta R.T.: 0.021 min
Response: 1106650
Conc: 0.38 ng/ml

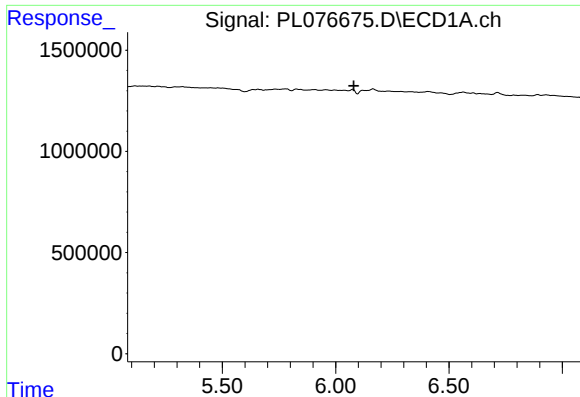

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.080 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

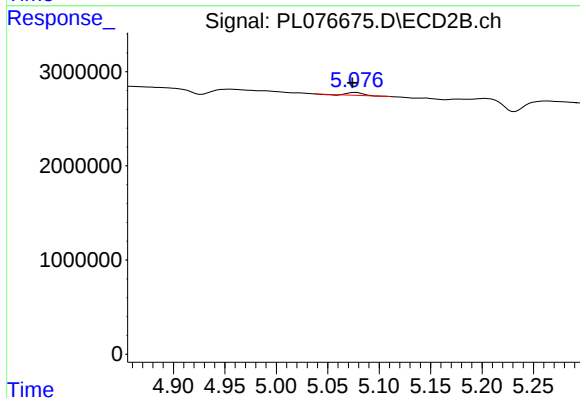


#12 4,4'-DDE

R.T.: 5.077 min
Delta R.T.: 0.003 min
Response: 303833
Conc: 0.10 ng/ml

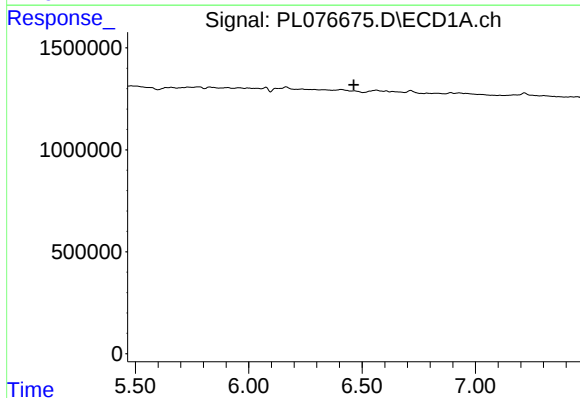


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.464 min
Response: 0
Conc: N.D.

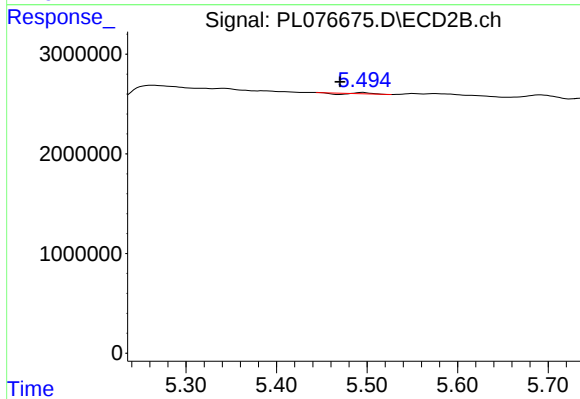

#14 Endrin


R.T.: 5.495 min
Delta R.T.: 0.025 min
Response: 38277
Conc: 0.02 ng/ml

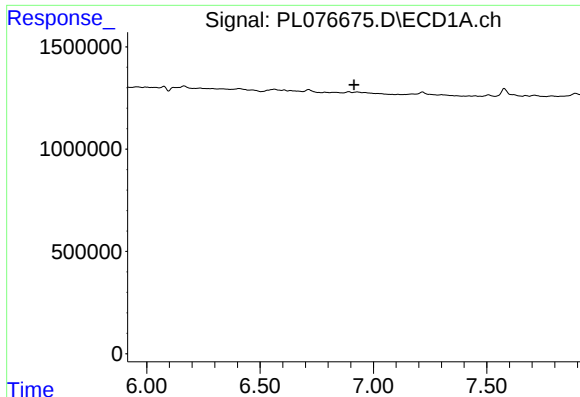

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.915 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

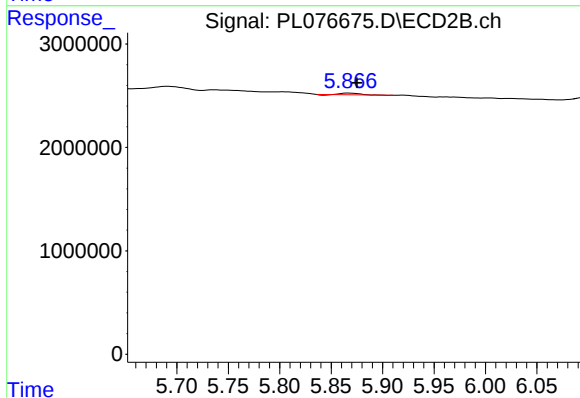


#17 4,4'-DDT

R.T.: 5.868 min
Delta R.T.: -0.007 min
Response: 149448
Conc: 0.06 ng/ml

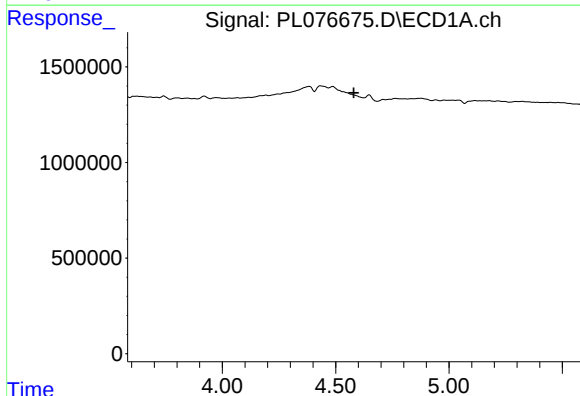


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.580 min
Response: 0
Conc: N.D.

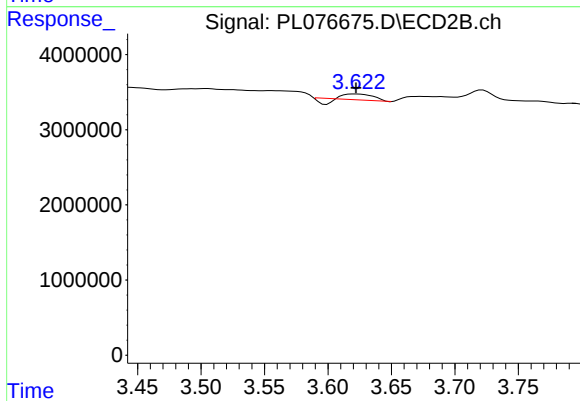

#23 Chlordane-1


R.T.: 3.622 min
Delta R.T.: 0.000 min
Response: 767778
Conc: 8.50 ng/ml

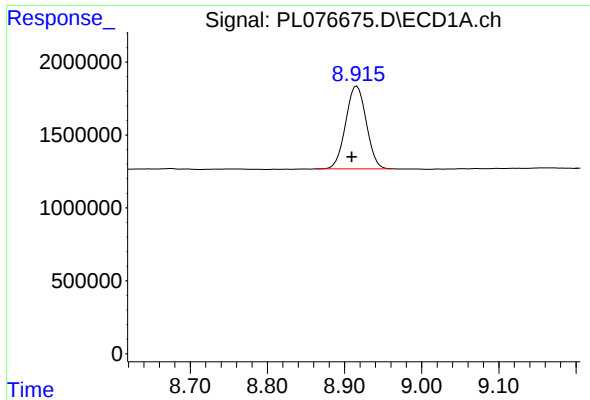

#28 Decachlorobiphenyl

R.T.: 8.916 min
Delta R.T.: 0.007 min
Response: 10523741
Conc: 11.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

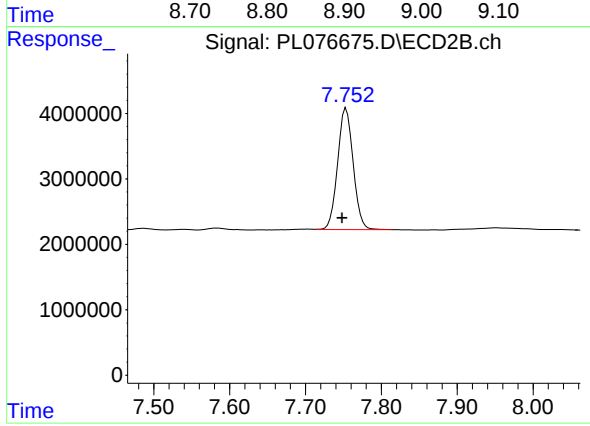

#28 Decachlorobiphenyl

R.T.: 7.754 min
Delta R.T.: 0.005 min
Response: 26405433
Conc: 10.29 ng/ml