

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072723\
 Data File : PL084294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2023 12:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/28/2023
 Supervised By :Ankita Jodhani 07/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 16:46:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.476	2.688	39389820	19310781	19.696	17.388
2) SA Decachlor...	9.023	7.869	27874159	22294848	21.414m	20.065

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072723\
Data File : PL084294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2023 12:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/28/2023
Supervised By : Ankita Jodhani 07/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 16:46:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

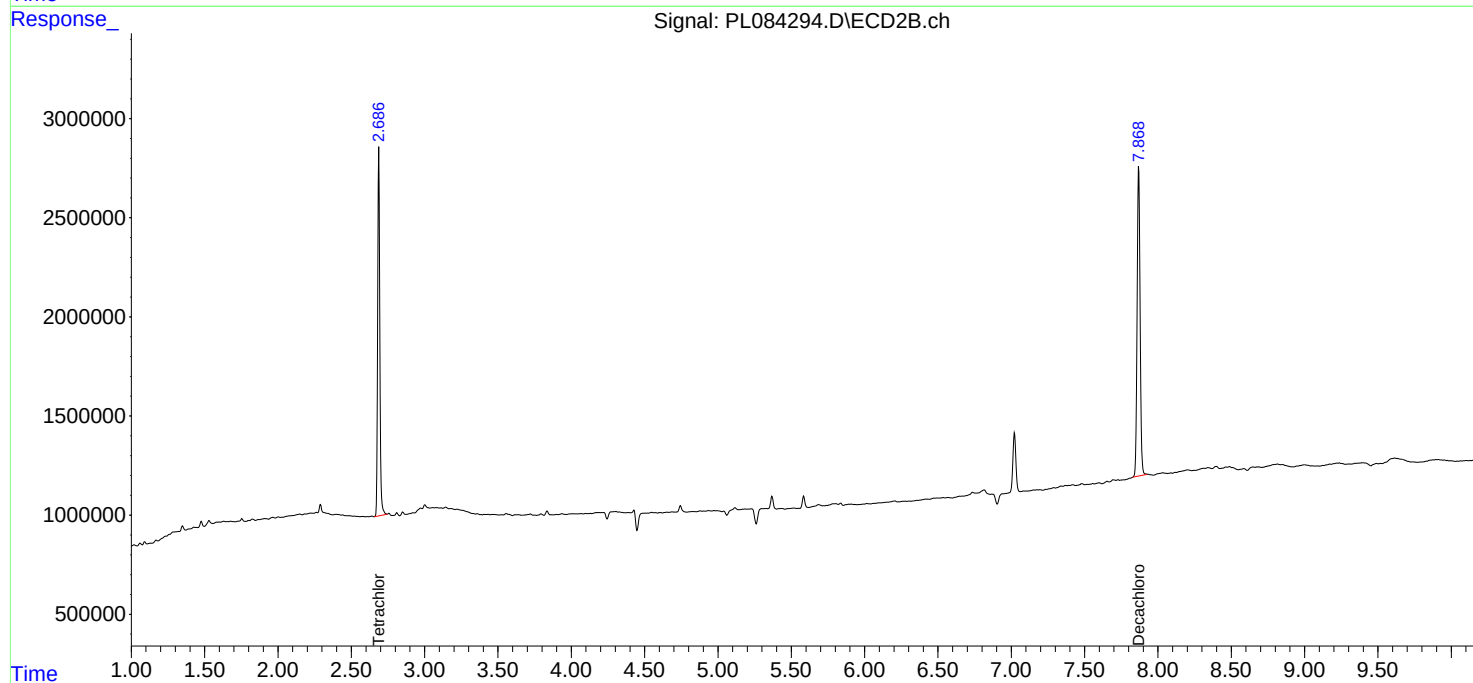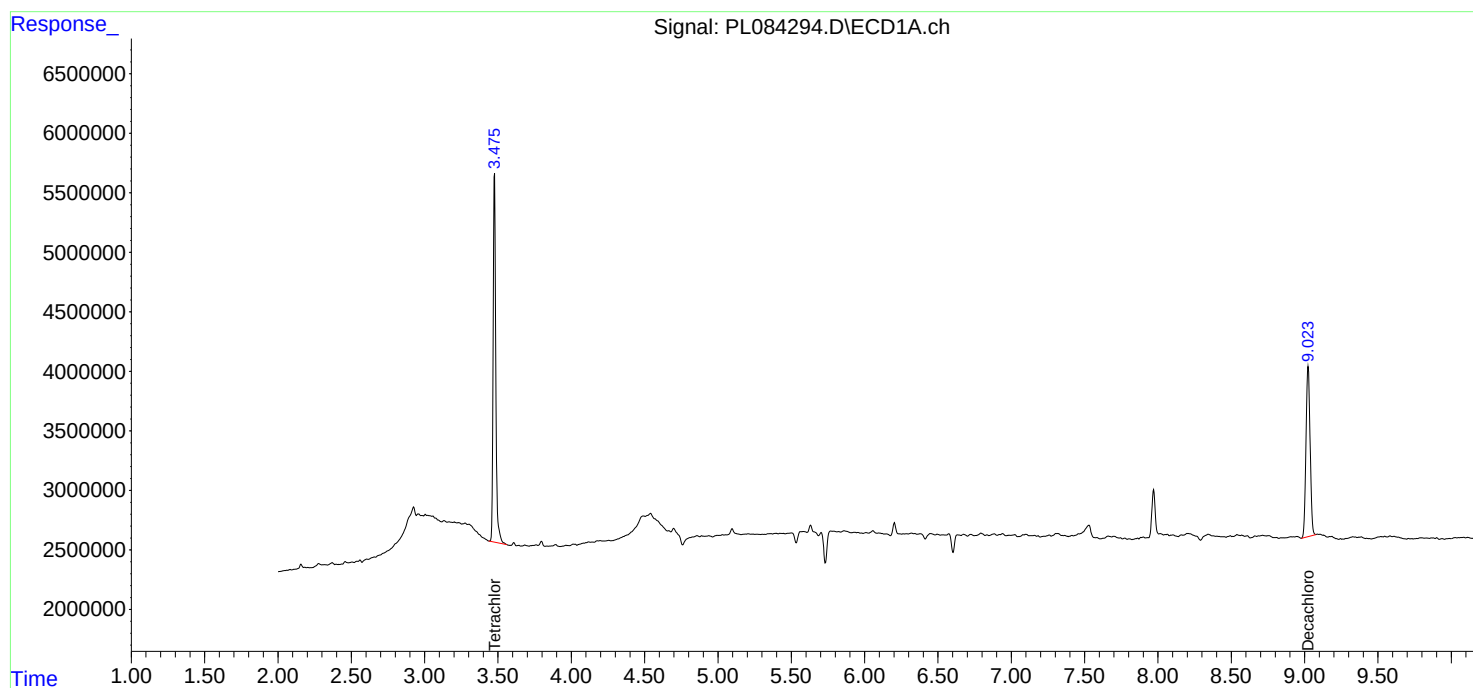

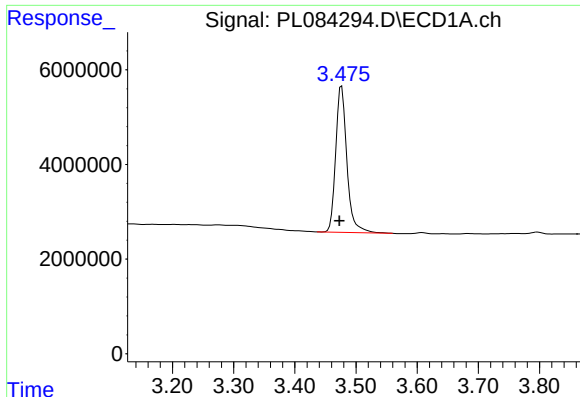


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 39389820
Conc: 19.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/28/2023
Supervised By :Ankita Jodhani 07/28/2023

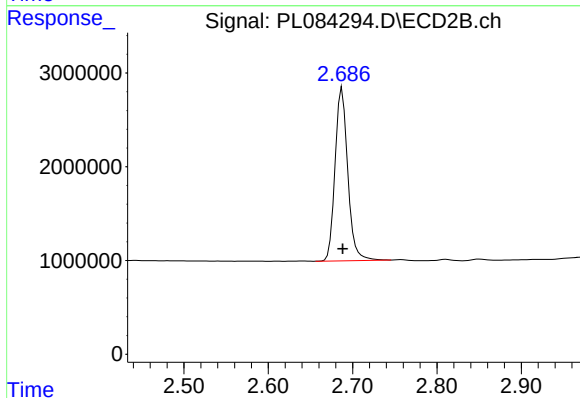


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: 0.000 min
Response: 19310781
Conc: 17.39 ng/ml

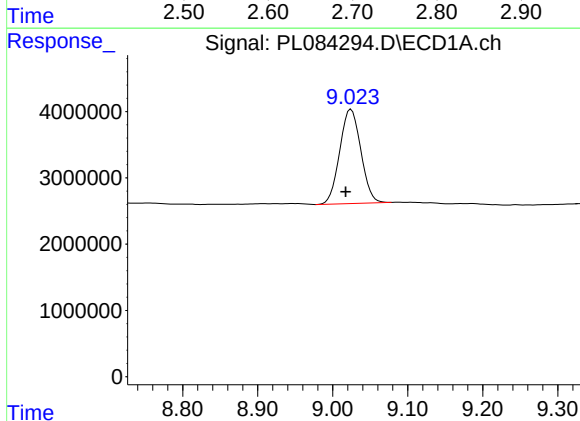

#28 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.006 min
Response: 27874159
Conc: 21.41 ng/ml m

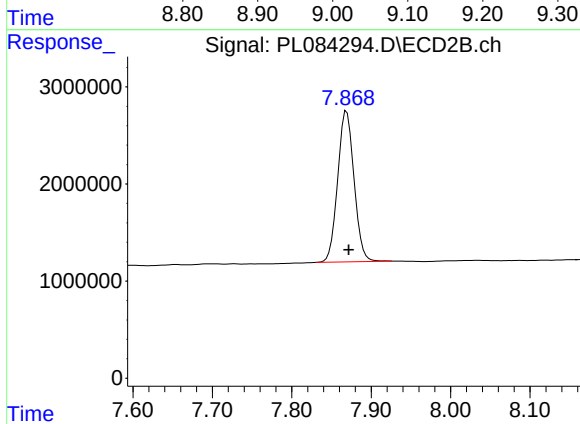

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: -0.002 min
Response: 22294848
Conc: 20.07 ng/ml