

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072723\
 Data File : PL084311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2023 17:55
 Operator : AR\AJ
 Sample : 03775-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BUILDING-A-10-(0-5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 21:36:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	2.687	15212438	7193291	7.607	6.477
28)	SA Decachlor...	9.025	7.869	15895088	11991489	12.211	10.792

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072723\
Data File : PL084311.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2023 17:55
Operator : AR\AJ
Sample : 03775-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BUILDING-A-10-(0-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 21:36:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

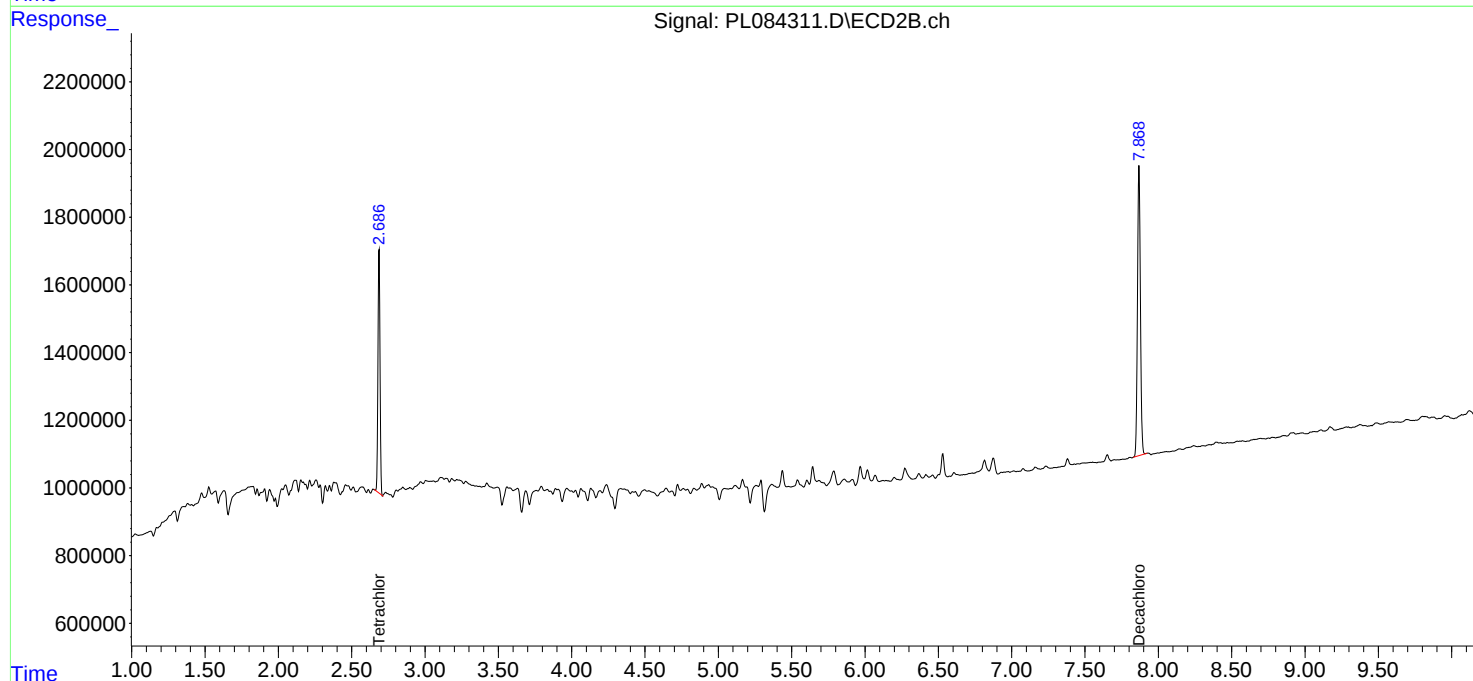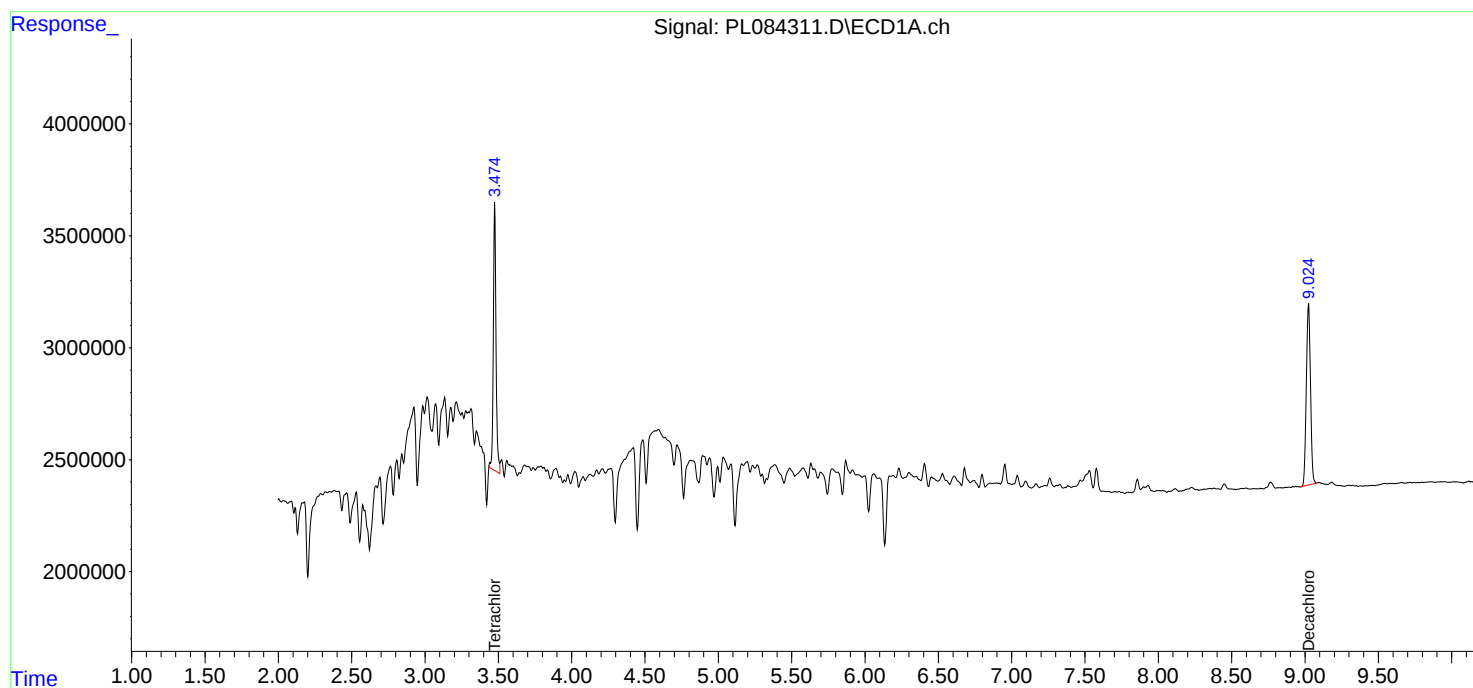


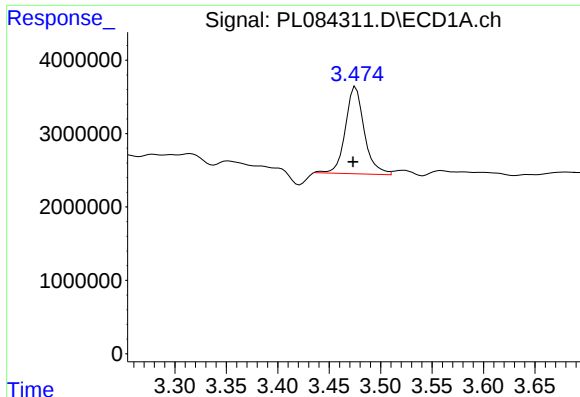

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 15212438
Conc: 7.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
BUILDING-A-10-(0-5)

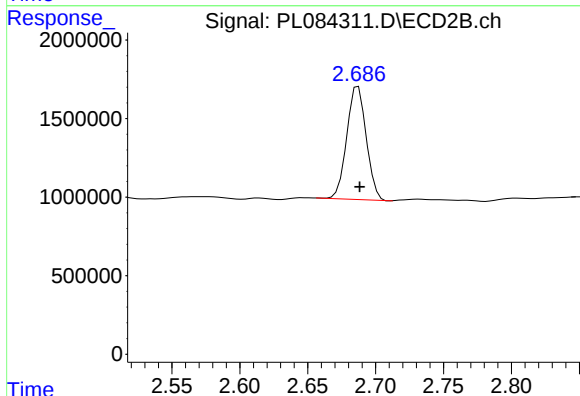


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: -0.001 min
Response: 7193291
Conc: 6.48 ng/ml

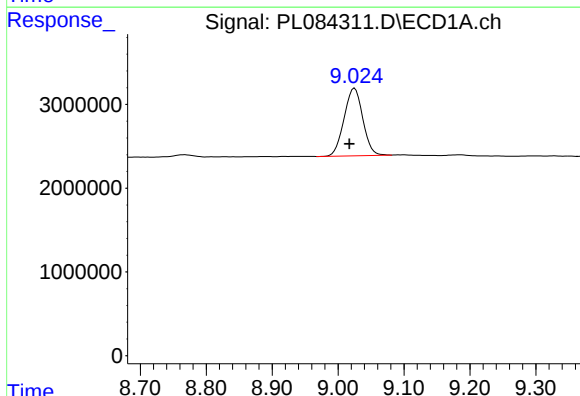

#28 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.008 min
Response: 15895088
Conc: 12.21 ng/ml

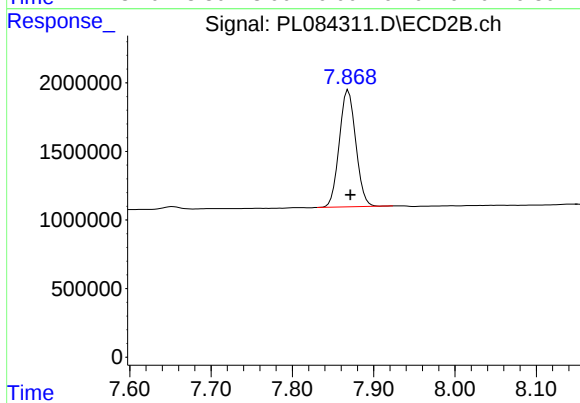

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: -0.003 min
Response: 11991489
Conc: 10.79 ng/ml