

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072723\
 Data File : PL084319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2023 20:29
 Operator : AR\AJ
 Sample : 03781-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OS-1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/28/2023
 Supervised By : Ankita Jodhani 07/28/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 21:43:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 14 00:03:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.497f	2.688	34458235	18176570	17.230	16.367
28) SA Decachlor...	9.044f	7.869	22839249	18483161	17.546m	16.635
Target Compounds						
17) MA 4,4'-DDT	6.975	5.969	990475	790426	0.621	0.868 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072723\
Data File : PL084319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2023 20:29
Operator : AR\AJ
Sample : 03781-01
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OS-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/28/2023
Supervised By : Ankita Jodhani 07/28/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 21:43:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071223.M
Quant Title : GC Extractables
QLast Update : Fri Jul 14 00:03:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

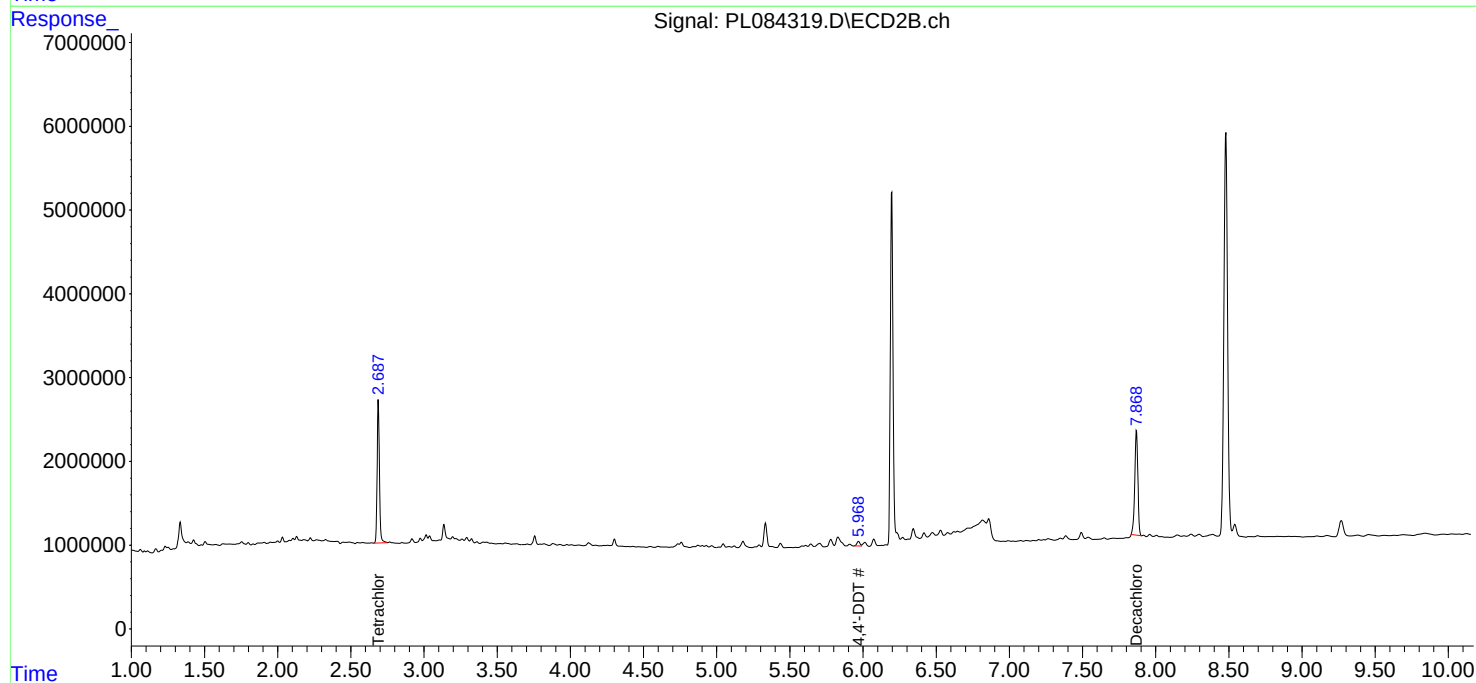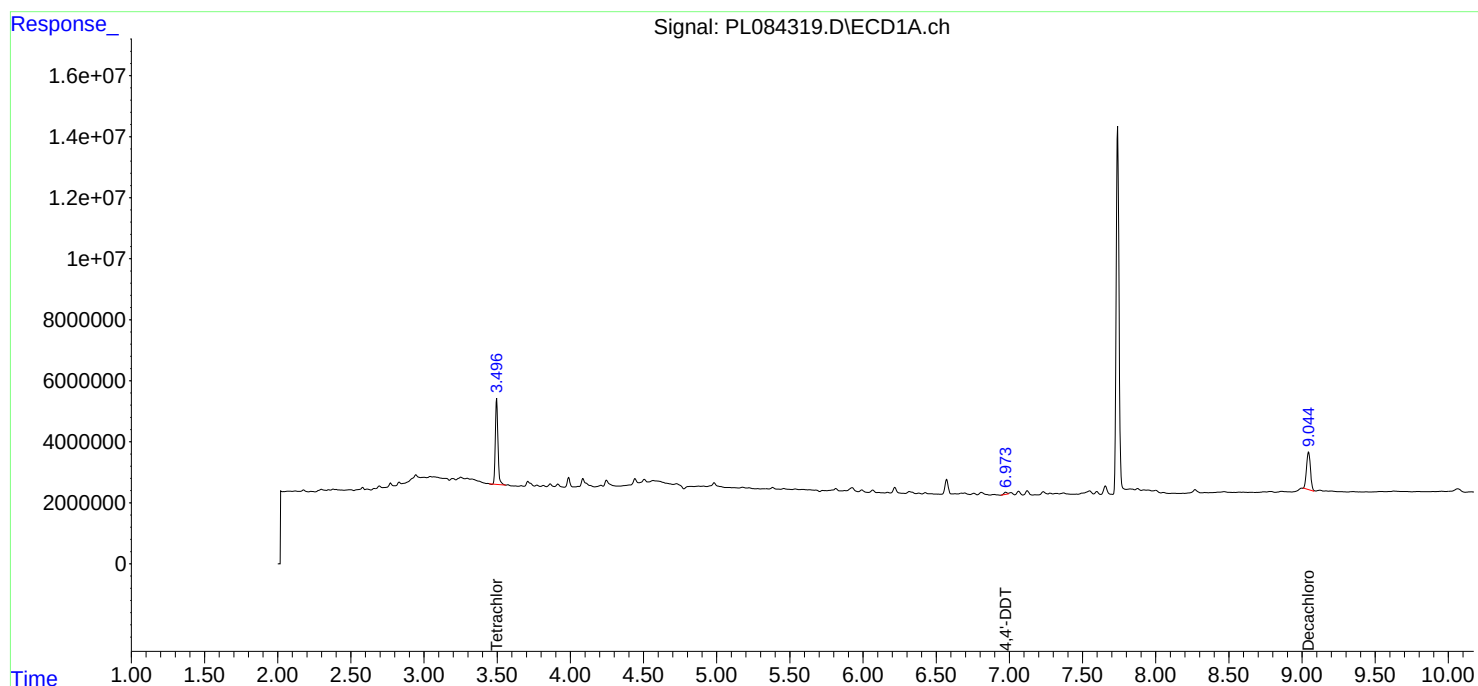

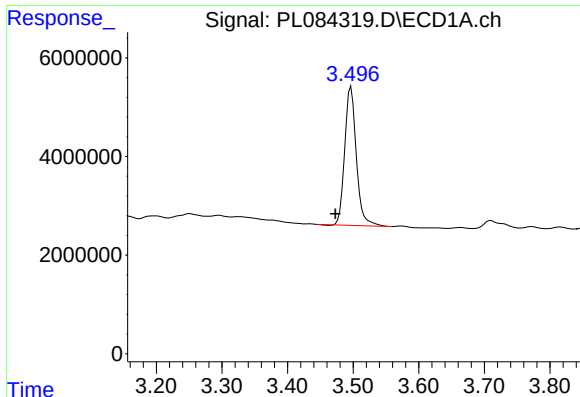


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: 0.024 min
Response: 34458235
Conc: 17.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
OS-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/28/2023
Supervised By :Ankita Jodhani 07/28/2023

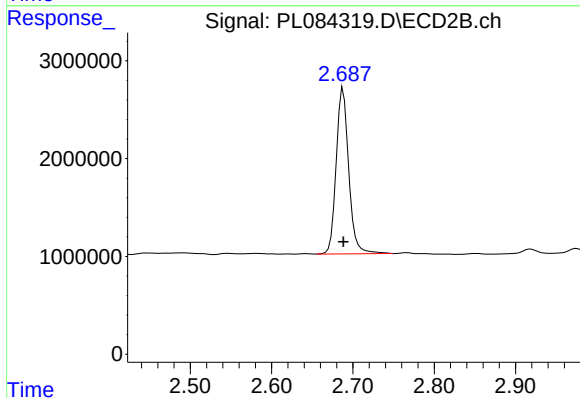


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: 0.000 min
Response: 18176570
Conc: 16.37 ng/ml

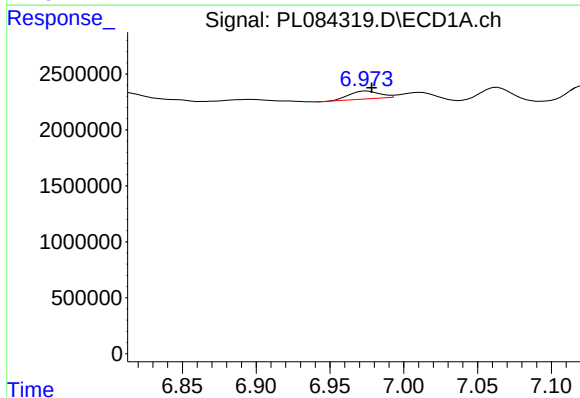


#17 4,4'-DDT

R.T.: 6.975 min
Delta R.T.: -0.003 min
Response: 990475
Conc: 0.62 ng/ml

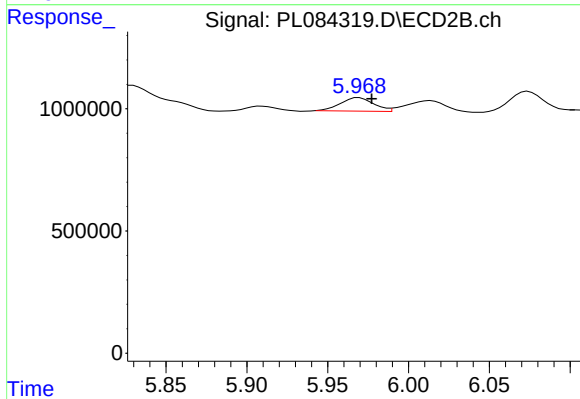

#17 4,4'-DDT

R.T.: 5.969 min
Delta R.T.: -0.008 min
Response: 790426
Conc: 0.87 ng/ml

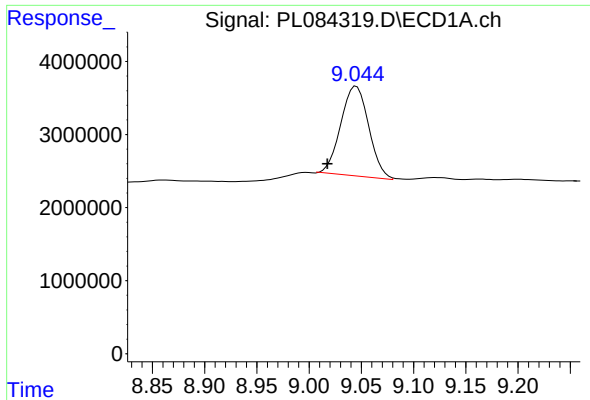


#28 Decachlorobiphenyl

R.T.: 9.044 min
Delta R.T.: 0.026 min
Response: 22839249
Conc: 17.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
OS-1

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/28/2023
Supervised By :Ankita Jodhani 07/28/2023

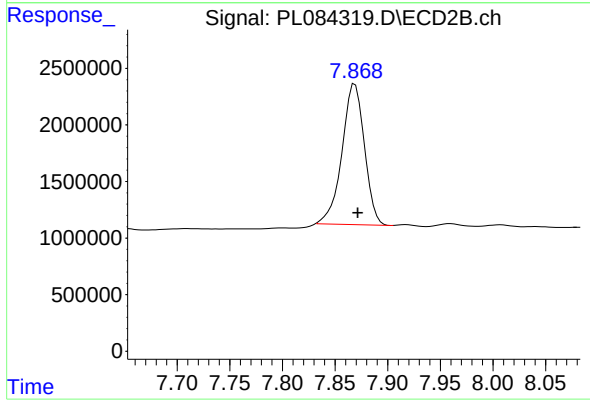

#28 Decachlorobiphenyl

R.T.: 7.869 min
Delta R.T.: -0.003 min
Response: 18483161
Conc: 16.63 ng/ml