

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072821\
 Data File : PL068513.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2021 08:26
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 02:14:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
8) B	Heptachlo...	0.000	8.035	0	33067	N.D.	0.029 #
9) A	Endosulfan I	0.000	8.446	0	20041	N.D.	0.019 #
11) B	alpha-Chl...	0.000	8.387	0	38923	N.D.	0.035 #
13) MA	Dieldrin	0.000	8.729	0	240052	N.D.	0.226 #
14) MA	Endrin	0.000	8.989f	0	60933	N.D.	0.068 #
15) B	Endosulfa...	0.000	9.218f	0	107282	N.D.	0.118 #
19) B	Endosulfa...	0.000	9.580	0	10908	N.D.	0.012 #
20) A	Methoxychlor	0.000	9.902	0	30229	N.D.	0.060 #
22)	Mirex	0.000	10.541	0	295840	N.D.	0.382 #
26)	Chlordane-4	0.000	8.387	0	38923	N.D.	0.208 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072821\
Data File : PL068513.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2021 08:26
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 02:14:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

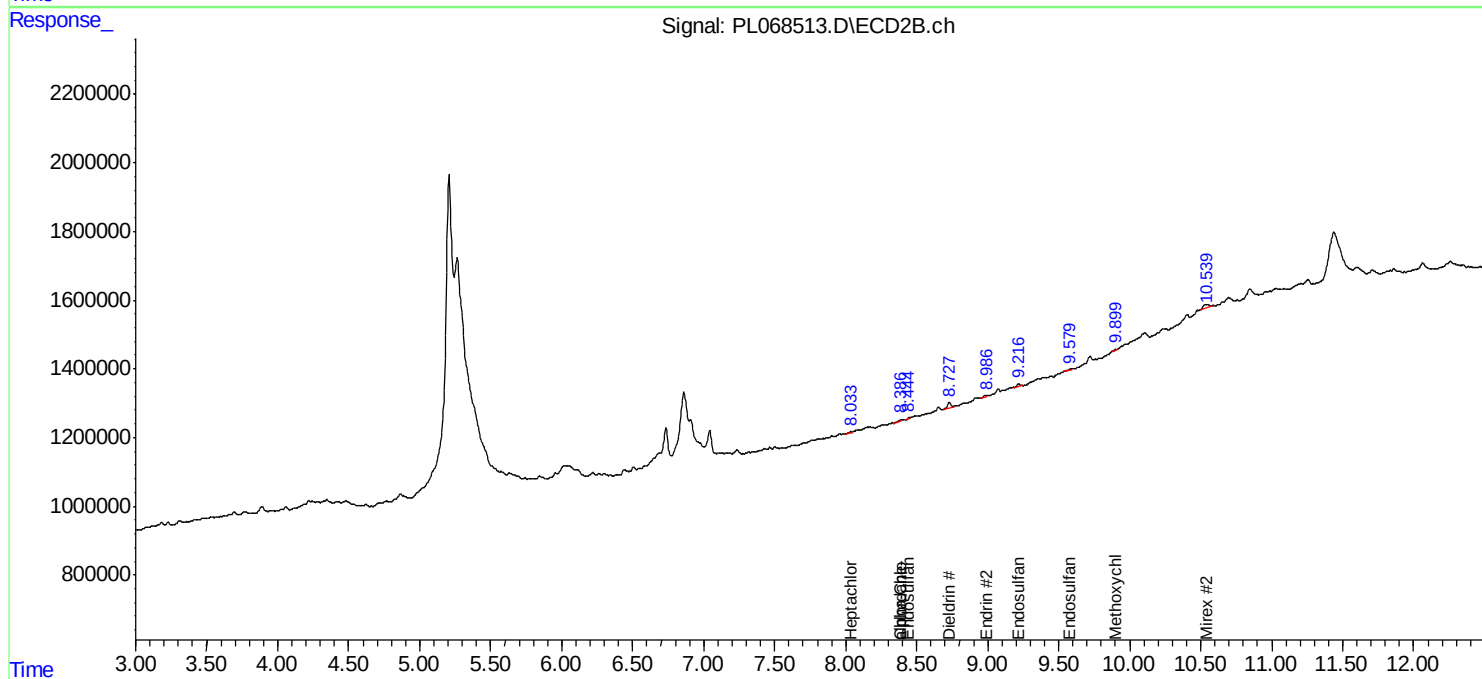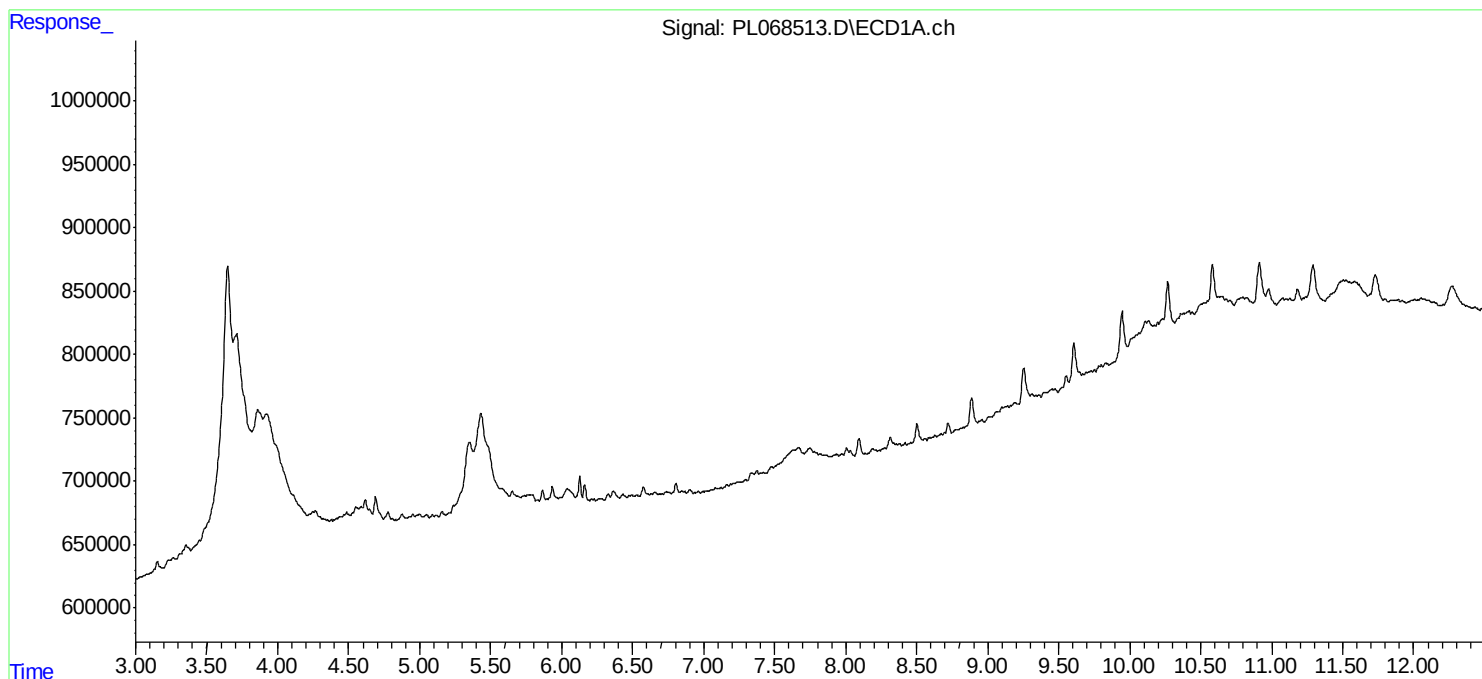


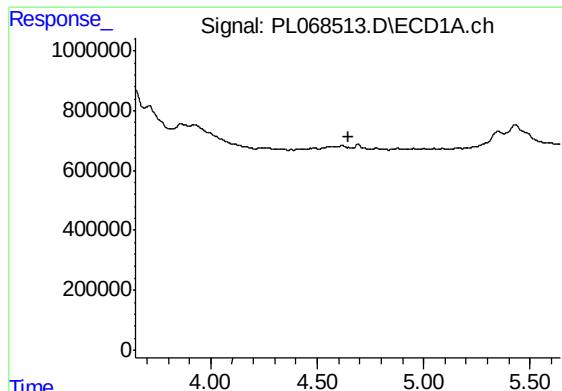

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

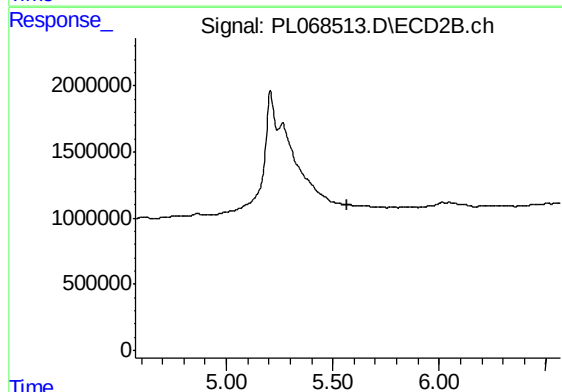


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.571 min
Response: 0
Conc: N.D.

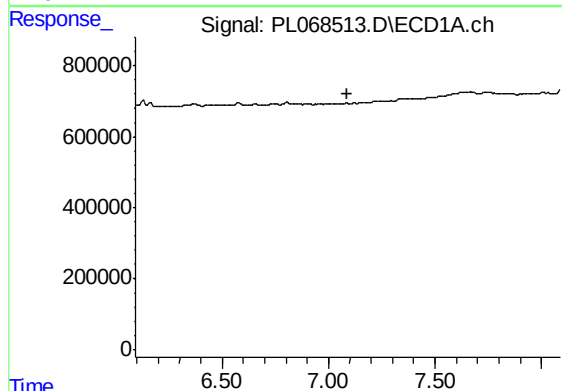


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

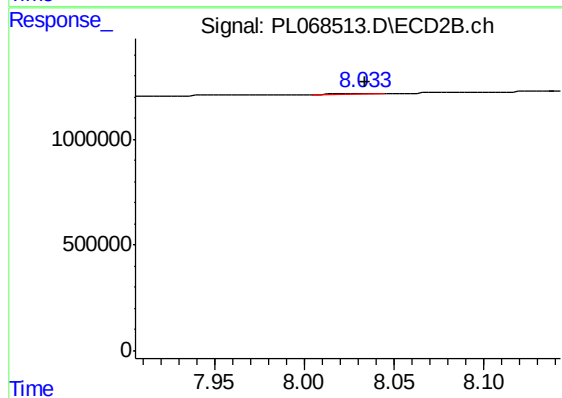

#8 Heptachlor epoxide


R.T.: 8.035 min
Delta R.T.: 0.001 min
Response: 33067
Conc: 0.03 ng/ml

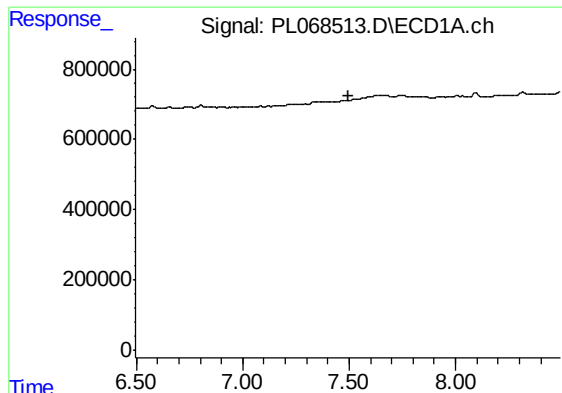

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

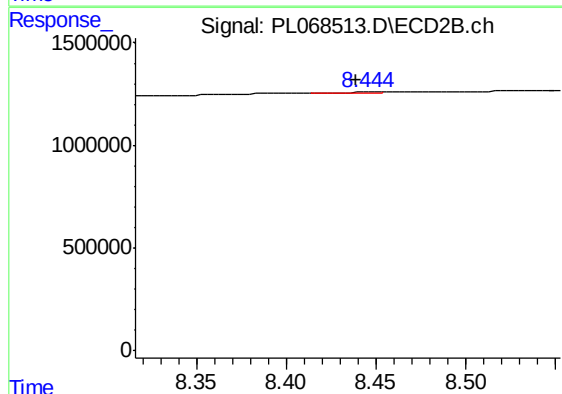


#9 Endosulfan I

R.T.: 8.446 min
Delta R.T.: 0.007 min
Response: 20041
Conc: 0.02 ng/ml

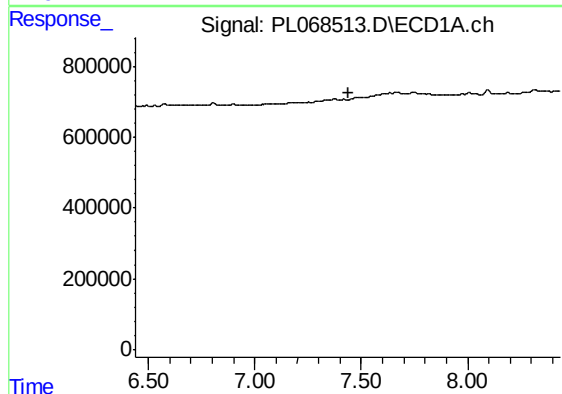


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.438 min
Response: 0
Conc: N.D.

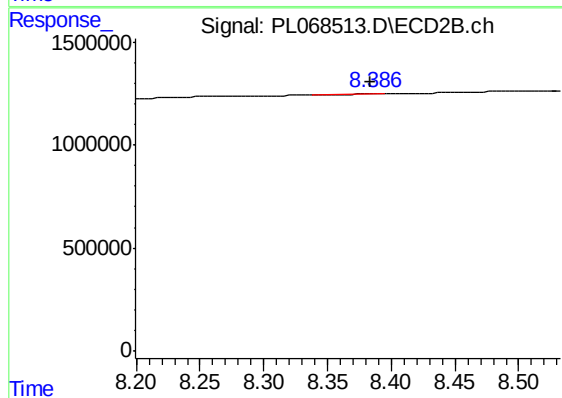

#11 alpha-Chlordane


R.T.: 8.387 min
Delta R.T.: 0.004 min
Response: 38923
Conc: 0.03 ng/ml

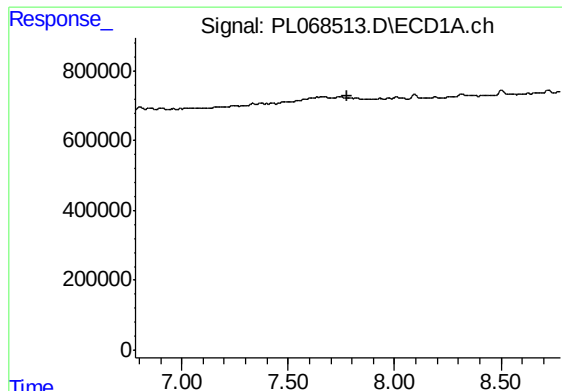

#13 Dielldrin


R.T.: 0.000 min
Exp R.T. : 7.781 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

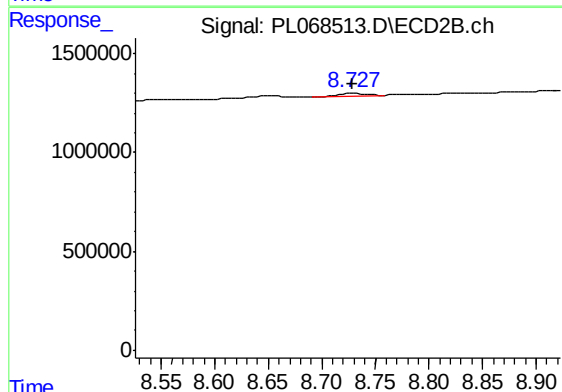


#13 Dielldrin

R.T.: 8.729 min
Delta R.T.: 0.000 min
Response: 240052
Conc: 0.23 ng/ml

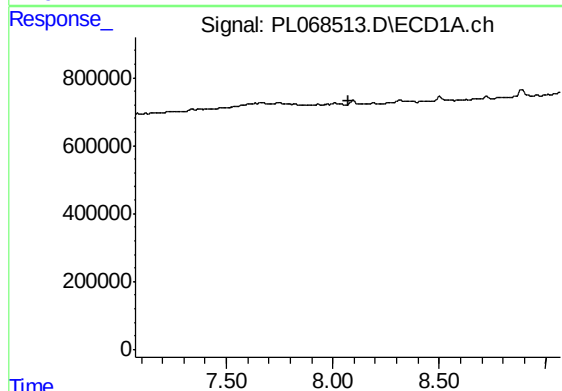


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.072 min
Response: 0
Conc: N.D.

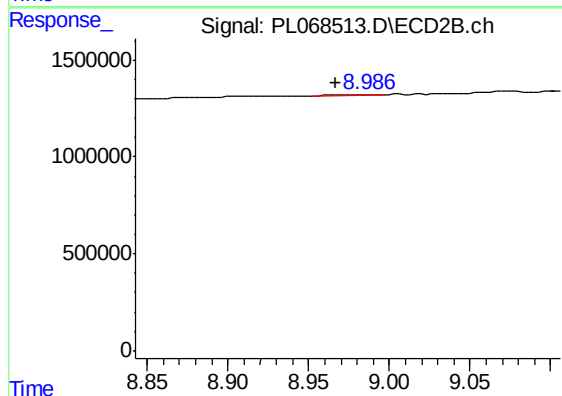

#14 Endrin


R.T.: 8.989 min
Delta R.T.: 0.022 min
Response: 60933
Conc: 0.07 ng/ml

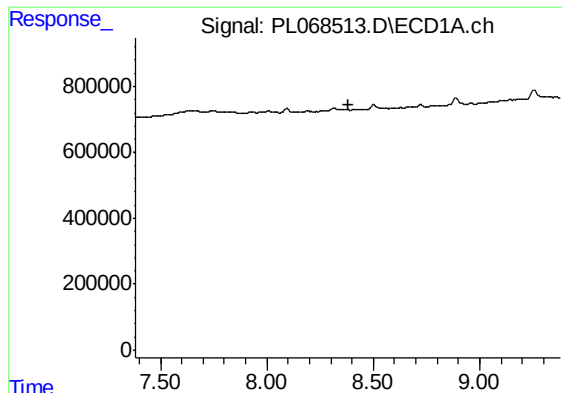

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

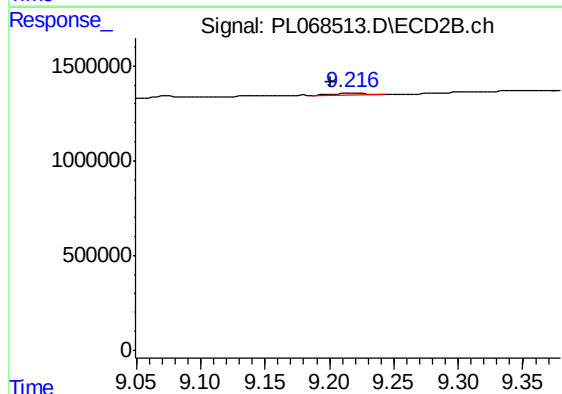


#15 Endosulfan II

R.T.: 9.218 min
Delta R.T.: 0.017 min
Response: 107282
Conc: 0.12 ng/ml

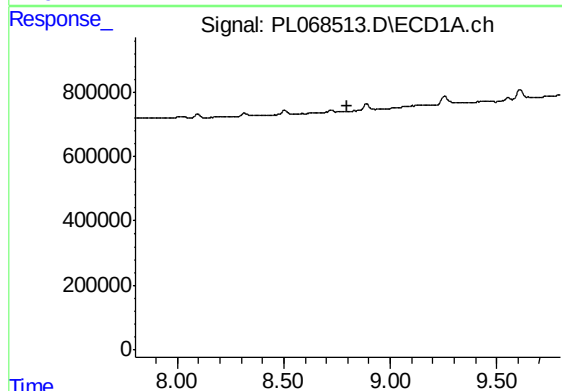


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.801 min
Response: 0
Conc: N.D.

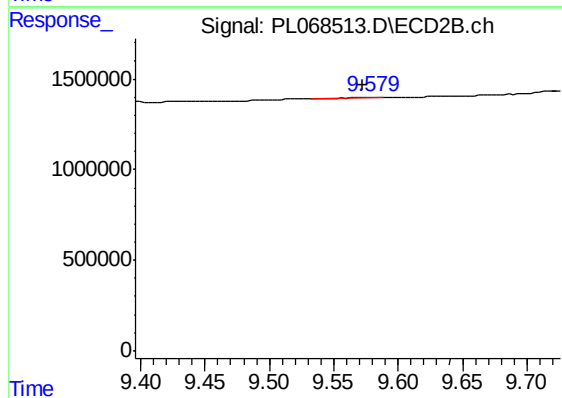

#19 Endosulfan Sulfate


R.T.: 9.580 min
Delta R.T.: 0.008 min
Response: 10908
Conc: 0.01 ng/ml

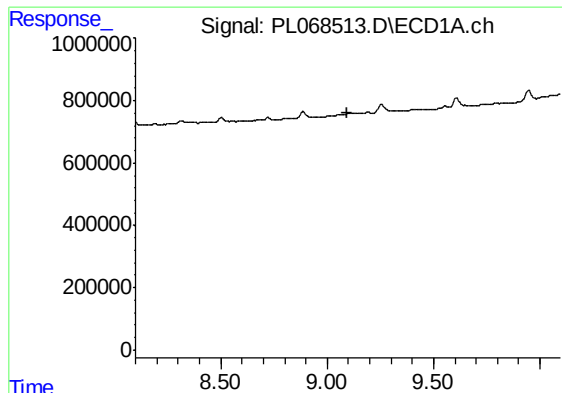

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

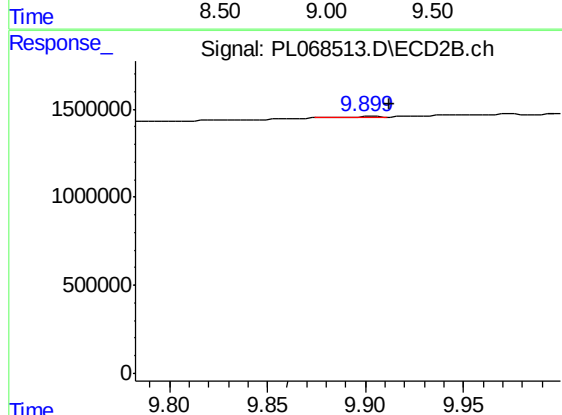


#20 Methoxychlor

R.T.: 9.902 min
Delta R.T.: -0.011 min
Response: 30229
Conc: 0.06 ng/ml

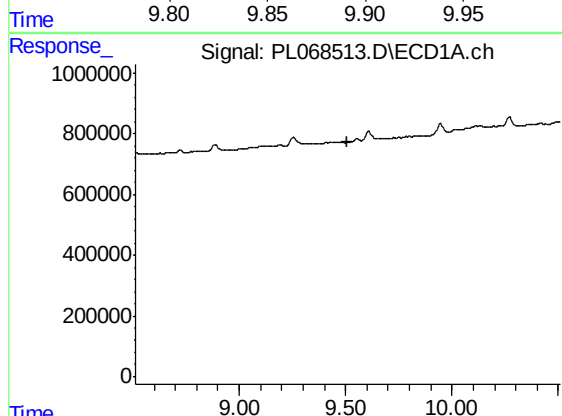


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.511 min
Response: 0
Conc: N.D.

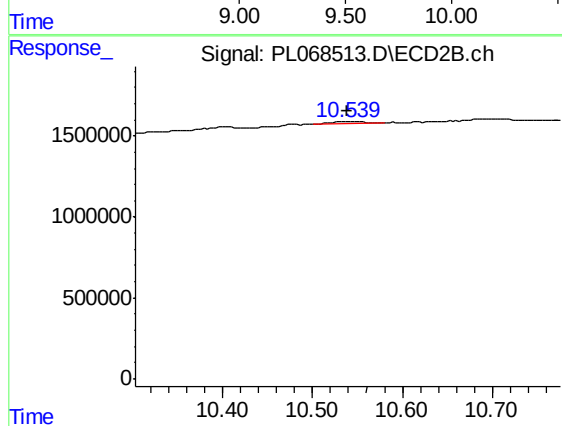

#22 Mirex


R.T.: 10.541 min
Delta R.T.: 0.002 min
Response: 295840
Conc: 0.38 ng/ml

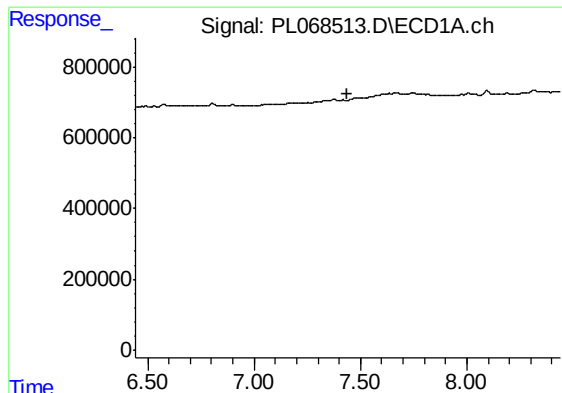

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

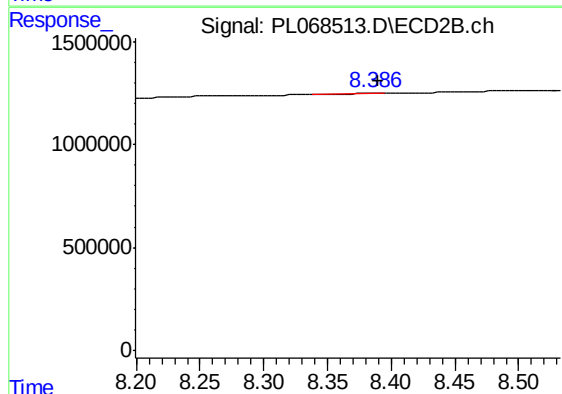


#26 Chlordane-4

R.T.: 8.387 min
Delta R.T.: -0.002 min
Response: 38923
Conc: 0.21 ng/ml

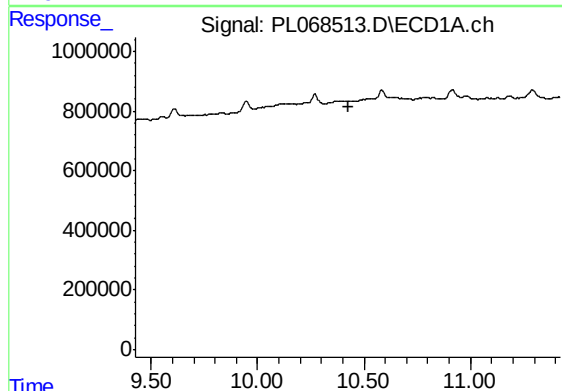

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.424 min
Response: 0
Conc: N.D.

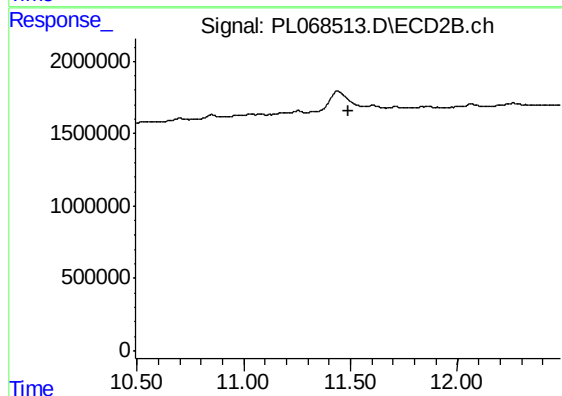

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.492 min
Response: 0
Conc: N.D.