

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072821\
 Data File : PL068521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2021 14:49
 Operator : AR\AJ
 Sample : M3198-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 02:18:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.643	5.572	6469162	13632866	15.073	13.360
28)	SA Decachlor...	10.420	11.497	7256142	11382472	12.902	12.761
Target Compounds							
10)	B gamma-Chl...	7.365	8.304	286966	645133	0.500m	0.573m
11)	B alpha-Chl...	7.435	8.388	499646	912662	0.870	0.811
12)	B 4,4'-DDE	7.650	8.570	750104	916665	1.489	0.889 #
17)	MA 4,4'-DDT	8.497	9.429	365326	450742	0.728	0.478 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072821\
Data File : PL068521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2021 14:49
Operator : AR\AJ
Sample : M3198-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 02:18:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

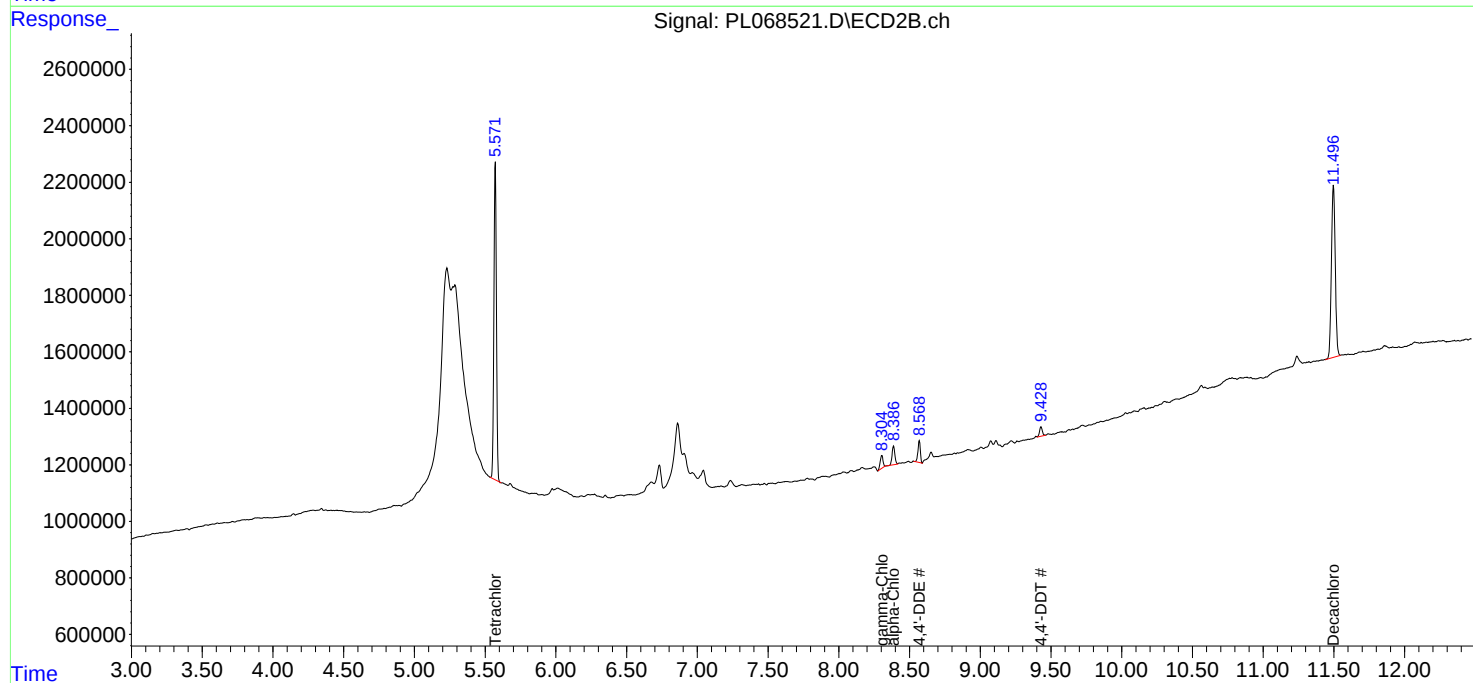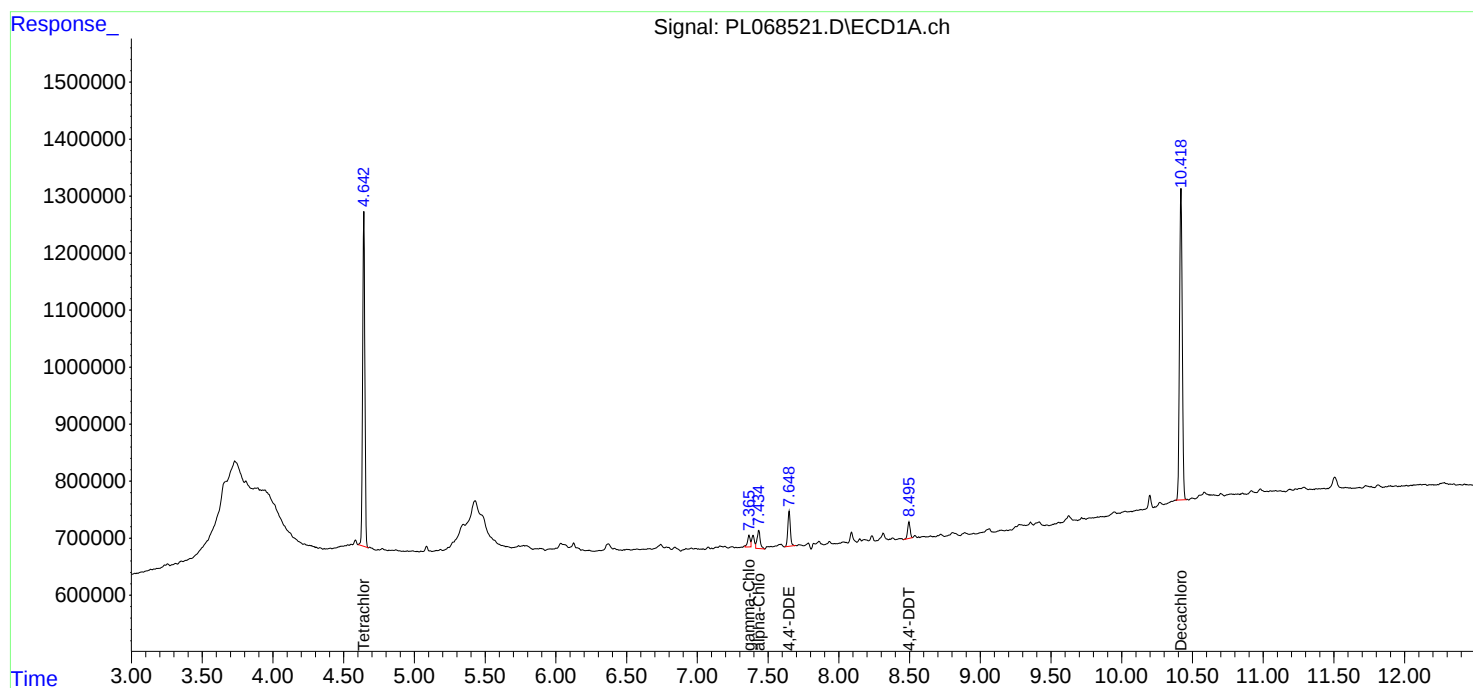


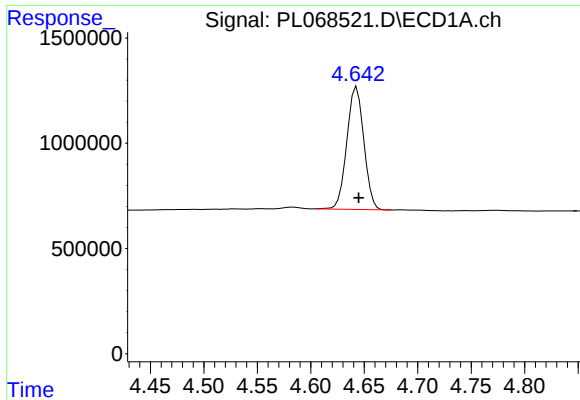

#1 Tetrachloro-m-xylene


R.T.: 4.643 min
Delta R.T.: -0.002 min
Response: 6469162
Conc: 15.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

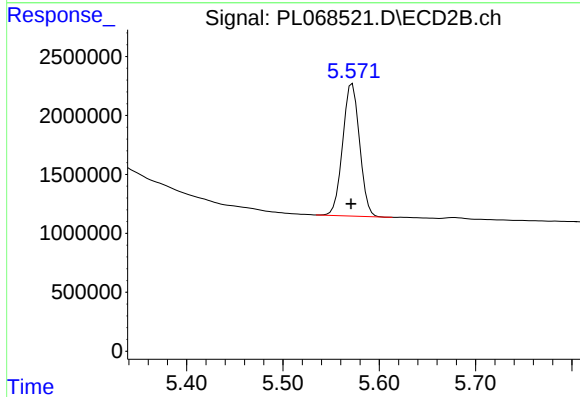


#1 Tetrachloro-m-xylene

R.T.: 5.572 min
Delta R.T.: 0.001 min
Response: 13632866
Conc: 13.36 ng/ml

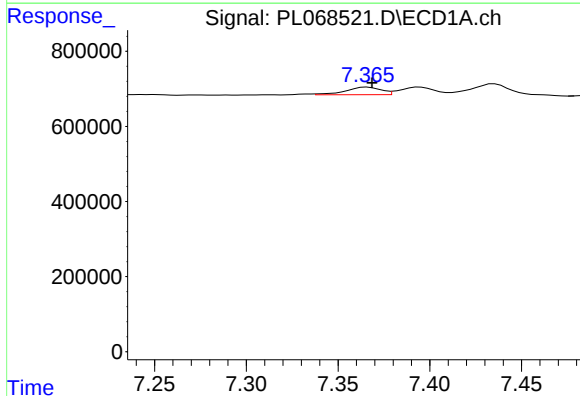


#10 gamma-Chlordane

R.T.: 7.365 min
Delta R.T.: -0.004 min
Response: 286966
Conc: 0.50 ng/ml m

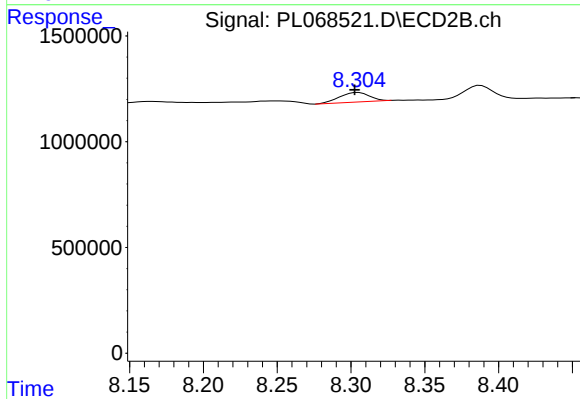

#10 gamma-Chlordane


R.T.: 8.304 min
Delta R.T.: 0.001 min
Response: 645133
Conc: 0.57 ng/ml m

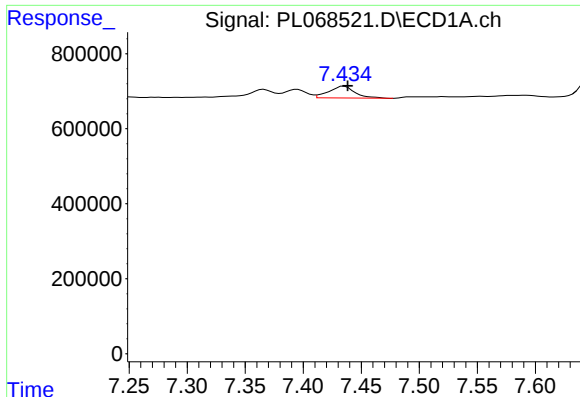

#11 alpha-Chlordane


R.T.: 7.435 min
Delta R.T.: -0.003 min
Response: 499646
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

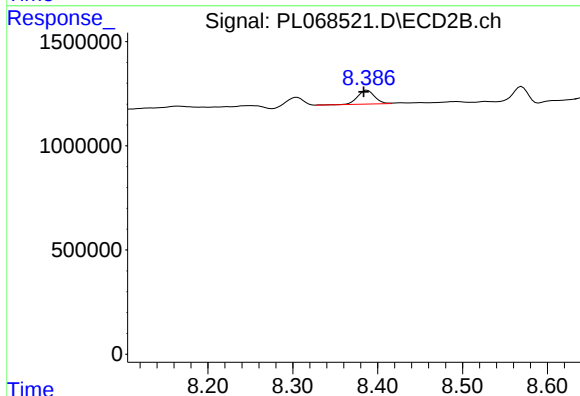


#11 alpha-Chlordane

R.T.: 8.388 min
Delta R.T.: 0.004 min
Response: 912662
Conc: 0.81 ng/ml

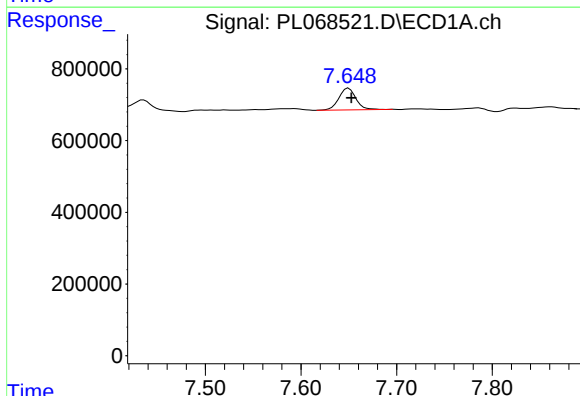


#12 4,4'-DDE

R.T.: 7.650 min
Delta R.T.: -0.003 min
Response: 750104
Conc: 1.49 ng/ml

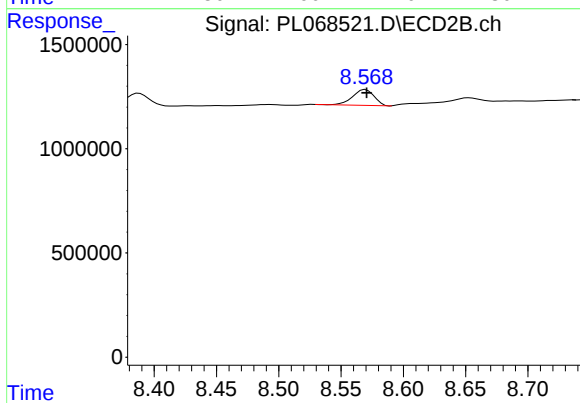

#12 4,4'-DDE


R.T.: 8.570 min
Delta R.T.: 0.000 min
Response: 916665
Conc: 0.89 ng/ml

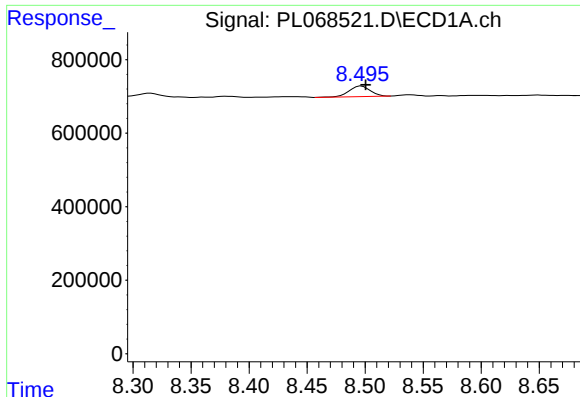

#17 4,4'-DDT


R.T.: 8.497 min
Delta R.T.: -0.004 min
Response: 365326
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-7

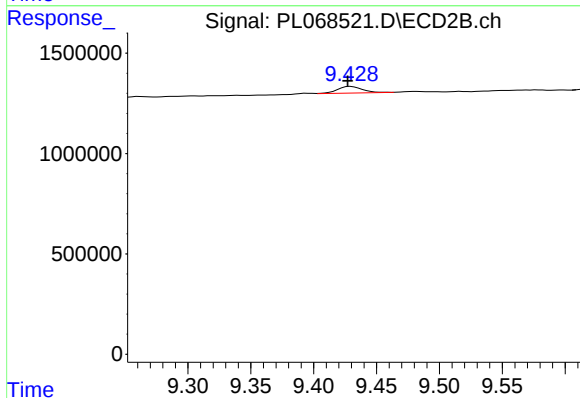


#17 4,4'-DDT

R.T.: 9.429 min
Delta R.T.: 0.002 min
Response: 450742
Conc: 0.48 ng/ml

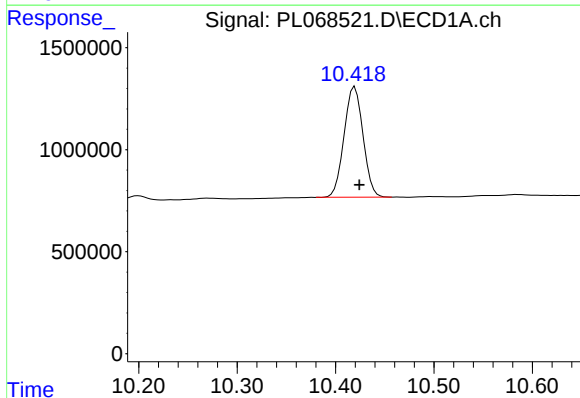

#28 Decachlorobiphenyl

R.T.: 10.420 min
Delta R.T.: -0.005 min
Response: 7256142
Conc: 12.90 ng/ml

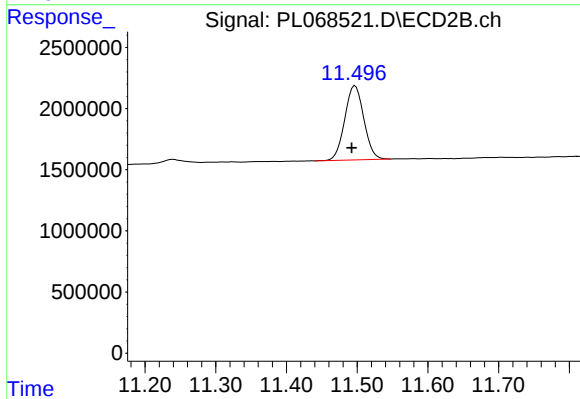

#28 Decachlorobiphenyl

R.T.: 11.497 min
Delta R.T.: 0.005 min
Response: 11382472
Conc: 12.76 ng/ml