

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072822\
 Data File : PL076695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2022 10:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 00:05:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	2.643	20798887	52465723	20.153	17.688
28)	SA Decachlor...	8.922	7.756	19556150	50211643	22.174	19.562
Target Compounds							
4)	MA Heptachlor	4.801	3.768f	256338	543462	0.191	0.144
5)	MB Aldrin	0.000	4.088f	0	78943	N.D.	0.022 #
6)	B beta-BHC	0.000	3.768	0	543462	N.D.	0.321 #
7)	B delta-BHC	4.655f	0.000	823077	0	0.743	N.D. #
8)	B Heptachlo...	5.579	0.000	602505	0	0.540	N.D. #
14)	MA Endrin	0.000	5.498f	0	1269680	N.D.	0.506 #
15)	B Endosulfa...	6.701	0.000	1267793	0	1.413	N.D. #
16)	A 4,4'-DDD	0.000	5.627	0	2587031	N.D.	1.092 #
20)	A Methoxychlor	0.000	6.429f	0	156020	N.D.	0.119 #
21)	B Endrin ke...	7.570f	6.639f	1075320	-4268	1.052	N.D. #
27)	Chlordane-5	0.000	5.526f	0	1239335	N.D.	15.478 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072822\
Data File : PL076695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2022 10:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 00:05:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

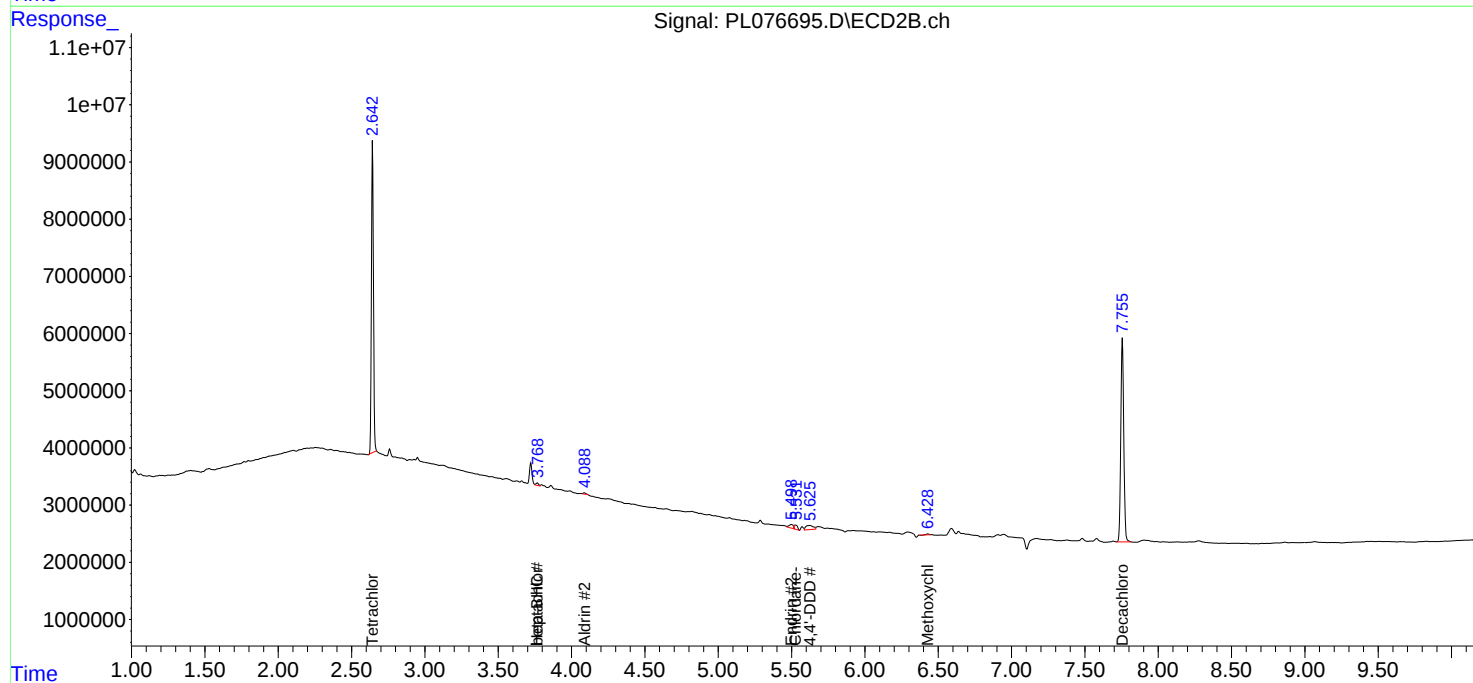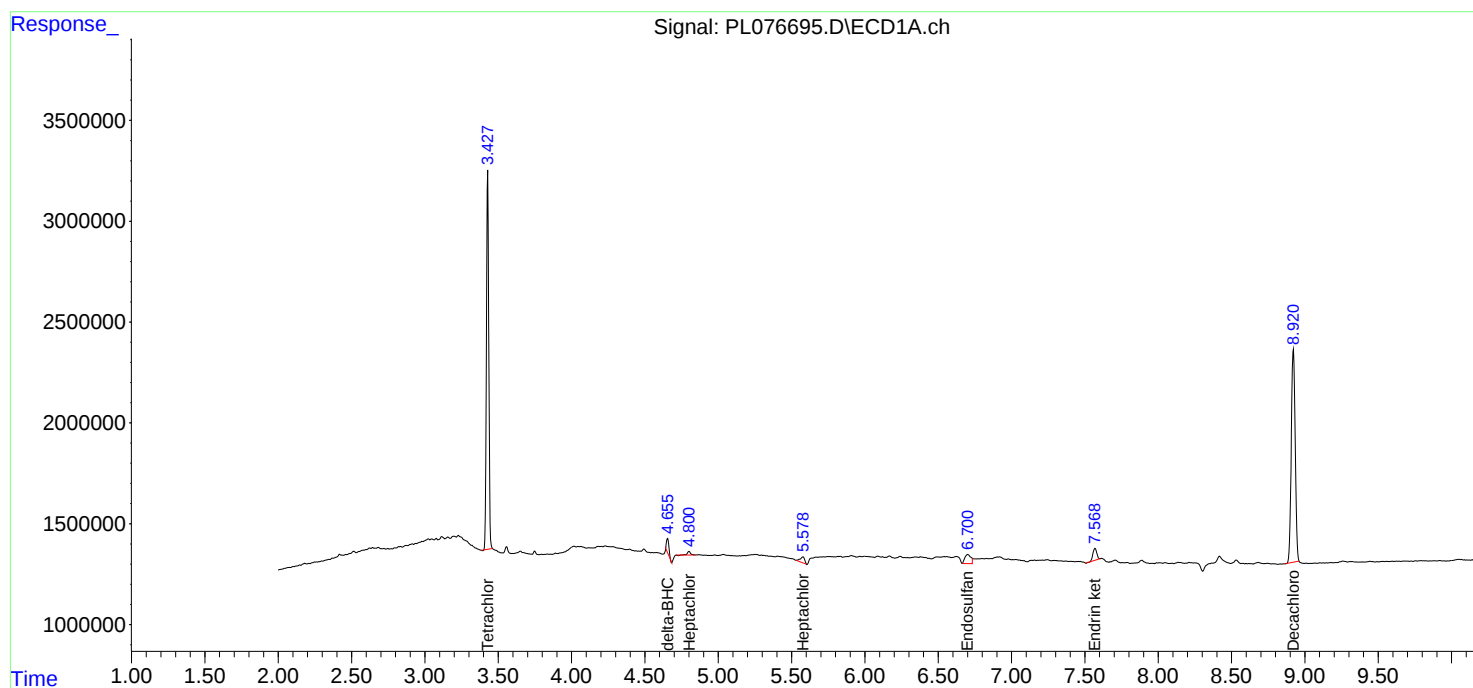


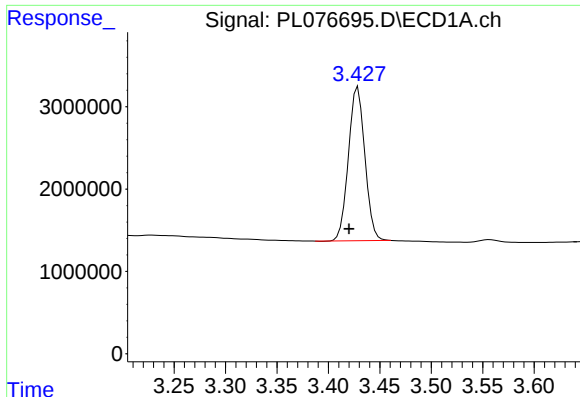

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.009 min
Response: 20798887
Conc: 20.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

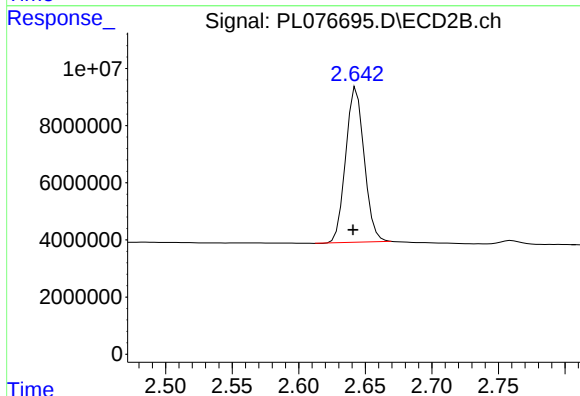


#1 Tetrachloro-m-xylene

R.T.: 2.643 min
Delta R.T.: 0.003 min
Response: 52465723
Conc: 17.69 ng/ml

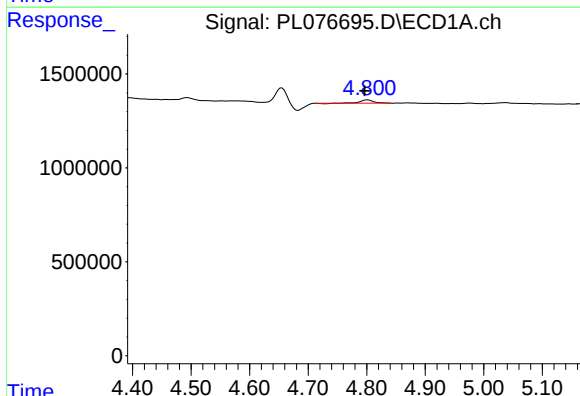


#4 Heptachlor

R.T.: 4.801 min
Delta R.T.: 0.005 min
Response: 256338
Conc: 0.19 ng/ml

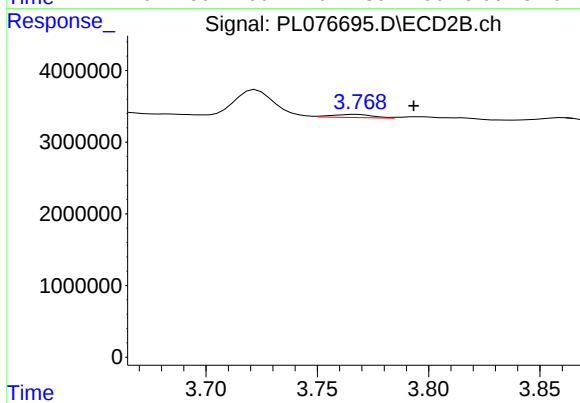

#4 Heptachlor


R.T.: 3.768 min
Delta R.T.: -0.026 min
Response: 543462
Conc: 0.14 ng/ml

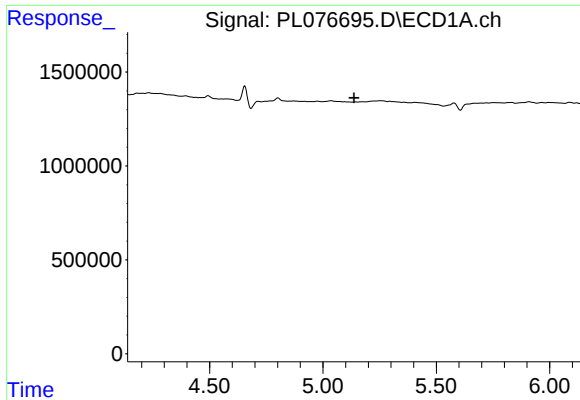

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.137 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

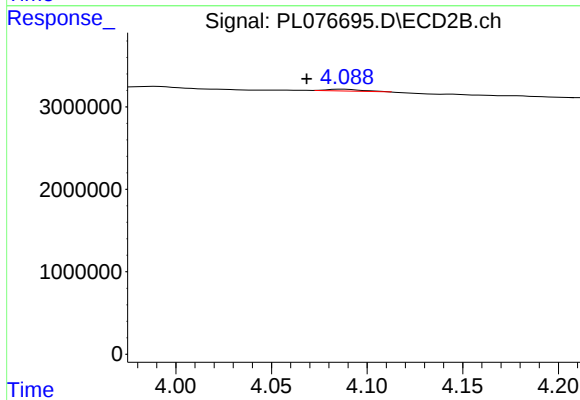


#5 Aldrin

R.T.: 4.088 min
Delta R.T.: 0.019 min
Response: 78943
Conc: 0.02 ng/ml

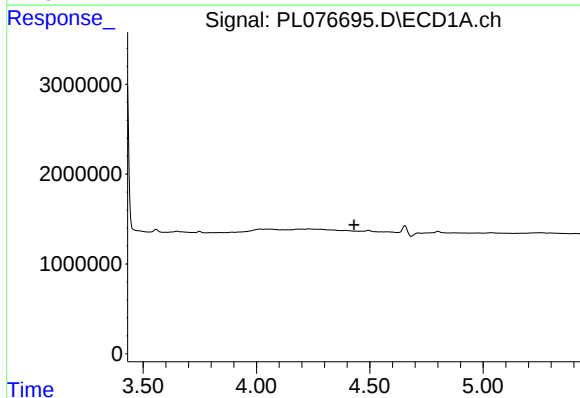


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.431 min
Response: 0
Conc: N.D.

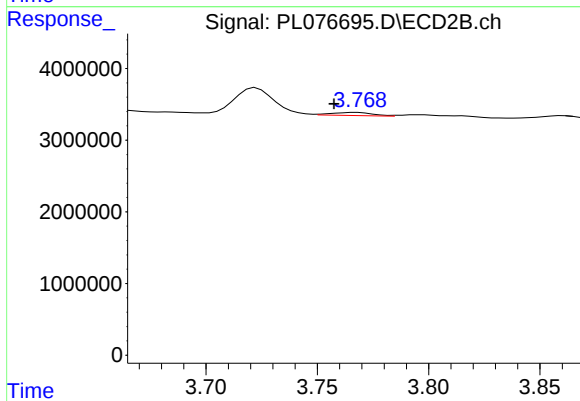

#6 beta-BHC


R.T.: 3.768 min
Delta R.T.: 0.010 min
Response: 543462
Conc: 0.32 ng/ml

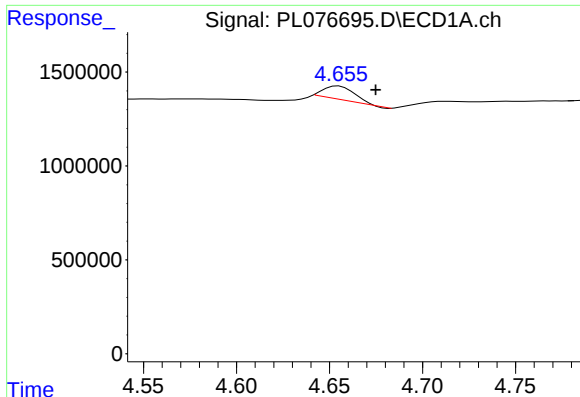

#7 delta-BHC


R.T.: 4.655 min
Delta R.T.: -0.020 min
Response: 823077
Conc: 0.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

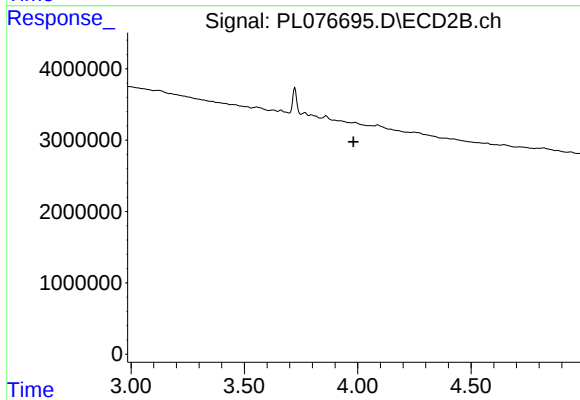


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 3.982 min
Response: 0
Conc: N.D.

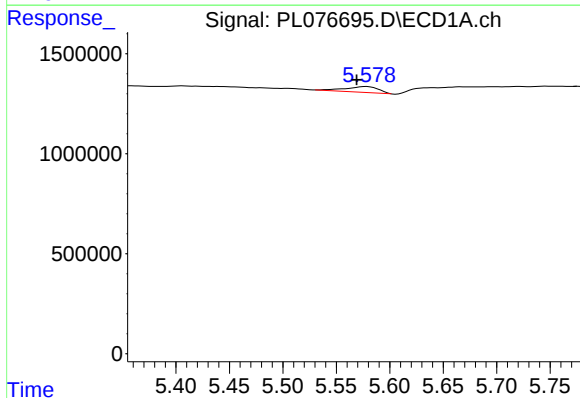


#8 Heptachlor epoxide

R.T.: 5.579 min
Delta R.T.: 0.010 min
Response: 602505
Conc: 0.54 ng/ml

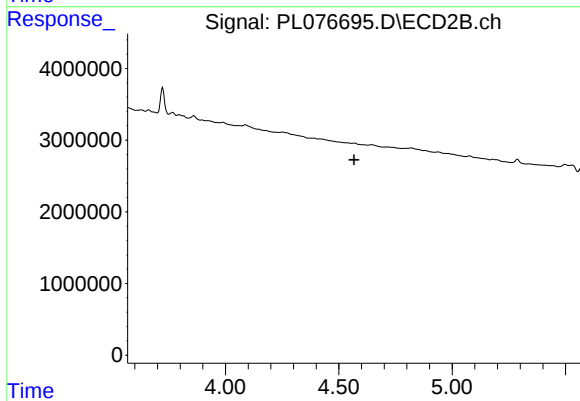

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.568 min
Response: 0
Conc: N.D.

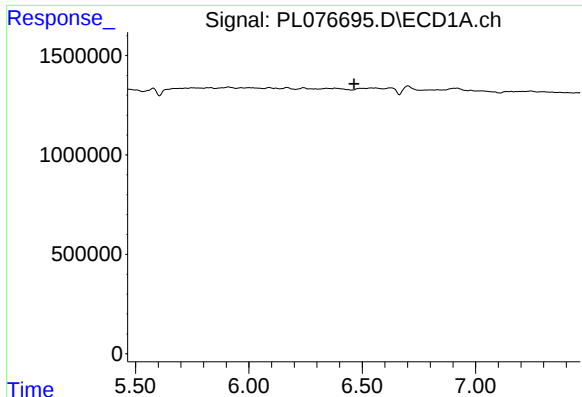

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

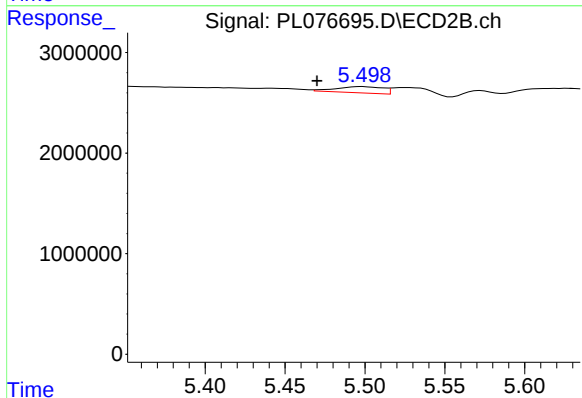


#14 Endrin

R.T.: 5.498 min
Delta R.T.: 0.028 min
Response: 1269680
Conc: 0.51 ng/ml

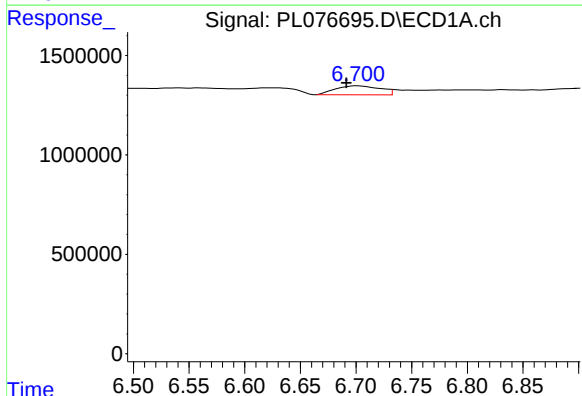


#15 Endosulfan II

R.T.: 6.701 min
Delta R.T.: 0.010 min
Response: 1267793
Conc: 1.41 ng/ml

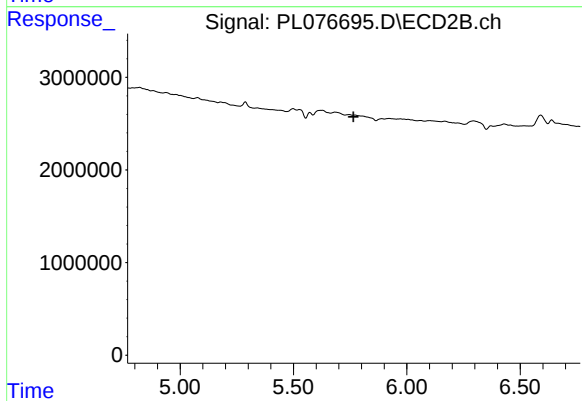

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 5.765 min
Response: 0
Conc: N.D.

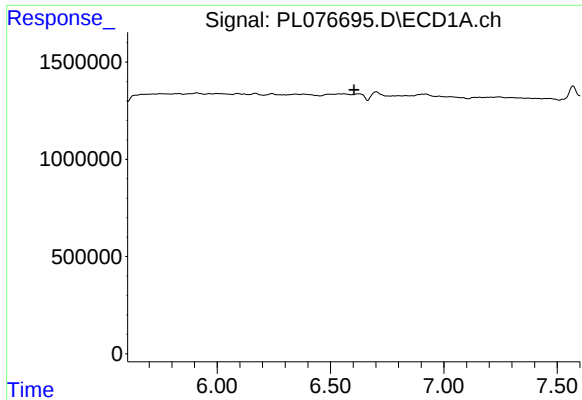

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.605 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

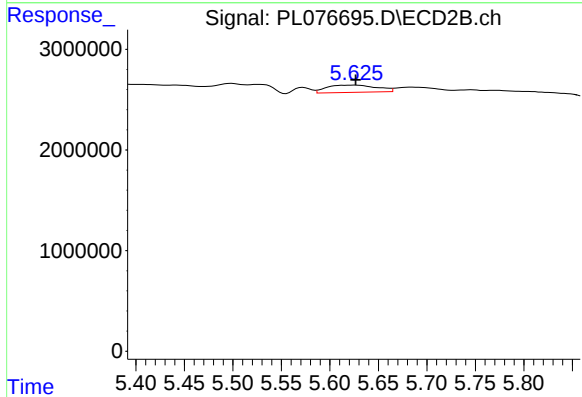


#16 4,4'-DDD

R.T.: 5.627 min
Delta R.T.: 0.000 min
Response: 2587031
Conc: 1.09 ng/ml

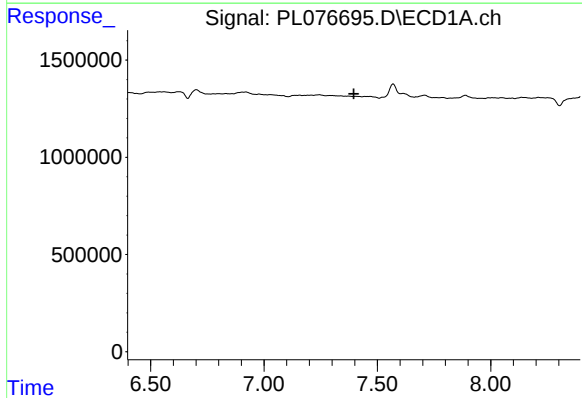


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.396 min
Response: 0
Conc: N.D.

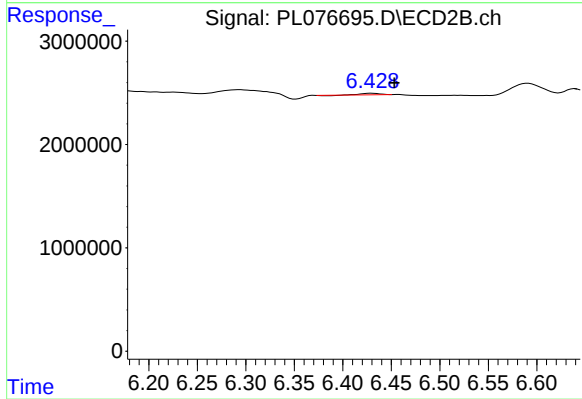

#20 Methoxychlor


R.T.: 6.429 min
Delta R.T.: -0.024 min
Response: 156020
Conc: 0.12 ng/ml

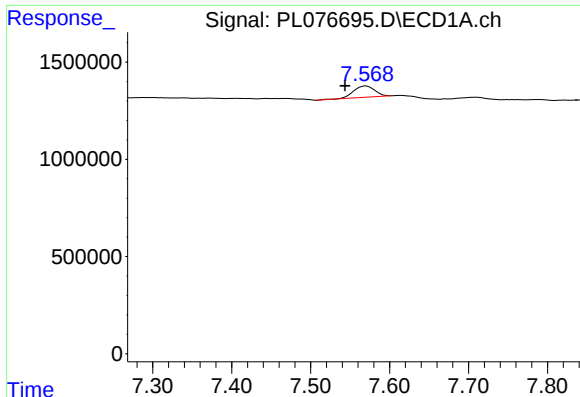

#21 Endrin ketone


R.T.: 7.570 min
Delta R.T.: 0.027 min
Response: 1075320
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

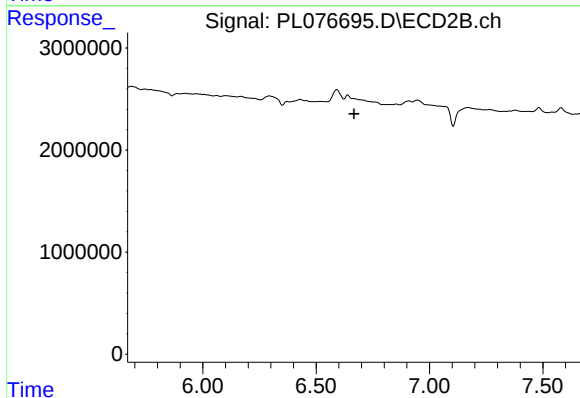


#21 Endrin ketone

R.T.: 6.639 min
Delta R.T.: -0.028 min
Response: -4268
Conc: N.D.

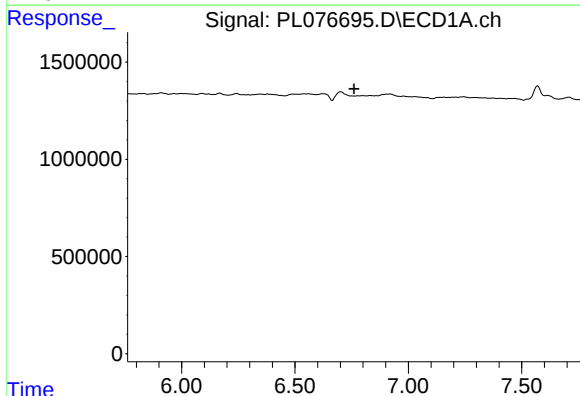


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.761 min
Response: 0
Conc: N.D.

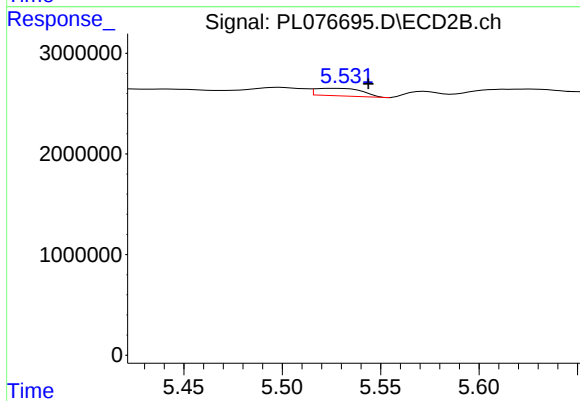

#27 Chlordane-5


R.T.: 5.526 min
Delta R.T.: -0.018 min
Response: 1239335
Conc: 15.48 ng/ml

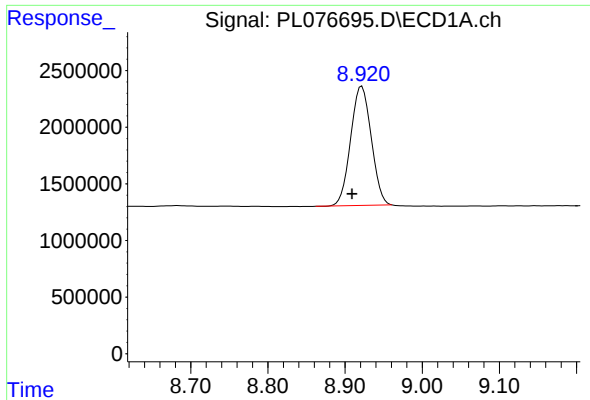

#28 Decachlorobiphenyl

R.T.: 8.922 min
Delta R.T.: 0.012 min
Response: 19556150
Conc: 22.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

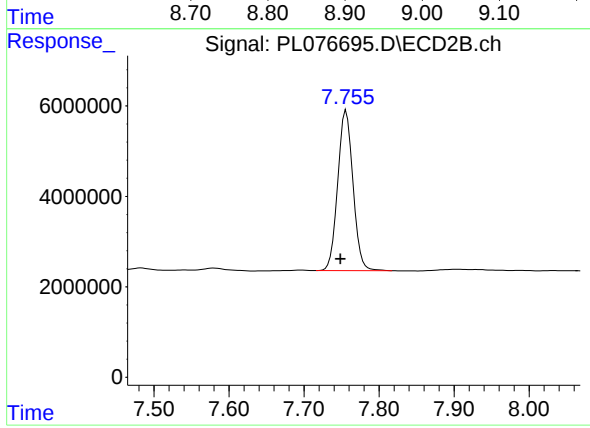

#28 Decachlorobiphenyl

R.T.: 7.756 min
Delta R.T.: 0.008 min
Response: 50211643
Conc: 19.56 ng/ml