

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072822\
 Data File : PL076701.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2022 14:14
 Operator : AR\AJ
 Sample : N3796-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-INFLUENT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/28/2022
 Supervised By :Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 00:08:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.424	2.640	21581422	51218030	20.912m	17.267m
2) SA Decachlor...	8.920	7.751	10339786	43117815	11.724m	16.798m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072822\
Data File : PL076701.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2022 14:14
Operator : AR\AJ
Sample : N3796-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/28/2022
Supervised By : Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 00:08:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

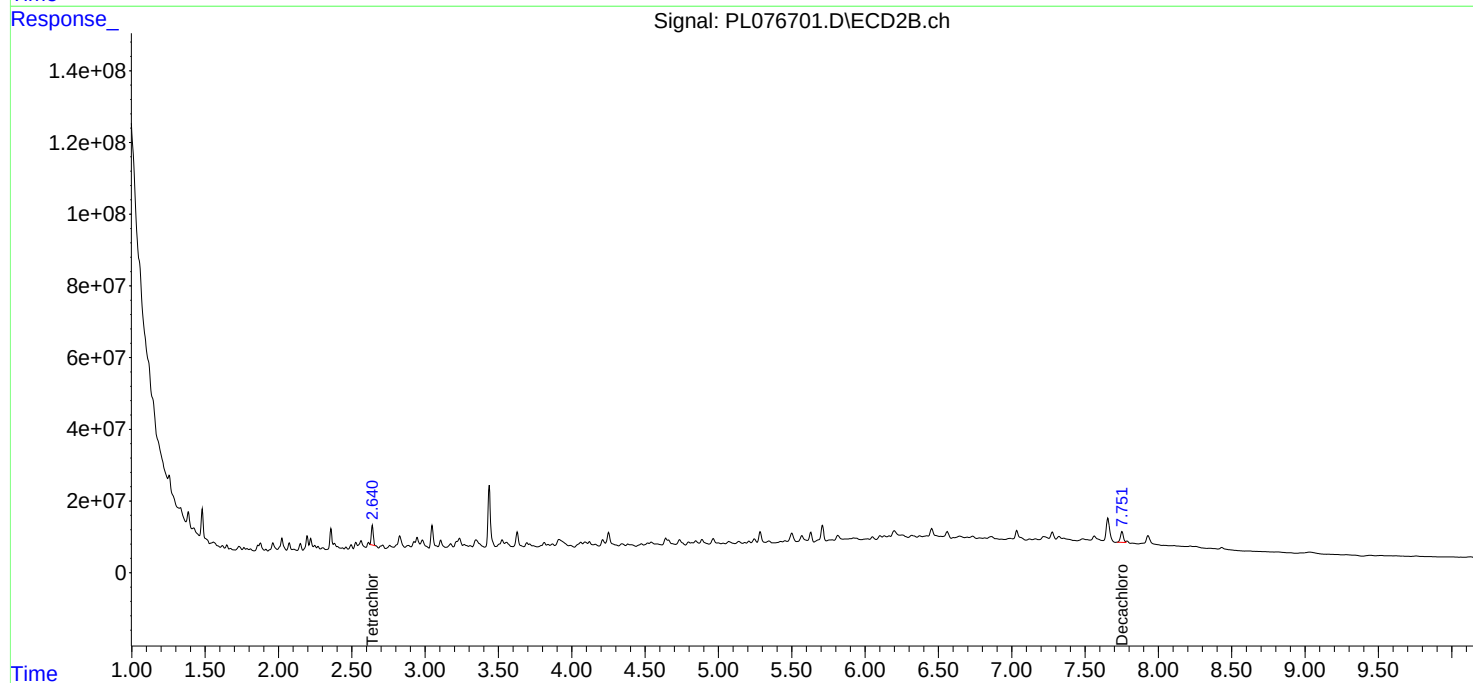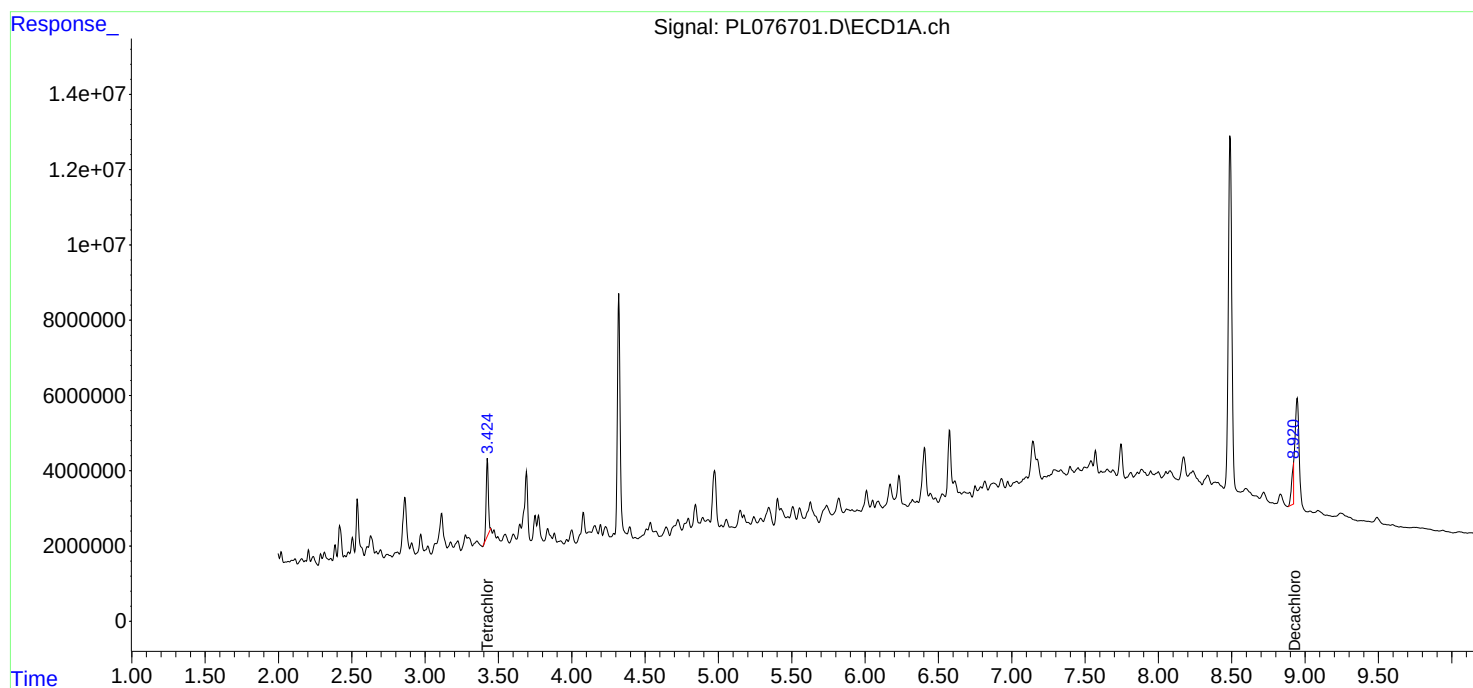

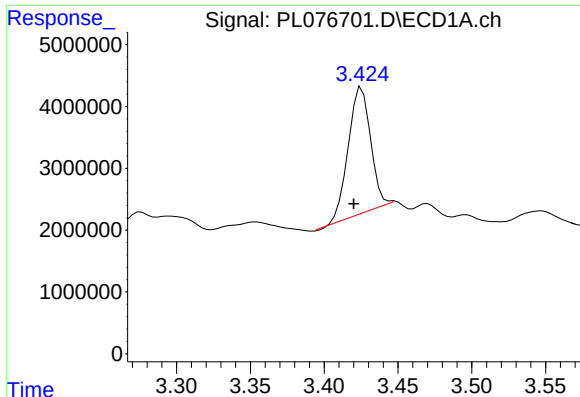


#1 Tetrachloro-m-xylene

R.T.: 3.424 min
Delta R.T.: 0.004 min
Response: 21581422
Conc: 20.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/28/2022
Supervised By :Ankita Jodhani 07/28/2022

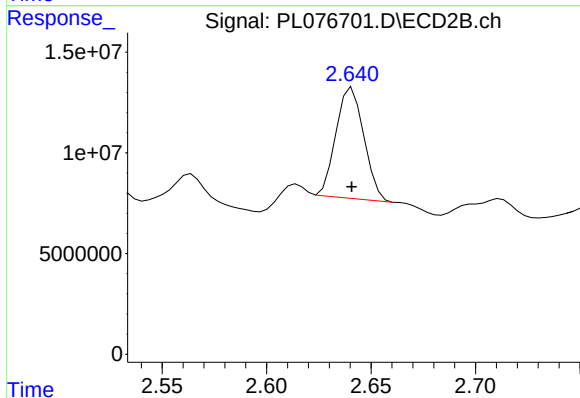


#1 Tetrachloro-m-xylene

R.T.: 2.640 min
Delta R.T.: -0.001 min
Response: 51218030
Conc: 17.27 ng/ml m

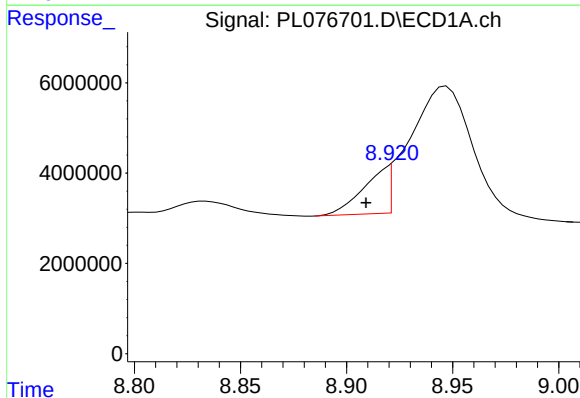

#28 Decachlorobiphenyl

R.T.: 8.920 min
Delta R.T.: 0.011 min
Response: 10339786
Conc: 11.72 ng/ml m

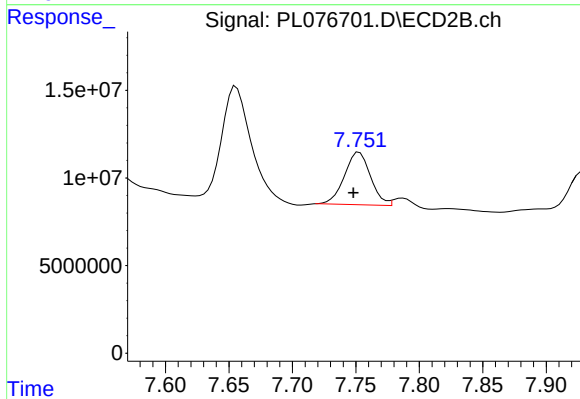

#28 Decachlorobiphenyl

R.T.: 7.751 min
Delta R.T.: 0.003 min
Response: 43117815
Conc: 16.80 ng/ml m