

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072822\
 Data File : PL076712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2022 17:39
 Operator : AR\AJ
 Sample : N3912-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 6601-S

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/28/2022
 Supervised By : Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 00:15:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.420	2.642	11382164	30843643	11.029	10.398
2) SA Decachlor...	8.910	7.748	9155982	23407356	10.382	9.119

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072822\
Data File : PL076712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2022 17:39
Operator : AR\AJ
Sample : N3912-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
6601-S


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/28/2022
Supervised By : Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 00:15:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

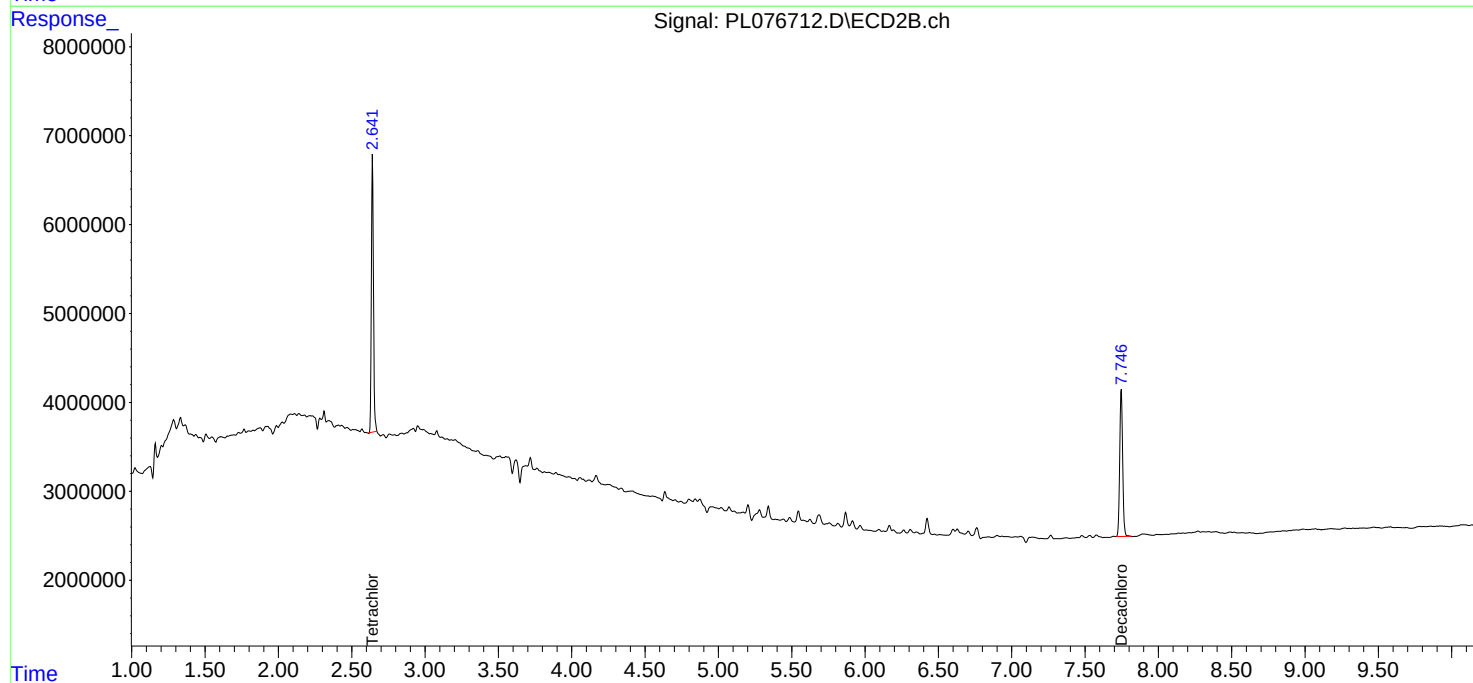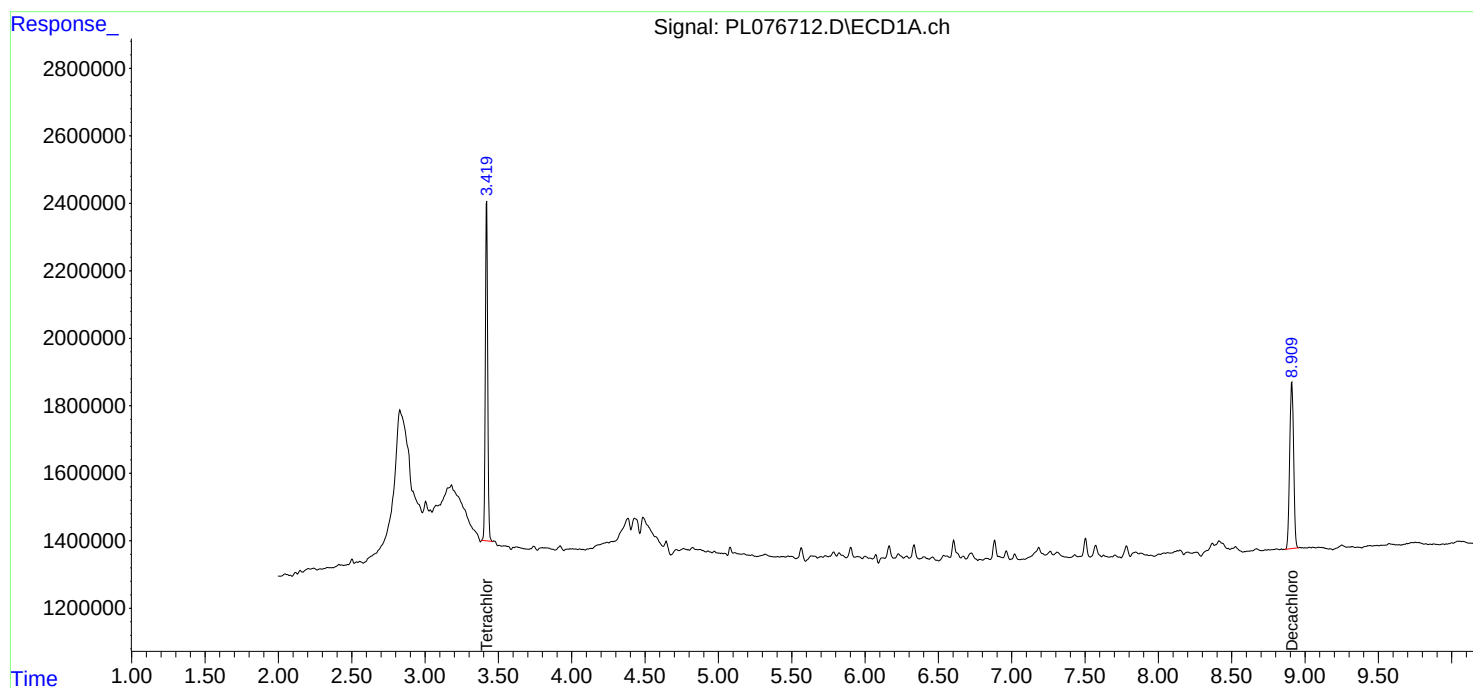

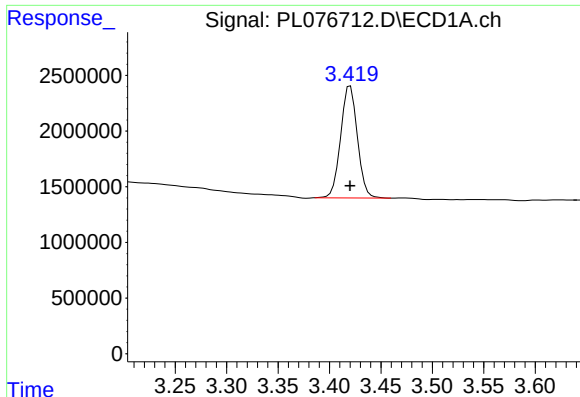


#1 Tetrachloro-m-xylene

R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 11382164
Conc: 11.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
6601-S


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/28/2022
Supervised By :Ankita Jodhani 07/28/2022

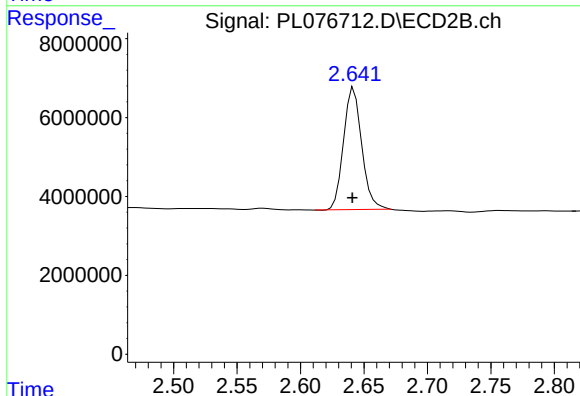


#1 Tetrachloro-m-xylene

R.T.: 2.642 min
Delta R.T.: 0.001 min
Response: 30843643
Conc: 10.40 ng/ml

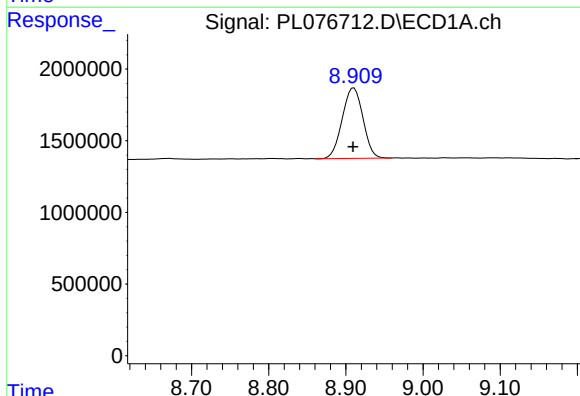

#28 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: 0.001 min
Response: 9155982
Conc: 10.38 ng/ml

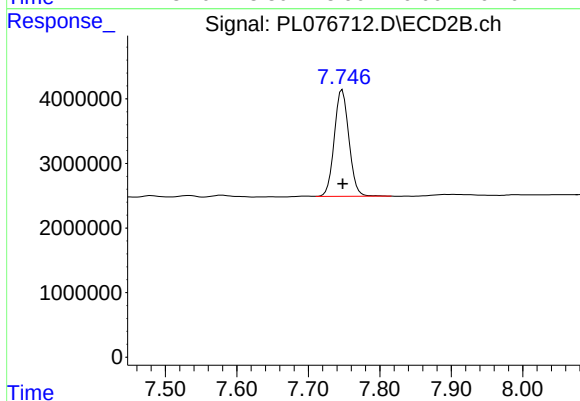

#28 Decachlorobiphenyl

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 23407356
Conc: 9.12 ng/ml