

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072822\
 Data File : PL076713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2022 17:53
 Operator : AR\AJ
 Sample : N3918-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-02-07-26-2022

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/28/2022
 Supervised By :Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 00:15:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.418	2.641	900280	3241366	0.872m	1.093m#
2) SA Decachlor...	8.909	7.746	1094559	2884842	1.241	1.124m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072822\
Data File : PL076713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2022 17:53
Operator : AR\AJ
Sample : N3918-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OR-02-07-26-2022


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/28/2022
Supervised By : Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 00:15:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

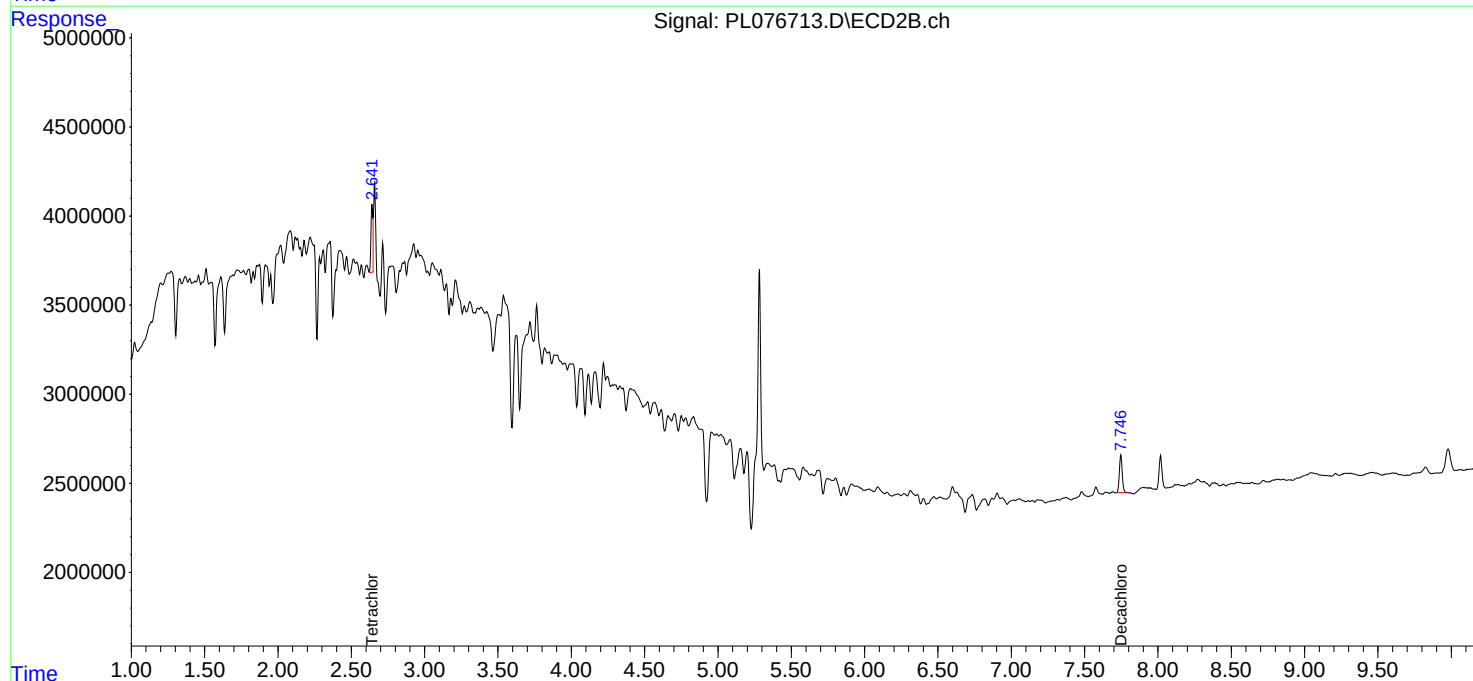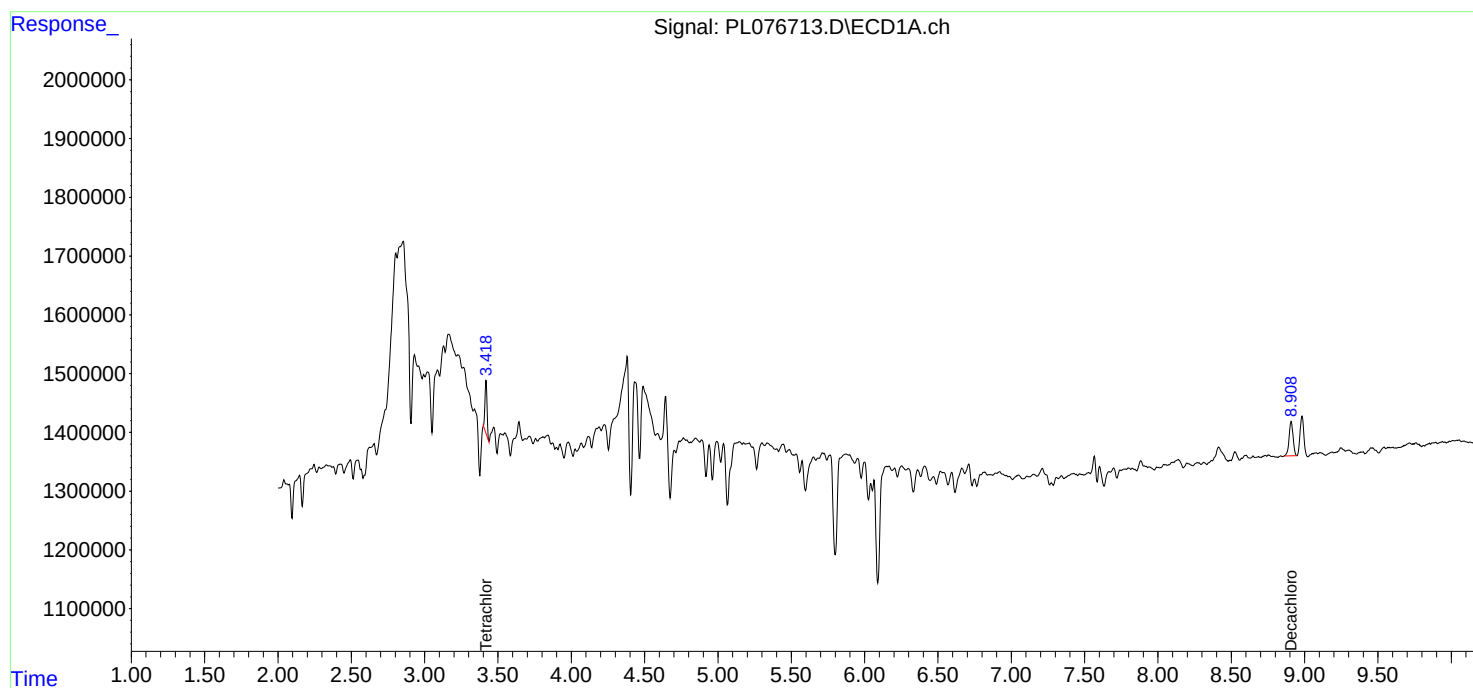

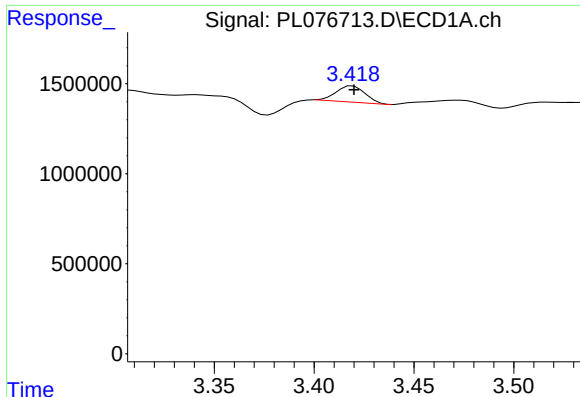


#1 Tetrachloro-m-xylene

R.T.: 3.418 min
Delta R.T.: -0.002 min
Response: 900280
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-02-07-26-2022


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/28/2022
Supervised By :Ankita Jodhani 07/28/2022

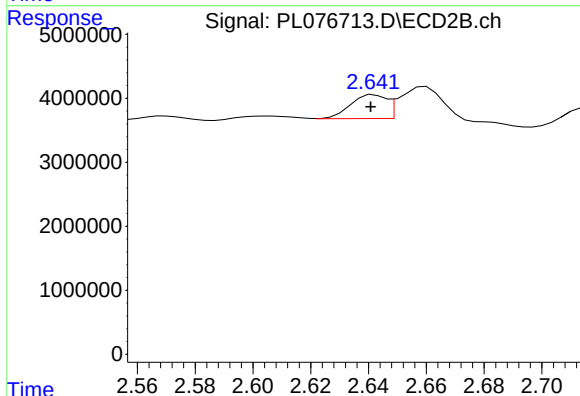


#1 Tetrachloro-m-xylene

R.T.: 2.641 min
Delta R.T.: 0.000 min
Response: 3241366
Conc: 1.09 ng/ml m

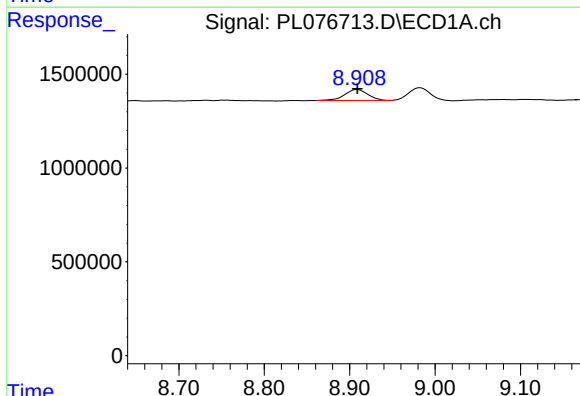

#28 Decachlorobiphenyl

R.T.: 8.909 min
Delta R.T.: 0.000 min
Response: 1094559
Conc: 1.24 ng/ml

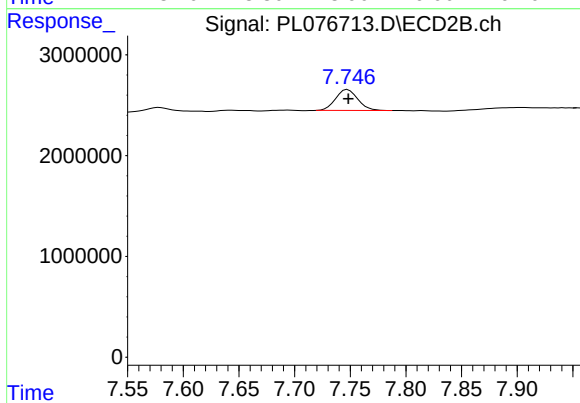

#28 Decachlorobiphenyl

R.T.: 7.746 min
Delta R.T.: -0.002 min
Response: 2884842
Conc: 1.12 ng/ml m