

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072825\
 Data File : PL096601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2025 18:00
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 08:10:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:08:04 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.827	308.2E6	613.0E6	99.614	100.364
28)	SA Decachlor...	9.015	7.992	220.5E6	411.8E6	97.034	97.851
Target Compounds							
23)	Chlordane-1	4.690	3.838	161.5E6	203.4E6	996.669	1016.563
24)	Chlordane-2	5.214	4.418	162.9E6	224.2E6	976.392	974.867
25)	Chlordane-3	5.916	5.052	666.4E6	692.8E6	1020.421	1030.726
26)	Chlordane-4	6.001	5.115	815.6E6	616.1E6	1010.572	1024.705
27)	Chlordane-5	6.838	6.009	130.0E6	247.0E6	1015.497	1009.096



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072825\
Data File : PL096601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2025 18:00
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 08:10:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:08:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

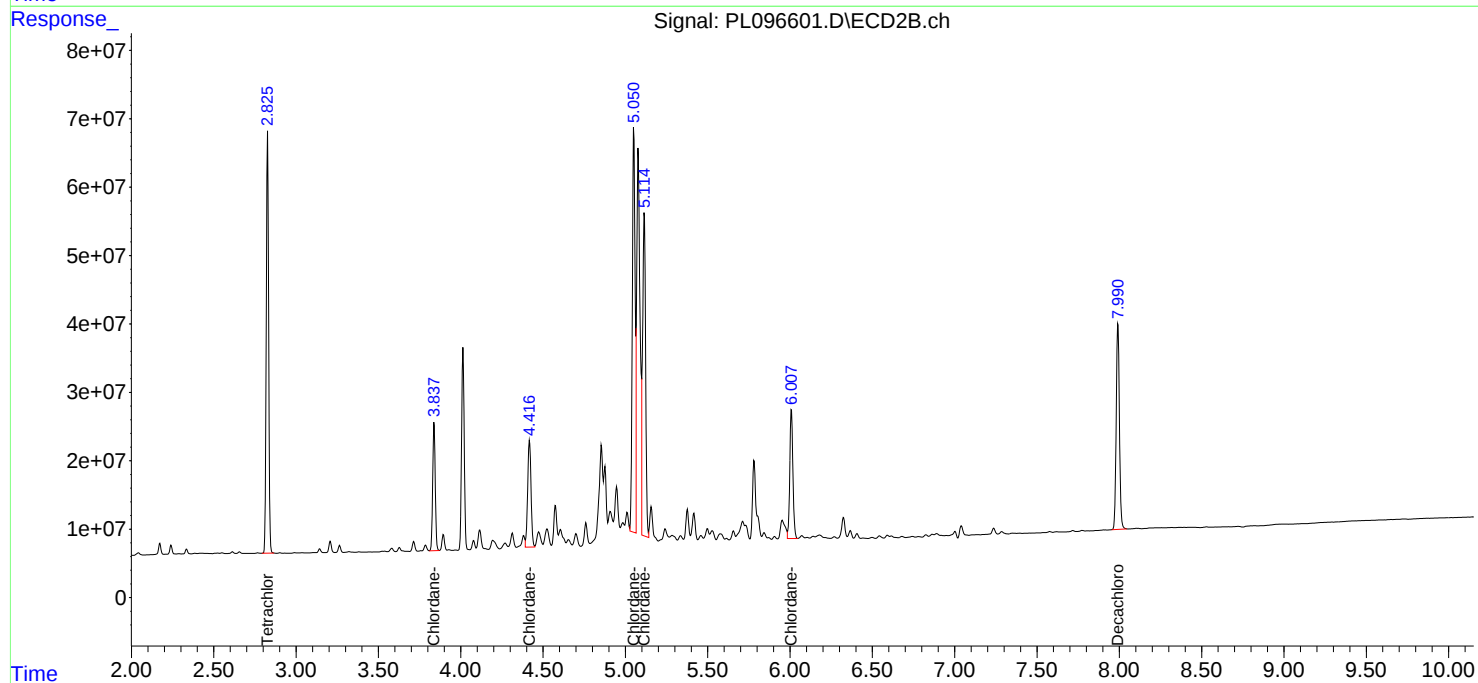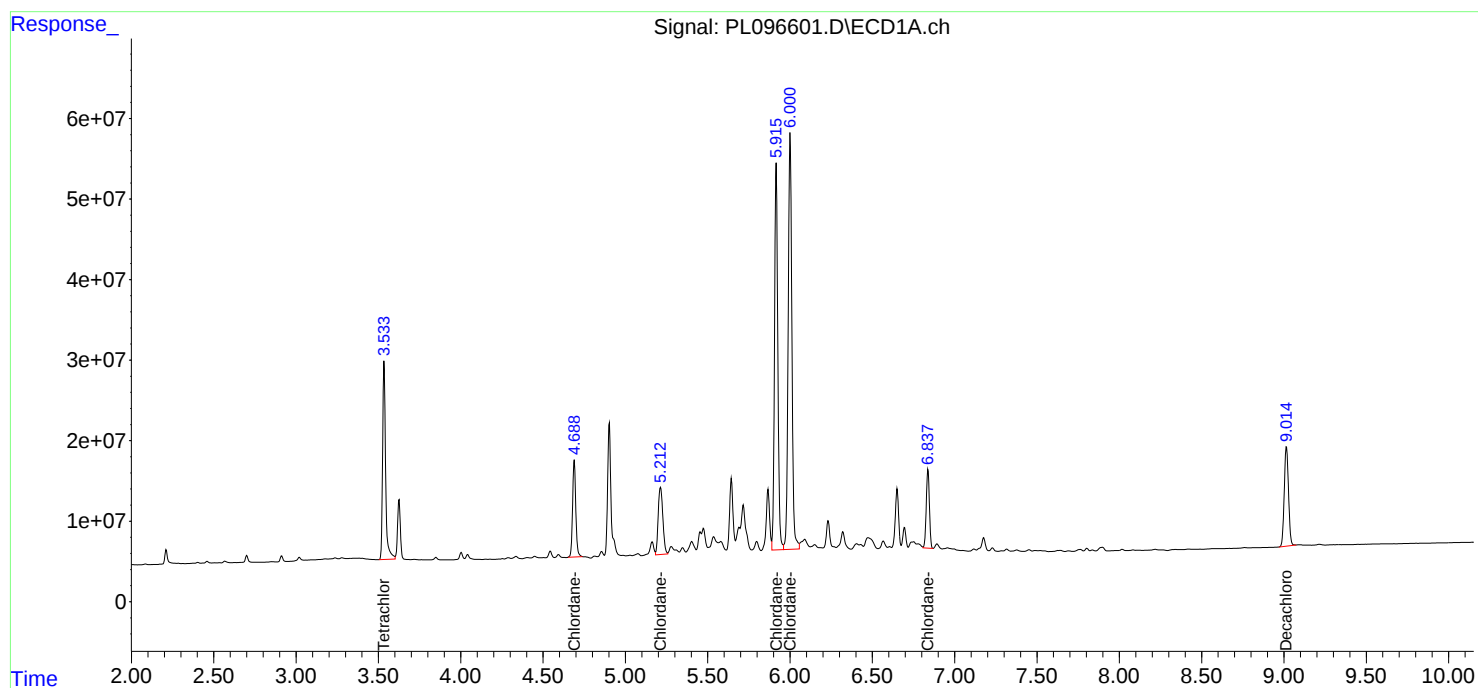


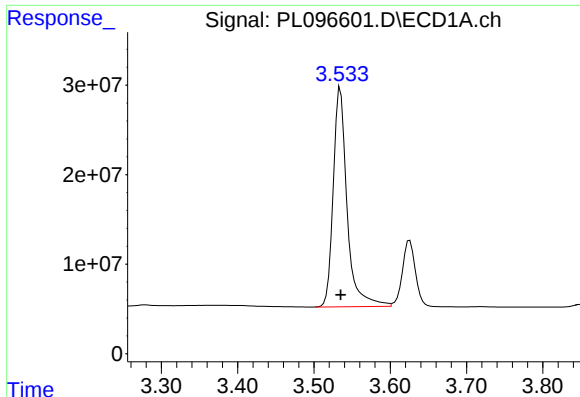

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 308167735
Conc: 99.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

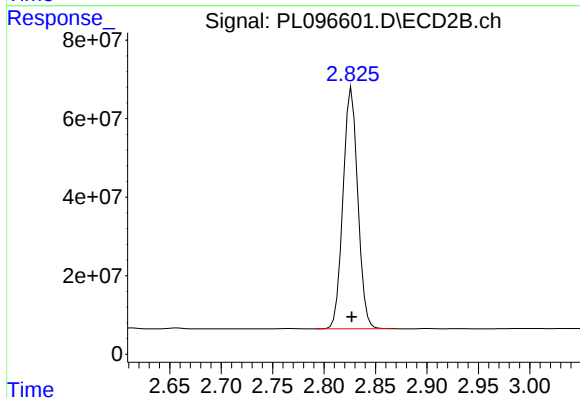


#1 Tetrachloro-m-xylene

R.T.: 2.827 min
Delta R.T.: 0.000 min
Response: 612988712
Conc: 100.36 ng/ml

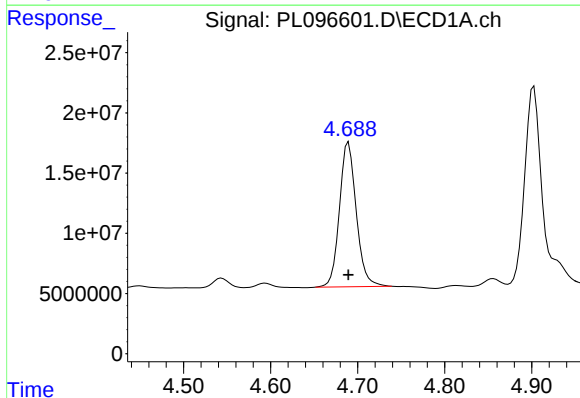


#23 Chlordane-1

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 161458999
Conc: 996.67 ng/ml

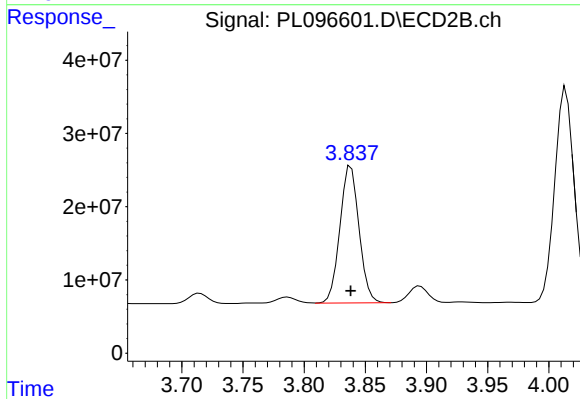

#23 Chlordane-1


R.T.: 3.838 min
Delta R.T.: 0.000 min
Response: 203448277
Conc: 1016.56 ng/ml

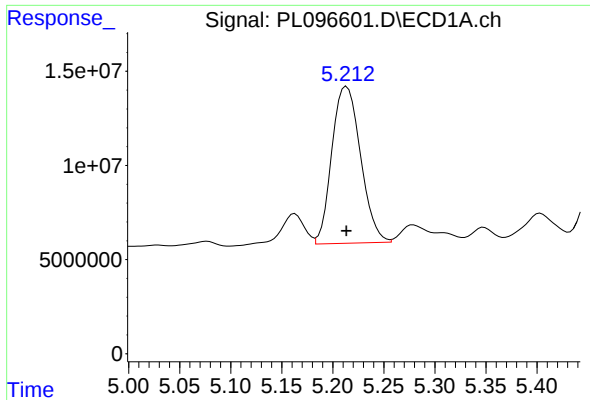

#24 Chlordane-2


R.T.: 5.214 min
Delta R.T.: 0.000 min
Response: 162881508
Conc: 976.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

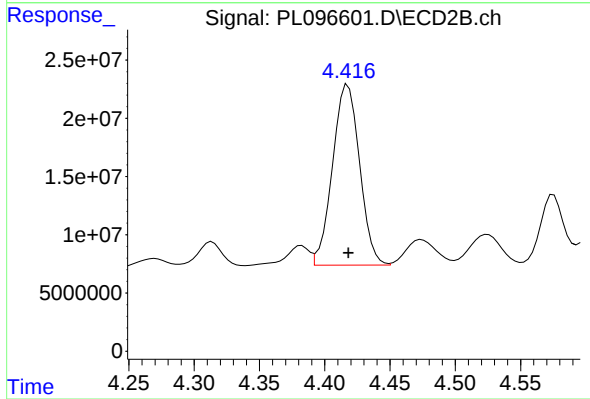


#24 Chlordane-2

R.T.: 4.418 min
Delta R.T.: 0.000 min
Response: 224225681
Conc: 974.87 ng/ml

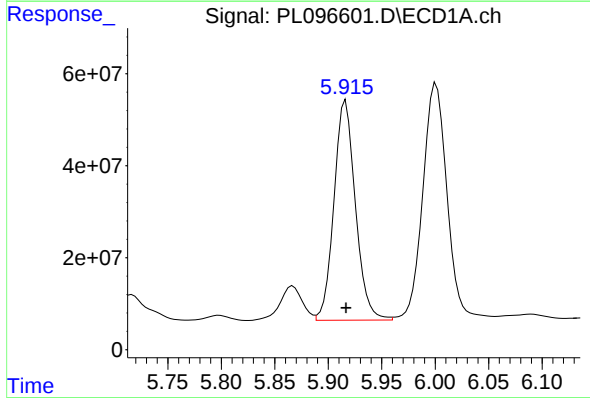


#25 Chlordane-3

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 666362934
Conc: 1020.42 ng/ml

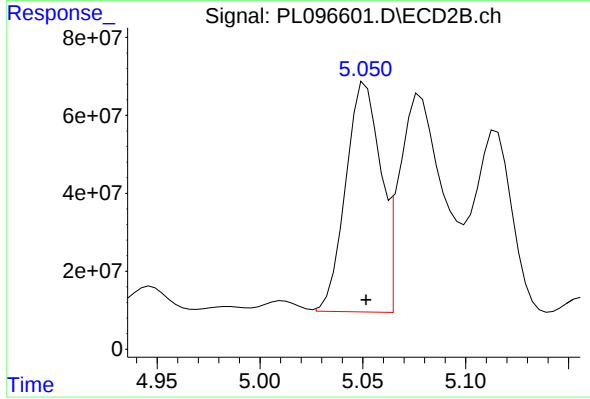

#25 Chlordane-3


R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 692840994
Conc: 1030.73 ng/ml

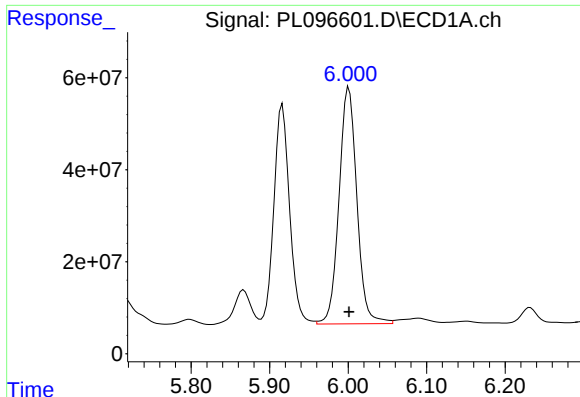

#26 Chlordane-4


R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 815595191
Conc: 1010.57 ng/m

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

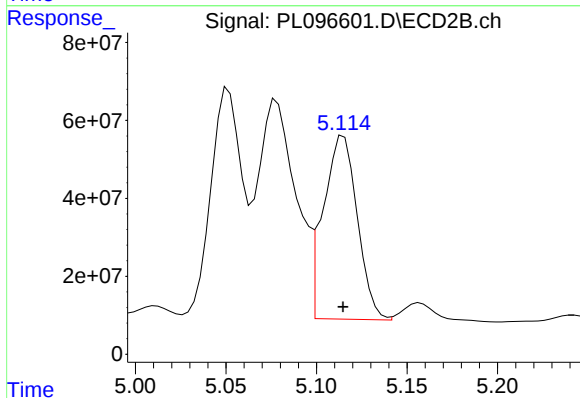


#26 Chlordane-4

R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 616095983
Conc: 1024.71 ng/ml

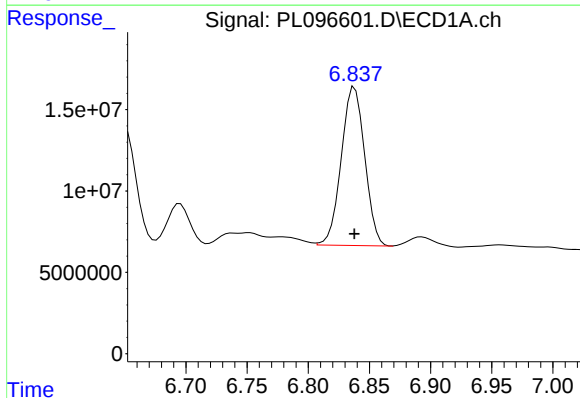


#27 Chlordane-5

R.T.: 6.838 min
Delta R.T.: 0.000 min
Response: 129976578
Conc: 1015.50 ng/ml

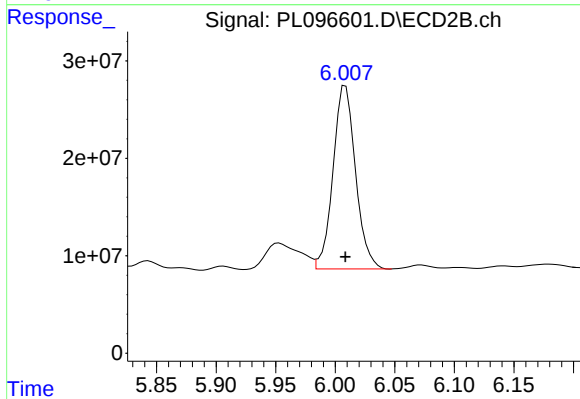

#27 Chlordane-5


R.T.: 6.009 min
Delta R.T.: 0.000 min
Response: 247024418
Conc: 1009.10 ng/ml

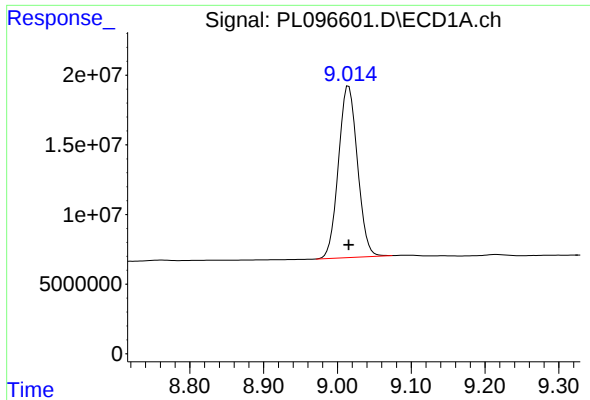

#28 Decachlorobiphenyl

R.T.: 9.015 min
Delta R.T.: 0.000 min
Response: 220521210
Conc: 97.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

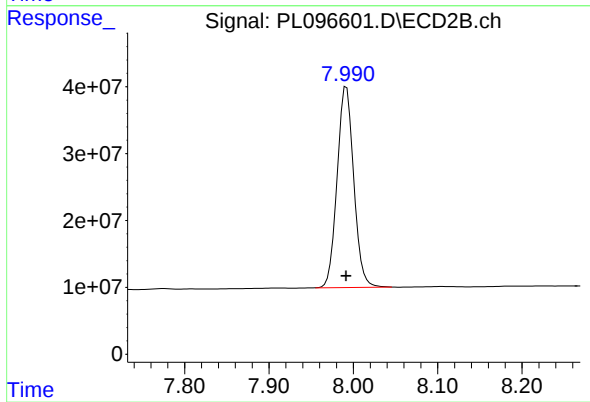

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 411782263
Conc: 97.85 ng/ml