

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072825\
 Data File : PL096602.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2025 18:14
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 08:11:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:08:04 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.827	230.6E6	459.4E6	74.544	75.218
28)	SA Decachlor...	9.015	7.992	166.4E6	311.4E6	73.203	74.006
Target Compounds							
23)	Chlordane-1	4.690	3.838	120.7E6	151.6E6	744.957	757.466
24)	Chlordane-2	5.213	4.418	122.2E6	169.9E6	732.337	738.550
25)	Chlordane-3	5.917	5.051	493.4E6	512.8E6	755.598	762.829
26)	Chlordane-4	6.001	5.115	605.8E6	455.6E6	750.590	757.734
27)	Chlordane-5	6.838	6.009	96480039	185.0E6	753.791	755.736



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072825\
Data File : PL096602.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2025 18:14
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 08:11:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:08:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

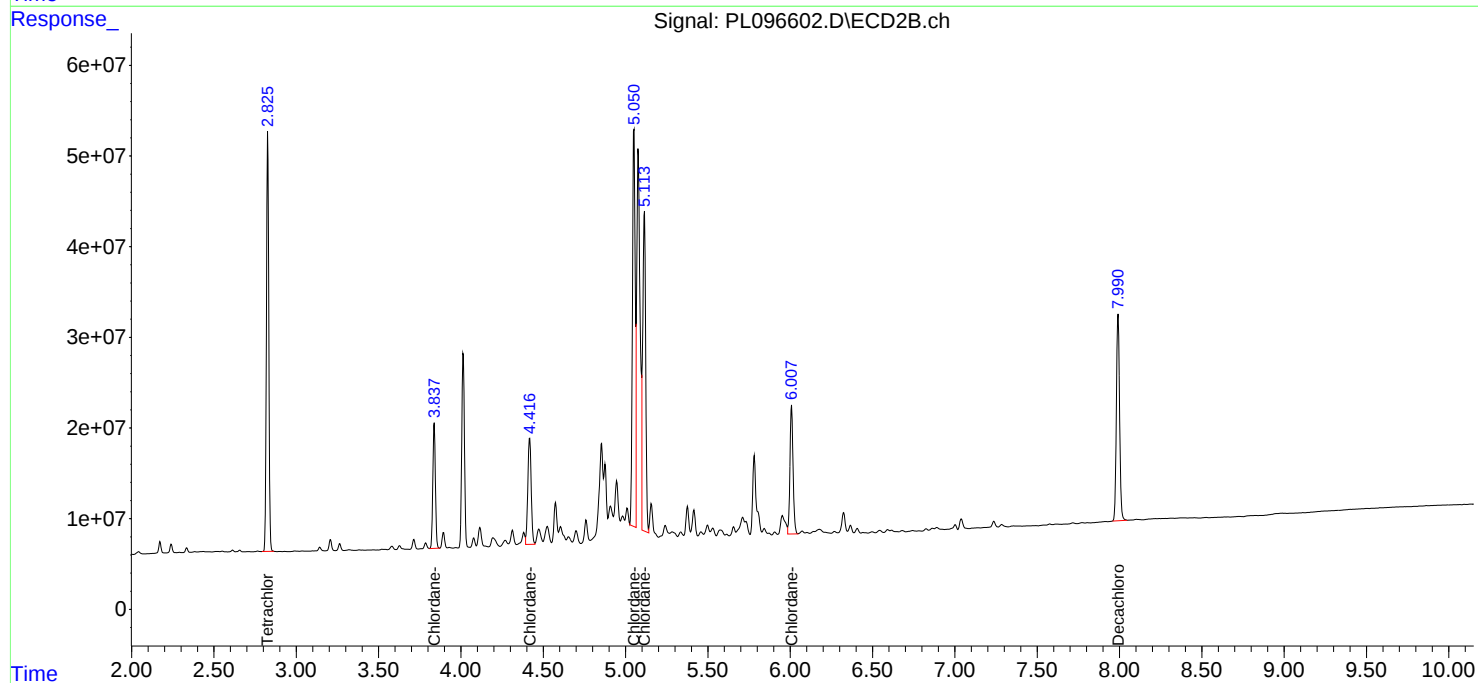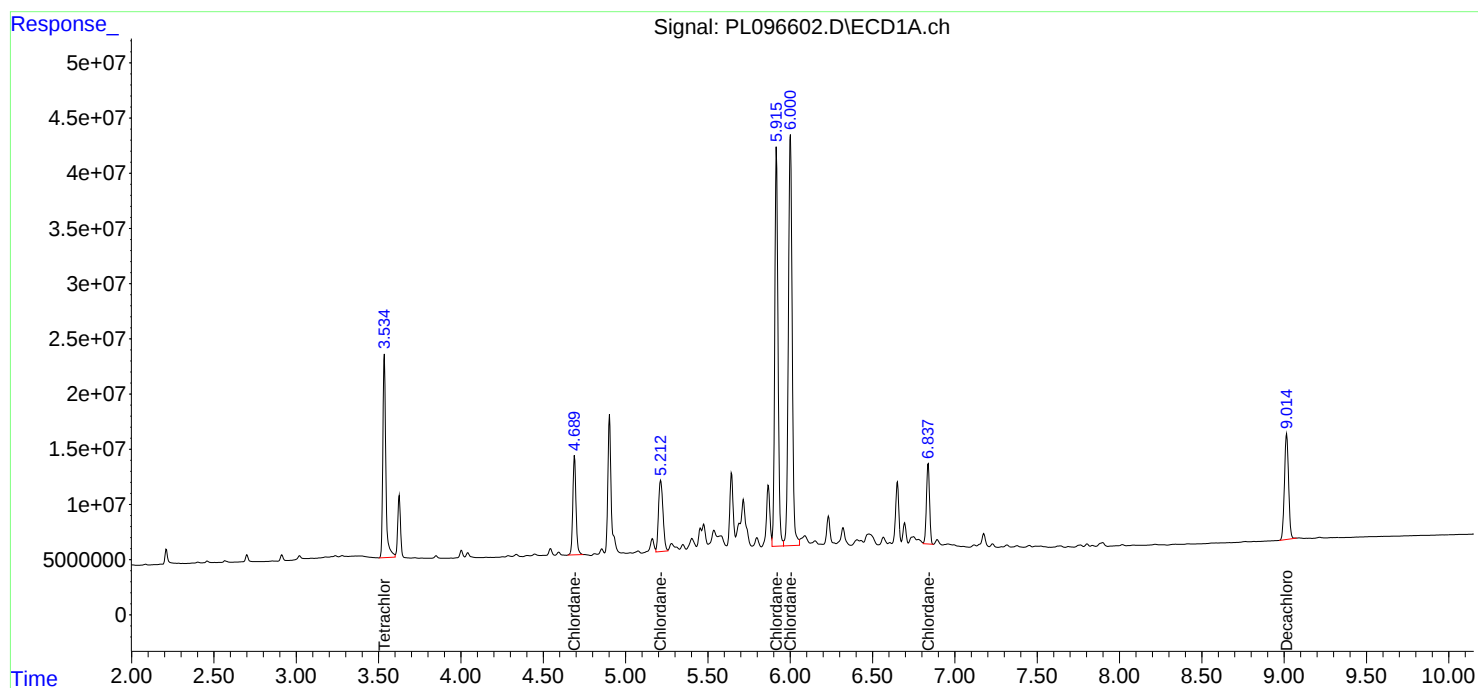


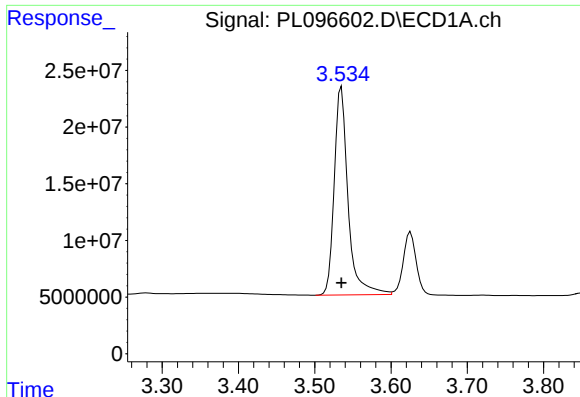

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 230610440
Conc: 74.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

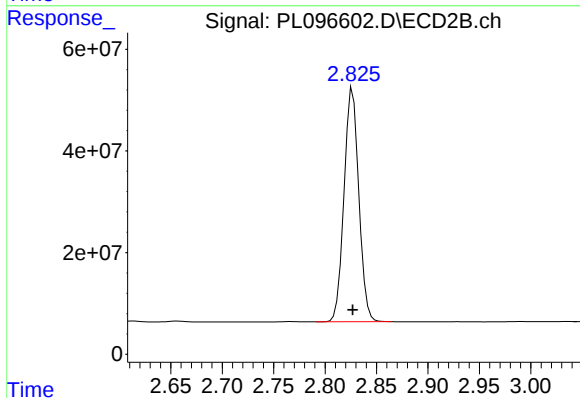


#1 Tetrachloro-m-xylene

R.T.: 2.827 min
Delta R.T.: 0.000 min
Response: 459404398
Conc: 75.22 ng/ml

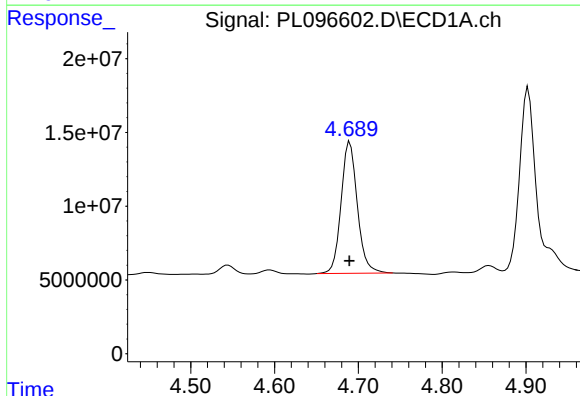


#23 Chlordane-1

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 120682000
Conc: 744.96 ng/ml

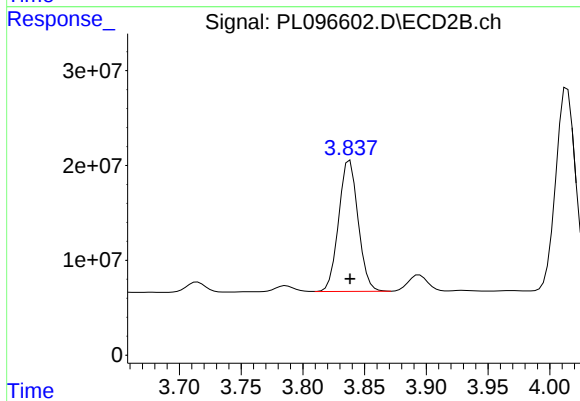

#23 Chlordane-1


R.T.: 3.838 min
Delta R.T.: 0.000 min
Response: 151594407
Conc: 757.47 ng/ml

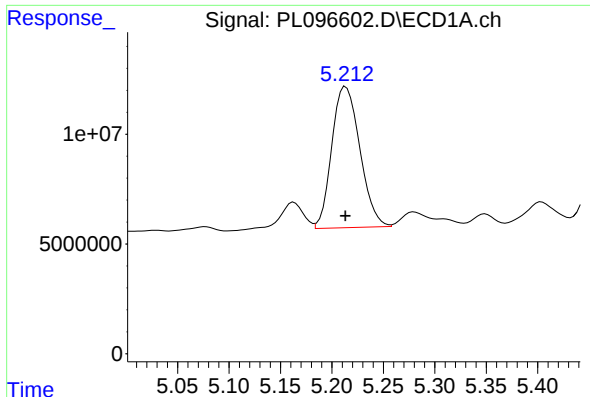

#24 Chlordane-2


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 122168275
Conc: 732.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

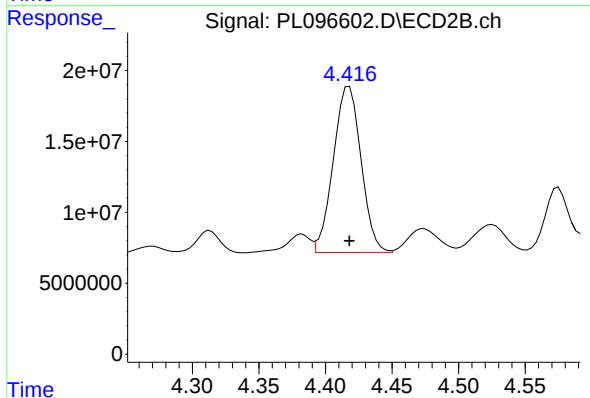


#24 Chlordane-2

R.T.: 4.418 min
Delta R.T.: 0.000 min
Response: 169871170
Conc: 738.55 ng/ml

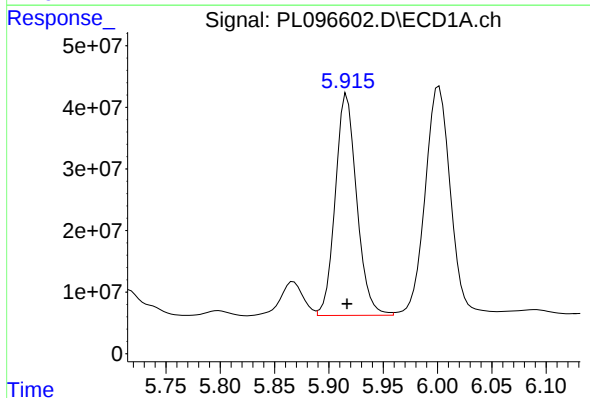


#25 Chlordane-3

R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 493426580
Conc: 755.60 ng/ml

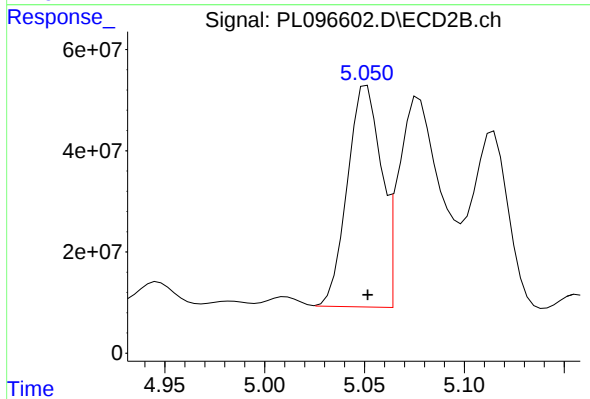

#25 Chlordane-3


R.T.: 5.051 min
Delta R.T.: 0.000 min
Response: 512764268
Conc: 762.83 ng/ml

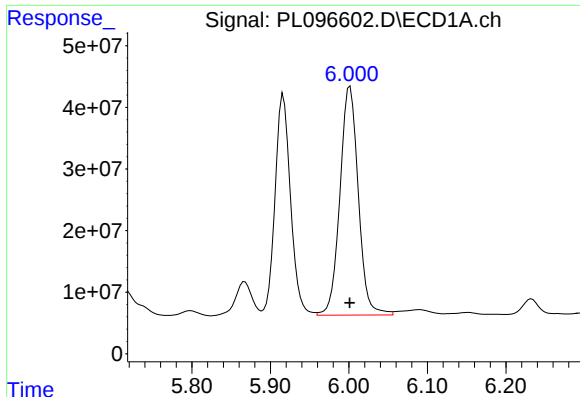

#26 Chlordane-4


R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 605772923
Conc: 750.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

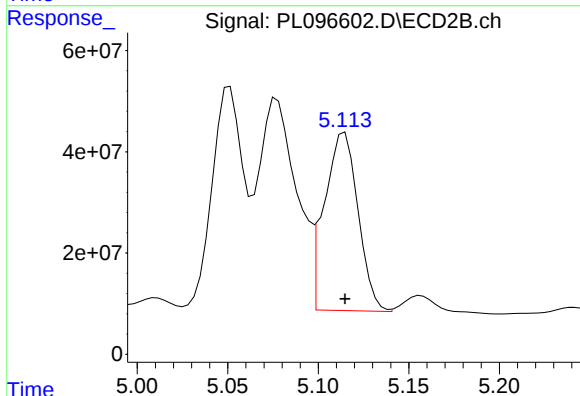


#26 Chlordane-4

R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 455581767
Conc: 757.73 ng/ml

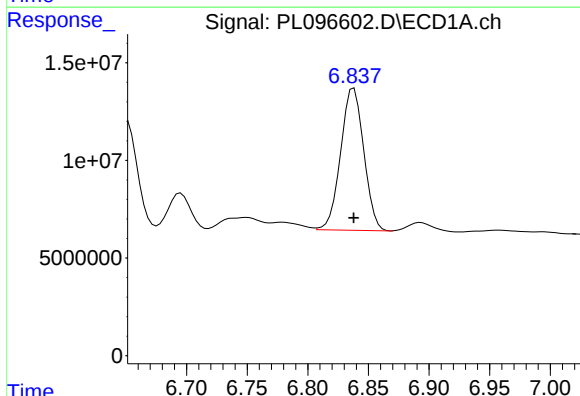


#27 Chlordane-5

R.T.: 6.838 min
Delta R.T.: 0.000 min
Response: 96480039
Conc: 753.79 ng/ml

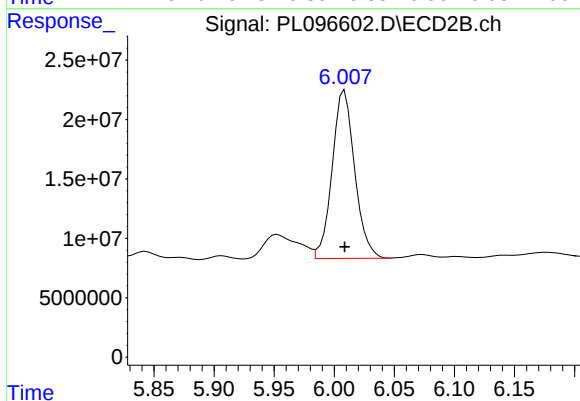

#27 Chlordane-5


R.T.: 6.009 min
Delta R.T.: 0.000 min
Response: 185002548
Conc: 755.74 ng/ml

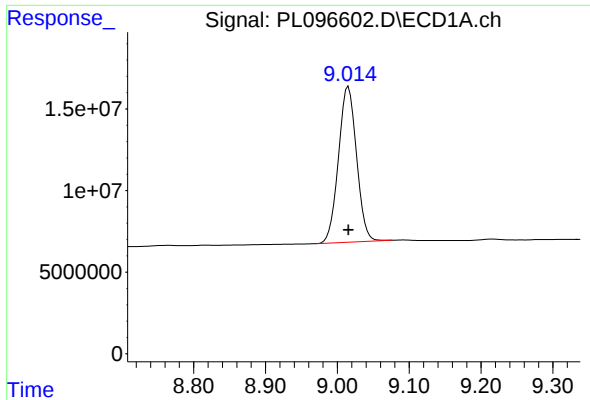

#28 Decachlorobiphenyl

R.T.: 9.015 min
Delta R.T.: 0.000 min
Response: 166363788
Conc: 73.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

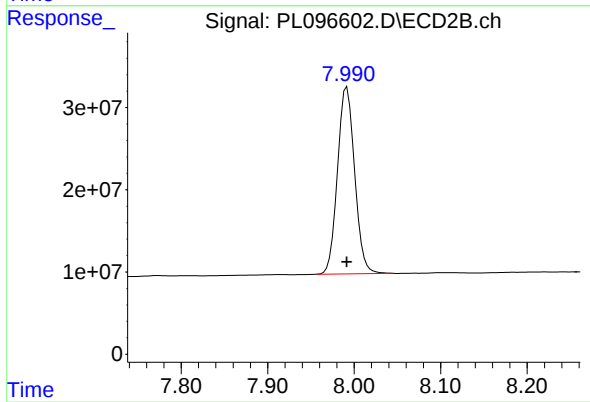

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 311437522
Conc: 74.01 ng/ml