

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072825\
 Data File : PL096604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2025 18:41
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 08:11:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:08:04 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.827	77979760	152.2E6	25.207	24.928
28)	SA Decachlor...	9.015	7.991	58824826	109.3E6	25.884	25.974
Target Compounds							
23)	Chlordane-1	4.690	3.838	40601168	49824738	250.627	248.957
24)	Chlordane-2	5.213	4.418	43296060	58687662	259.538	255.157
25)	Chlordane-3	5.916	5.051	157.2E6	165.4E6	240.753	246.130
26)	Chlordane-4	6.001	5.115	193.9E6	147.7E6	240.222	245.741
27)	Chlordane-5	6.837	6.008	30148657	61383648	235.549	250.753



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072825\
Data File : PL096604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2025 18:41
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 08:11:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:08:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

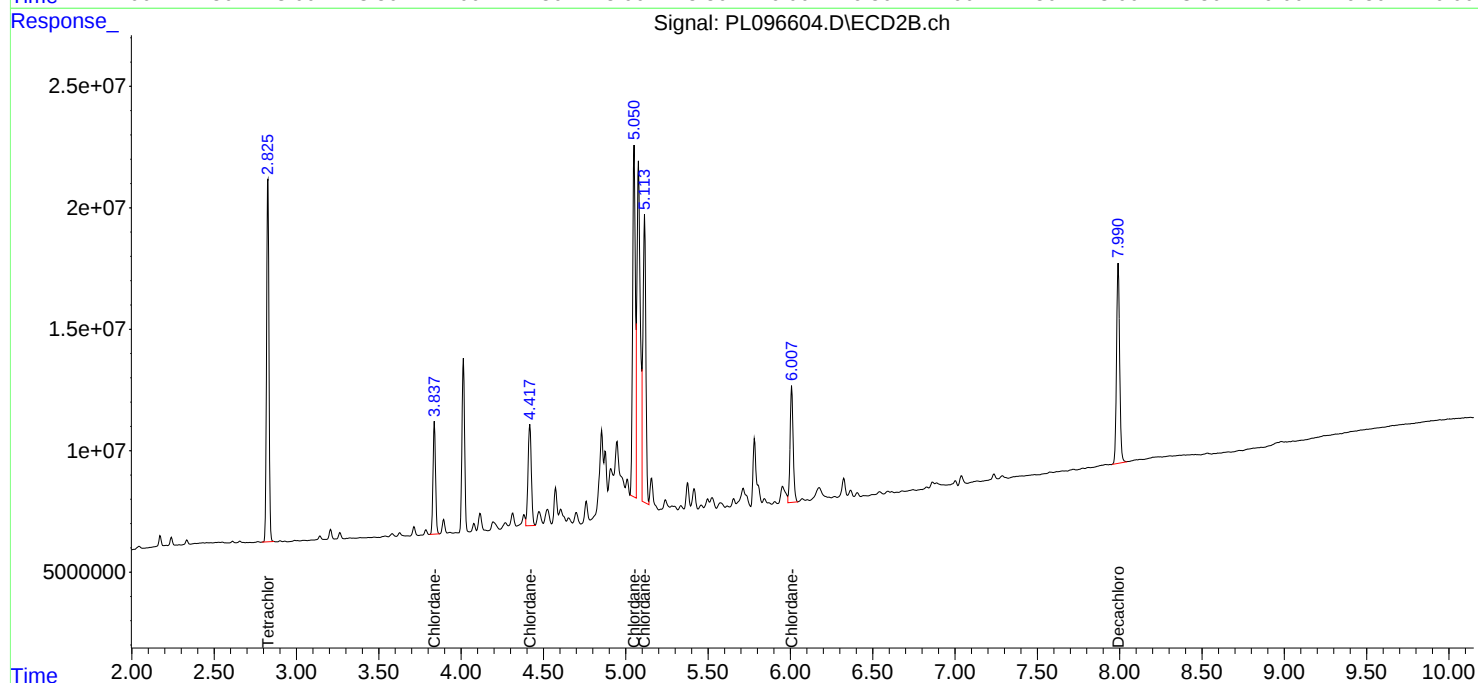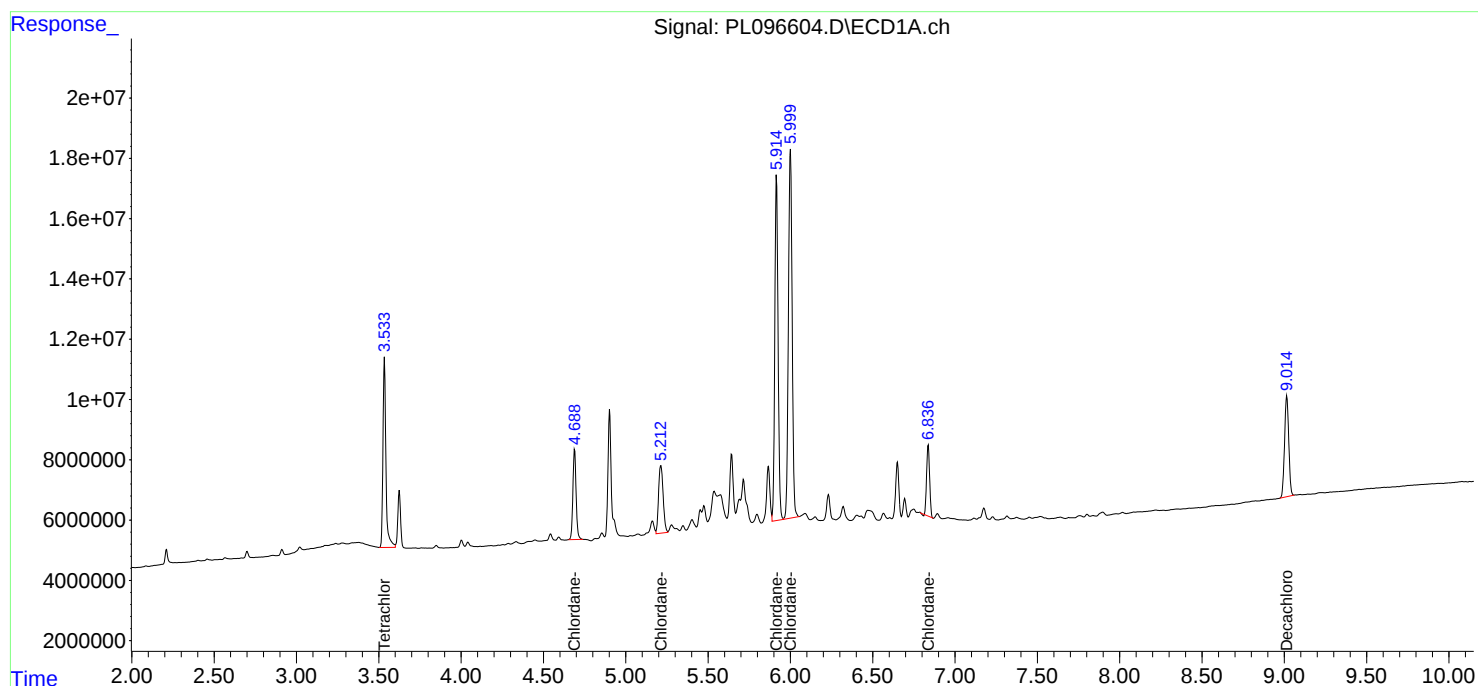


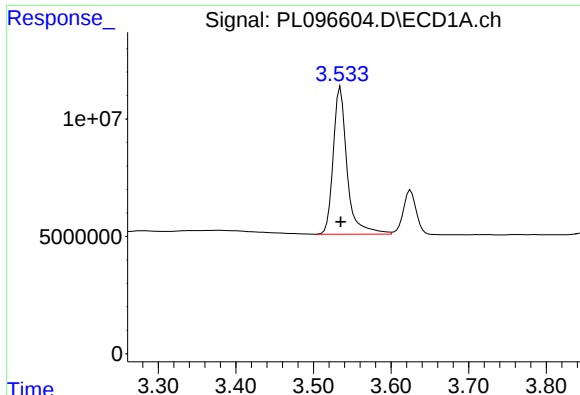

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 77979760
Conc: 25.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

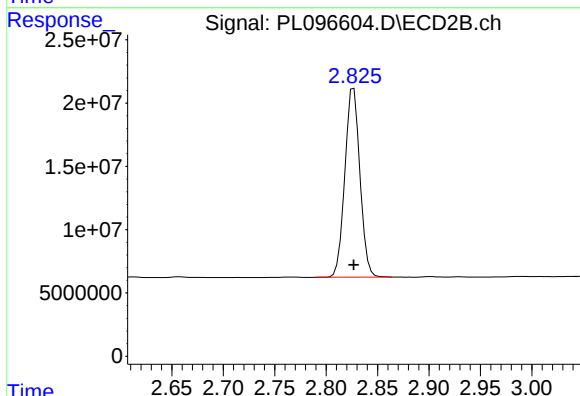


#1 Tetrachloro-m-xylene

R.T.: 2.827 min
Delta R.T.: 0.000 min
Response: 152249130
Conc: 24.93 ng/ml

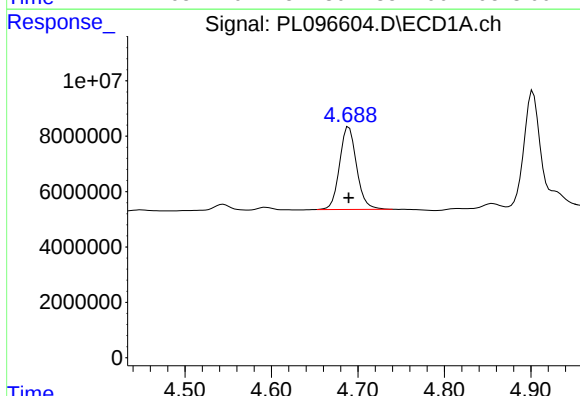


#23 Chlordane-1

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 40601168
Conc: 250.63 ng/ml

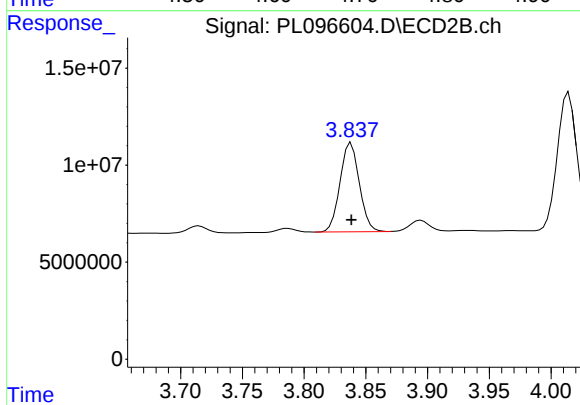

#23 Chlordane-1


R.T.: 3.838 min
Delta R.T.: 0.000 min
Response: 49824738
Conc: 248.96 ng/ml

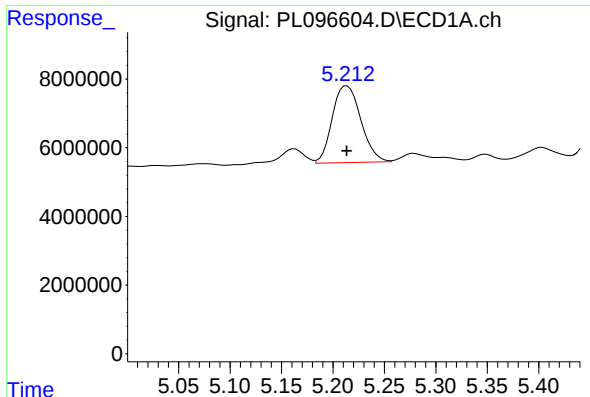

#24 Chlordane-2


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 43296060
Conc: 259.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

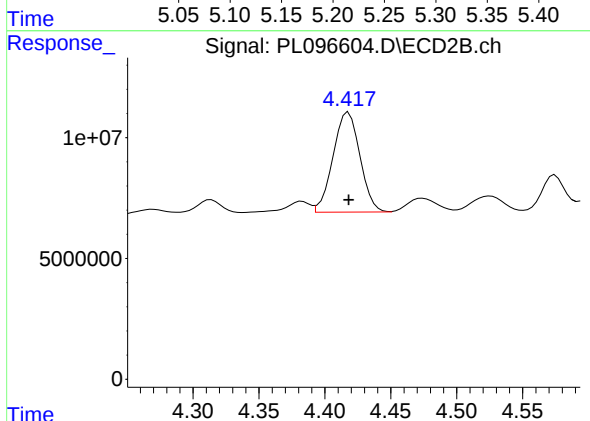


#24 Chlordane-2

R.T.: 4.418 min
Delta R.T.: 0.000 min
Response: 58687662
Conc: 255.16 ng/ml

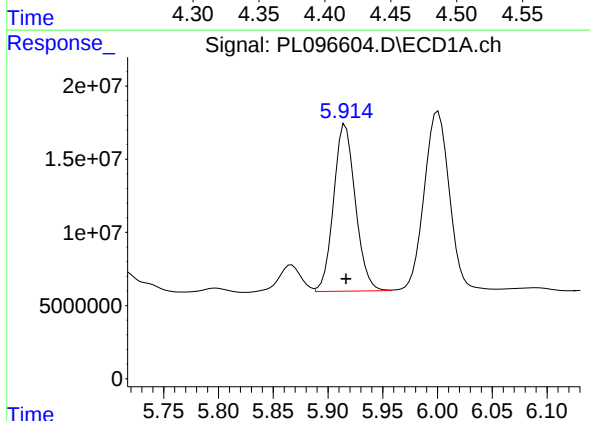


#25 Chlordane-3

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 157218375
Conc: 240.75 ng/ml

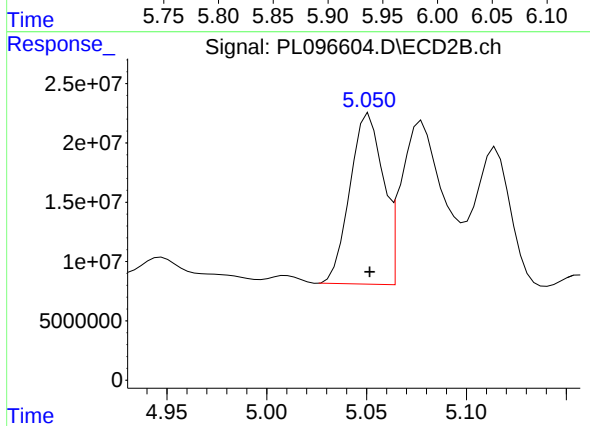

#25 Chlordane-3


R.T.: 5.051 min
Delta R.T.: 0.000 min
Response: 165445678
Conc: 246.13 ng/ml

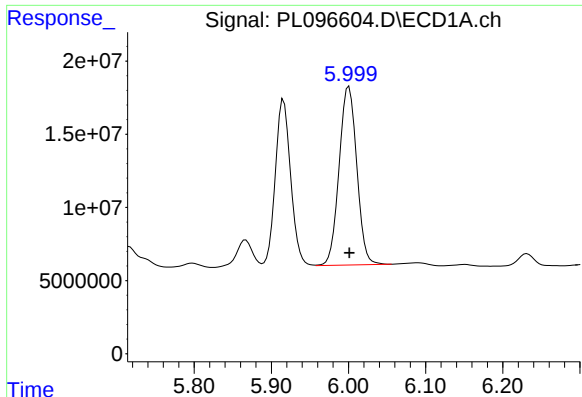

#26 Chlordane-4


R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 193874640
Conc: 240.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

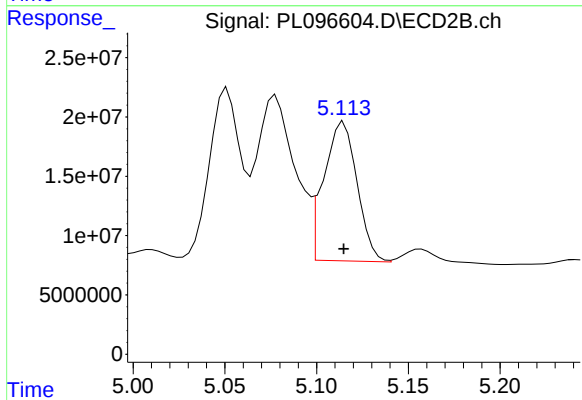


#26 Chlordane-4

R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 147749771
Conc: 245.74 ng/ml

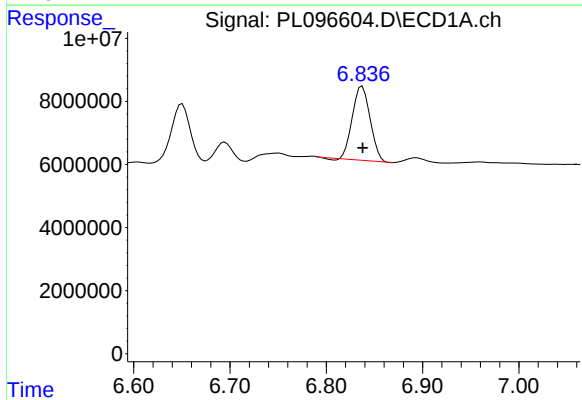


#27 Chlordane-5

R.T.: 6.837 min
Delta R.T.: 0.000 min
Response: 30148657
Conc: 235.55 ng/ml

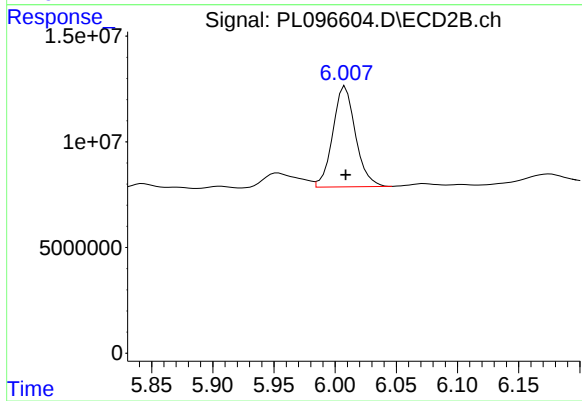

#27 Chlordane-5


R.T.: 6.008 min
Delta R.T.: 0.000 min
Response: 61383648
Conc: 250.75 ng/ml

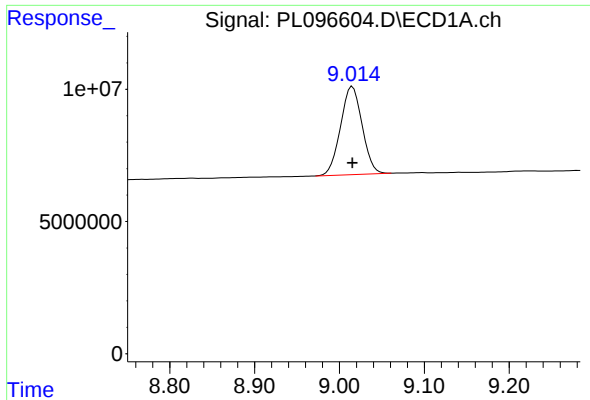

#28 Decachlorobiphenyl

R.T.: 9.015 min
Delta R.T.: 0.000 min
Response: 58824826
Conc: 25.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

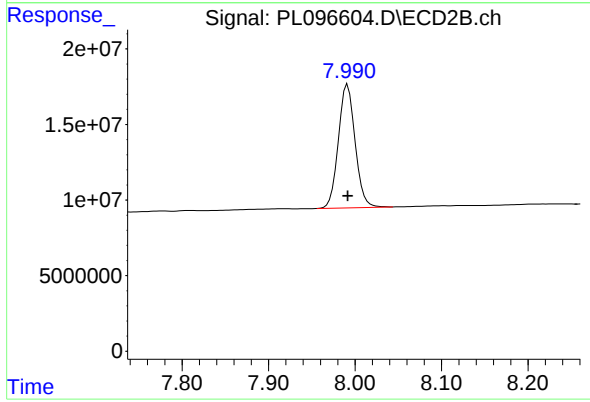

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: 0.000 min
Response: 109306046
Conc: 25.97 ng/ml