

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072919\
 Data File : PL050846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 10:32
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 00:39:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.341f	0.000	3326772	0	0.331	N.D. #
Target Compounds							
2)	A alpha-BHC	0.000	4.344f	0	3875912	N.D.	0.939 #
3)	MA gamma-BHC...	0.000	4.581f	0	25978251	N.D.	6.707 #
4)	MA Heptachlor	4.286f	0.000	1992559	0	0.121	N.D. #
6)	B beta-BHC	4.286	0.000	1992559	0	0.304	N.D. #
9)	A Endosulfan I	5.305	0.000	114.3E6	0	7.859	N.D. #
10)	B gamma-Chl...	5.203	0.000	52305882	0	3.314	N.D. #
17)	MA 4,4'-DDT	6.154f	0.000	171.2E6	0	13.821	N.D. #
18)	B Endrin al...	6.242	0.000	27794014	0	2.409	N.D. #
24)	Chlordane-2	4.677f	0.000	32732968	0	73.129	N.D. #
25)	Chlordane-3	5.203	0.000	52305882	0	37.367	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072919\
Data File : PL050846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 10:32
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 00:39:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

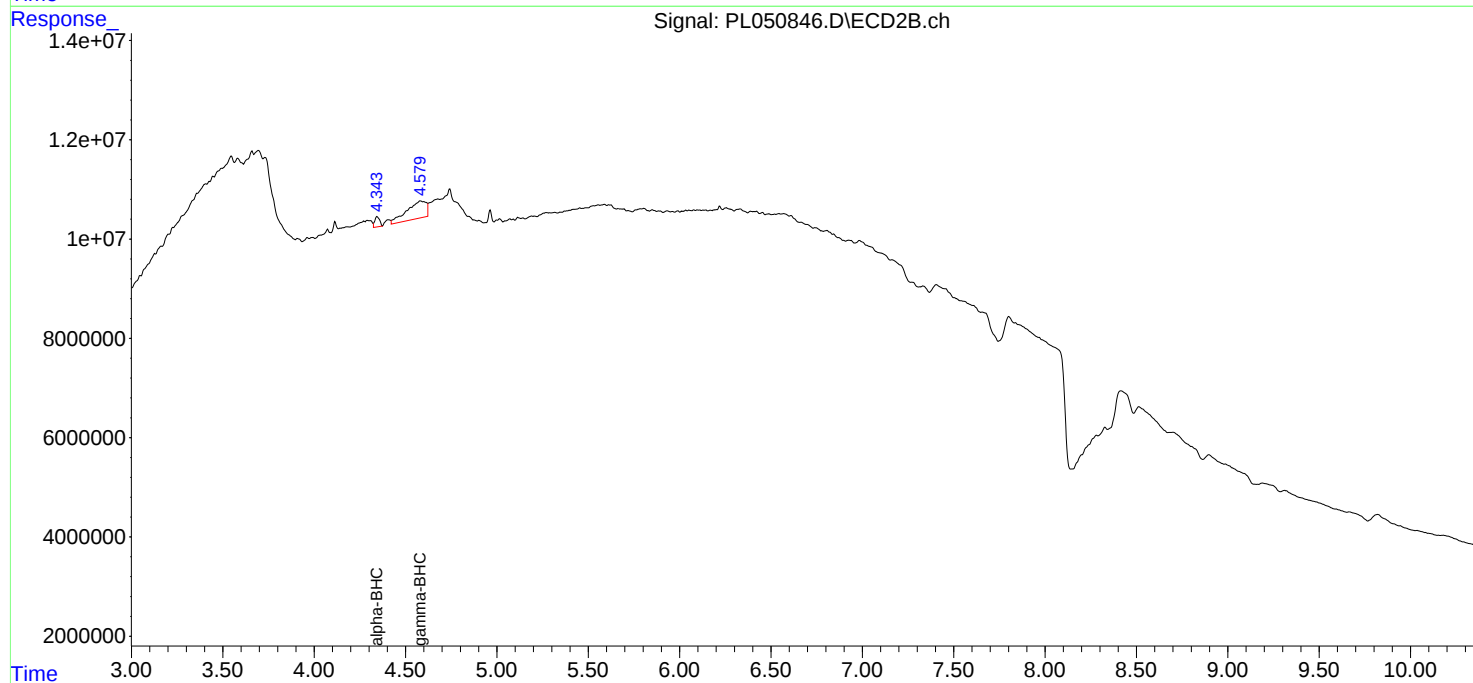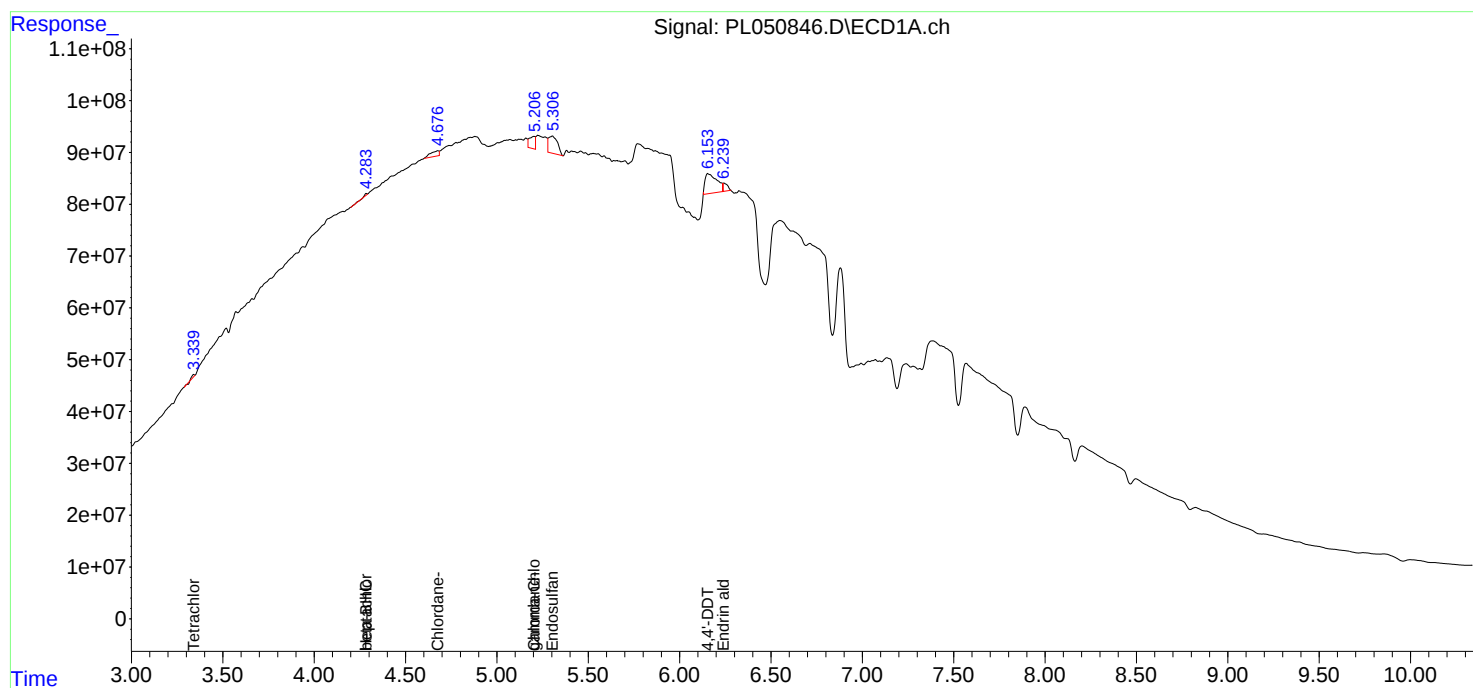


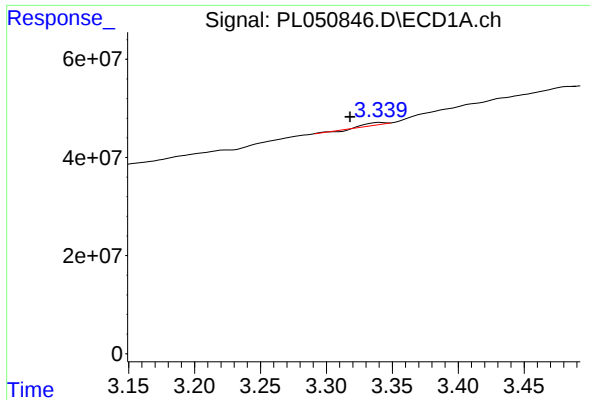

#1 Tetrachloro-m-xylene


R.T.: 3.341 min
Delta R.T.: 0.023 min
Response: 3326772
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

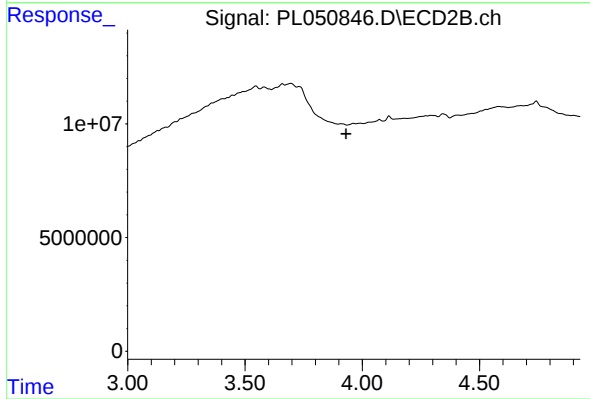


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.931 min
Response: 0
Conc: N.D.

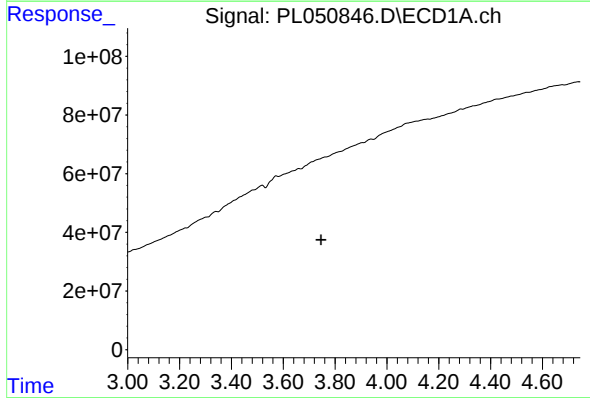


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.746 min
Response: 0
Conc: N.D.

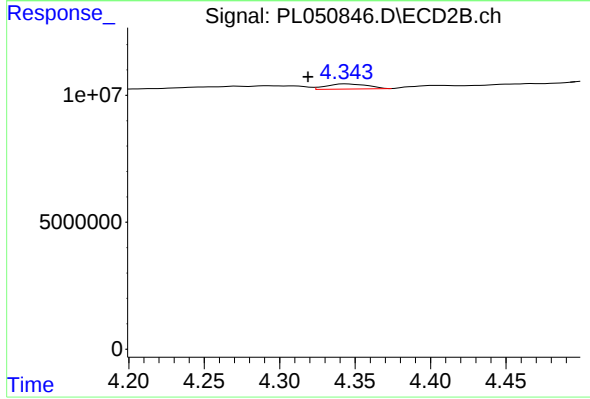

#2 alpha-BHC


R.T.: 4.344 min
Delta R.T.: 0.025 min
Response: 3875912
Conc: 0.94 ng/ml

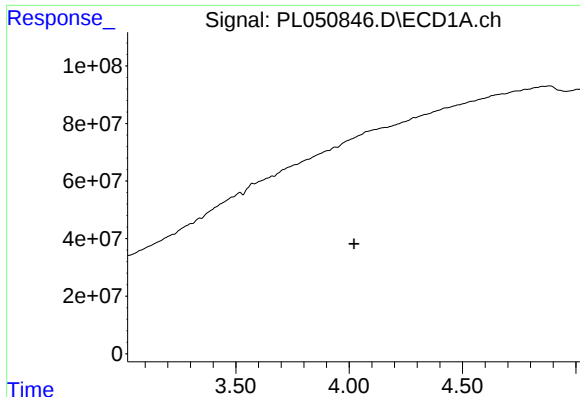

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

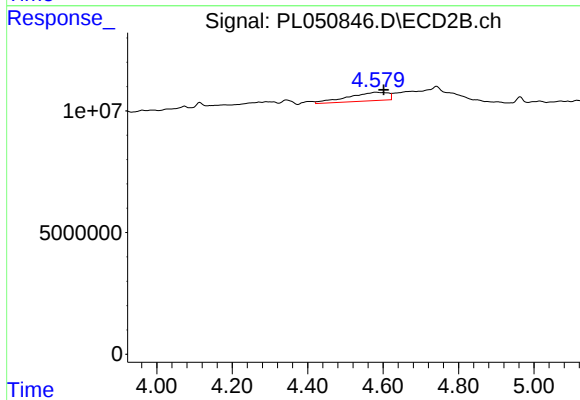


#3 gamma-BHC (Lindane)

R.T.: 4.581 min
Delta R.T.: -0.021 min
Response: 25978251
Conc: 6.71 ng/ml

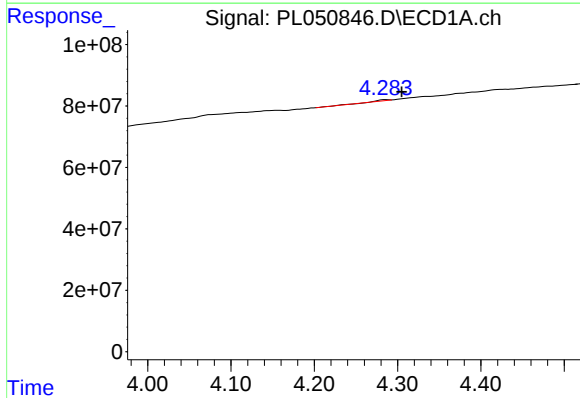


#4 Heptachlor

R.T.: 4.286 min
Delta R.T.: -0.019 min
Response: 1992559
Conc: 0.12 ng/ml

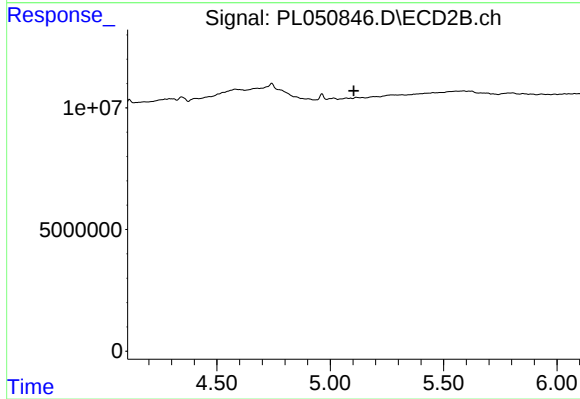

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.104 min
Response: 0
Conc: N.D.

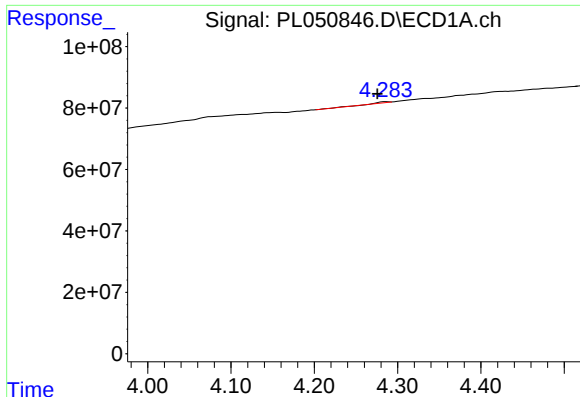

#6 beta-BHC


R.T.: 4.286 min
Delta R.T.: 0.010 min
Response: 1992559
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

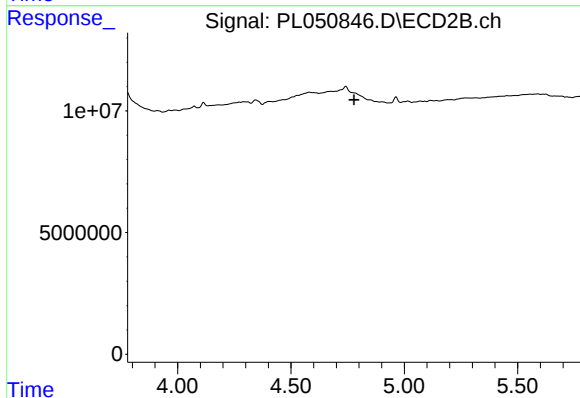


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.778 min
Response: 0
Conc: N.D.

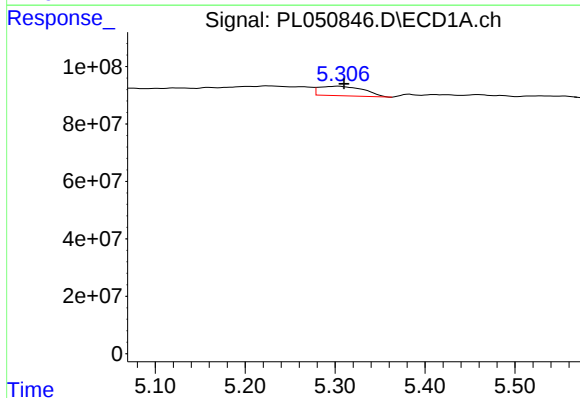


#9 Endosulfan I

R.T.: 5.305 min
Delta R.T.: -0.005 min
Response: 114297258
Conc: 7.86 ng/ml

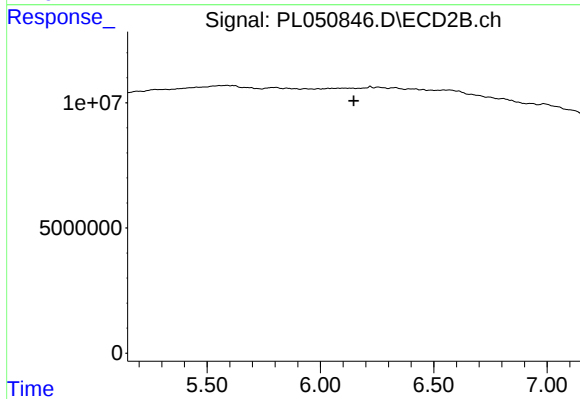

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

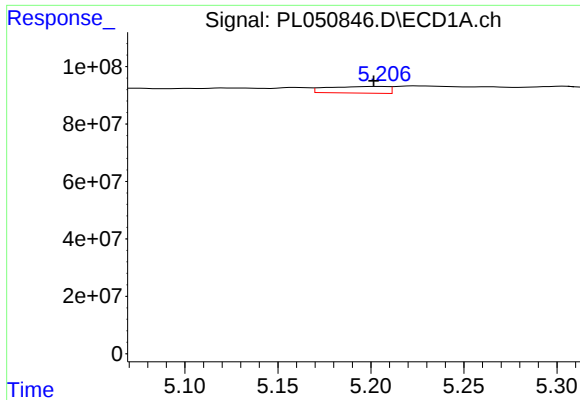

#10 gamma-Chlordane


R.T.: 5.203 min
Delta R.T.: 0.001 min
Response: 52305882
Conc: 3.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

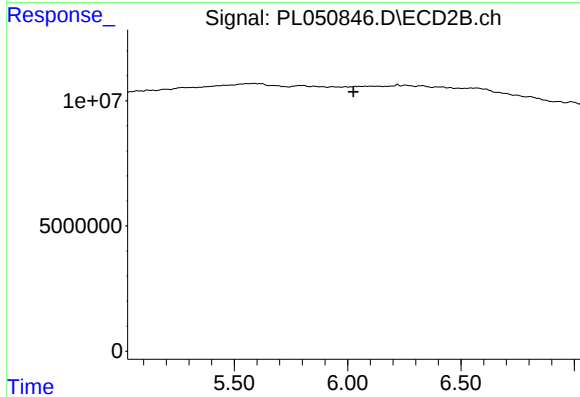


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

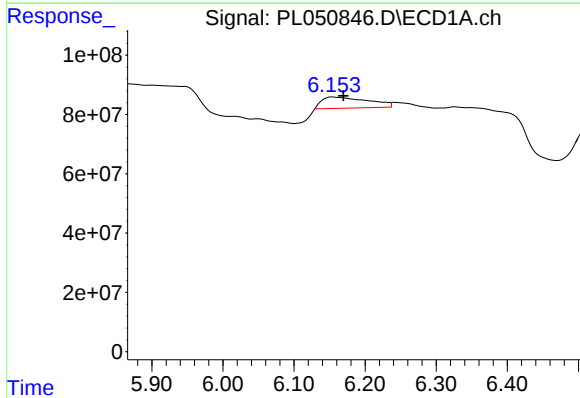


#17 4,4'-DDT

R.T.: 6.154 min
Delta R.T.: -0.016 min
Response: 171187671
Conc: 13.82 ng/ml

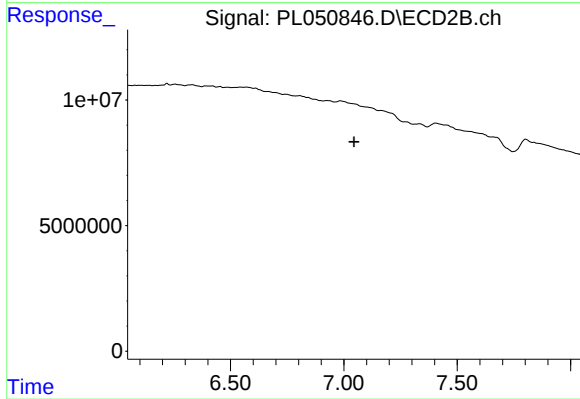

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

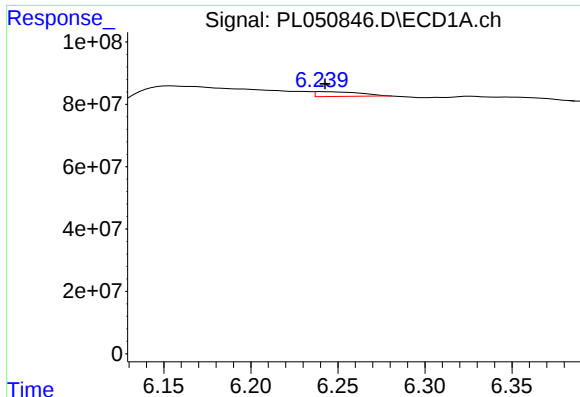

#18 Endrin aldehyde


R.T.: 6.242 min
Delta R.T.: 0.000 min
Response: 27794014
Conc: 2.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

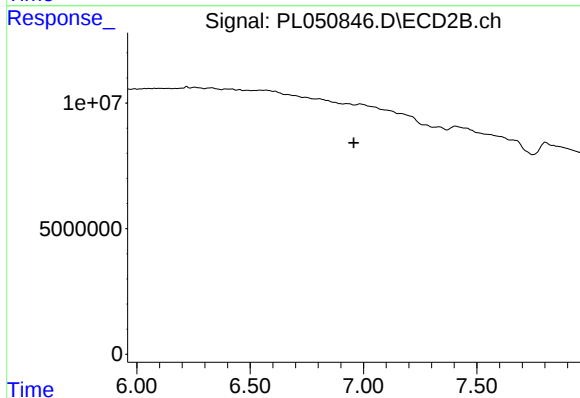


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.957 min
Response: 0
Conc: N.D.

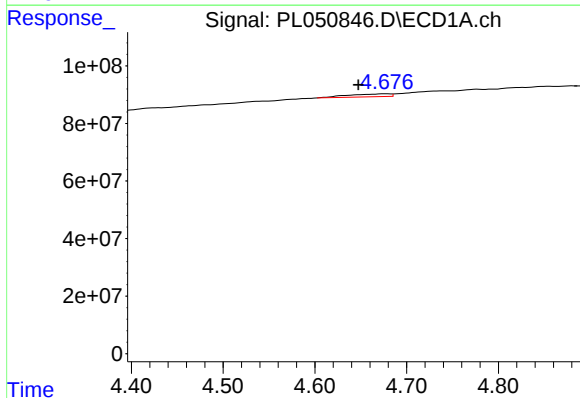


#24 Chlordane-2

R.T.: 4.677 min
Delta R.T.: 0.030 min
Response: 32732968
Conc: 73.13 ng/ml

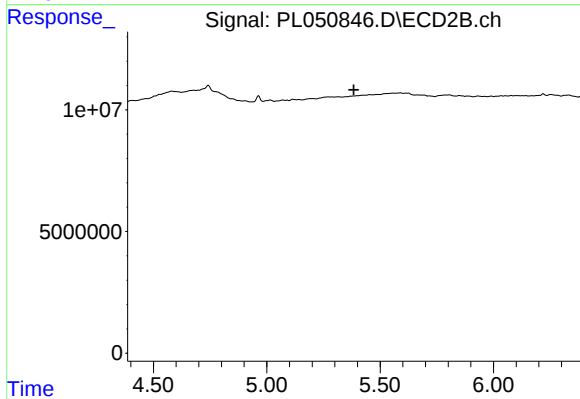

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.383 min
Response: 0
Conc: N.D.

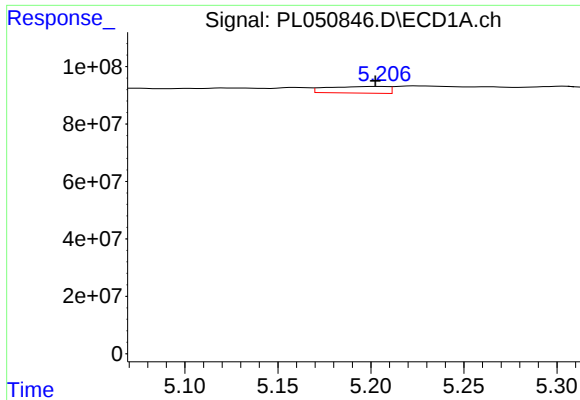

#25 Chlordane-3


R.T.: 5.203 min
Delta R.T.: 0.000 min
Response: 52305882
Conc: 37.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

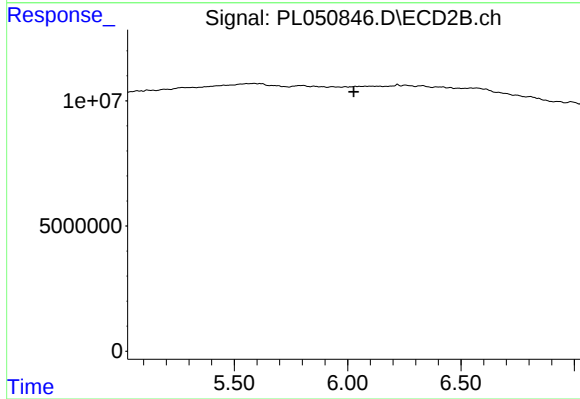


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

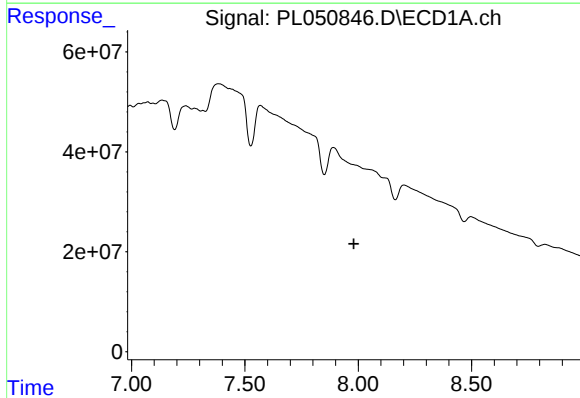

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.981 min
Response: 0
Conc: N.D.

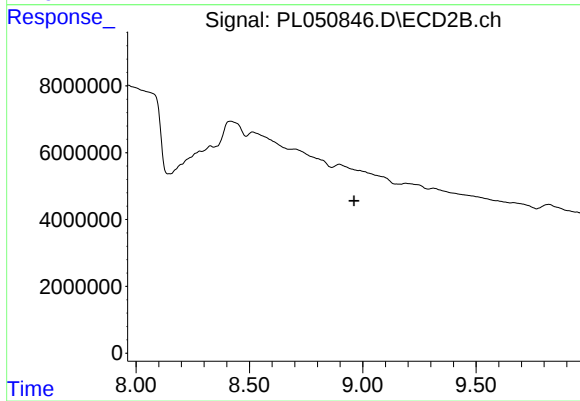

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.