

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072919\
 Data File : PL050858.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 14:53
 Operator : SM\AJ
 Sample : K4024-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 00:43:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.929	137.4E6	36365362	13.674	12.745
28)	SA Decachlor...	7.979	8.959	118.4E6	31748503	11.693	11.227
Target Compounds							
6)	B beta-BHC	0.000	4.797f	0	7981865	N.D.	4.617 #
8)	B Heptachlo...	0.000	5.805	0	4742203	N.D.	1.240 #
10)	B gamma-Chl...	5.221f	6.026	18919538	4515174	1.199	1.222
14)	MA Endrin	5.812	0.000	39927726	0	2.712	N.D. #
23)	Chlordane-1	4.159	0.000	6694196	0	18.193	N.D. #
25)	Chlordane-3	5.221f	6.026	18919538	4515174	13.516	9.387 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072919\
Data File : PL050858.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 14:53
Operator : SM\AJ
Sample : K4024-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 00:43:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

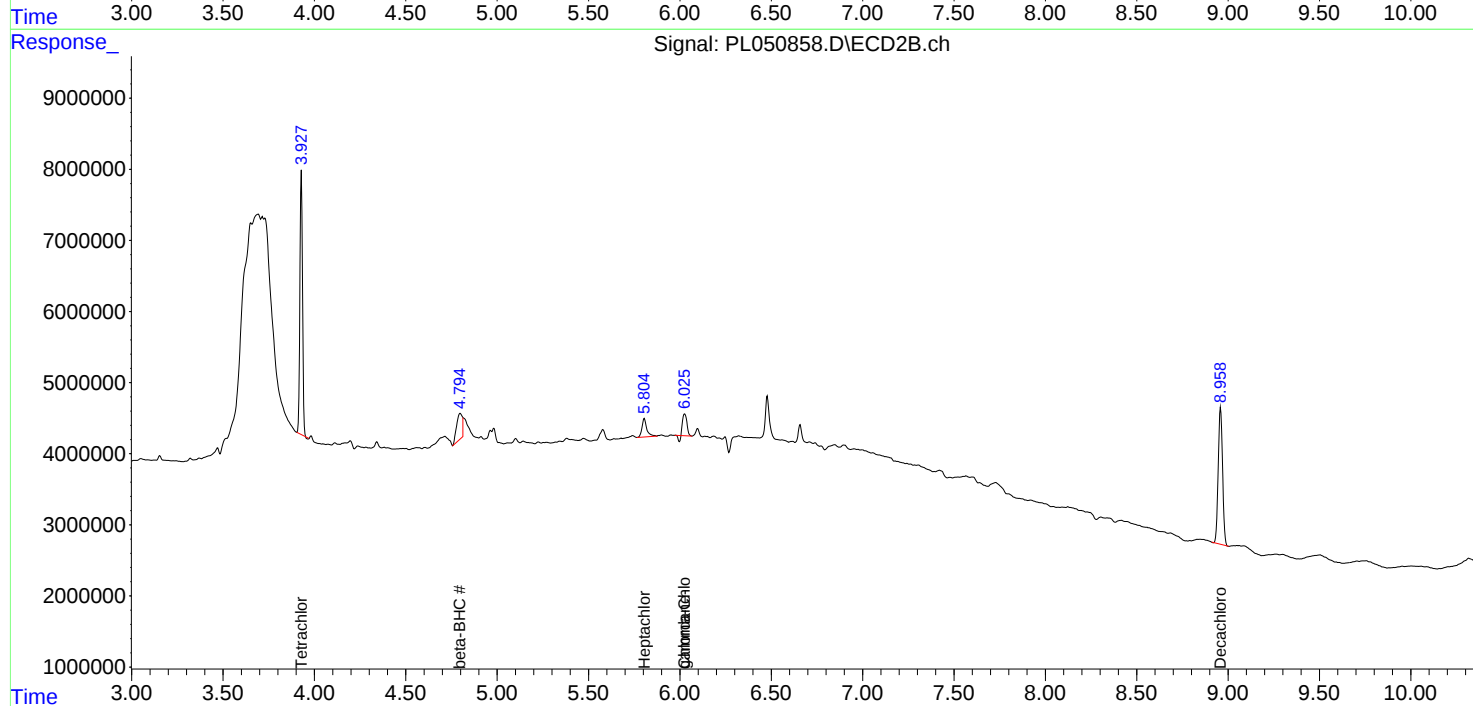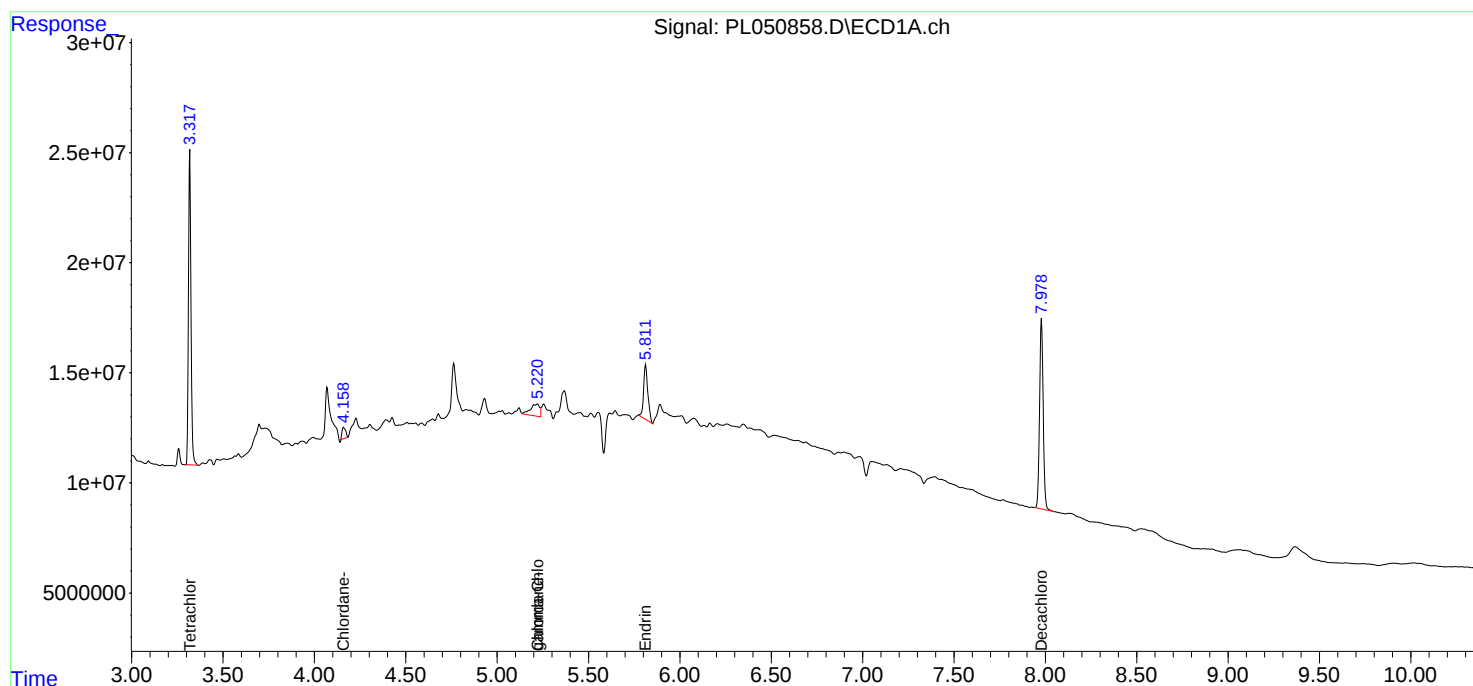


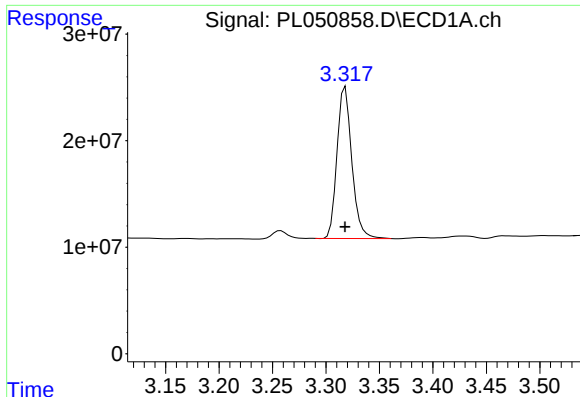

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 137396891
Conc: 13.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

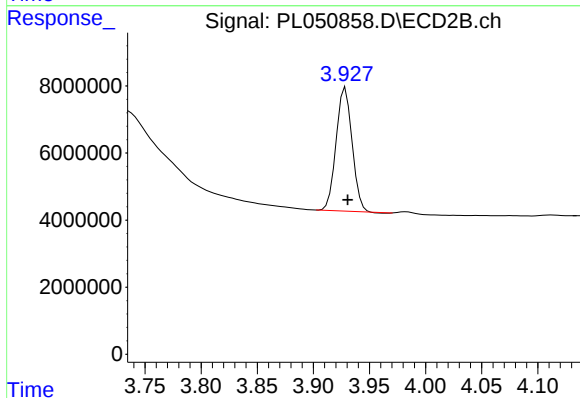


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 36365362
Conc: 12.75 ng/ml

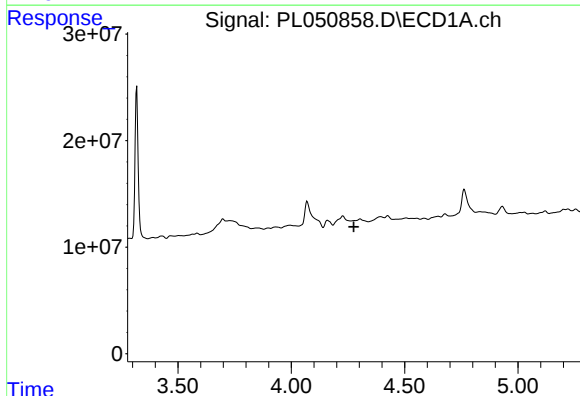


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

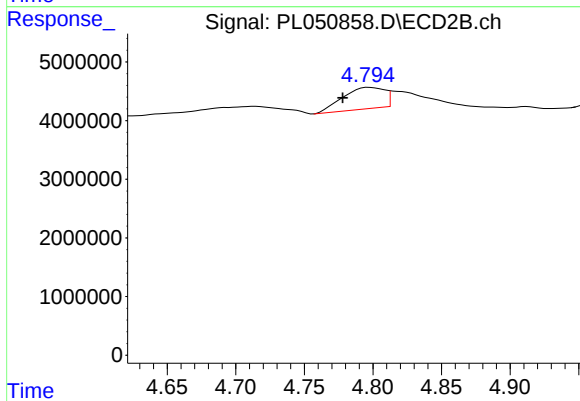

#6 beta-BHC


R.T.: 4.797 min
Delta R.T.: 0.019 min
Response: 7981865
Conc: 4.62 ng/ml

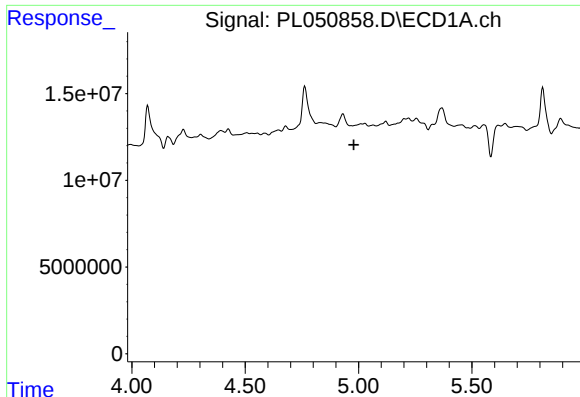

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

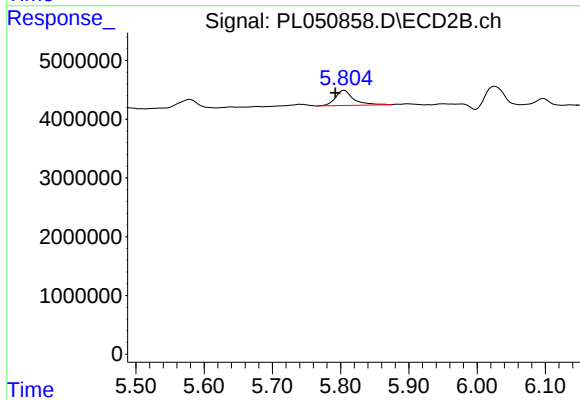


#8 Heptachlor epoxide

R.T.: 5.805 min
Delta R.T.: 0.013 min
Response: 4742203
Conc: 1.24 ng/ml

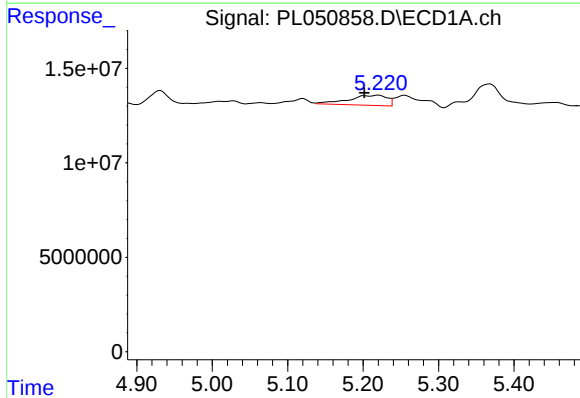


#10 gamma-Chlordane

R.T.: 5.221 min
Delta R.T.: 0.019 min
Response: 18919538
Conc: 1.20 ng/ml

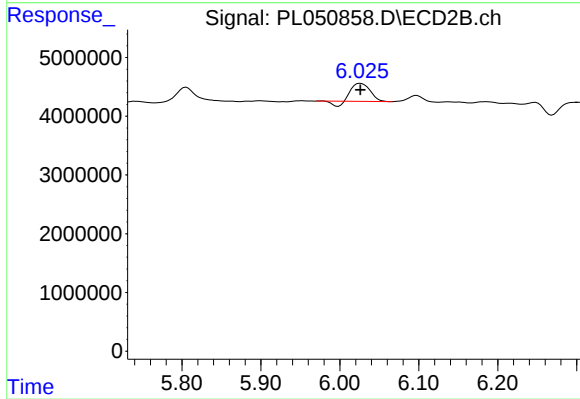

#10 gamma-Chlordane


R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 4515174
Conc: 1.22 ng/ml

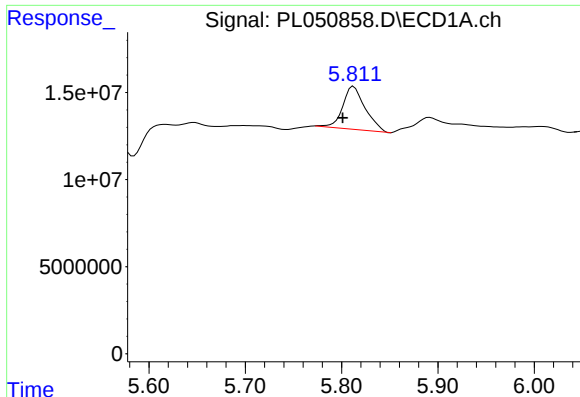

#14 Endrin


R.T.: 5.812 min
Delta R.T.: 0.011 min
Response: 39927726
Conc: 2.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

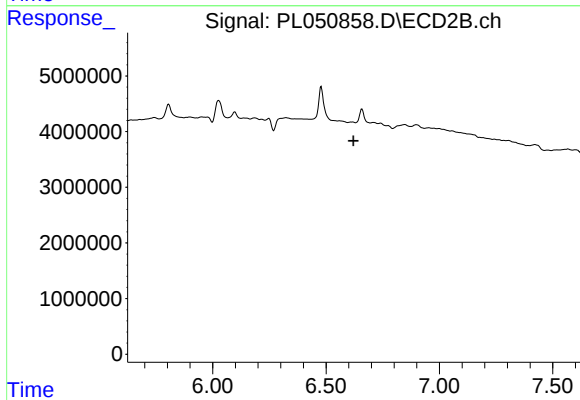


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.621 min
Response: 0
Conc: N.D.

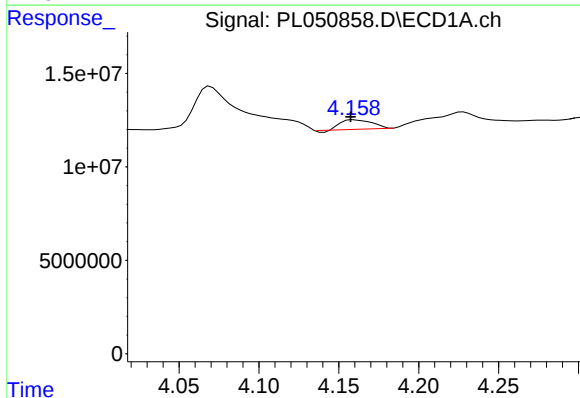


#23 Chlordane-1

R.T.: 4.159 min
Delta R.T.: 0.002 min
Response: 6694196
Conc: 18.19 ng/ml

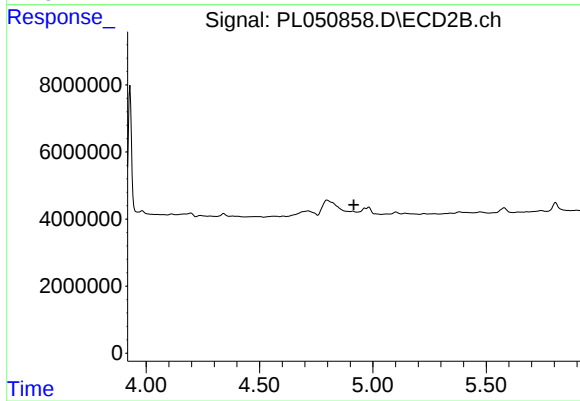

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.916 min
Response: 0
Conc: N.D.

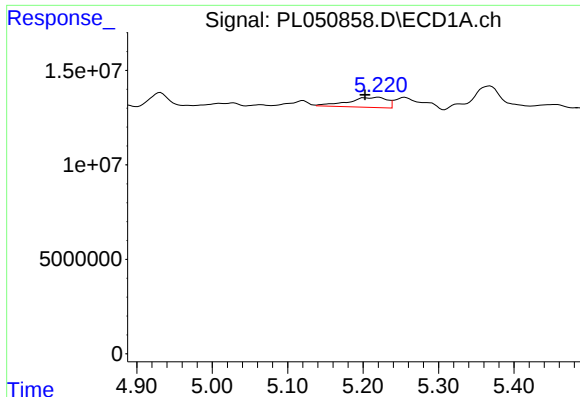

#25 Chlordane-3


R.T.: 5.221 min
Delta R.T.: 0.018 min
Response: 18919538
Conc: 13.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

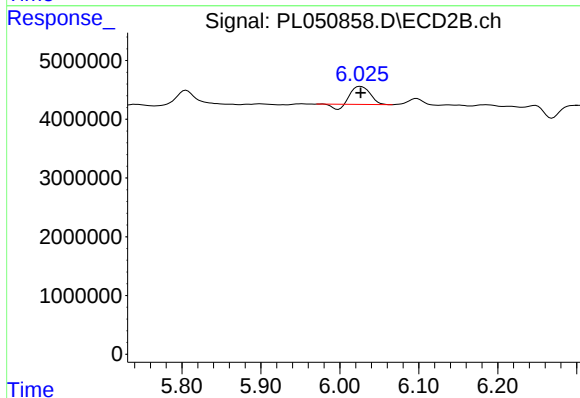


#25 Chlordane-3

R.T.: 6.026 min
Delta R.T.: 0.000 min
Response: 4515174
Conc: 9.39 ng/ml

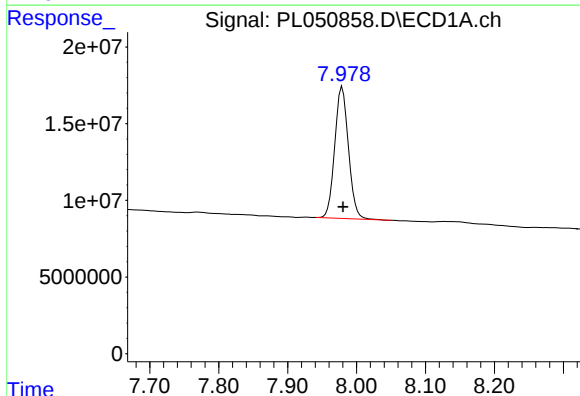

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.001 min
Response: 118396021
Conc: 11.69 ng/ml

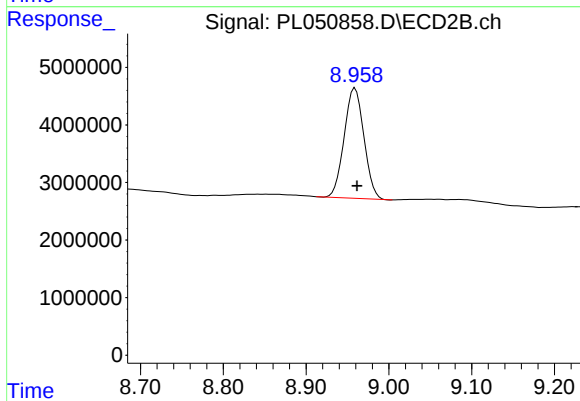

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.002 min
Response: 31748503
Conc: 11.23 ng/ml