

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072919\
 Data File : PL050855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 14:07
 Operator : SM\AJ
 Sample : K4021-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-8-A

Manual Integrations
 APPROVED

Ankita
 7/30/2019 10:02:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 00:42:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	205.1E6	53147348	20.416	18.627
28)	SA Decachlor...	7.979	8.959	175.0E6	45228882	17.286	15.994
Target Compounds							
10)	B gamma-Chl...	5.200	6.022	17640146	4734710	1.118m	1.281
11)	B alpha-Chl...	5.256	6.097	21440464	6215635	1.405m	1.696

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072919\
Data File : PL050855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 14:07
Operator : SM\AJ
Sample : K4021-13
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-8-A


Manual Integrations
APPROVED

Ankita
7/30/2019 10:02:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 00:42:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

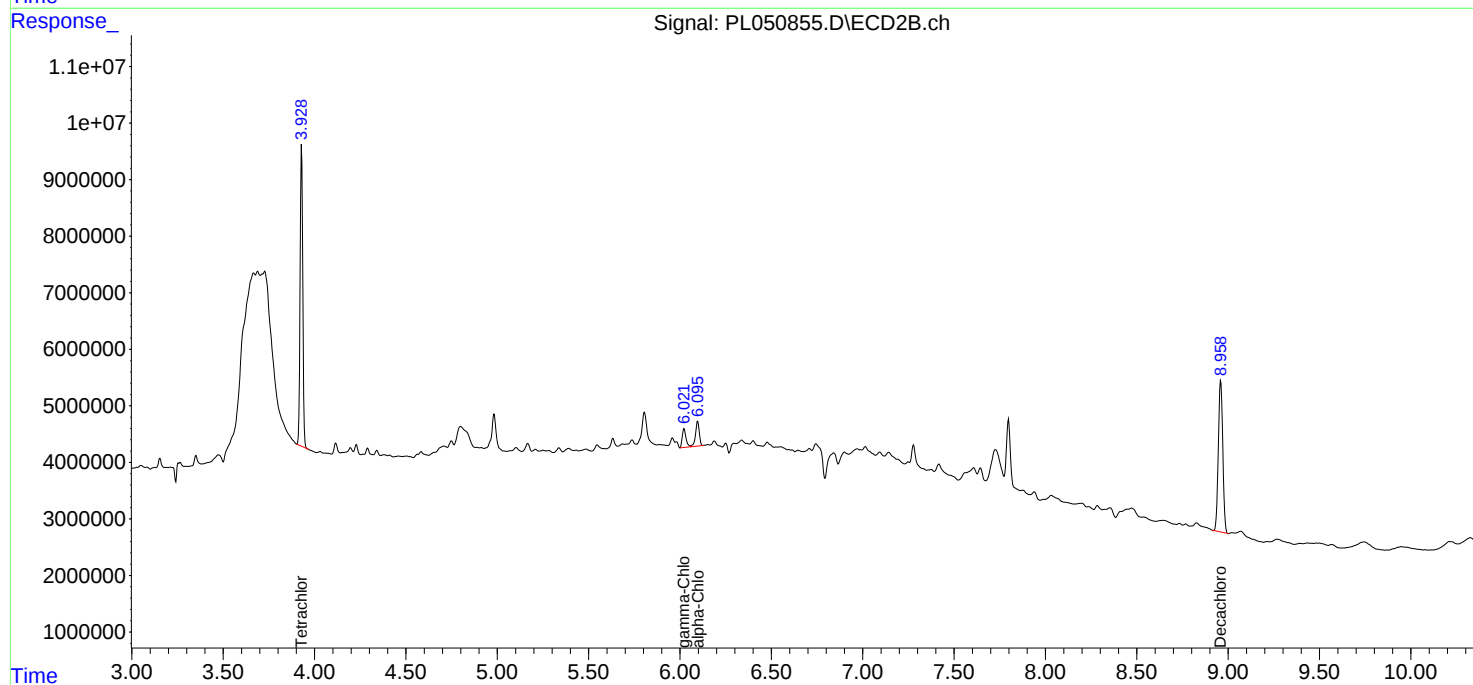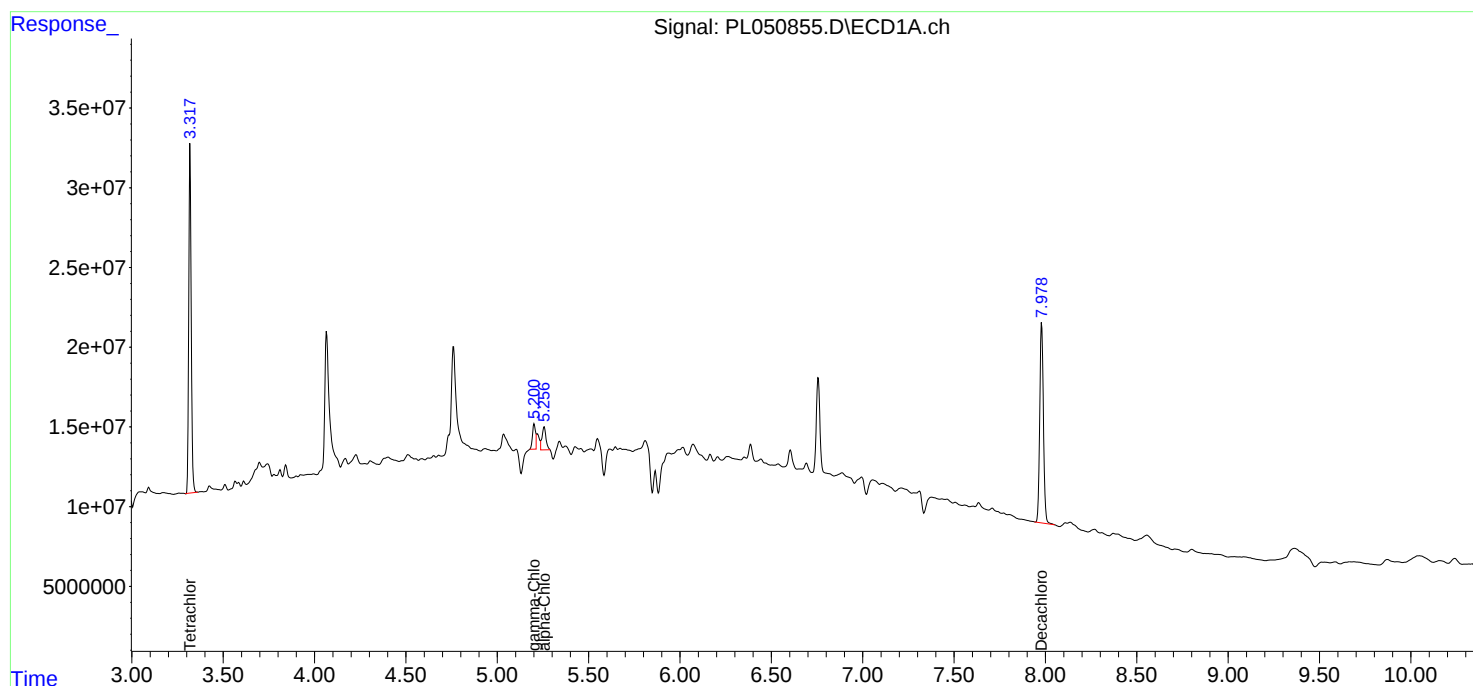

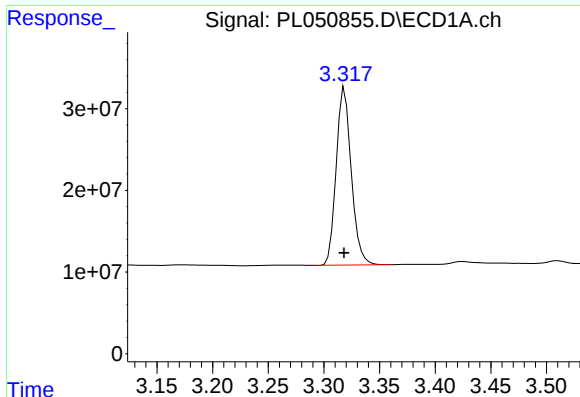


#1 Tetrachloro-m-xylene

R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 205141114
Conc: 20.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8-A


Manual Integrations
APPROVED

Ankita
7/30/2019 10:02:53 AM

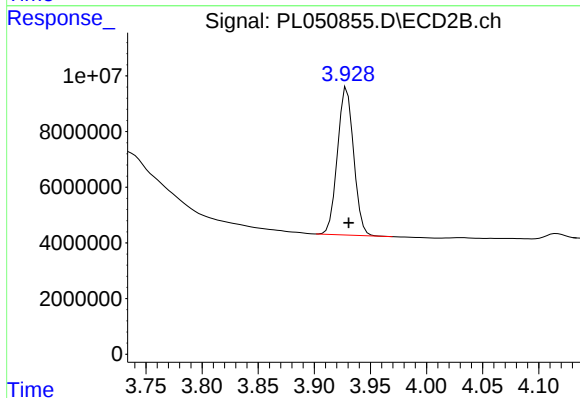


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.001 min
Response: 53147348
Conc: 18.63 ng/ml

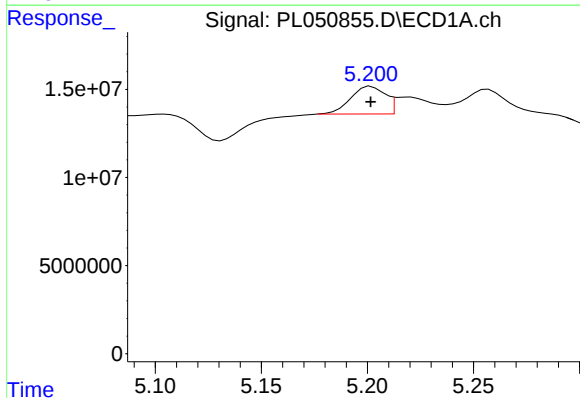


#10 gamma-Chlordane

R.T.: 5.200 min
Delta R.T.: -0.001 min
Response: 17640146
Conc: 1.12 ng/ml m

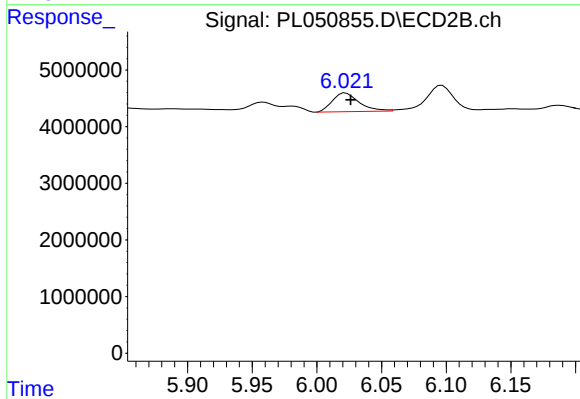

#10 gamma-Chlordane

R.T.: 6.022 min
Delta R.T.: -0.004 min
Response: 4734710
Conc: 1.28 ng/ml

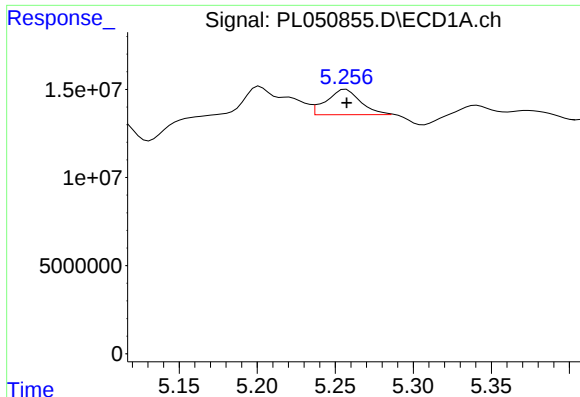


#11 alpha-Chlordane

R.T.: 5.256 min
Delta R.T.: -0.002 min
Response: 21440464
Conc: 1.41 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-8-A


Manual Integrations
APPROVED

Ankita
7/30/2019 10:02:53 AM

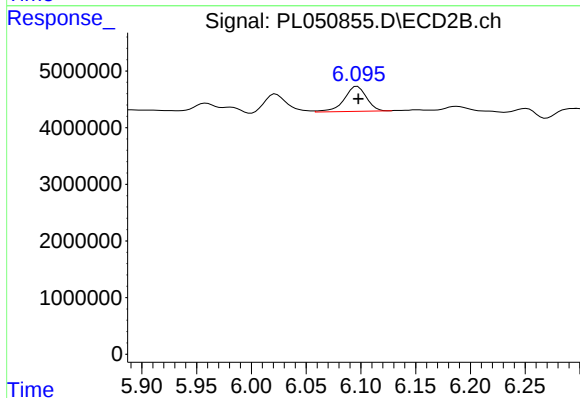


#11 alpha-Chlordane

R.T.: 6.097 min
Delta R.T.: -0.001 min
Response: 6215635
Conc: 1.70 ng/ml

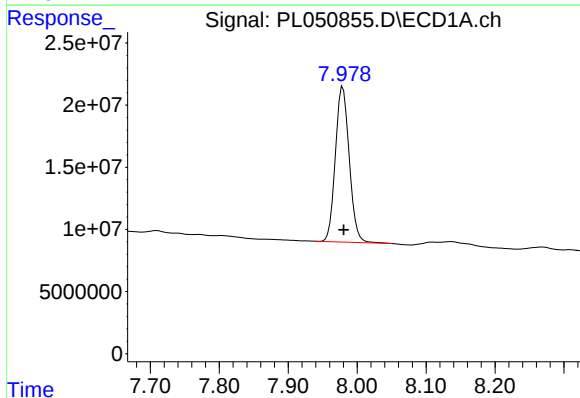

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.001 min
Response: 175023277
Conc: 17.29 ng/ml

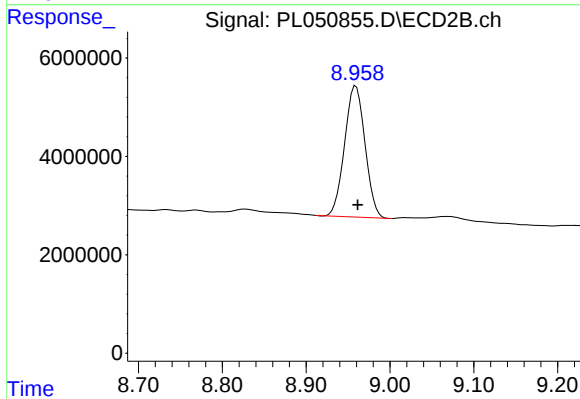

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.002 min
Response: 45228882
Conc: 15.99 ng/ml