

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072919\
 Data File : PL050859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2019 15:08
 Operator : SM\AJ
 Sample : K4024-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6-A

Manual Integrations
 APPROVED

Ankita
 7/30/2019 10:03:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 00:43:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.929	138.5E6	36770713	13.789	12.888
28)	SA Decachlor...	7.979	8.959	122.0E6	32540985	12.050	11.507
Target Compounds							
10)	B gamma-Chl...	5.201	6.023	4021677	954629	0.255m	0.258m
11)	B alpha-Chl...	5.254	6.095	4499270	1891547	0.295m	0.516m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072919\
Data File : PL050859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2019 15:08
Operator : SM\AJ
Sample : K4024-05
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-6-A


Manual Integrations
APPROVED

Ankita
7/30/2019 10:03:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 00:43:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

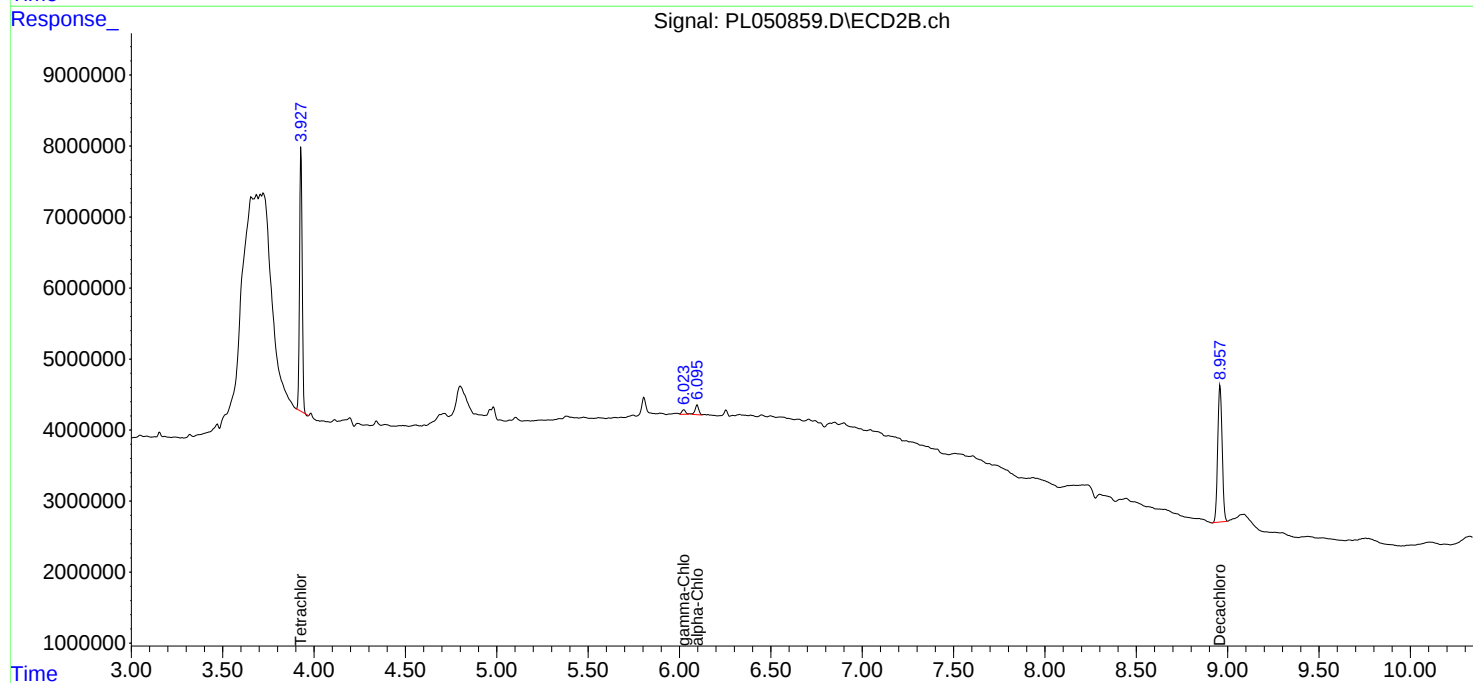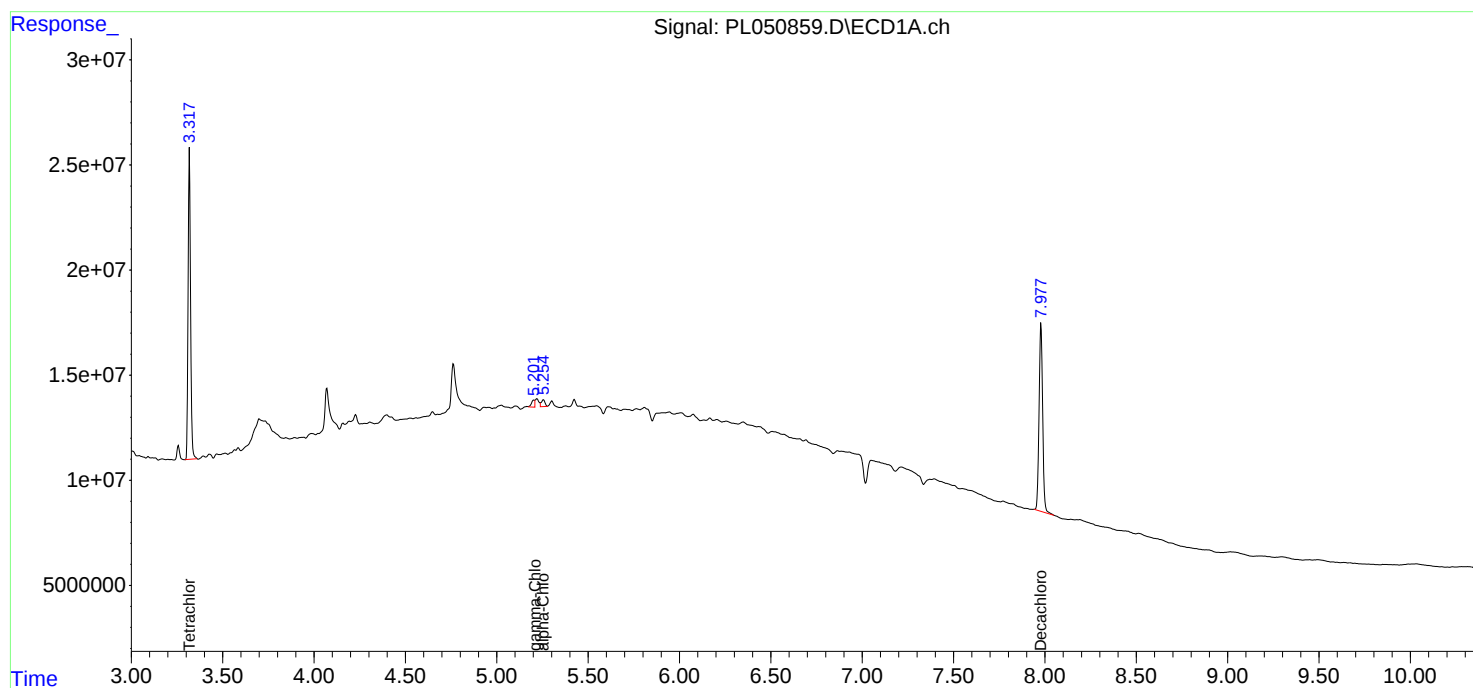

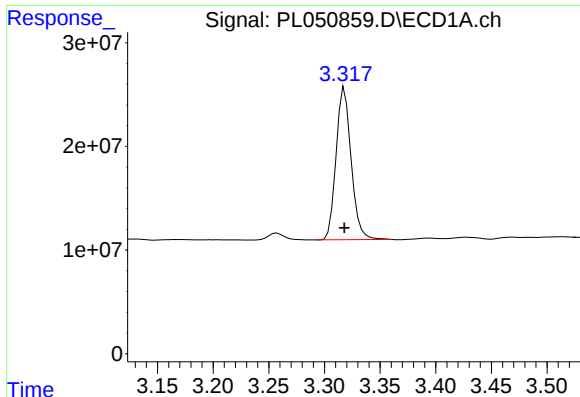


#1 Tetrachloro-m-xylene

R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 138549416
Conc: 13.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-A


Manual Integrations
APPROVED

Ankita
7/30/2019 10:03:01 AM

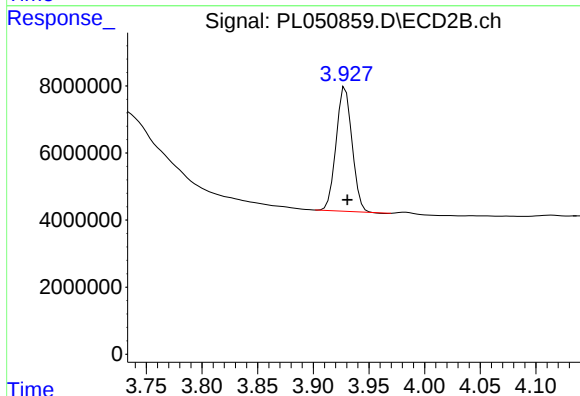


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 36770713
Conc: 12.89 ng/ml

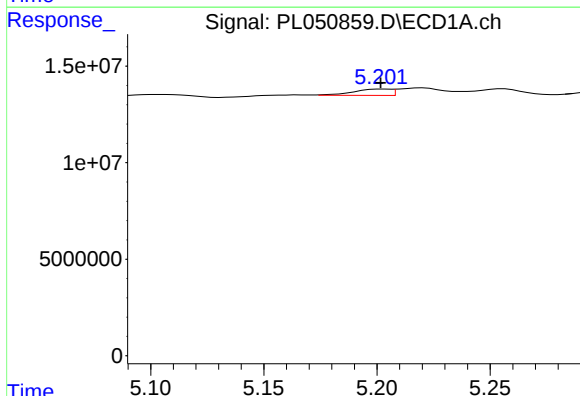


#10 gamma-Chlordane

R.T.: 5.201 min
Delta R.T.: 0.000 min
Response: 4021677
Conc: 0.25 ng/ml m

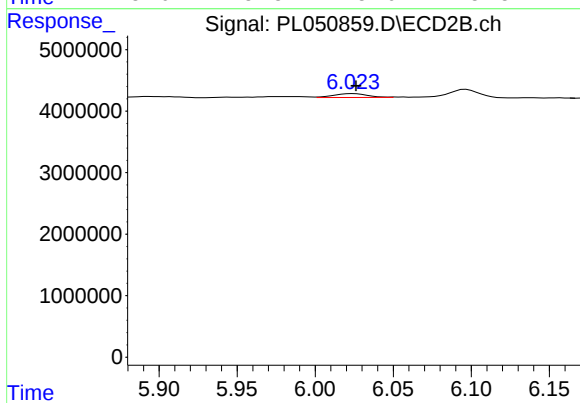

#10 gamma-Chlordane

R.T.: 6.023 min
Delta R.T.: -0.004 min
Response: 954629
Conc: 0.26 ng/ml m

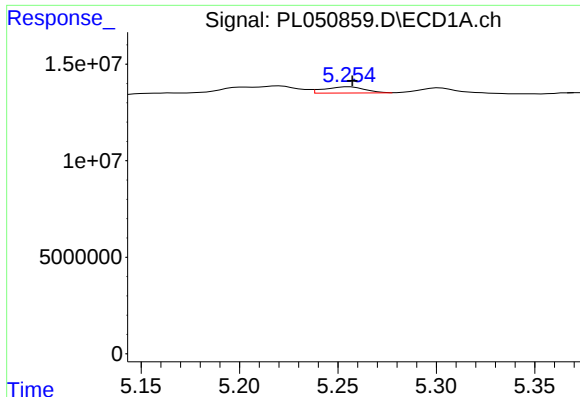


#11 alpha-Chlordane

R.T.: 5.254 min
Delta R.T.: -0.003 min
Response: 4499270
Conc: 0.29 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-6-A


Manual Integrations
APPROVED

Ankita
7/30/2019 10:03:01 AM

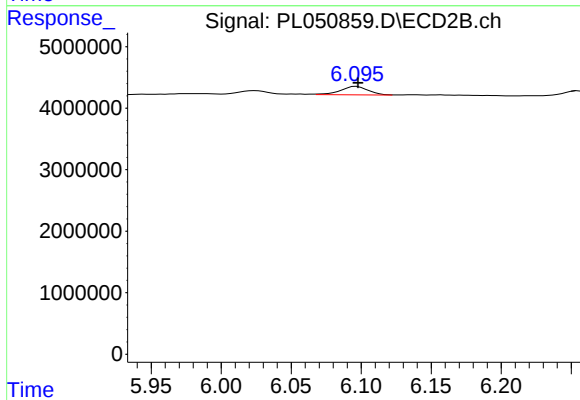


#11 alpha-Chlordane

R.T.: 6.095 min
Delta R.T.: -0.003 min
Response: 1891547
Conc: 0.52 ng/ml m

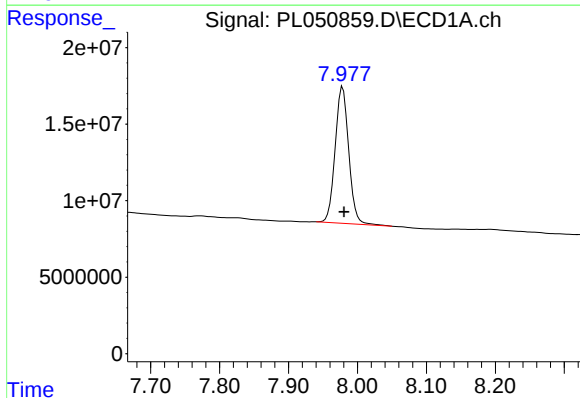

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 122008224
Conc: 12.05 ng/ml

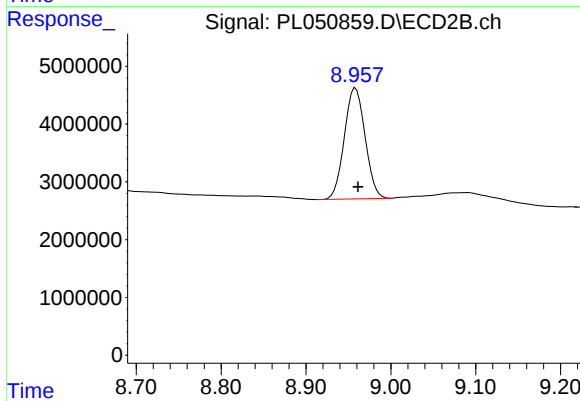

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.003 min
Response: 32540985
Conc: 11.51 ng/ml