

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072921\
 Data File : PL068560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2021 16:48
 Operator : AR\AJ
 Sample : PB138064TB
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB138064TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:22:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.570	9658104	21587693	22.503	21.156
28)	SA Decachlor...	10.417	11.491	12327179	19709648	21.918	22.096
Target Compounds							
9)	A Endosulfan I	0.000	8.446	0	34954	N.D.	0.034 #
11)	B alpha-Chl...	0.000	8.385	0	2656	N.D.	0.002 #
13)	MA Dieldrin	0.000	8.729	0	147977	N.D.	0.140 #
15)	B Endosulfa...	0.000	9.218f	0	624424	N.D.	0.689 #
17)	MA 4,4'-DDT	0.000	9.446f	0	14945	N.D.	0.016 #
19)	B Endosulfa...	0.000	9.568	0	68147	N.D.	0.076 #
23)	Chlordane-1	0.000	6.983f	0	123985	N.D.	3.061 #
26)	Chlordane-4	0.000	8.385	0	2656	N.D.	0.014 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072921\
Data File : PL068560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2021 16:48
Operator : AR\AJ
Sample : PB138064TB
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PB138064TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:22:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

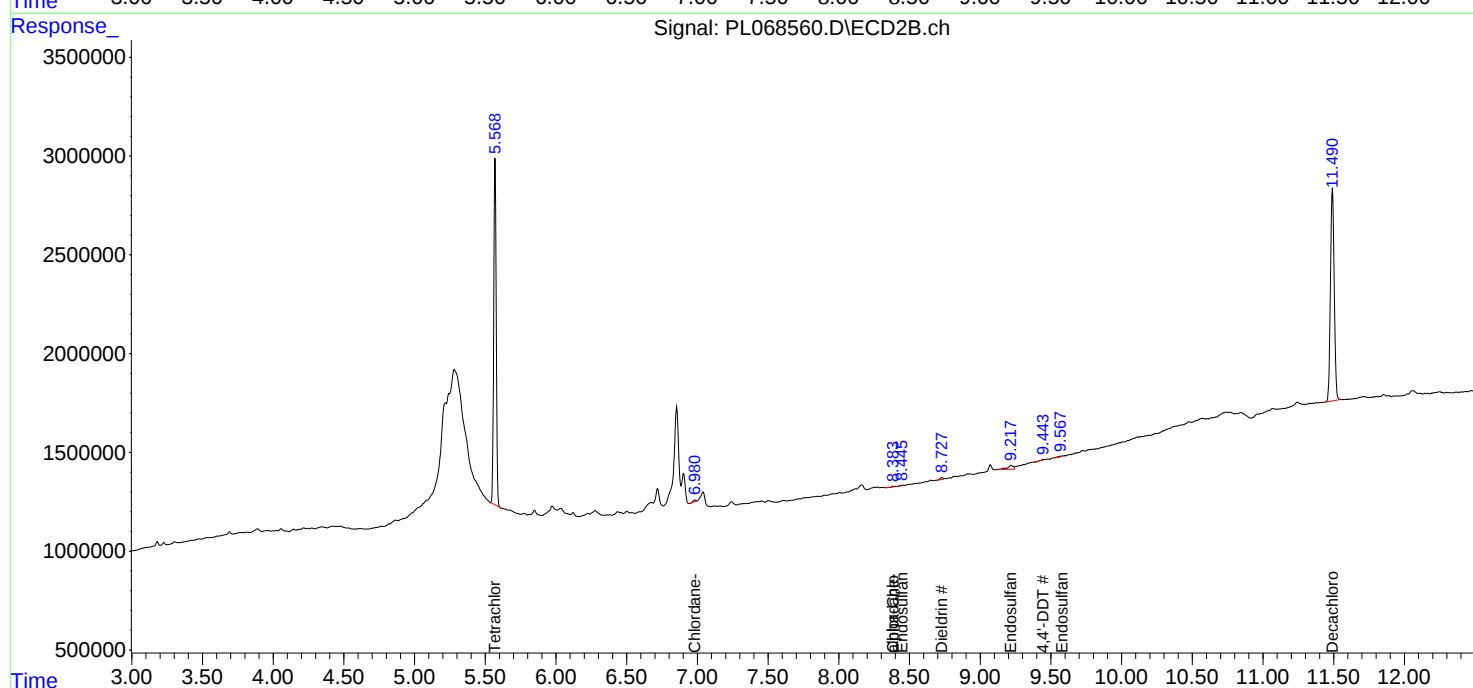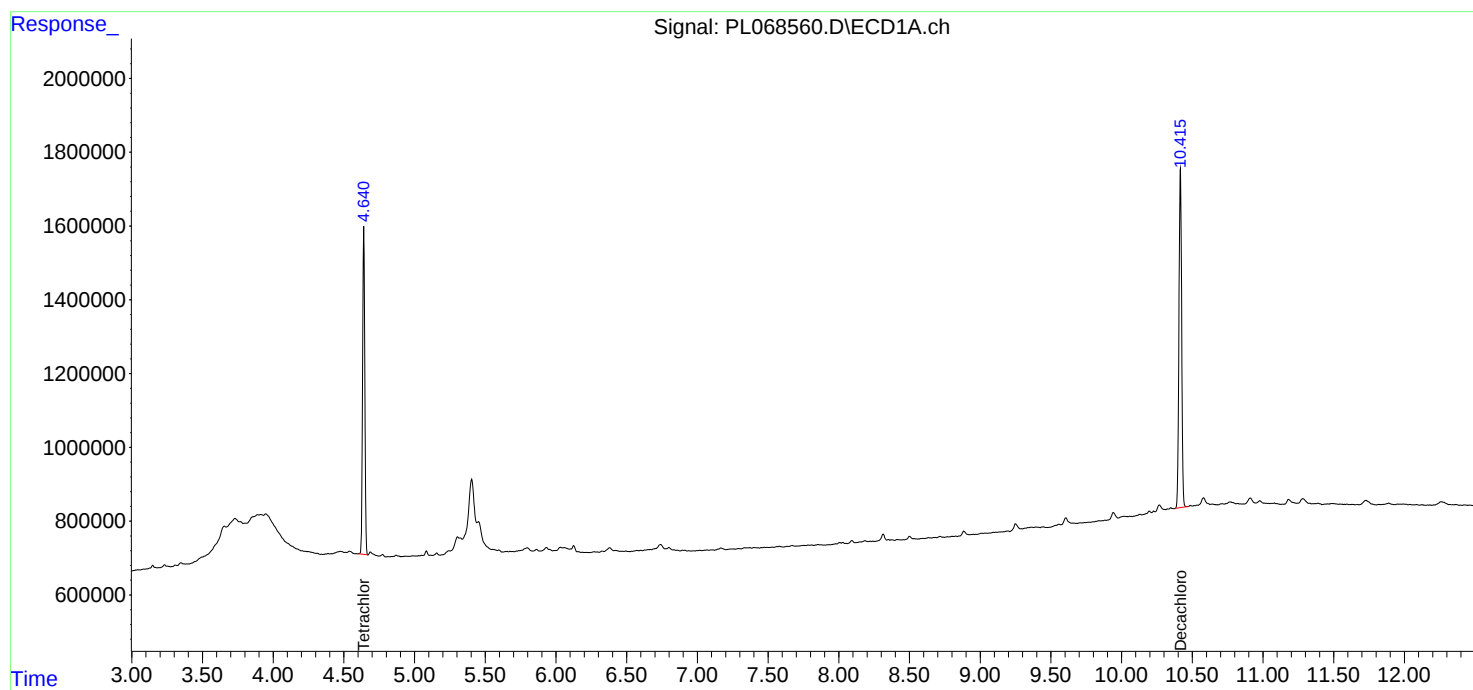


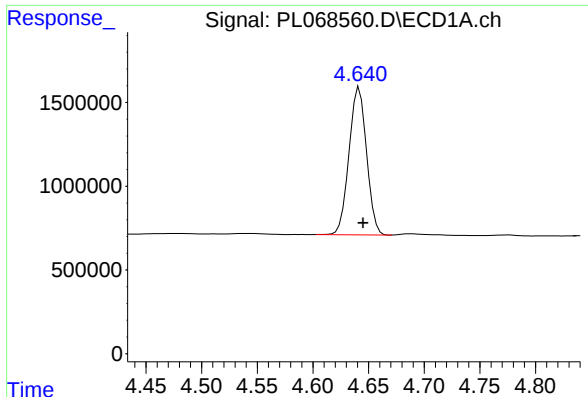

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.003 min
Response: 9658104
Conc: 22.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138064TB

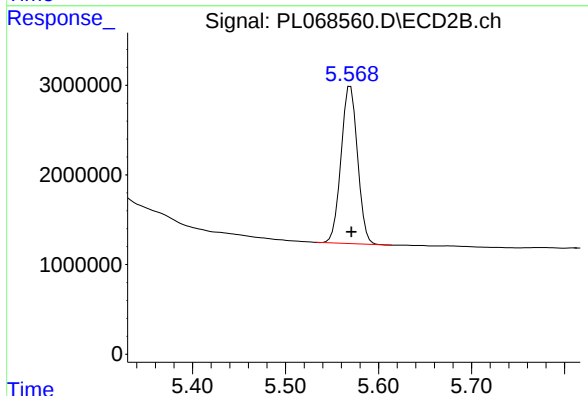


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 21587693
Conc: 21.16 ng/ml

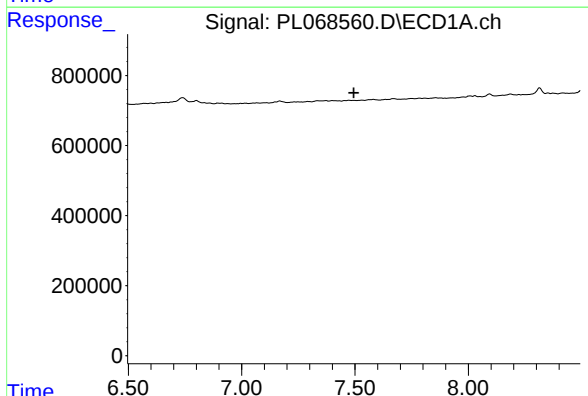


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.494 min
Response: 0
Conc: N.D.

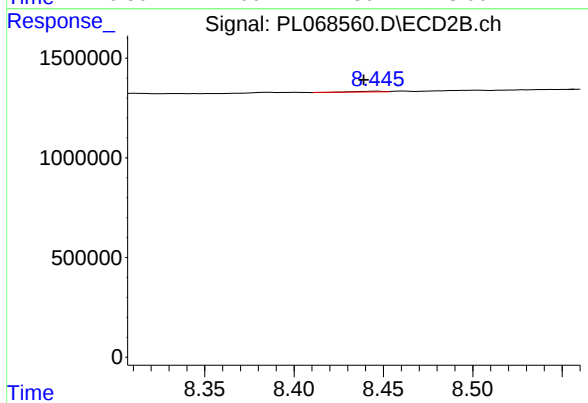

#9 Endosulfan I


R.T.: 8.446 min
Delta R.T.: 0.007 min
Response: 34954
Conc: 0.03 ng/ml

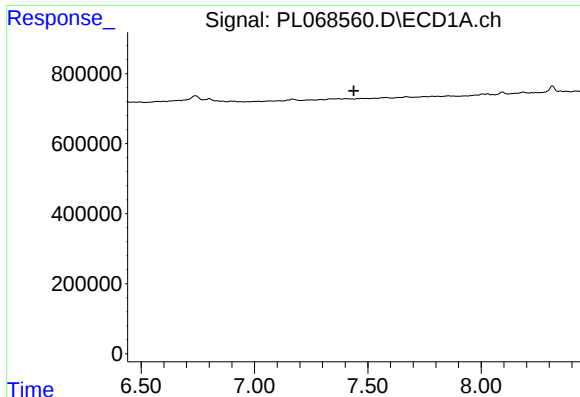

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138064TB

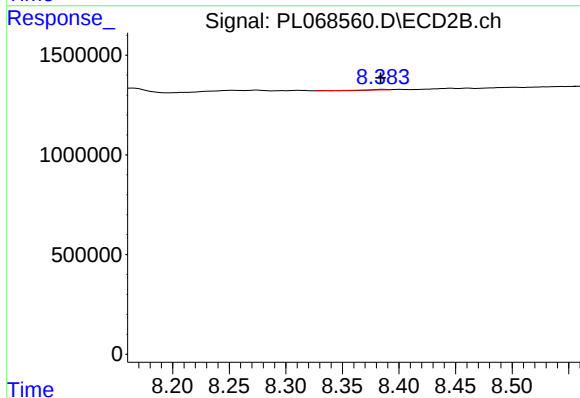


#11 alpha-Chlordane

R.T.: 8.385 min
Delta R.T.: 0.001 min
Response: 2656
Conc: 0.00 ng/ml

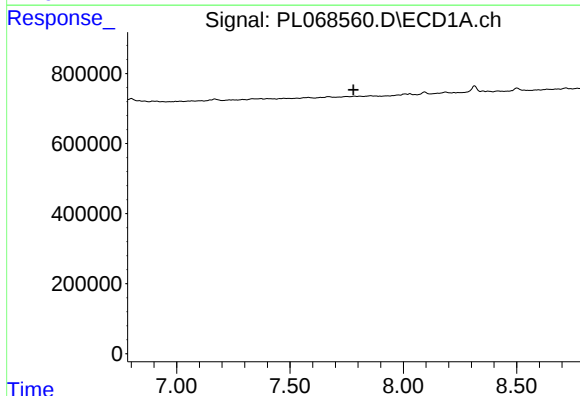


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.781 min
Response: 0
Conc: N.D.

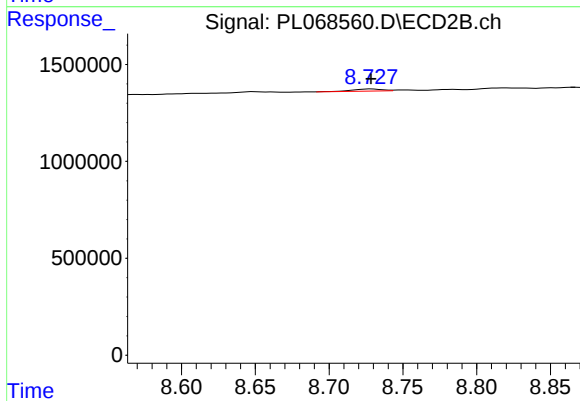

#13 Dieldrin


R.T.: 8.729 min
Delta R.T.: 0.000 min
Response: 147977
Conc: 0.14 ng/ml

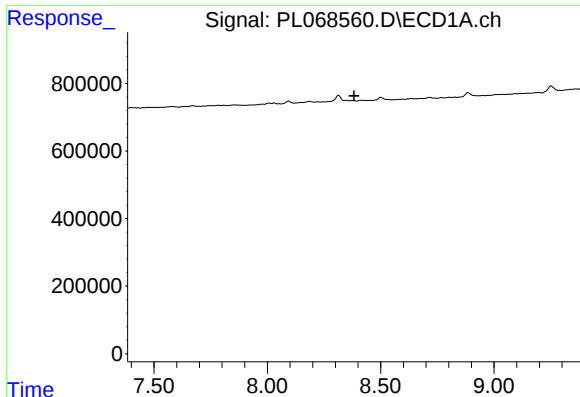

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138064TB

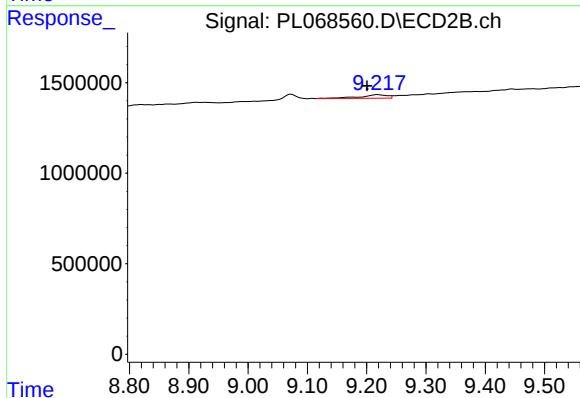


#15 Endosulfan II

R.T.: 9.218 min
Delta R.T.: 0.017 min
Response: 624424
Conc: 0.69 ng/ml

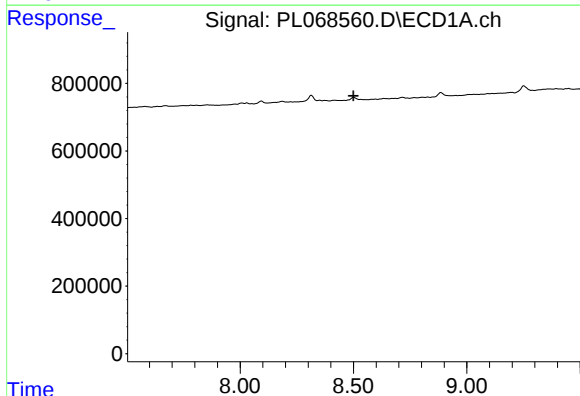


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.501 min
Response: 0
Conc: N.D.

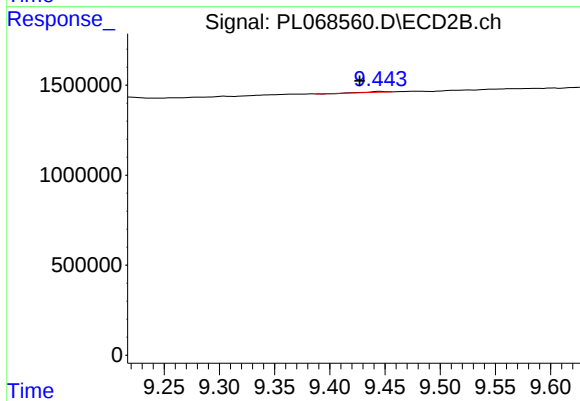

#17 4,4'-DDT


R.T.: 9.446 min
Delta R.T.: 0.018 min
Response: 14945
Conc: 0.02 ng/ml

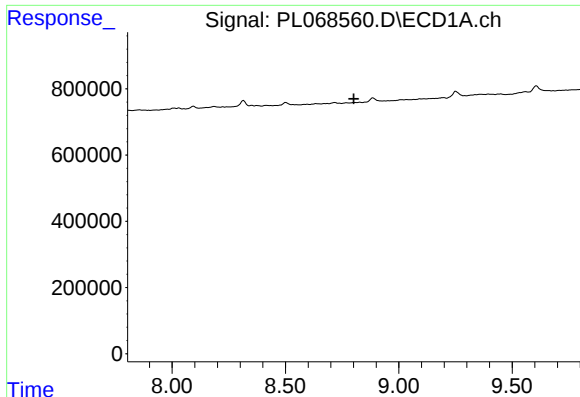

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138064TB

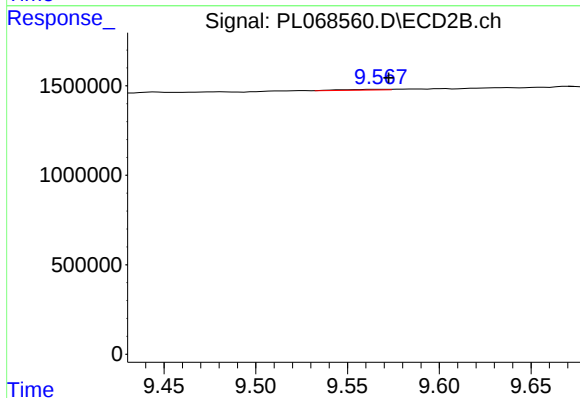


#19 Endosulfan Sulfate

R.T.: 9.568 min
Delta R.T.: -0.004 min
Response: 68147
Conc: 0.08 ng/ml

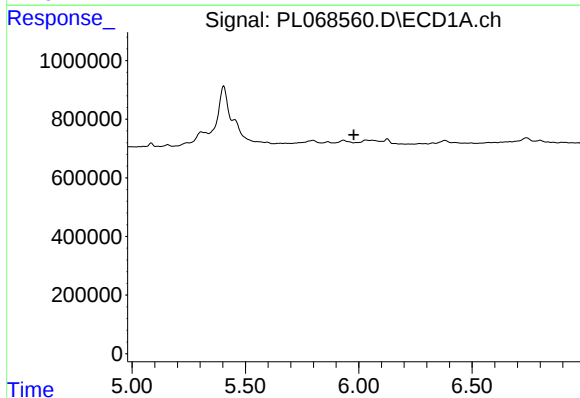


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

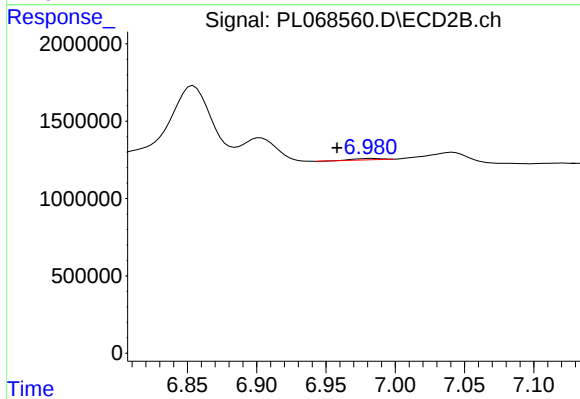

#23 Chlordane-1


R.T.: 6.983 min
Delta R.T.: 0.025 min
Response: 123985
Conc: 3.06 ng/ml

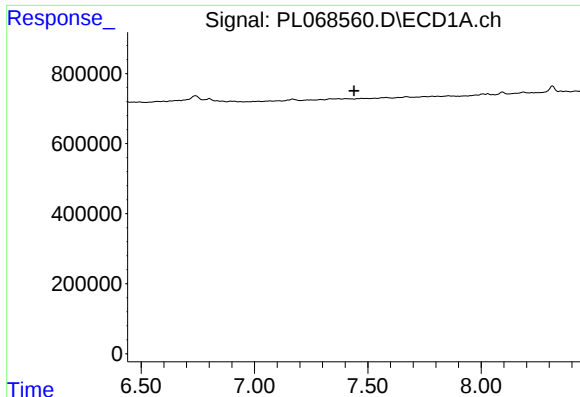

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138064TB

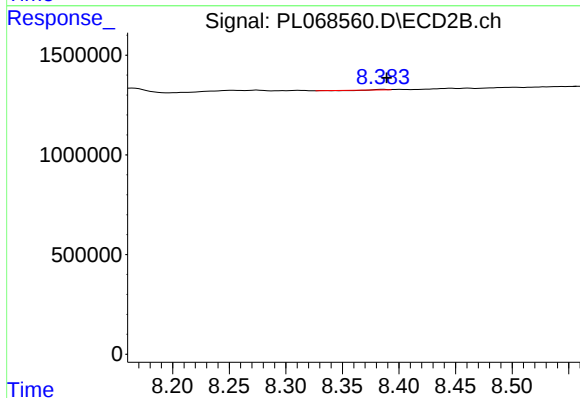


#26 Chlordane-4

R.T.: 8.385 min
Delta R.T.: -0.004 min
Response: 2656
Conc: 0.01 ng/ml

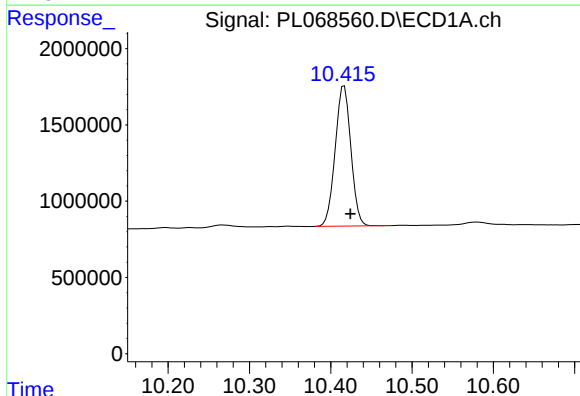

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.008 min
Response: 12327179
Conc: 21.92 ng/ml

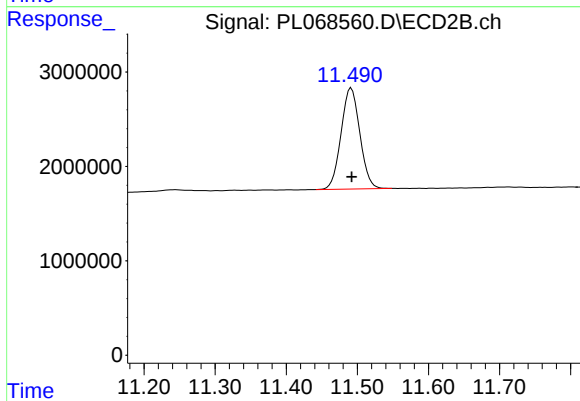

#28 Decachlorobiphenyl

R.T.: 11.491 min
Delta R.T.: 0.000 min
Response: 19709648
Conc: 22.10 ng/ml