

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072921\
 Data File : PL068561.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2021 17:05
 Operator : AR\AJ
 Sample : PB138070BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB138070BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:22:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.570	9208898	20471694	21.457	20.062
28)	SA Decachlor...	10.415	11.493	11863091	18812388	21.093	21.090
Target Compounds							
8)	B Heptachlo...	0.000	8.038	0	1387324	N.D.	1.227 #
9)	A Endosulfan I	0.000	8.447	0	8003	N.D.	0.008 #
13)	MA Dieldrin	7.782	8.725	-11228	293023	N.D.	0.276
14)	MA Endrin	8.088f	8.963	873140	1071232	1.746	1.198 #
15)	B Endosulfa...	0.000	9.217f	0	1253350	N.D.	1.383 #
17)	MA 4,4'-DDT	0.000	9.445f	0	157926	N.D.	0.167 #
18)	B Endrin al...	0.000	9.350	0	110250	N.D.	0.153 #
23)	Chlordane-1	0.000	6.977f	0	232771	N.D.	5.746 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072921\
Data File : PL068561.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2021 17:05
Operator : AR\AJ
Sample : PB138070BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PB138070BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:22:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

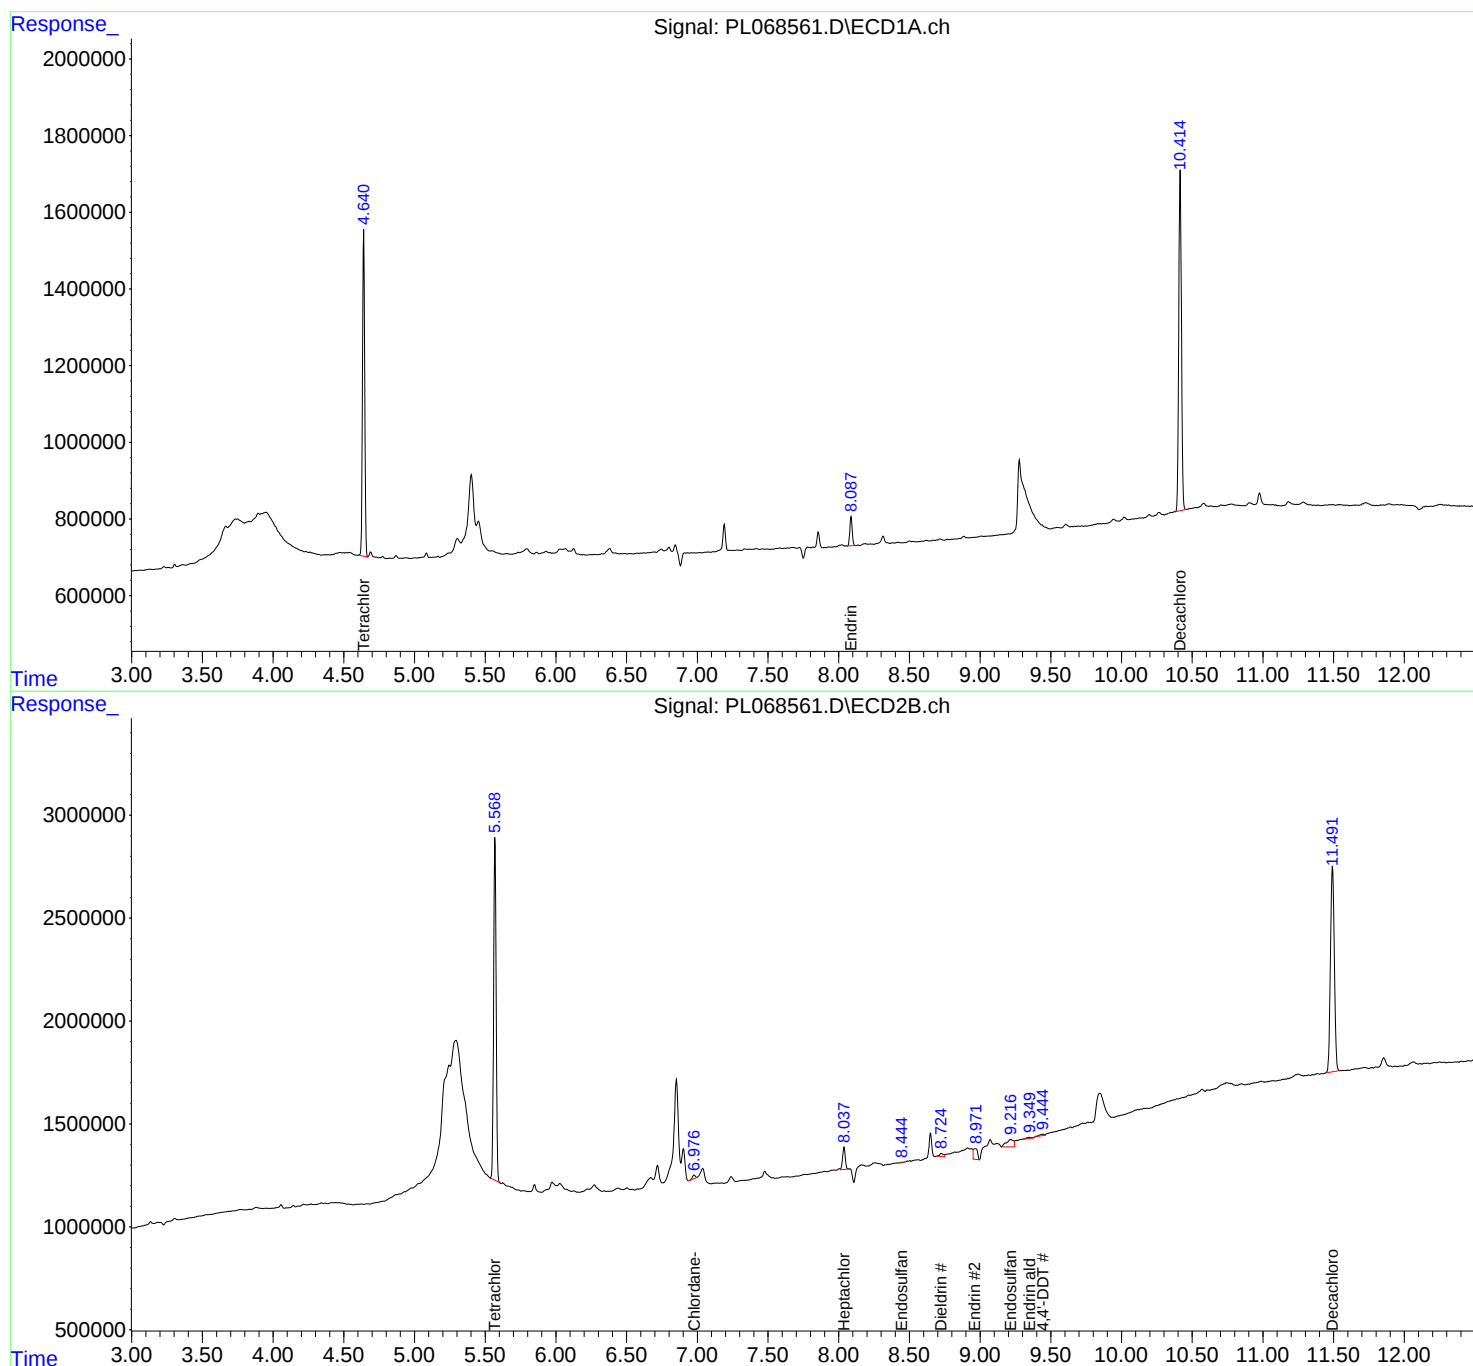


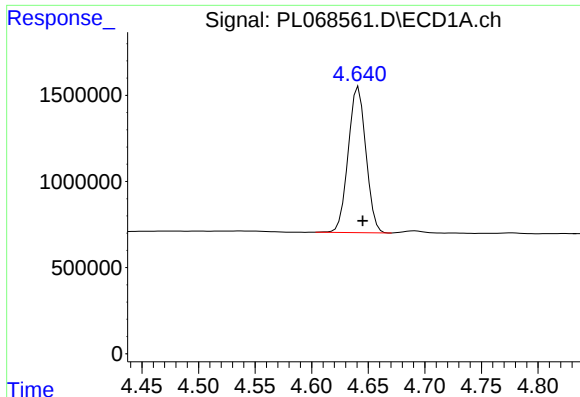

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.004 min
Response: 9208898
Conc: 21.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138070BL

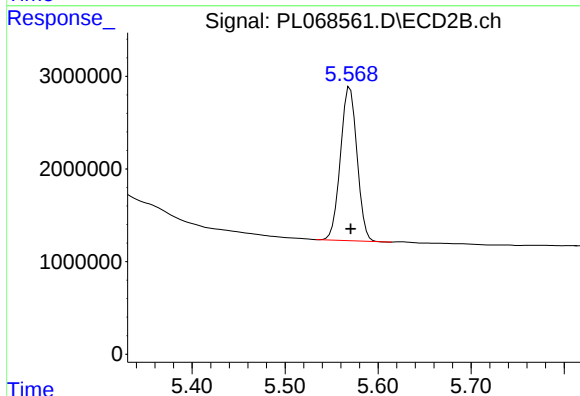


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 20471694
Conc: 20.06 ng/ml

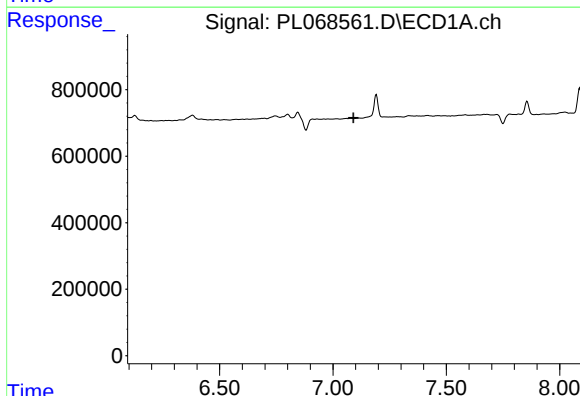


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

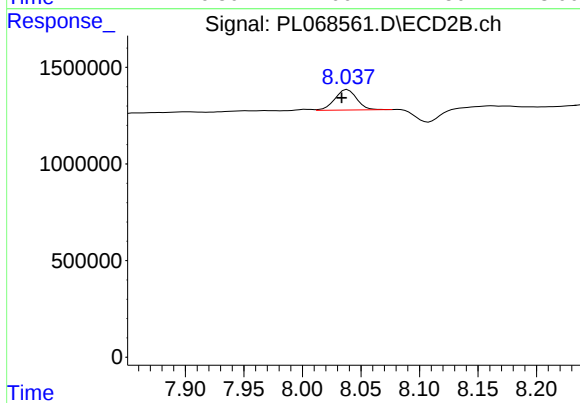

#8 Heptachlor epoxide


R.T.: 8.038 min
Delta R.T.: 0.005 min
Response: 1387324
Conc: 1.23 ng/ml

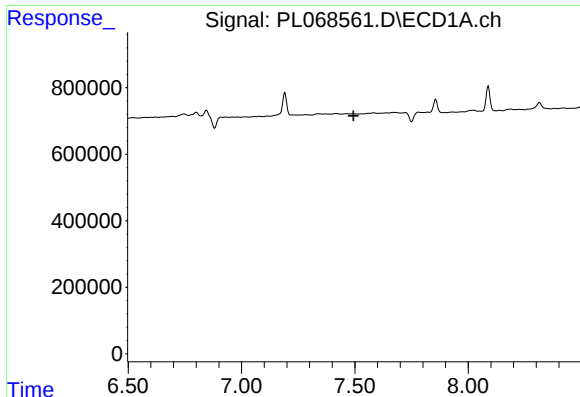

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138070BL

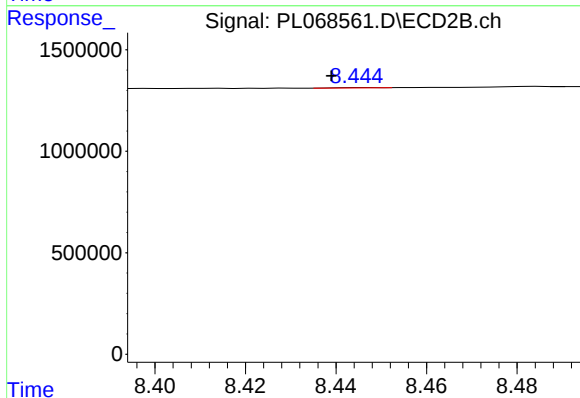


#9 Endosulfan I

R.T.: 8.447 min
Delta R.T.: 0.008 min
Response: 8003
Conc: 0.01 ng/ml

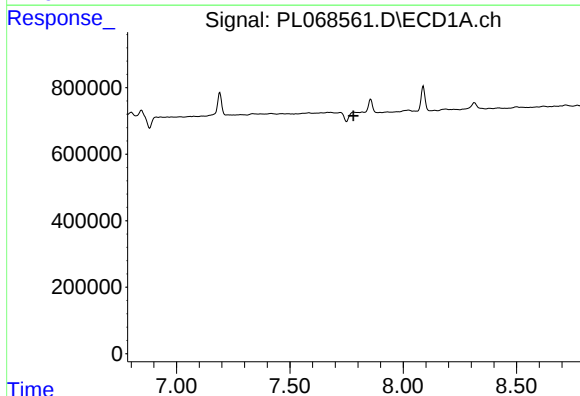


#13 Dieldrin

R.T.: 7.782 min
Delta R.T.: 0.001 min
Response: -11228
Conc: N.D.

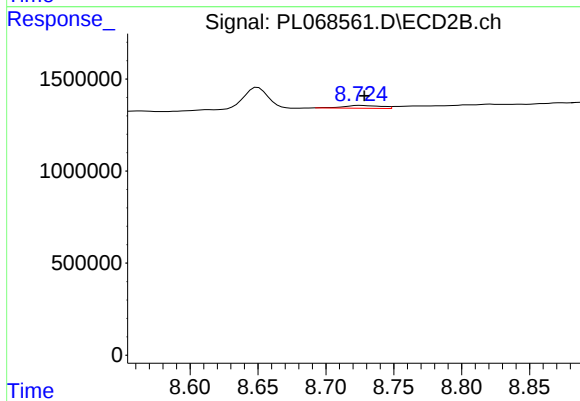

#13 Dieldrin


R.T.: 8.725 min
Delta R.T.: -0.003 min
Response: 293023
Conc: 0.28 ng/ml

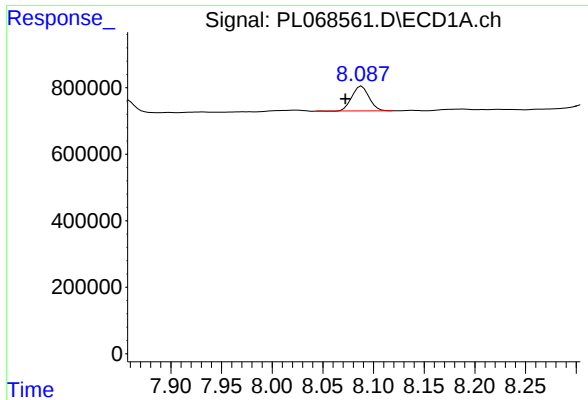

#14 Endrin


R.T.: 8.088 min
Delta R.T.: 0.016 min
Response: 873140
Conc: 1.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138070BL

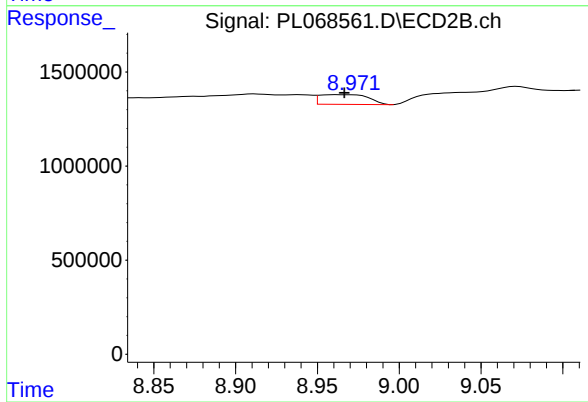


#14 Endrin

R.T.: 8.963 min
Delta R.T.: -0.004 min
Response: 1071232
Conc: 1.20 ng/ml

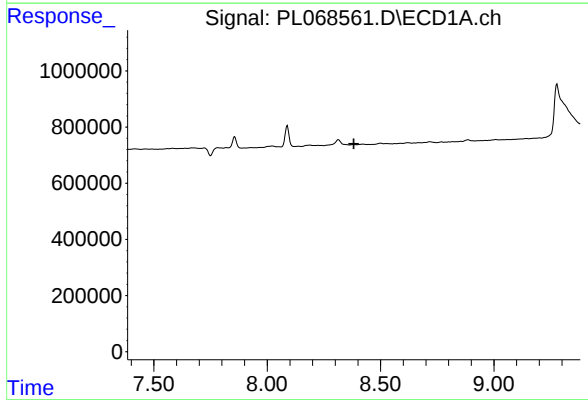


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.382 min
Response: 0
Conc: N.D.

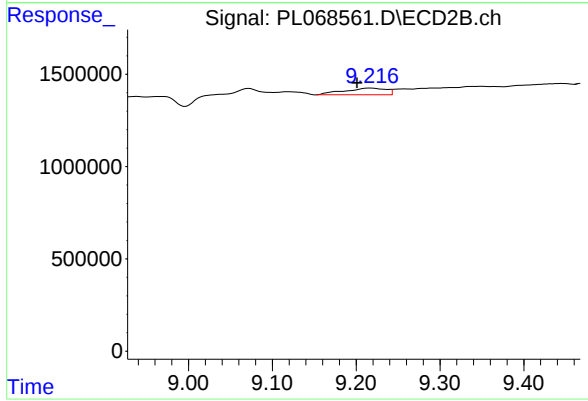

#15 Endosulfan II


R.T.: 9.217 min
Delta R.T.: 0.016 min
Response: 1253350
Conc: 1.38 ng/ml

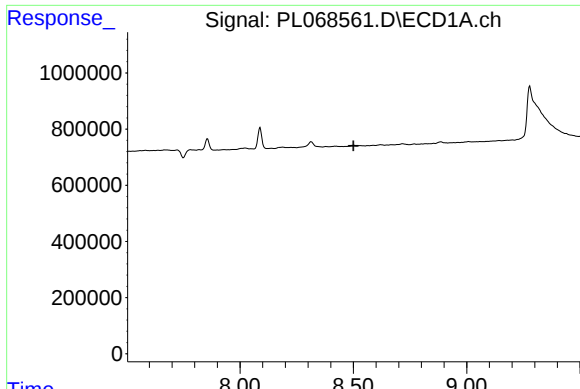

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.501 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138070BL

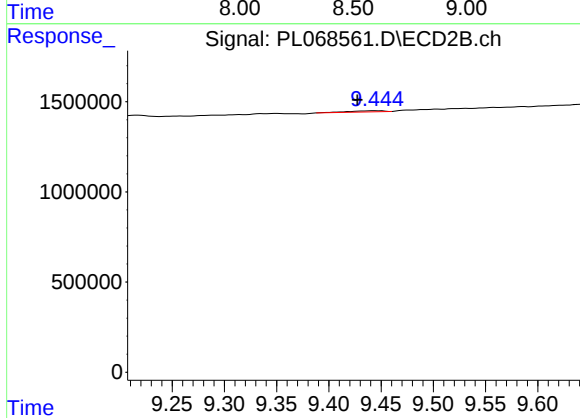


#17 4,4'-DDT

R.T.: 9.445 min
Delta R.T.: 0.018 min
Response: 157926
Conc: 0.17 ng/ml

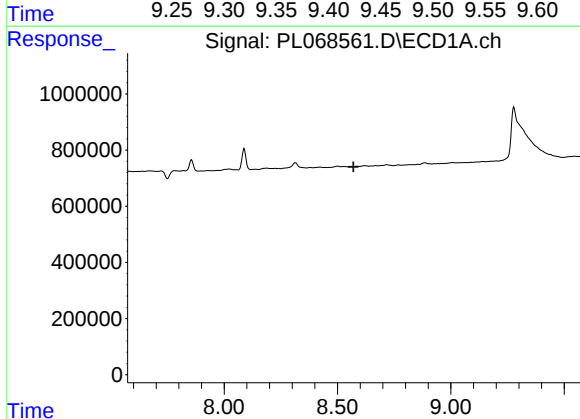


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.571 min
Response: 0
Conc: N.D.

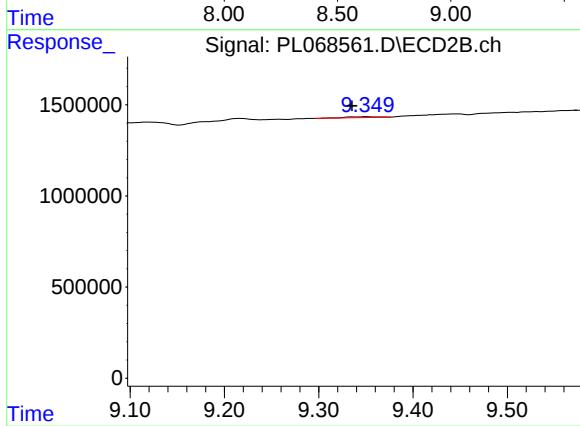

#18 Endrin aldehyde


R.T.: 9.350 min
Delta R.T.: 0.015 min
Response: 110250
Conc: 0.15 ng/ml

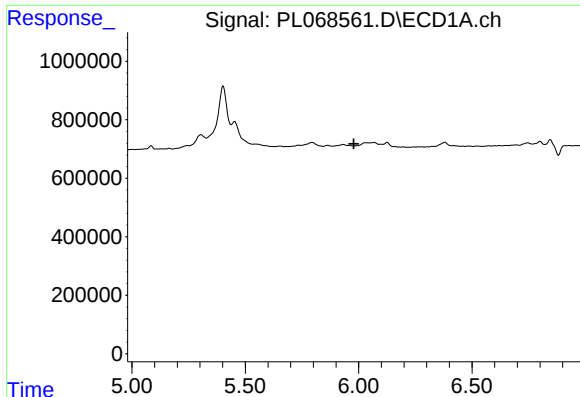

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138070BL

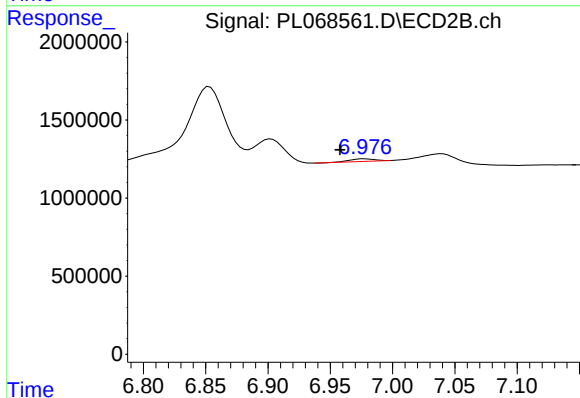


#23 Chlordane-1

R.T.: 6.977 min
Delta R.T.: 0.019 min
Response: 232771
Conc: 5.75 ng/ml

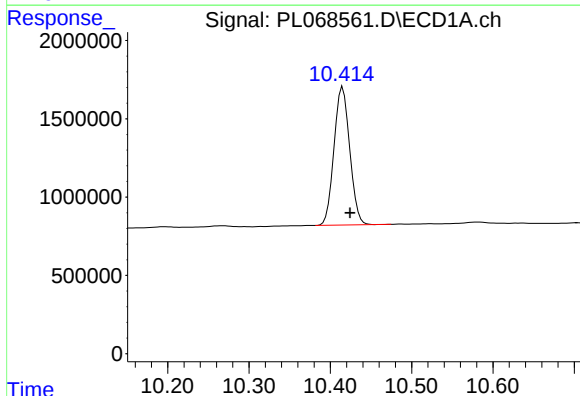

#28 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: -0.009 min
Response: 11863091
Conc: 21.09 ng/ml

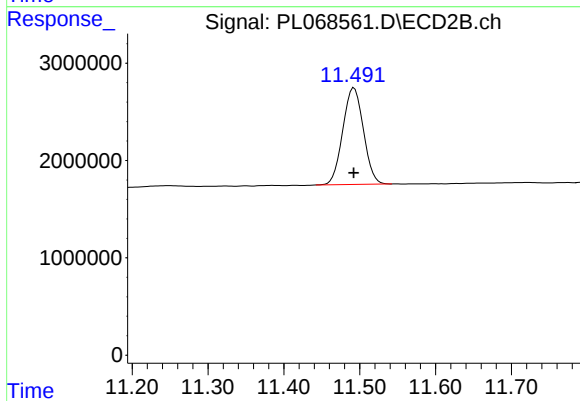

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 18812388
Conc: 21.09 ng/ml