

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072921\
 Data File : PL068562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2021 17:22
 Operator : AR\AJ
 Sample : PB138070TB
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB138070TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:22:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.570	9602488	21463057	22.374	21.033
28)	SA Decachlor...	10.416	11.492	12418851	19677341	22.081	22.060
Target Compounds							
8)	B Heptachlo...	0.000	8.007f	0	47044	N.D.	0.042 #
11)	B alpha-Chl...	0.000	8.401f	0	101375	N.D.	0.090 #
13)	MA Dieldrin	0.000	8.728	0	117746	N.D.	0.111 #
14)	MA Endrin	0.000	8.984f	0	73054	N.D.	0.082 #
15)	B Endosulfa...	0.000	9.219f	0	168979	N.D.	0.186 #
18)	B Endrin al...	0.000	9.355f	0	13577	N.D.	0.019 #
20)	A Methoxychlor	0.000	9.926	0	38668	N.D.	0.076 #
23)	Chlordane-1	0.000	6.979f	0	355278	N.D.	8.770 #
26)	Chlordane-4	0.000	8.401	0	101375	N.D.	0.541 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072921\
Data File : PL068562.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2021 17:22
Operator : AR\AJ
Sample : PB138070TB
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB138070TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:22:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

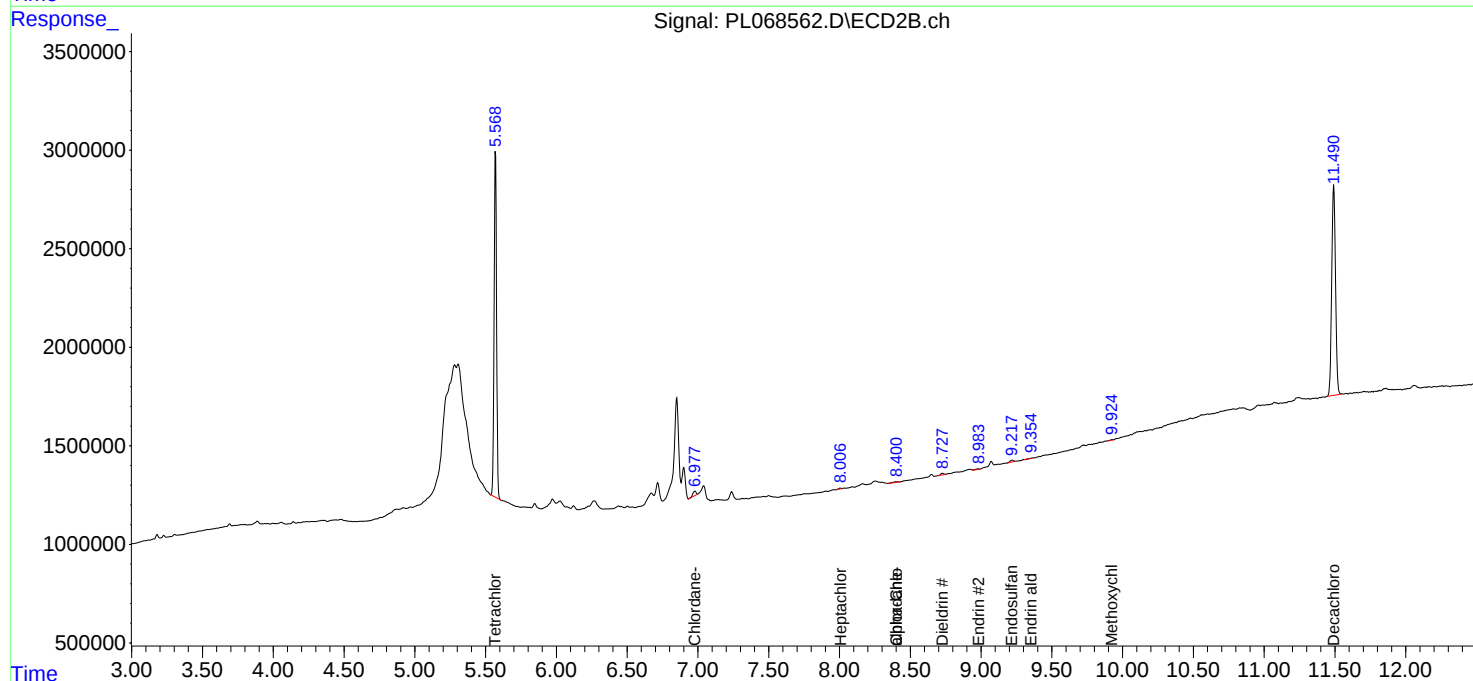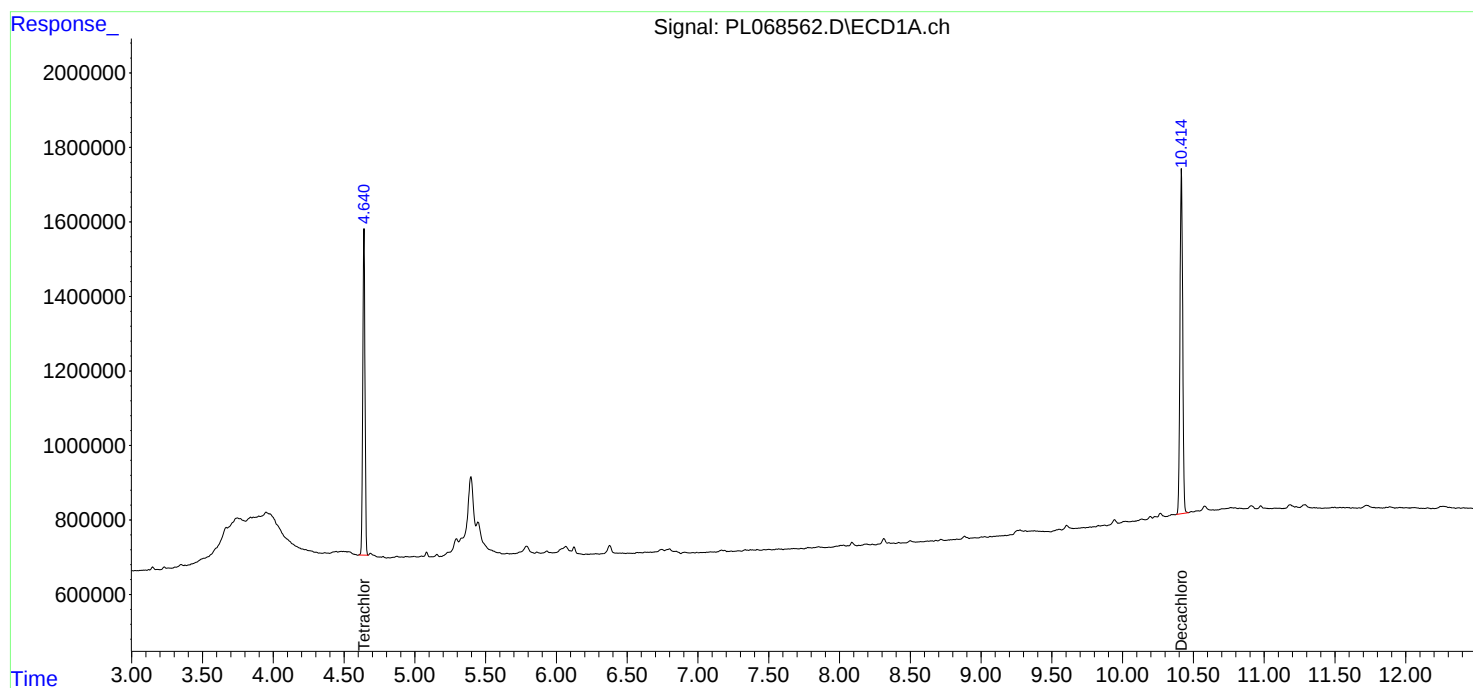


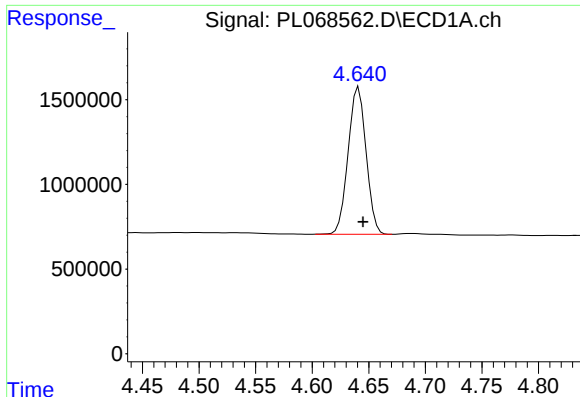

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.004 min
Response: 9602488
Conc: 22.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138070TB

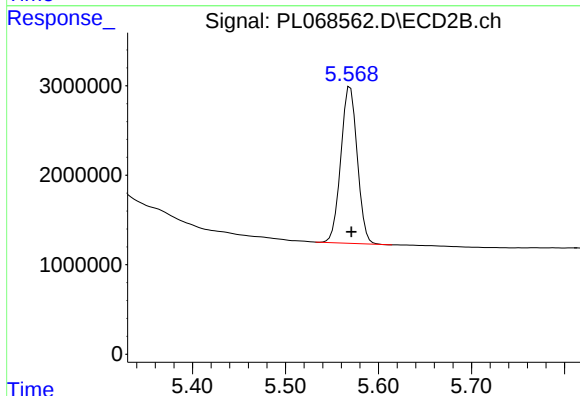


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: -0.001 min
Response: 21463057
Conc: 21.03 ng/ml

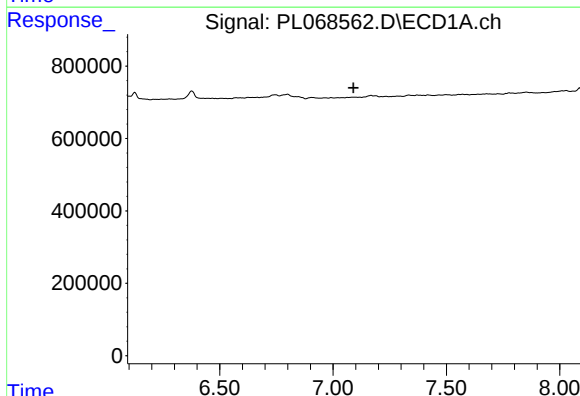


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

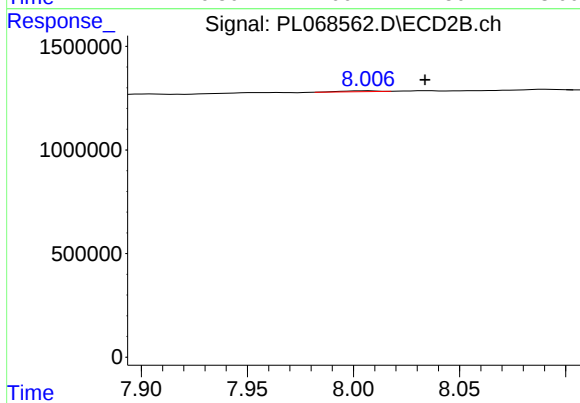

#8 Heptachlor epoxide


R.T.: 8.007 min
Delta R.T.: -0.027 min
Response: 47044
Conc: 0.04 ng/ml

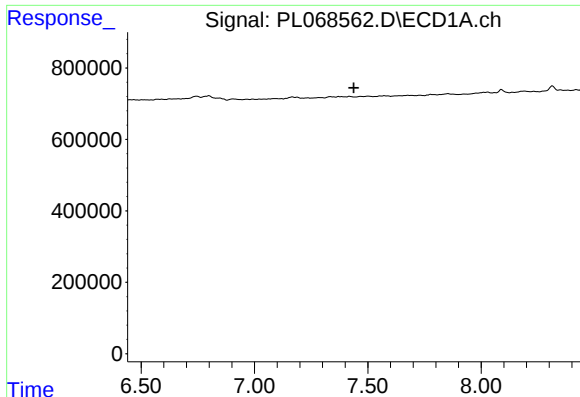

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.438 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138070TB

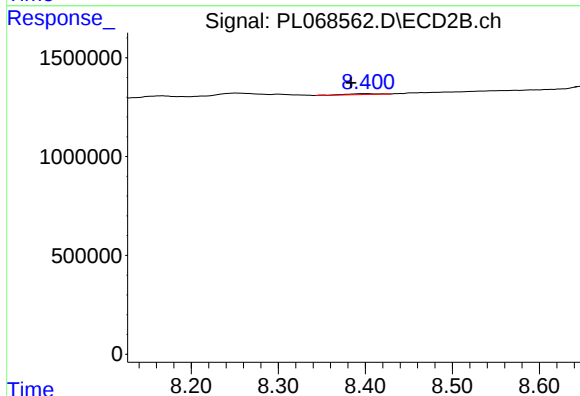


#11 alpha-Chlordane

R.T.: 8.401 min
Delta R.T.: 0.018 min
Response: 101375
Conc: 0.09 ng/ml

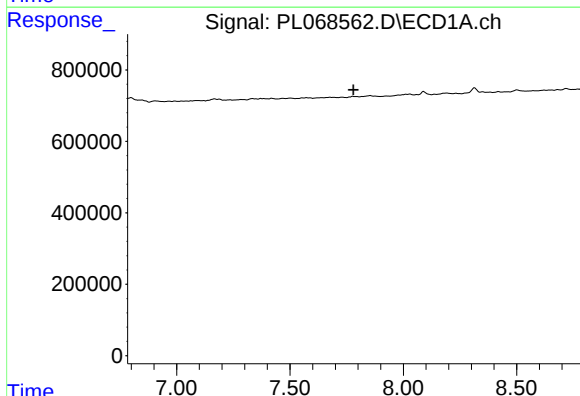


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.781 min
Response: 0
Conc: N.D.

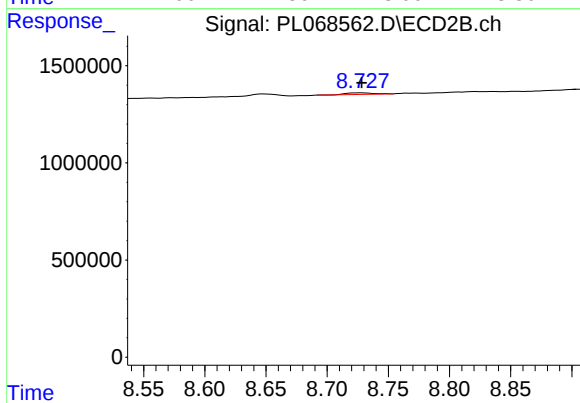

#13 Dieldrin


R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 117746
Conc: 0.11 ng/ml

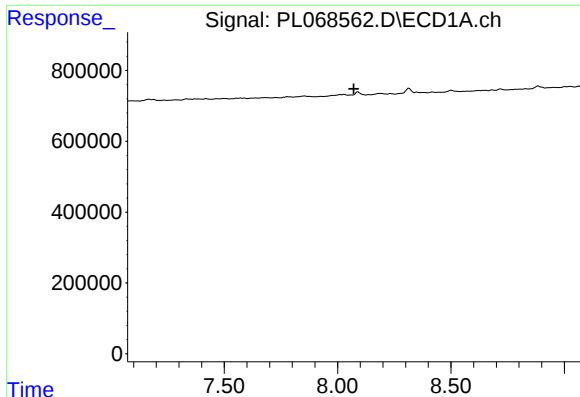

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.072 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138070TB

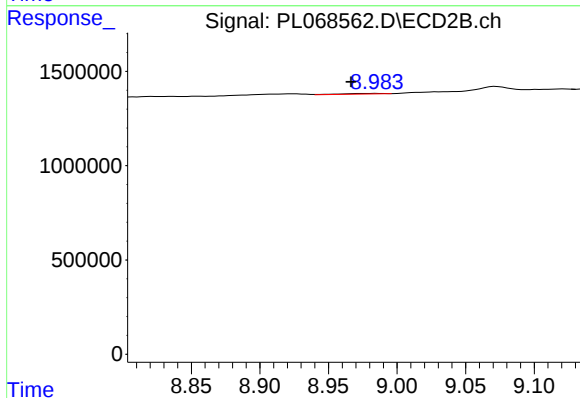


#14 Endrin

R.T.: 8.984 min
Delta R.T.: 0.018 min
Response: 73054
Conc: 0.08 ng/ml

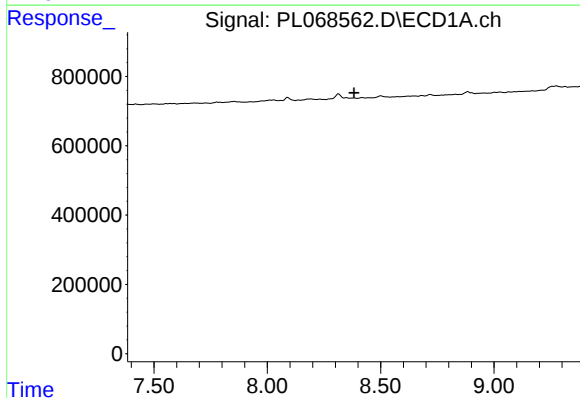


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

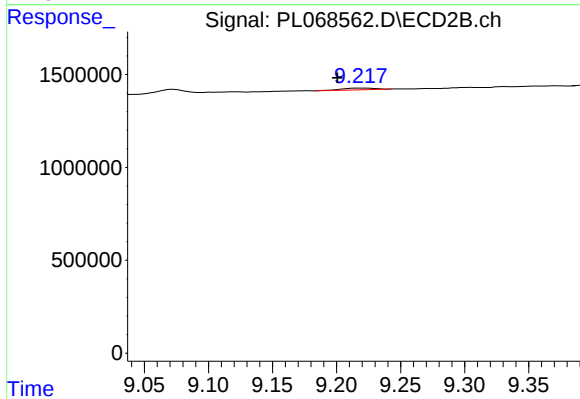

#15 Endosulfan II


R.T.: 9.219 min
Delta R.T.: 0.018 min
Response: 168979
Conc: 0.19 ng/ml

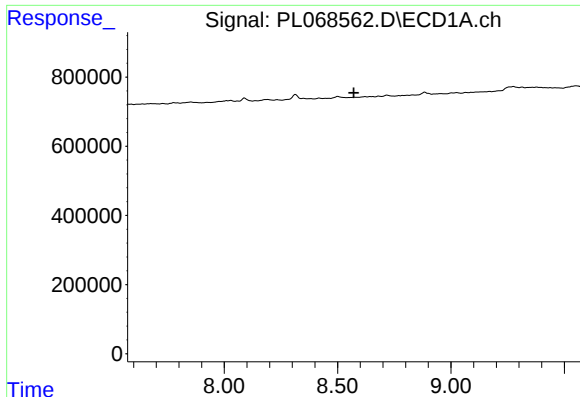

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.571 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138070TB

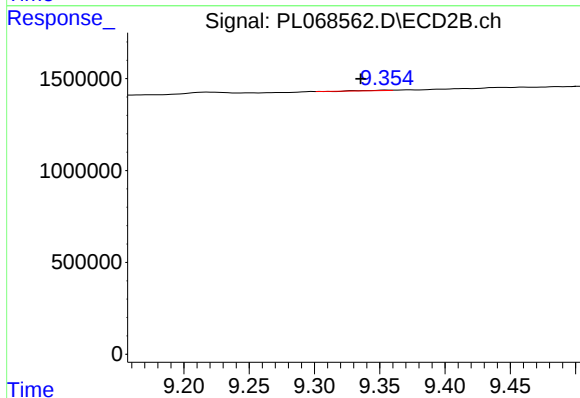


#18 Endrin aldehyde

R.T.: 9.355 min
Delta R.T.: 0.020 min
Response: 13577
Conc: 0.02 ng/ml

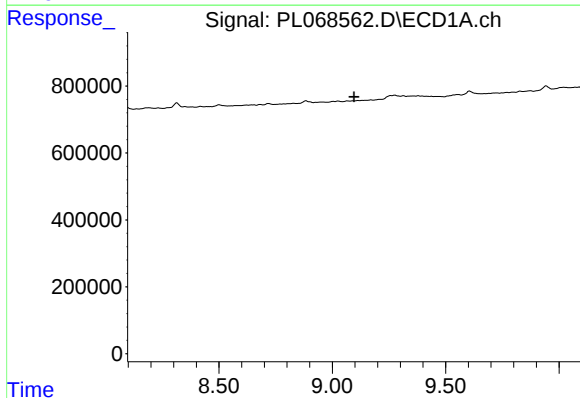


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 9.096 min
Response: 0
Conc: N.D.

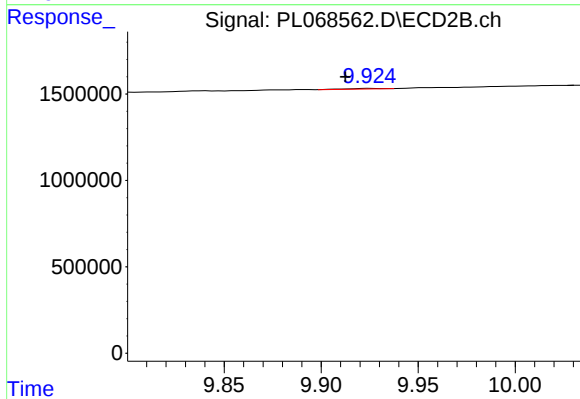

#20 Methoxychlor


R.T.: 9.926 min
Delta R.T.: 0.013 min
Response: 38668
Conc: 0.08 ng/ml

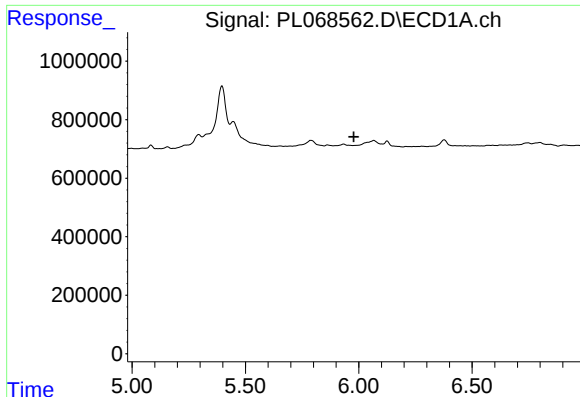

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.978 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138070TB

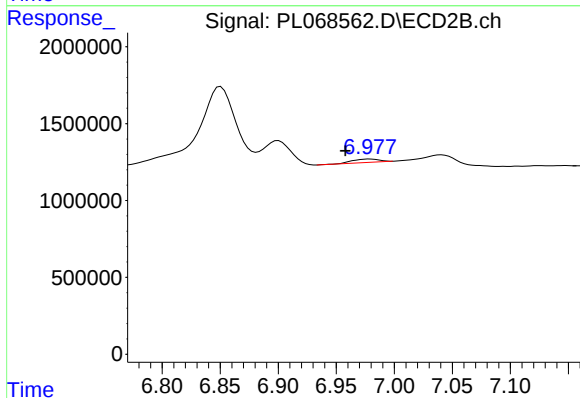


#23 Chlordane-1

R.T.: 6.979 min
Delta R.T.: 0.022 min
Response: 355278
Conc: 8.77 ng/ml

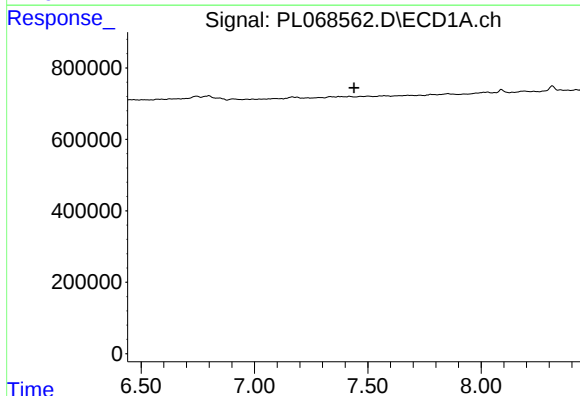


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.440 min
Response: 0
Conc: N.D.

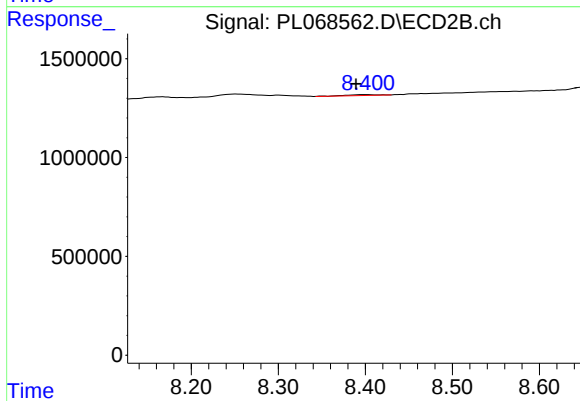

#26 Chlordane-4


R.T.: 8.401 min
Delta R.T.: 0.012 min
Response: 101375
Conc: 0.54 ng/ml

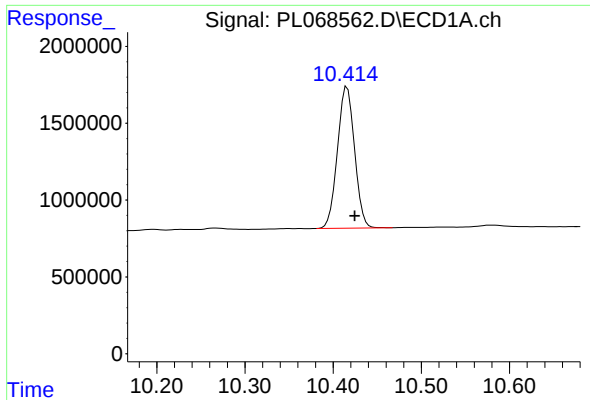

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.008 min
Response: 12418851
Conc: 22.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138070TB

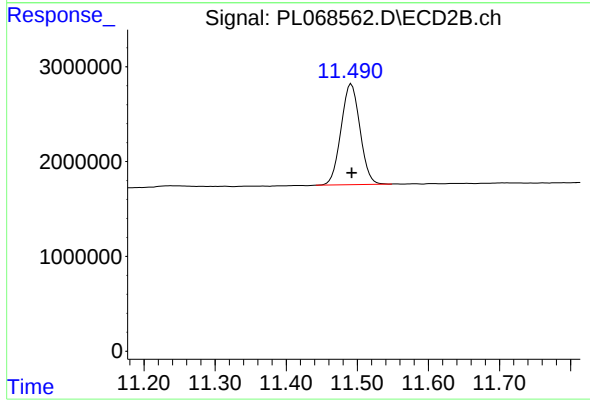

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: 0.000 min
Response: 19677341
Conc: 22.06 ng/ml