

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072921\
 Data File : PL068581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2021 23:11
 Operator : AR\AJ
 Sample : M3223-05
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:27:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.569	6142197	13753213	14.311	13.478
28)	SA Decachlor...	10.415	11.492	9587432	15577041	17.047	17.463
Target Compounds							
9)	A Endosulfan I	0.000	8.445	0	14141	N.D.	0.014 #
13)	MA Dieldrin	0.000	8.726	0	168674	N.D.	0.159 #
14)	MA Endrin	0.000	8.944f	0	10391	N.D.	0.012 #
15)	B Endosulfa...	0.000	9.215	0	102790	N.D.	0.113 #
17)	MA 4,4'-DDT	0.000	9.435	0	13680	N.D.	0.014 #
22)	Mirex	0.000	10.565f	0	112588	N.D.	0.146 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072921\
Data File : PL068581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2021 23:11
Operator : AR\AJ
Sample : M3223-05
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:27:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

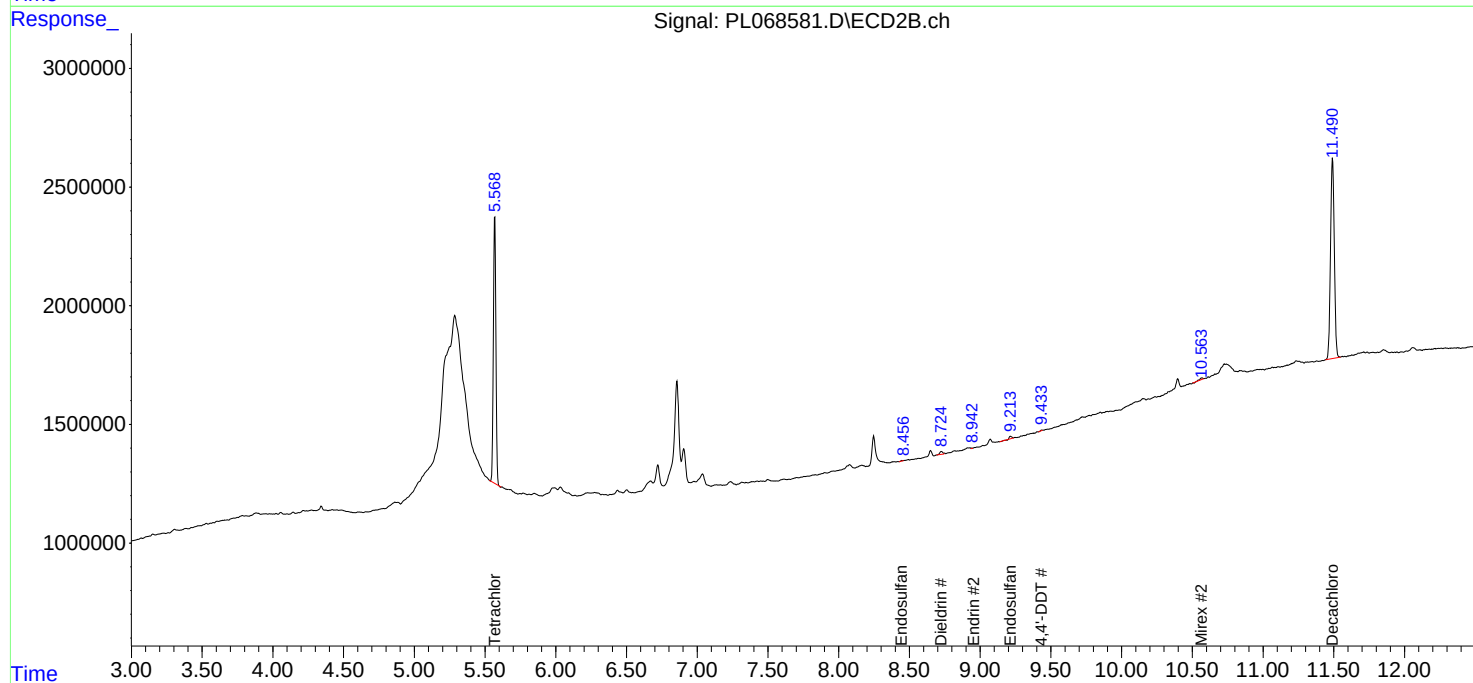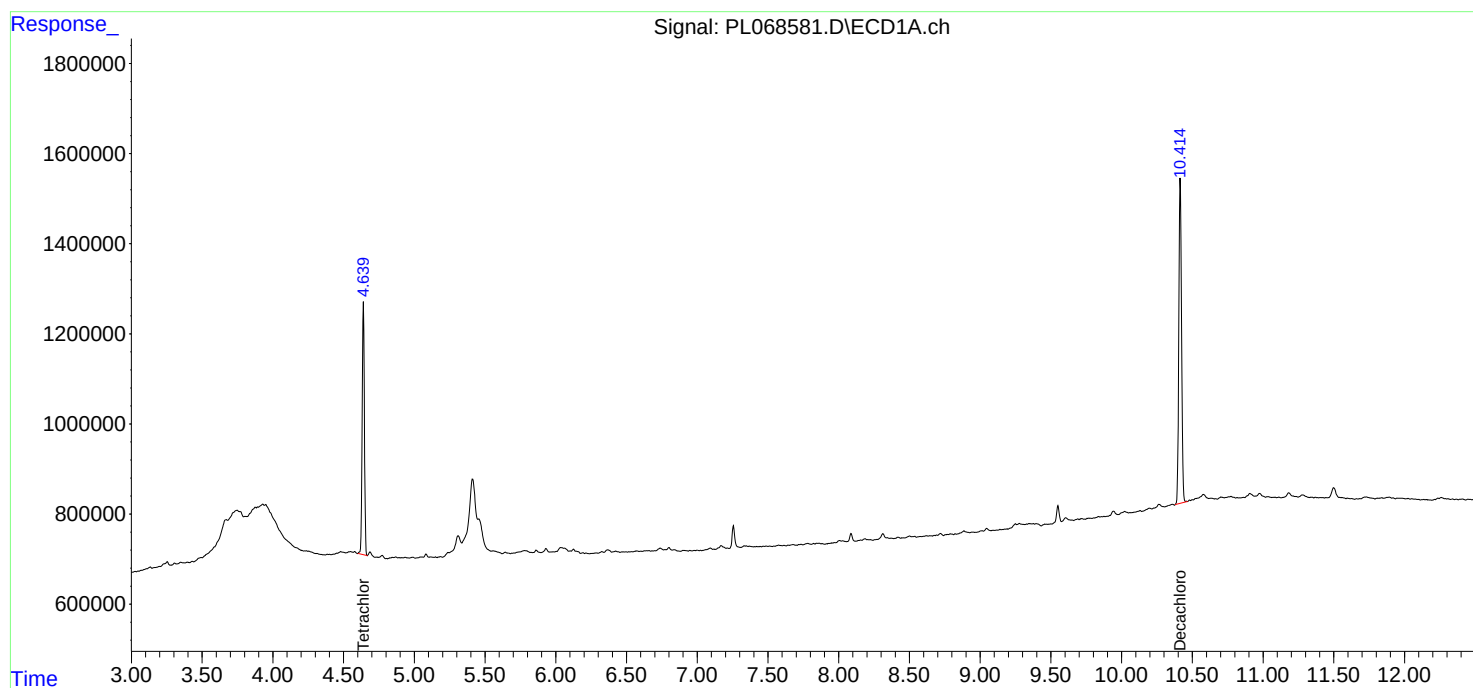


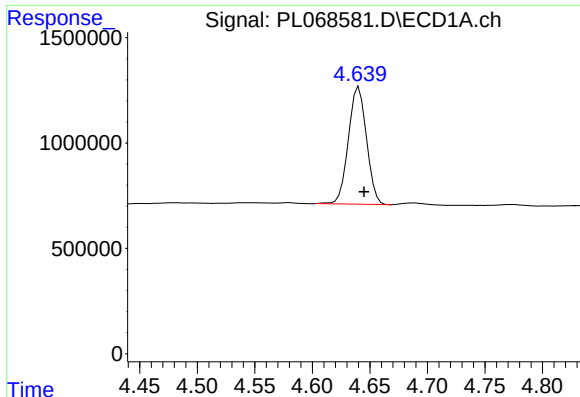

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.004 min
Response: 6142197
Conc: 14.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-11

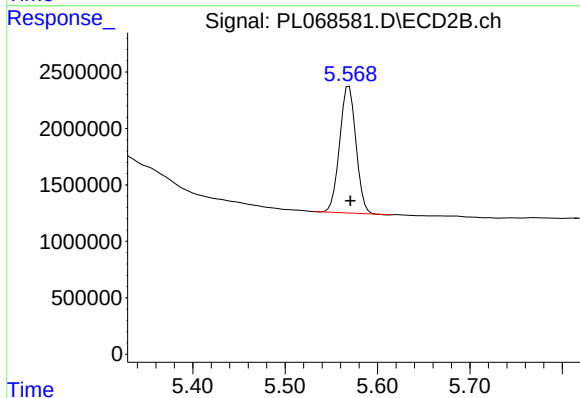


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 13753213
Conc: 13.48 ng/ml

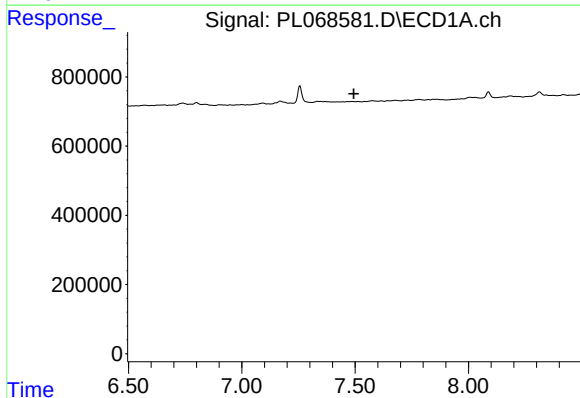


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.494 min
Response: 0
Conc: N.D.

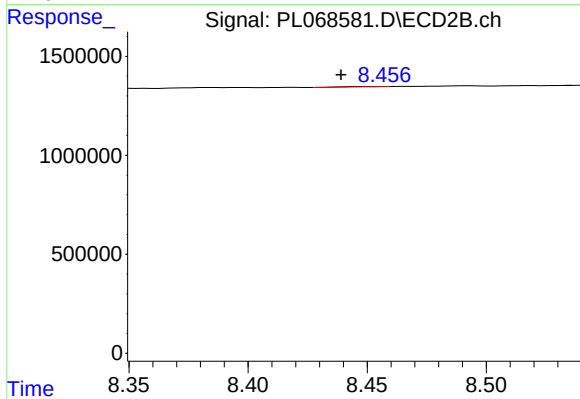

#9 Endosulfan I


R.T.: 8.445 min
Delta R.T.: 0.006 min
Response: 14141
Conc: 0.01 ng/ml

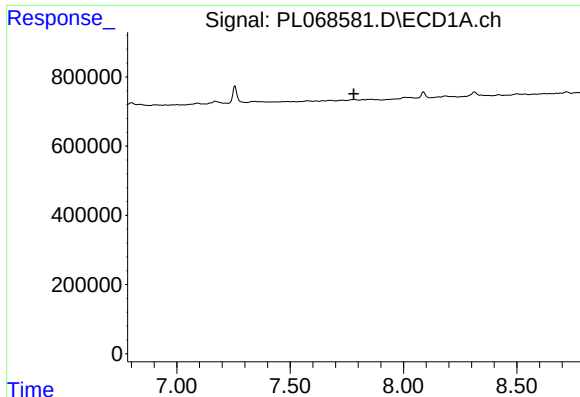

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.781 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-11

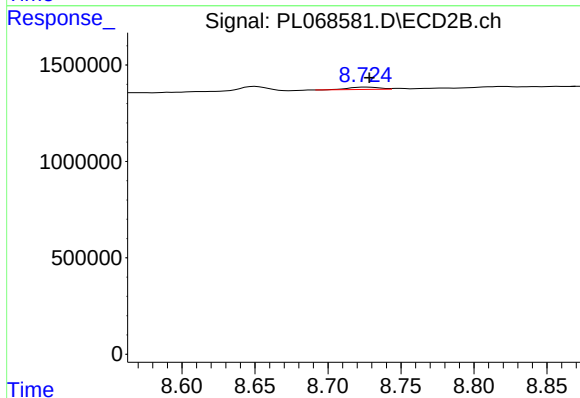


#13 Dieldrin

R.T.: 8.726 min
Delta R.T.: -0.003 min
Response: 168674
Conc: 0.16 ng/ml

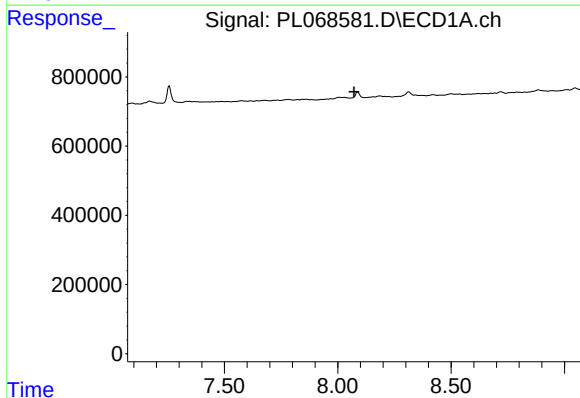


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 8.072 min
Response: 0
Conc: N.D.

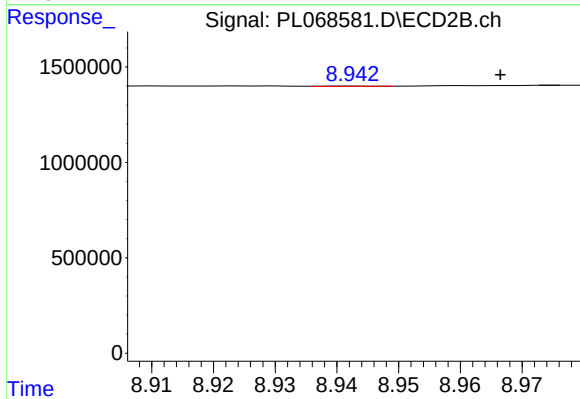

#14 Endrin


R.T.: 8.944 min
Delta R.T.: -0.023 min
Response: 10391
Conc: 0.01 ng/ml

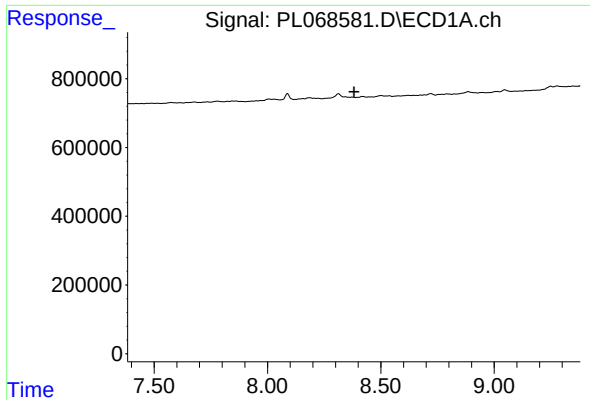

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-11

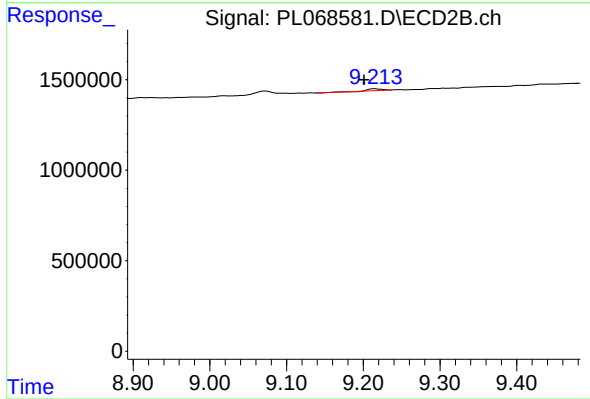


#15 Endosulfan II

R.T.: 9.215 min
Delta R.T.: 0.014 min
Response: 102790
Conc: 0.11 ng/ml

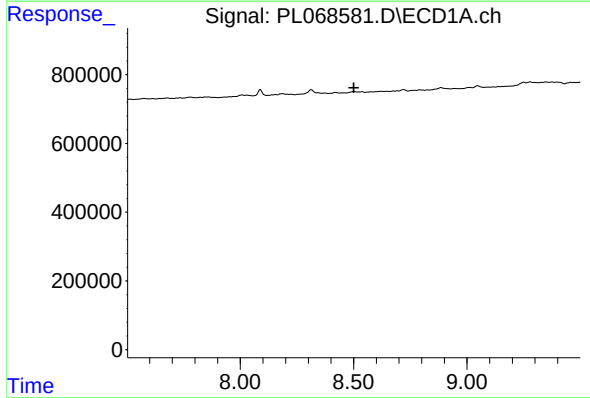


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.501 min
Response: 0
Conc: N.D.

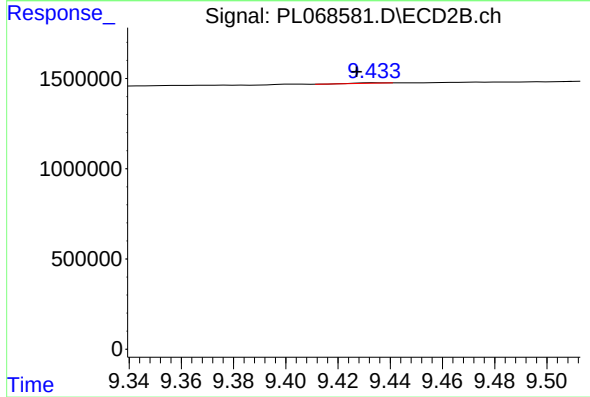

#17 4,4'-DDT


R.T.: 9.435 min
Delta R.T.: 0.008 min
Response: 13680
Conc: 0.01 ng/ml

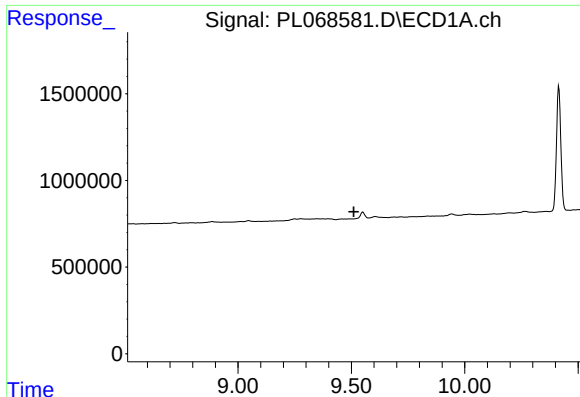

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-11

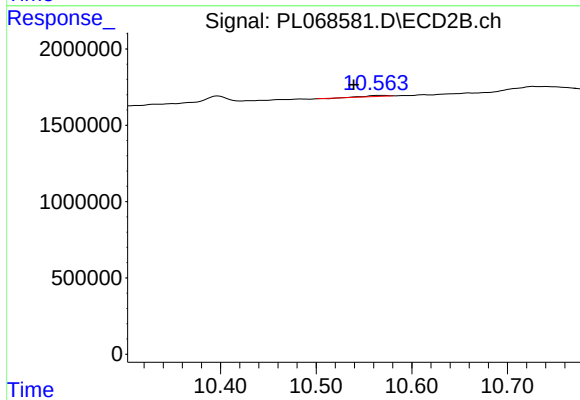


#22 Mirex

R.T.: 10.565 min
Delta R.T.: 0.026 min
Response: 112588
Conc: 0.15 ng/ml

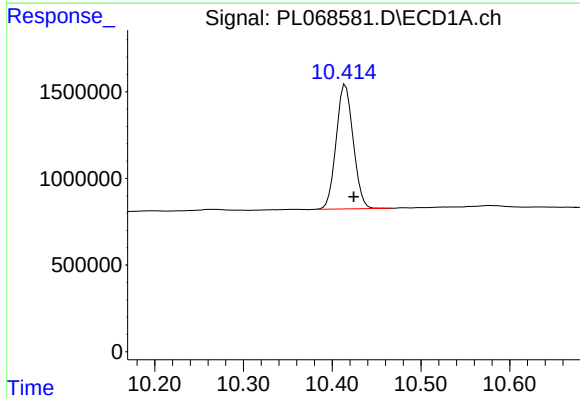

#28 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: -0.009 min
Response: 9587432
Conc: 17.05 ng/ml

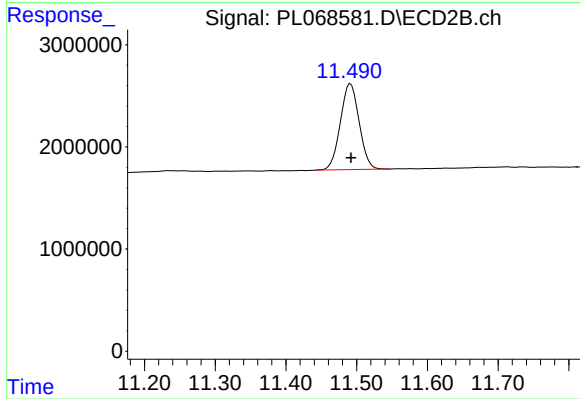

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: 0.000 min
Response: 15577041
Conc: 17.46 ng/ml