

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072921\
 Data File : PL068586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2021 01:07
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:35:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 20 11:44:21 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.570	25115651	56917118	58.520	55.778
28)	SA Decachlor...	10.417	11.493	26702170	46121035	47.477	51.706
Target Compounds							
2)	A alpha-BHC	5.348	6.150	33823204	76714764	57.779	56.424
3)	MA gamma-BHC...	5.771	6.546	33047442	70226768	58.137	54.431
4)	MA Heptachlor	6.183	7.196	32670956	64956246	53.601	49.839
5)	MB Aldrin	6.508	7.567	32464758	63971498	57.771	53.917
6)	B beta-BHC	6.151	6.798	17044271	34021936	58.247	48.158
7)	B delta-BHC	6.412	7.066	32867410	66106034	58.826	53.955
8)	B Heptachlo...	7.086	8.033	31105808	59671441	55.991	52.778
9)	A Endosulfan I	7.489	8.439	29210130	53285320	55.294	51.754
10)	B gamma-Chl...	7.363	8.302	31873727	58649484	55.551	52.077
11)	B alpha-Chl...	7.433	8.384	31632832	57789405	55.076	51.382
12)	B 4,4'-DDE	7.647	8.570	28198976	52730660	55.959	51.166
13)	MA Dieldrin	7.775	8.728	29838563	54430134	55.433	51.318
14)	MA Endrin	8.066	8.968	25827383	42310887	51.645	47.319
15)	B Endosulfa...	8.377	9.200	25539770	44814277	51.730	49.442
16)	A 4,4'-DDD	8.232	9.110	26661900	47560807	59.689	55.857
17)	MA 4,4'-DDT	8.494	9.427	20213718	35793403	40.299	37.923
18)	B Endrin al...	8.565	9.335	20453951	34954810	51.634	48.500
19)	B Endosulfa...	8.796	9.572	26997189	43806719	51.377	48.648
20)	A Methoxychlor	9.089	9.912	12539457	19190194	40.087	37.773
21)	B Endrin ke...	9.316	10.071	30357182	49698833	51.269	49.832
22)	Mirex	9.505	10.539	24453597	37656883	49.519	48.675
24)	Chlordane-2	6.656	7.567f	348459	63971498	16.247	1537.592 #
25)	Chlordane-3	7.363	8.302	31873727	58649484	591.856	378.702 #
26)	Chlordane-4	7.433	8.384	31632832	57789405	560.272	308.242 #
27)	Chlordane-5	8.377	0.000	25539770	0	1268.978	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072921\
Data File : PL068586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2021 01:07
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:35:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071921.M
Quant Title : GC Extractables
QLast Update : Tue Jul 20 11:44:21 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

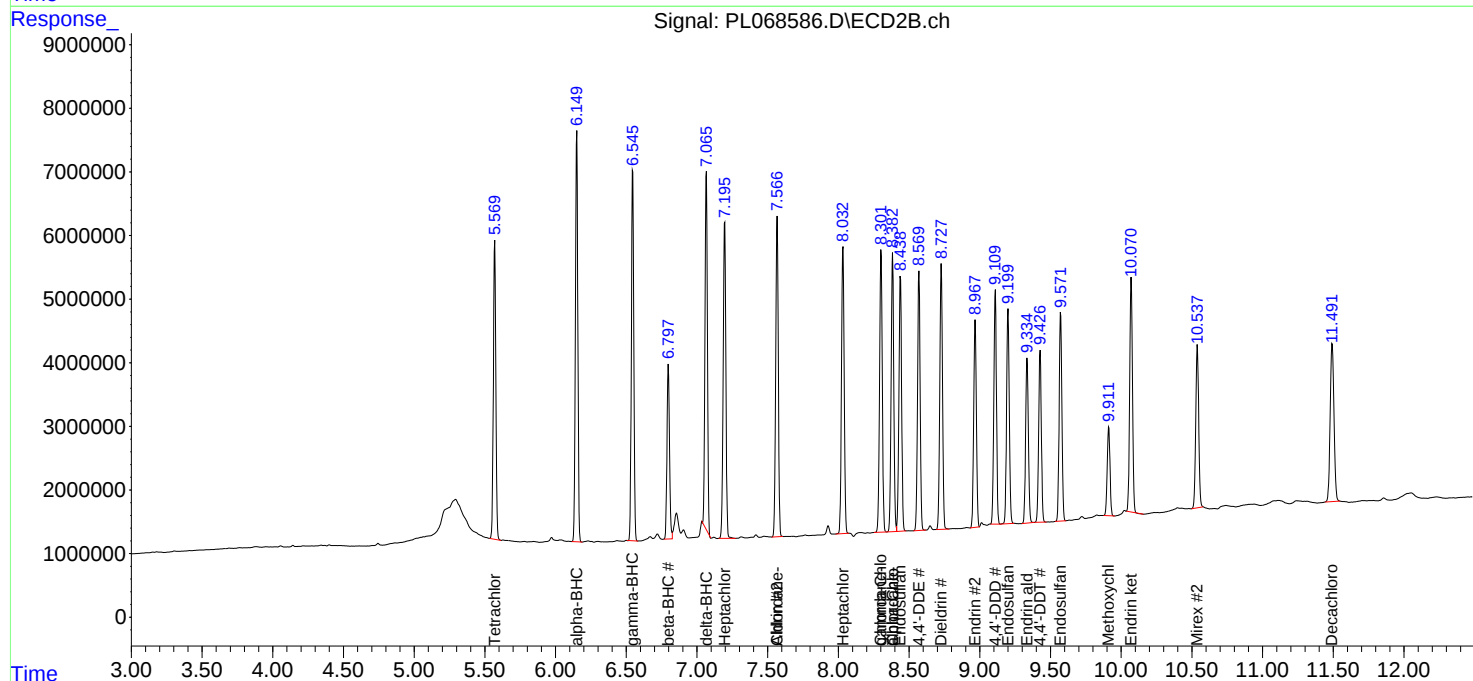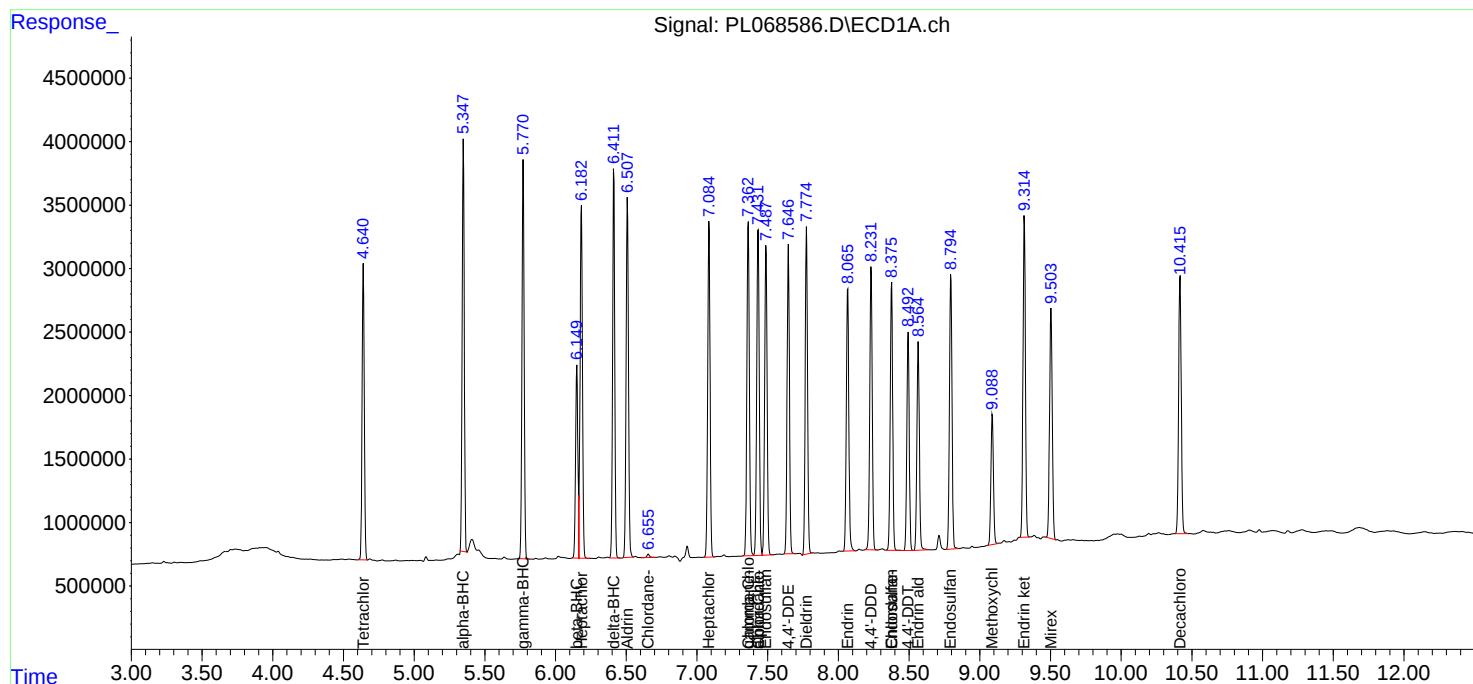


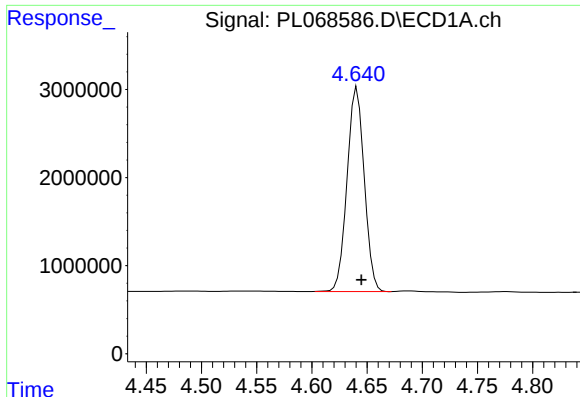

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.004 min
Response: 25115651
Conc: 58.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

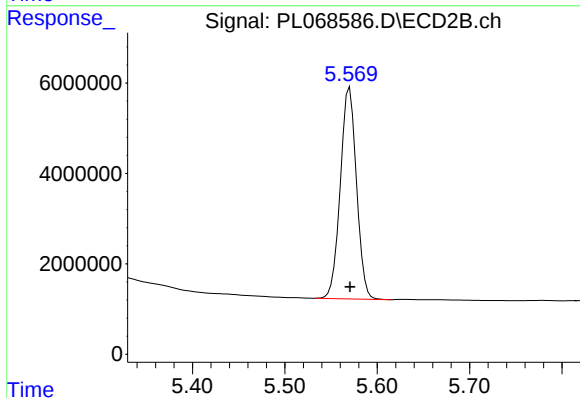


#1 Tetrachloro-m-xylene

R.T.: 5.570 min
Delta R.T.: 0.000 min
Response: 56917118
Conc: 55.78 ng/ml

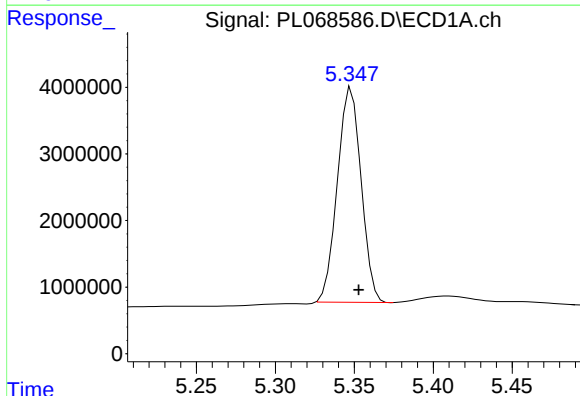


#2 alpha-BHC

R.T.: 5.348 min
Delta R.T.: -0.004 min
Response: 33823204
Conc: 57.78 ng/ml

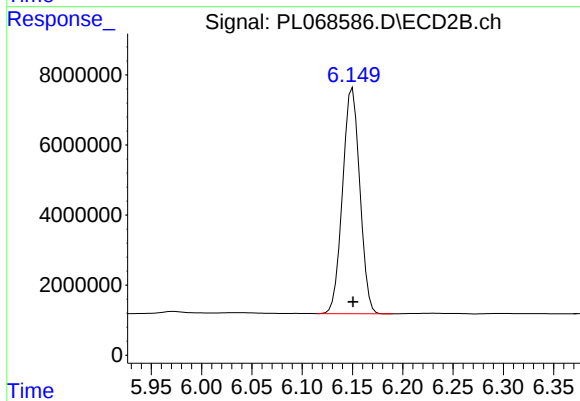

#2 alpha-BHC


R.T.: 6.150 min
Delta R.T.: 0.000 min
Response: 76714764
Conc: 56.42 ng/ml

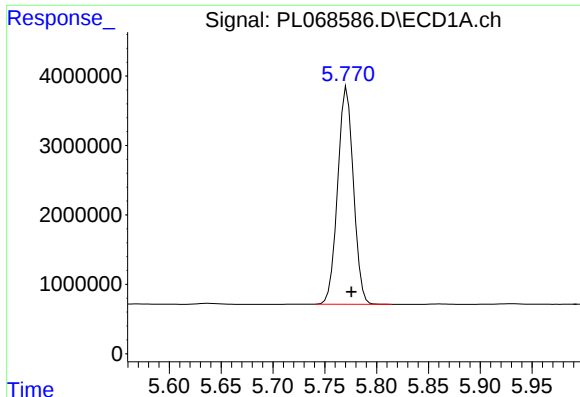

#3 gamma-BHC (Lindane)


R.T.: 5.771 min
Delta R.T.: -0.004 min
Response: 33047442
Conc: 58.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

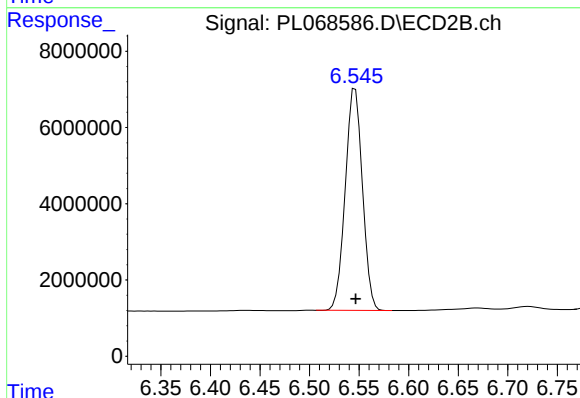


#3 gamma-BHC (Lindane)

R.T.: 6.546 min
Delta R.T.: 0.000 min
Response: 70226768
Conc: 54.43 ng/ml

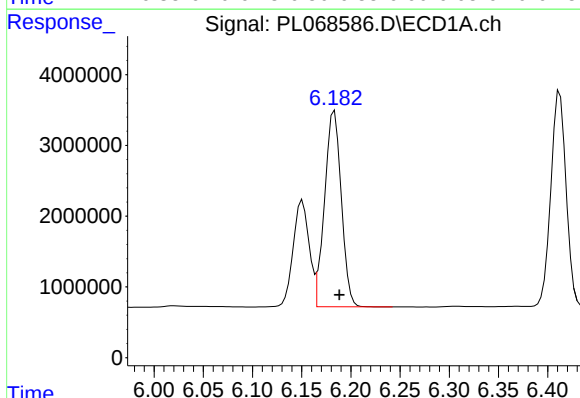


#4 Heptachlor

R.T.: 6.183 min
Delta R.T.: -0.005 min
Response: 32670956
Conc: 53.60 ng/ml

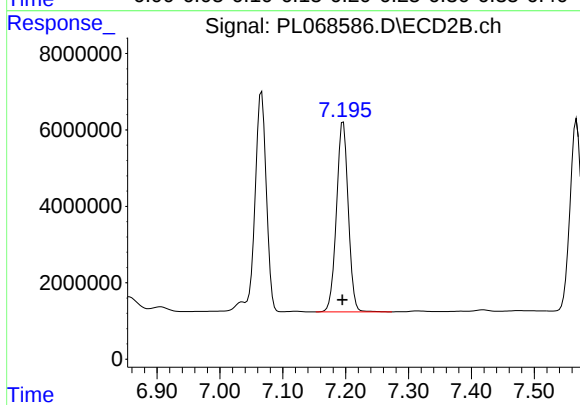

#4 Heptachlor


R.T.: 7.196 min
Delta R.T.: 0.001 min
Response: 64956246
Conc: 49.84 ng/ml

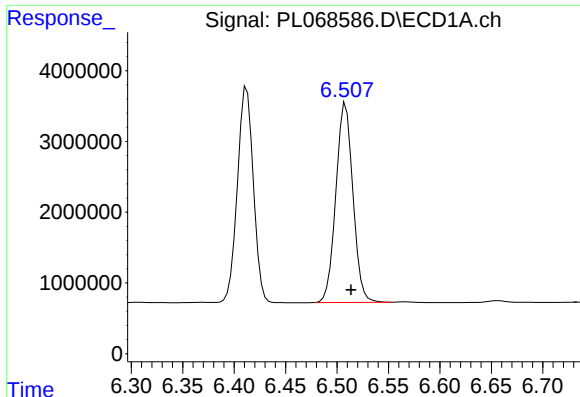

#5 Aldrin


R.T.: 6.508 min
Delta R.T.: -0.005 min
Response: 32464758
Conc: 57.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

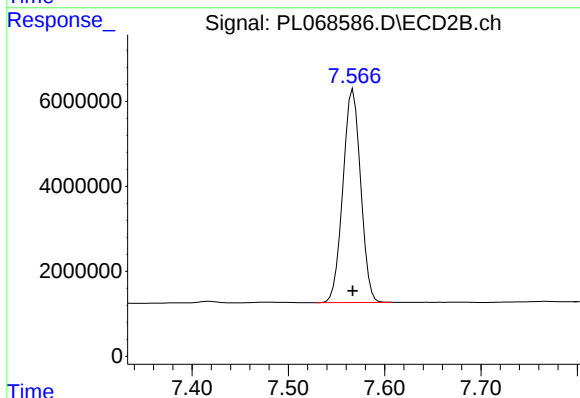


#5 Aldrin

R.T.: 7.567 min
Delta R.T.: 0.000 min
Response: 63971498
Conc: 53.92 ng/ml

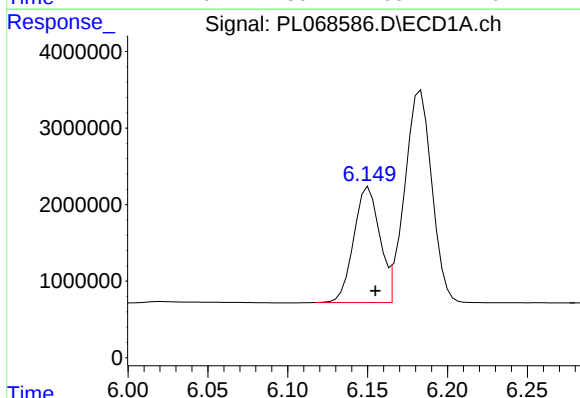


#6 beta-BHC

R.T.: 6.151 min
Delta R.T.: -0.004 min
Response: 17044271
Conc: 58.25 ng/ml

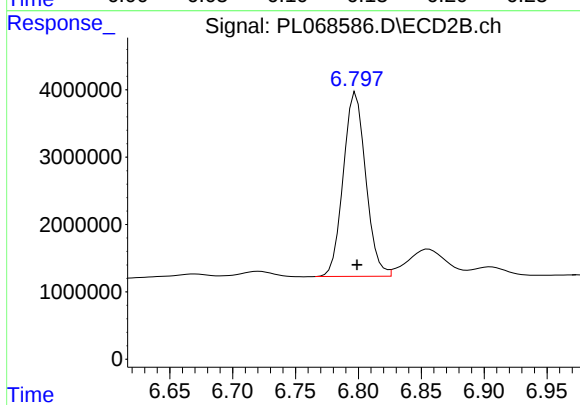

#6 beta-BHC


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 34021936
Conc: 48.16 ng/ml

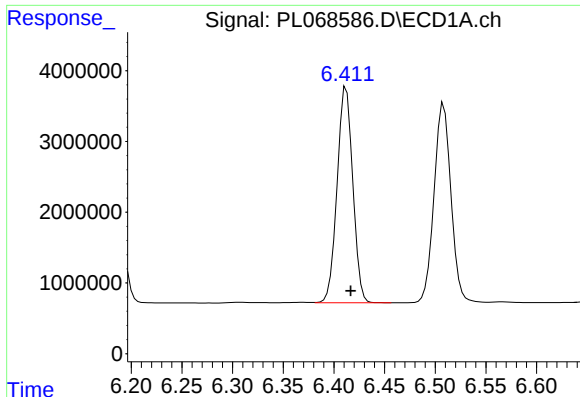

#7 delta-BHC


R.T.: 6.412 min
Delta R.T.: -0.004 min
Response: 32867410
Conc: 58.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

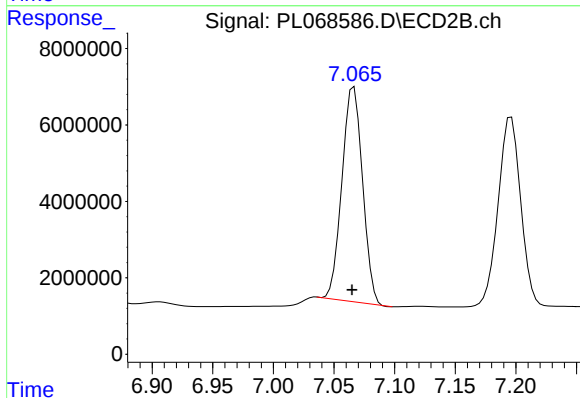


#7 delta-BHC

R.T.: 7.066 min
Delta R.T.: 0.002 min
Response: 66106034
Conc: 53.95 ng/ml

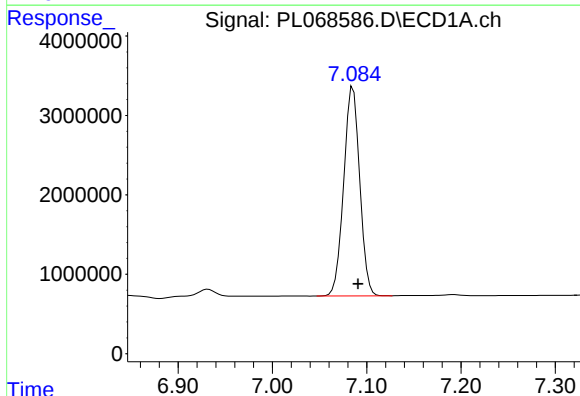


#8 Heptachlor epoxide

R.T.: 7.086 min
Delta R.T.: -0.005 min
Response: 31105808
Conc: 55.99 ng/ml

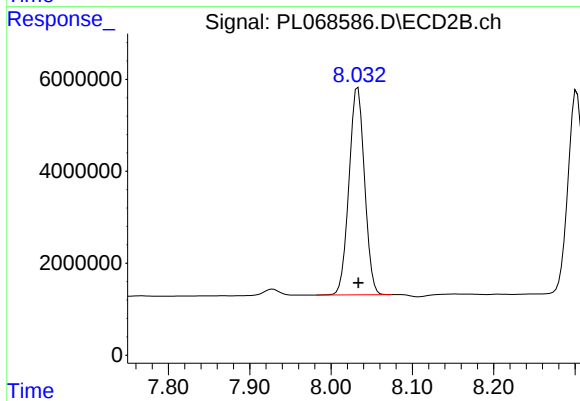

#8 Heptachlor epoxide


R.T.: 8.033 min
Delta R.T.: 0.000 min
Response: 59671441
Conc: 52.78 ng/ml

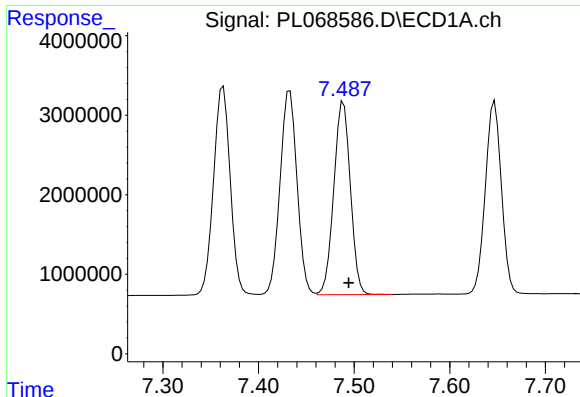

#9 Endosulfan I


R.T.: 7.489 min
Delta R.T.: -0.006 min
Response: 29210130
Conc: 55.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

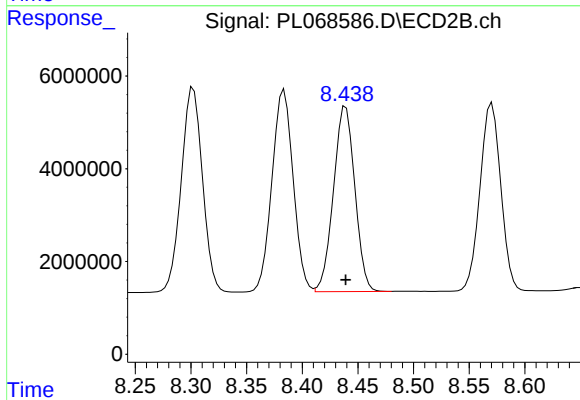


#9 Endosulfan I

R.T.: 8.439 min
Delta R.T.: 0.000 min
Response: 53285320
Conc: 51.75 ng/ml

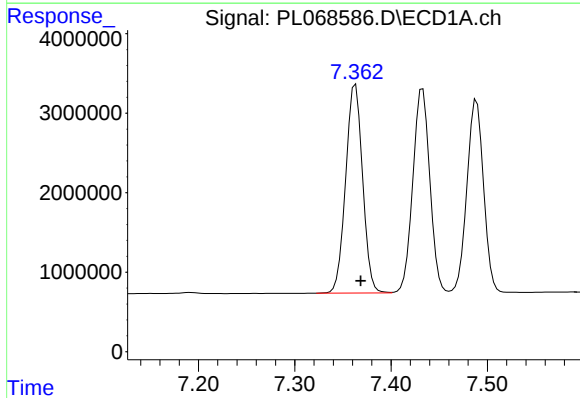


#10 gamma-Chlordane

R.T.: 7.363 min
Delta R.T.: -0.006 min
Response: 31873727
Conc: 55.55 ng/ml

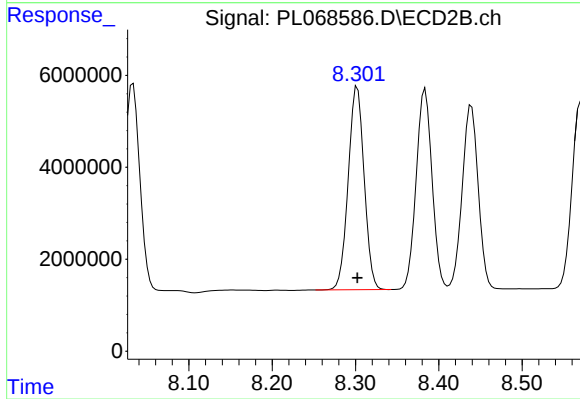

#10 gamma-Chlordane


R.T.: 8.302 min
Delta R.T.: 0.000 min
Response: 58649484
Conc: 52.08 ng/ml

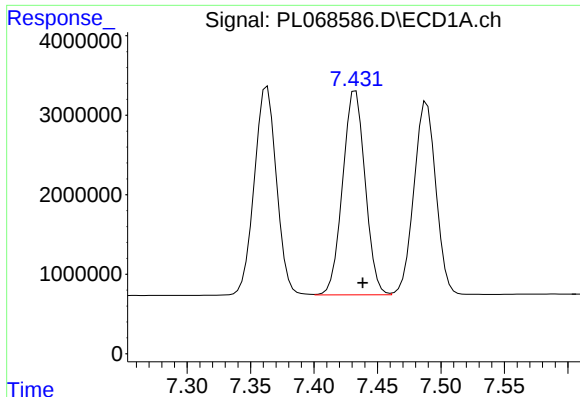

#11 alpha-Chlordane


R.T.: 7.433 min
Delta R.T.: -0.006 min
Response: 31632832
Conc: 55.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

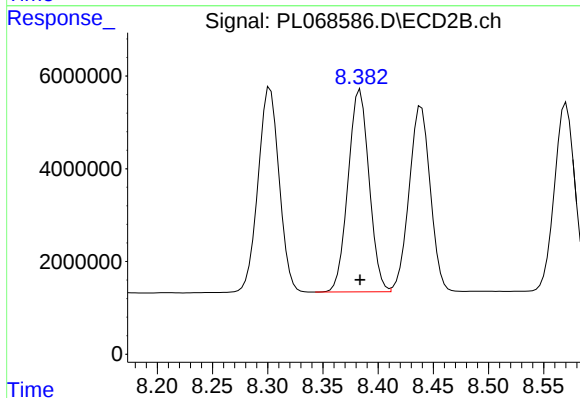


#11 alpha-Chlordane

R.T.: 8.384 min
Delta R.T.: 0.000 min
Response: 57789405
Conc: 51.38 ng/ml

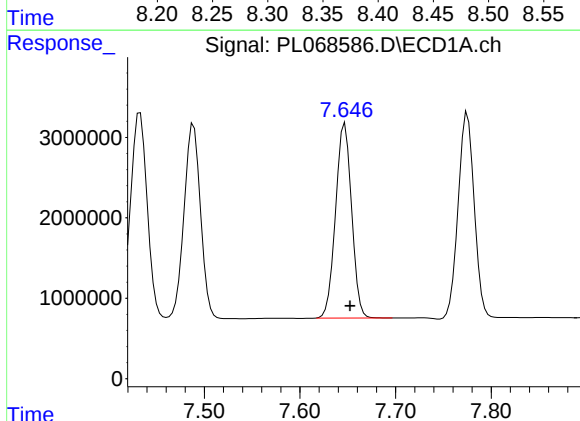


#12 4,4'-DDE

R.T.: 7.647 min
Delta R.T.: -0.005 min
Response: 28198976
Conc: 55.96 ng/ml

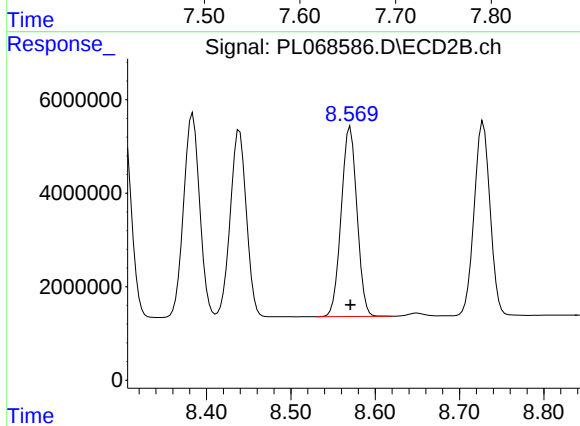

#12 4,4'-DDE


R.T.: 8.570 min
Delta R.T.: 0.000 min
Response: 52730660
Conc: 51.17 ng/ml

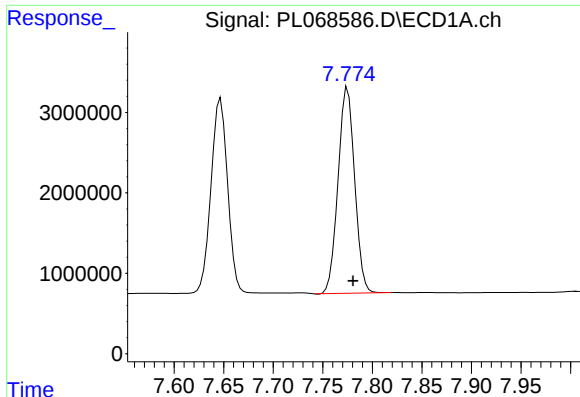

#13 Dieldrin


R.T.: 7.775 min
Delta R.T.: -0.006 min
Response: 29838563
Conc: 55.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

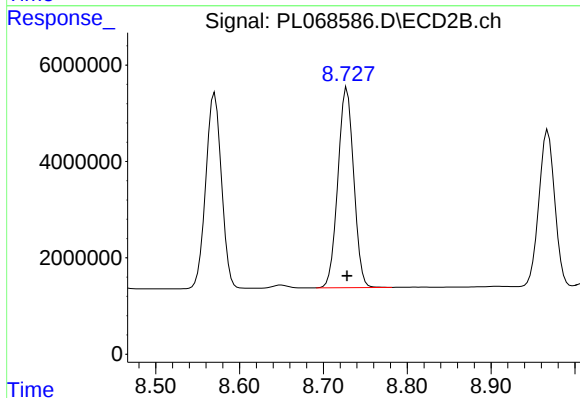


#13 Dieldrin

R.T.: 8.728 min
Delta R.T.: 0.000 min
Response: 54430134
Conc: 51.32 ng/ml

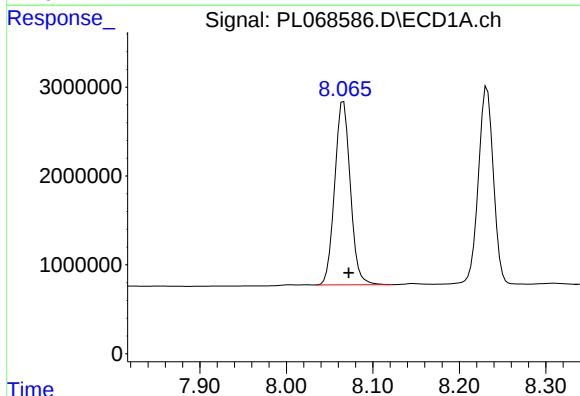


#14 Endrin

R.T.: 8.066 min
Delta R.T.: -0.006 min
Response: 25827383
Conc: 51.65 ng/ml

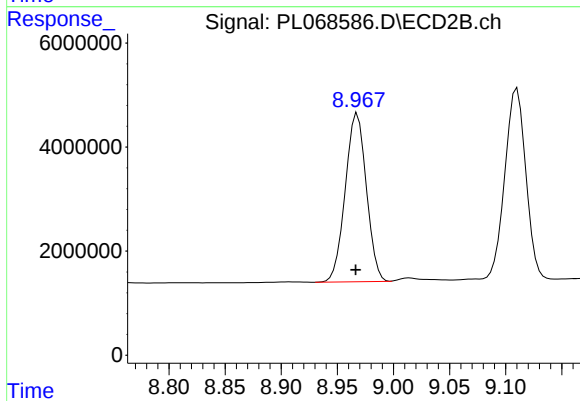

#14 Endrin


R.T.: 8.968 min
Delta R.T.: 0.001 min
Response: 42310887
Conc: 47.32 ng/ml

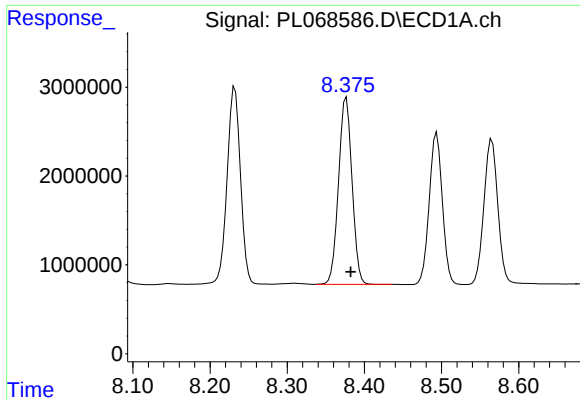

#15 Endosulfan II


R.T.: 8.377 min
Delta R.T.: -0.006 min
Response: 25539770
Conc: 51.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

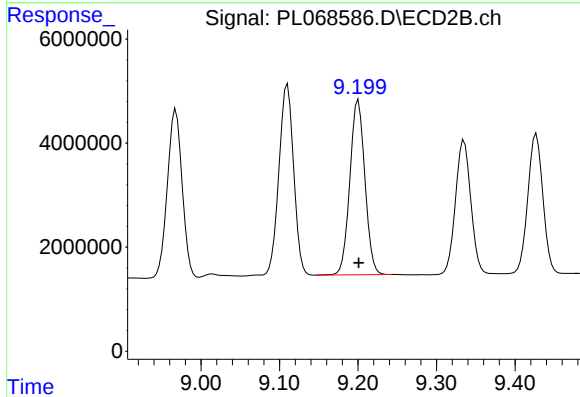


#15 Endosulfan II

R.T.: 9.200 min
Delta R.T.: 0.000 min
Response: 44814277
Conc: 49.44 ng/ml

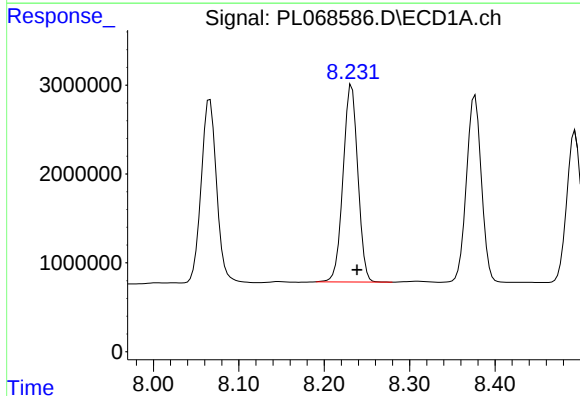


#16 4,4'-DDD

R.T.: 8.232 min
Delta R.T.: -0.006 min
Response: 26661900
Conc: 59.69 ng/ml

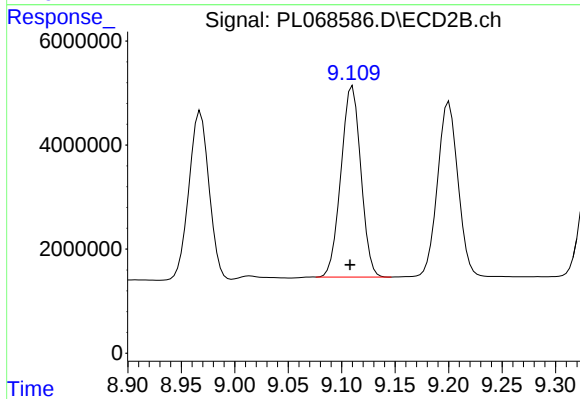

#16 4,4'-DDD


R.T.: 9.110 min
Delta R.T.: 0.002 min
Response: 47560807
Conc: 55.86 ng/ml

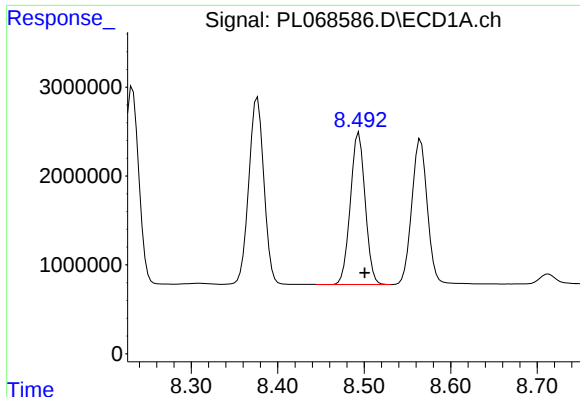

#17 4,4'-DDT


R.T.: 8.494 min
Delta R.T.: -0.007 min
Response: 20213718
Conc: 40.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

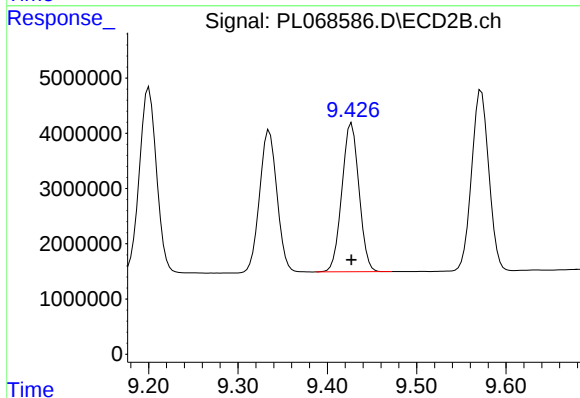


#17 4,4'-DDT

R.T.: 9.427 min
Delta R.T.: 0.000 min
Response: 35793403
Conc: 37.92 ng/ml

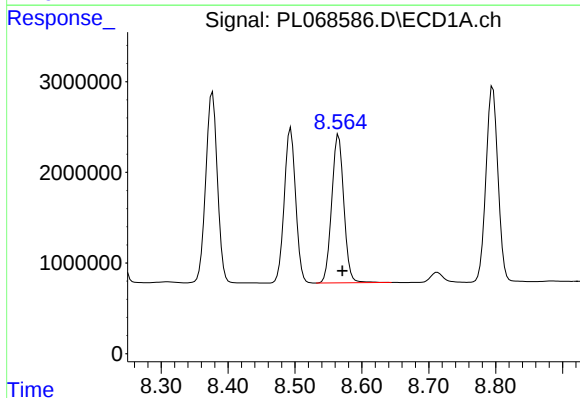


#18 Endrin aldehyde

R.T.: 8.565 min
Delta R.T.: -0.006 min
Response: 20453951
Conc: 51.63 ng/ml

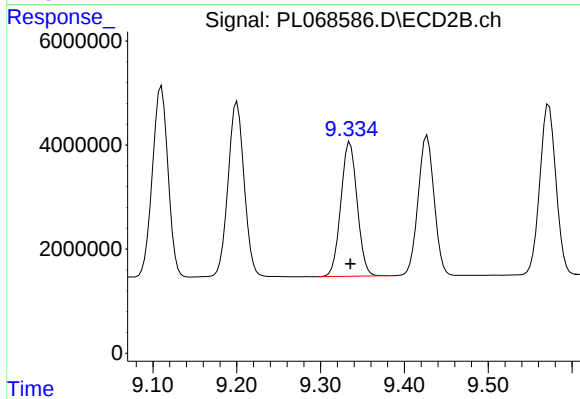

#18 Endrin aldehyde


R.T.: 9.335 min
Delta R.T.: 0.000 min
Response: 34954810
Conc: 48.50 ng/ml

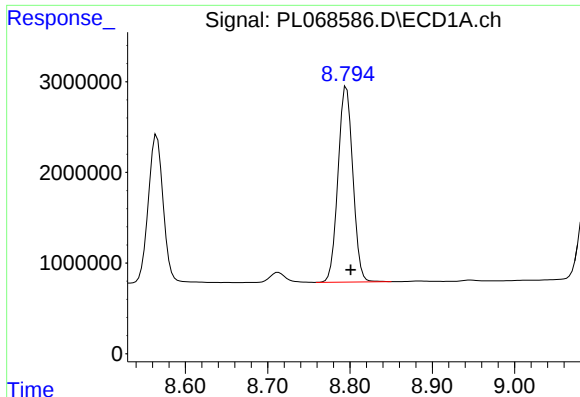

#19 Endosulfan Sulfate


R.T.: 8.796 min
Delta R.T.: -0.005 min
Response: 26997189
Conc: 51.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

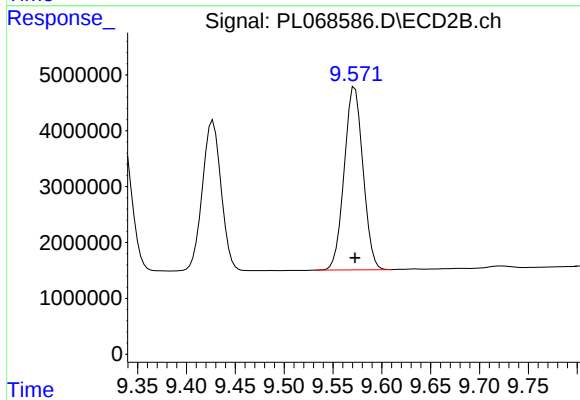


#19 Endosulfan Sulfate

R.T.: 9.572 min
Delta R.T.: 0.000 min
Response: 43806719
Conc: 48.65 ng/ml

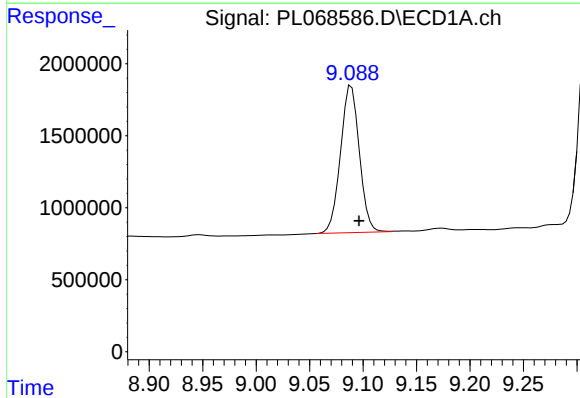


#20 Methoxychlor

R.T.: 9.089 min
Delta R.T.: -0.007 min
Response: 12539457
Conc: 40.09 ng/ml

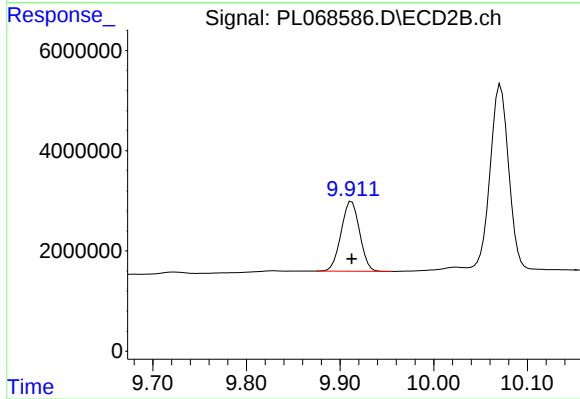

#20 Methoxychlor


R.T.: 9.912 min
Delta R.T.: 0.000 min
Response: 19190194
Conc: 37.77 ng/ml

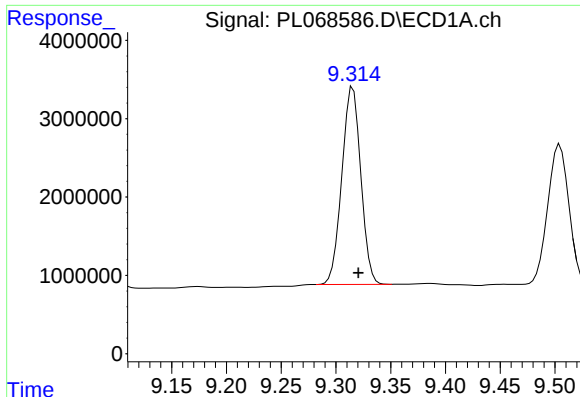

#21 Endrin ketone


R.T.: 9.316 min
Delta R.T.: -0.005 min
Response: 30357182
Conc: 51.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

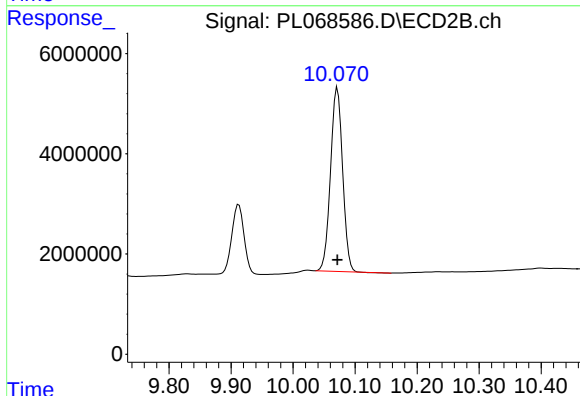


#21 Endrin ketone

R.T.: 10.071 min
Delta R.T.: 0.000 min
Response: 49698833
Conc: 49.83 ng/ml

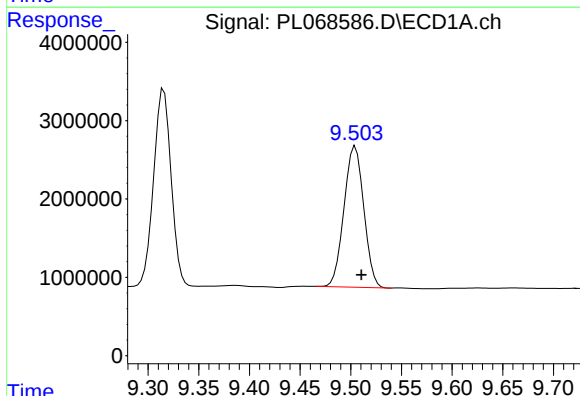


#22 Mirex

R.T.: 9.505 min
Delta R.T.: -0.006 min
Response: 24453597
Conc: 49.52 ng/ml

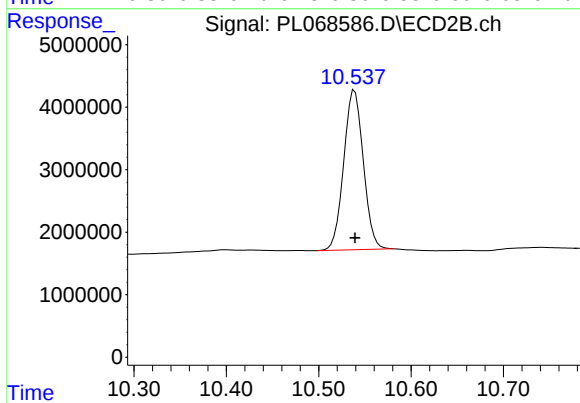

#22 Mirex


R.T.: 10.539 min
Delta R.T.: 0.000 min
Response: 37656883
Conc: 48.68 ng/ml

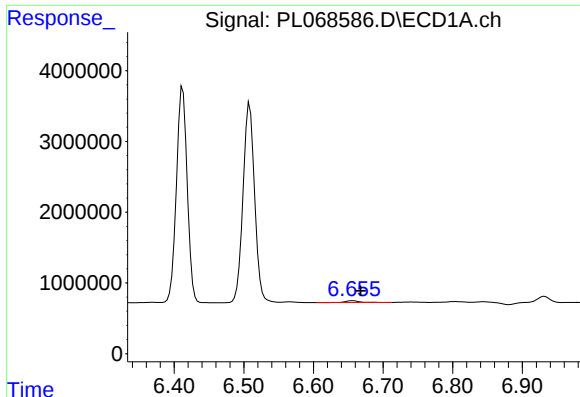

#24 Chlordane-2


R.T.: 6.656 min
Delta R.T.: -0.012 min
Response: 348459
Conc: 16.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

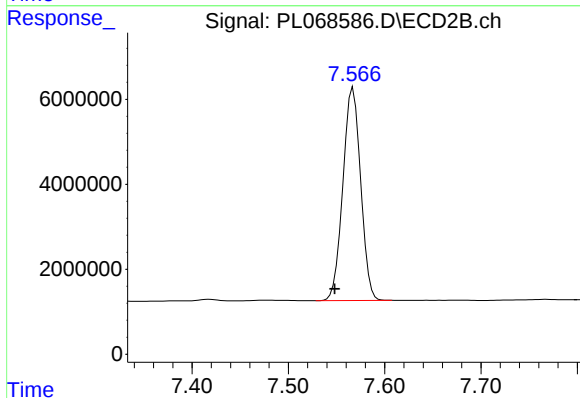


#24 Chlordane-2

R.T.: 7.567 min
Delta R.T.: 0.019 min
Response: 63971498
Conc: 1537.59 ng/ml

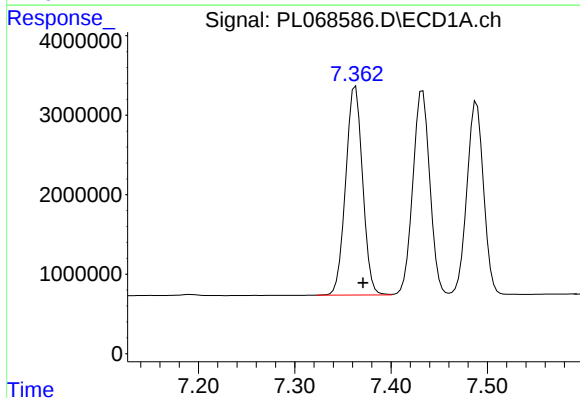


#25 Chlordane-3

R.T.: 7.363 min
Delta R.T.: -0.008 min
Response: 31873727
Conc: 591.86 ng/ml

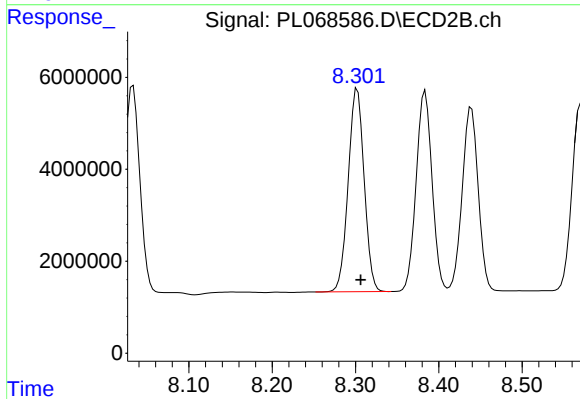

#25 Chlordane-3


R.T.: 8.302 min
Delta R.T.: -0.004 min
Response: 58649484
Conc: 378.70 ng/ml

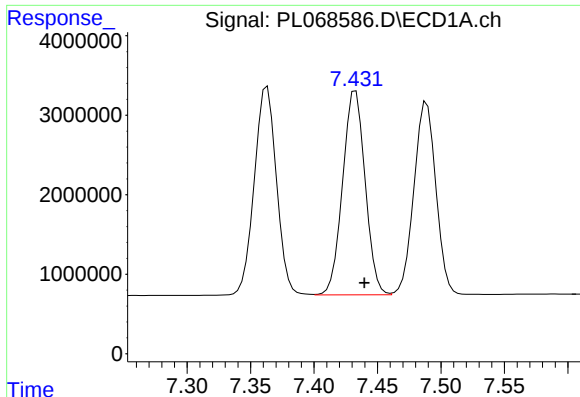

#26 Chlordane-4


R.T.: 7.433 min
Delta R.T.: -0.007 min
Response: 31632832
Conc: 560.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

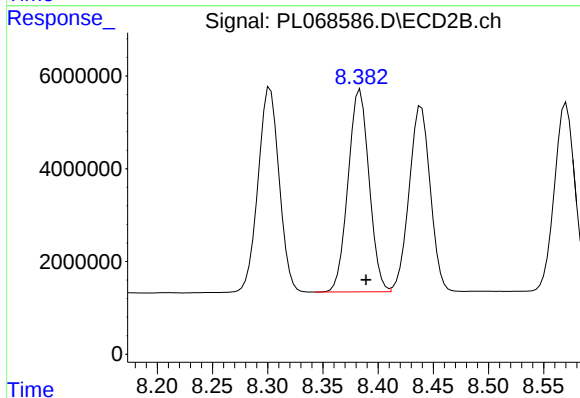


#26 Chlordane-4

R.T.: 8.384 min
Delta R.T.: -0.005 min
Response: 57789405
Conc: 308.24 ng/ml

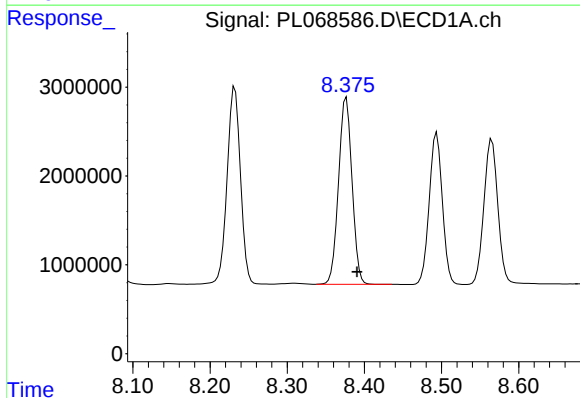


#27 Chlordane-5

R.T.: 8.377 min
Delta R.T.: -0.014 min
Response: 25539770
Conc: 1268.98 ng/ml

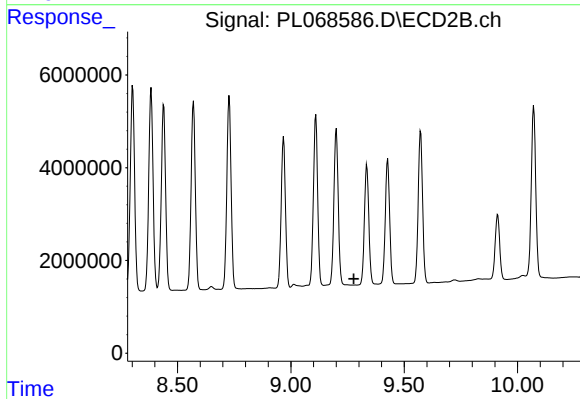

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.277 min
Response: 0
Conc: N.D.

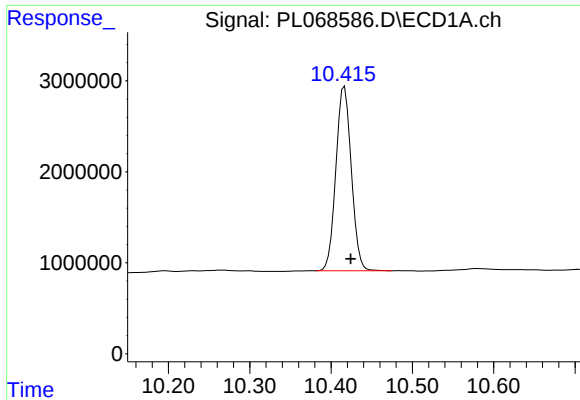

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.008 min
Response: 26702170
Conc: 47.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

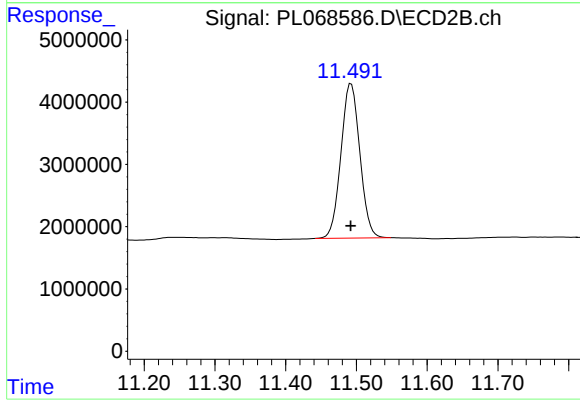

#28 Decachlorobiphenyl

R.T.: 11.493 min
Delta R.T.: 0.000 min
Response: 46121035
Conc: 51.71 ng/ml