

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072922\
 Data File : PL076734.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2022 14:11
 Operator : AR\AJ
 Sample : N3895-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 00:06:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	2.644	11360602	28531494	11.008	9.619
28)	SA Decachlor...	8.916	7.753	11742486	30383723	13.314	11.837
Target Compounds							
10)	B gamma-Chl...	0.000	4.802f	0	396546	N.D.	0.124 #
11)	B alpha-Chl...	5.907	0.000	213229	0	0.193	N.D. #
12)	B 4,4'-DDE	6.084	5.077	6718629	18533486	6.845	6.236
13)	MA Dieldrin	0.000	5.205	0	581680	N.D.	0.187 #
14)	MA Endrin	0.000	5.490f	0	1695804	N.D.	0.675 #
16)	A 4,4'-DDD	6.609	5.629	647536	998005	0.777	0.421 #
17)	MA 4,4'-DDT	6.920	5.878	3204099	7449845	3.526	3.101
19)	B Endosulfa...	0.000	6.170	0	65985	N.D.	0.027 #
20)	A Methoxychlor	0.000	6.428f	0	582548	N.D.	0.445 #
25)	Chlordane-3	0.000	4.802f	0	396546	N.D.	1.401 #
26)	Chlordane-4	5.907	0.000	213229	0	1.243	N.D. #
27)	Chlordane-5	0.000	5.549	0	550457	N.D.	6.875 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072922\
Data File : PL076734.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2022 14:11
Operator : AR\AJ
Sample : N3895-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 00:06:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

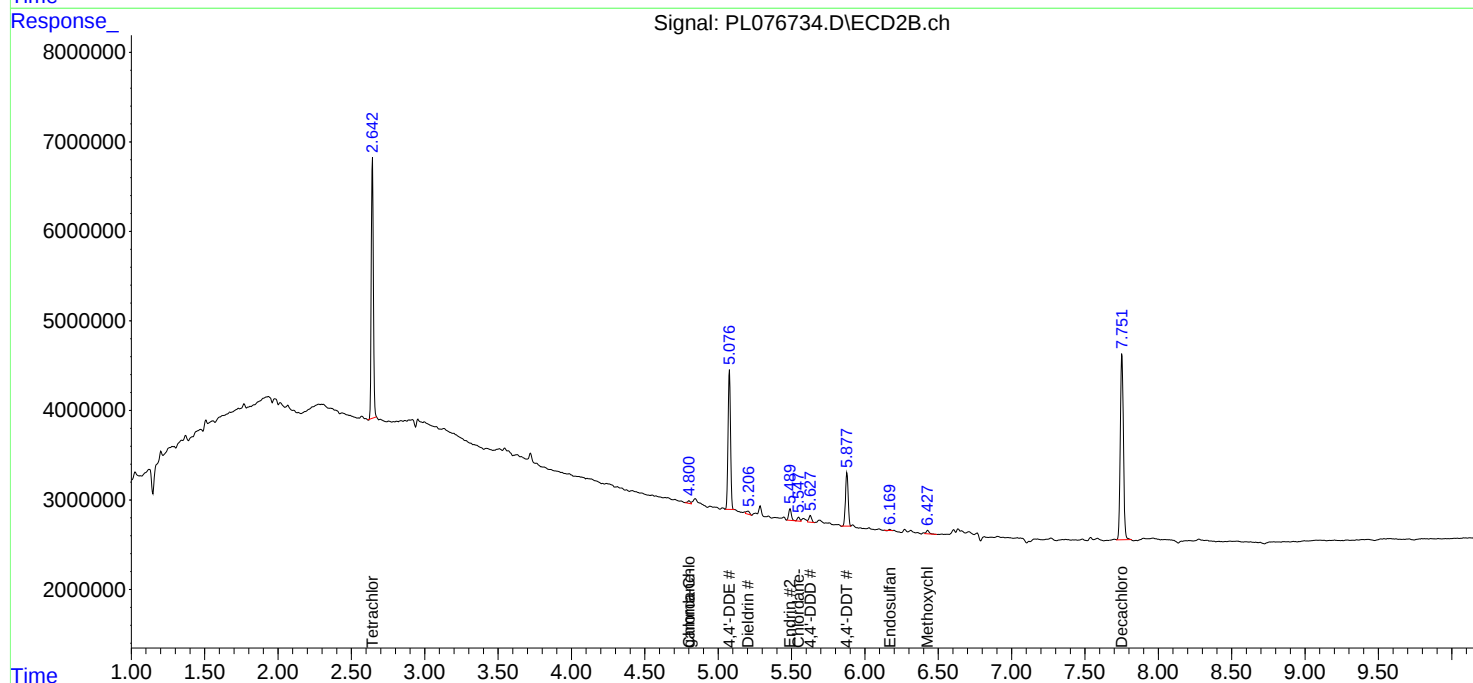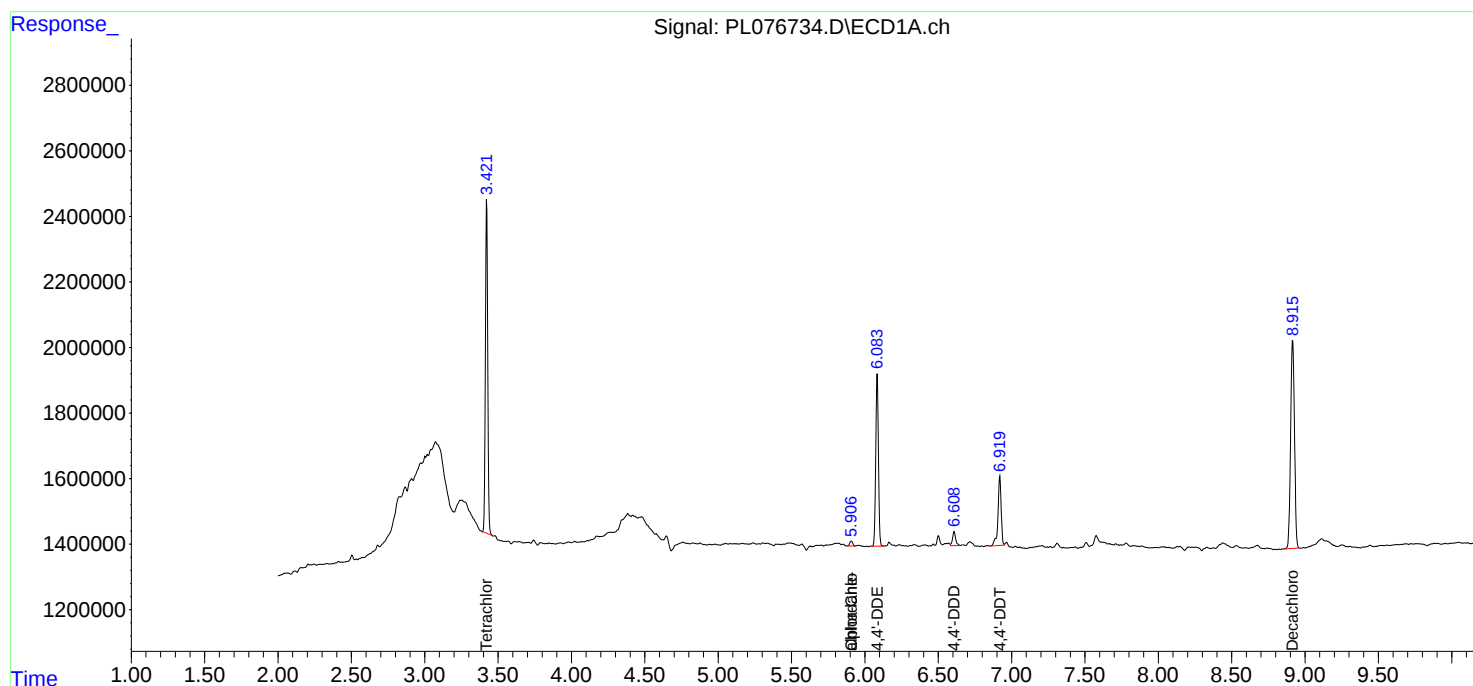


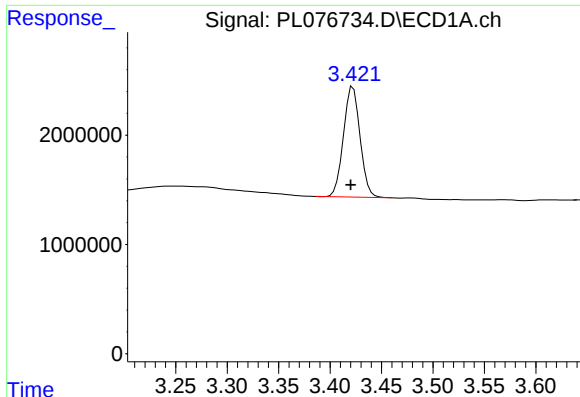

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.002 min
Response: 11360602
Conc: 11.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

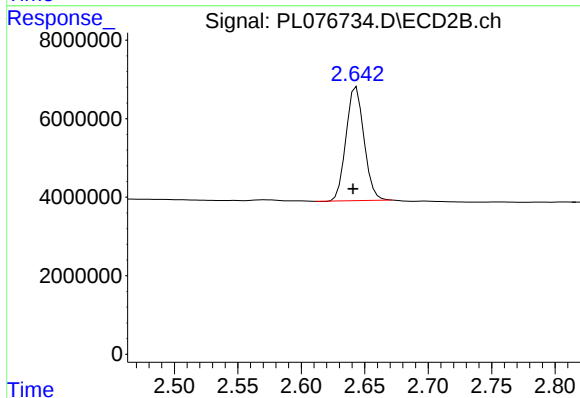


#1 Tetrachloro-m-xylene

R.T.: 2.644 min
Delta R.T.: 0.003 min
Response: 28531494
Conc: 9.62 ng/ml

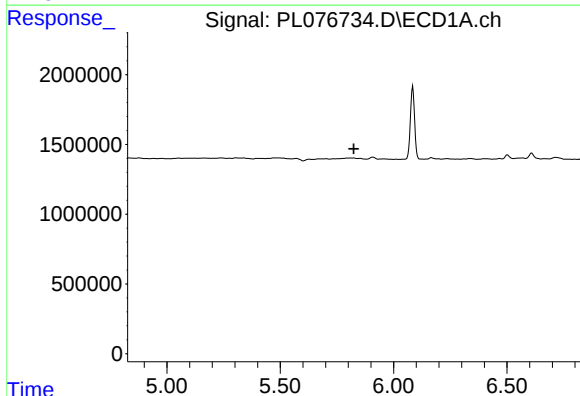


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.825 min
Response: 0
Conc: N.D.

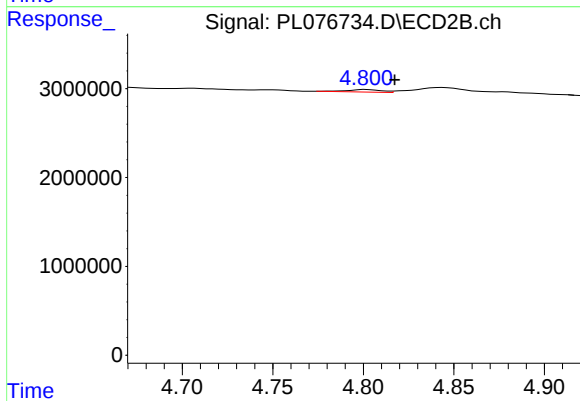

#10 gamma-Chlordane


R.T.: 4.802 min
Delta R.T.: -0.016 min
Response: 396546
Conc: 0.12 ng/ml

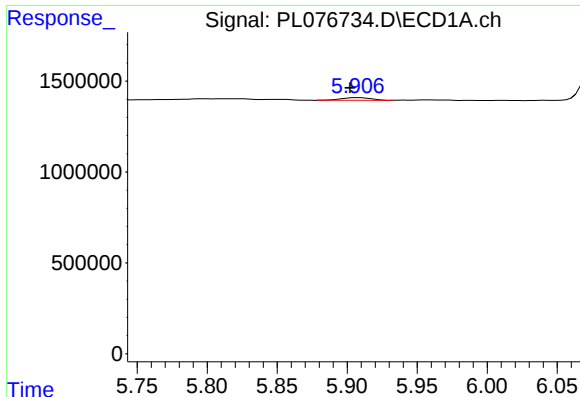

#11 alpha-Chlordane


R.T.: 5.907 min
Delta R.T.: 0.005 min
Response: 213229
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

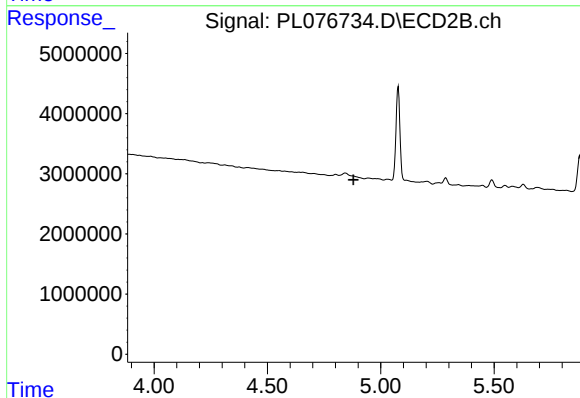


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.880 min
Response: 0
Conc: N.D.

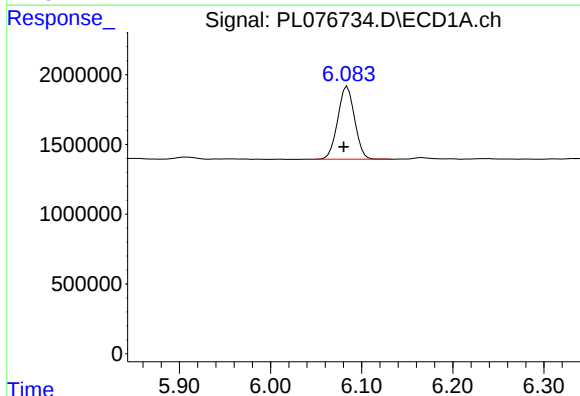


#12 4,4'-DDE

R.T.: 6.084 min
Delta R.T.: 0.004 min
Response: 6718629
Conc: 6.85 ng/ml

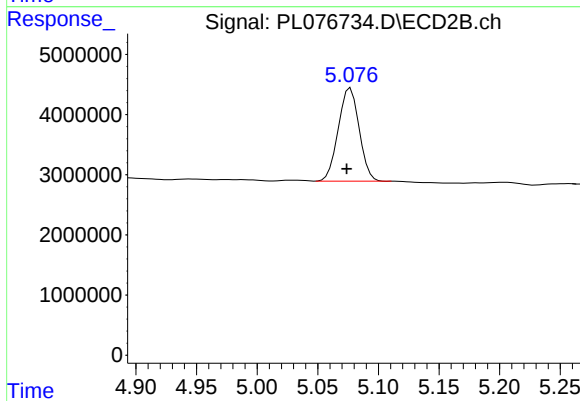

#12 4,4'-DDE


R.T.: 5.077 min
Delta R.T.: 0.003 min
Response: 18533486
Conc: 6.24 ng/ml

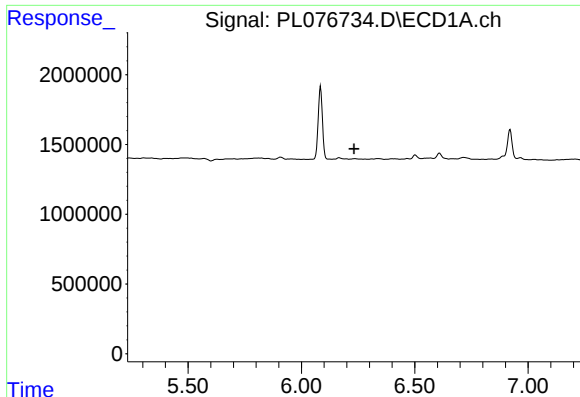

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.233 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

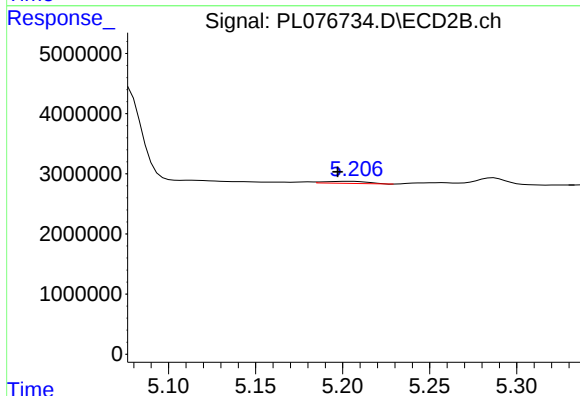


#13 Dieldrin

R.T.: 5.205 min
Delta R.T.: 0.008 min
Response: 581680
Conc: 0.19 ng/ml

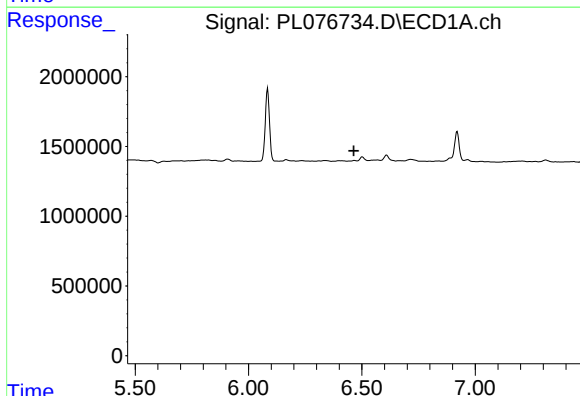


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.464 min
Response: 0
Conc: N.D.

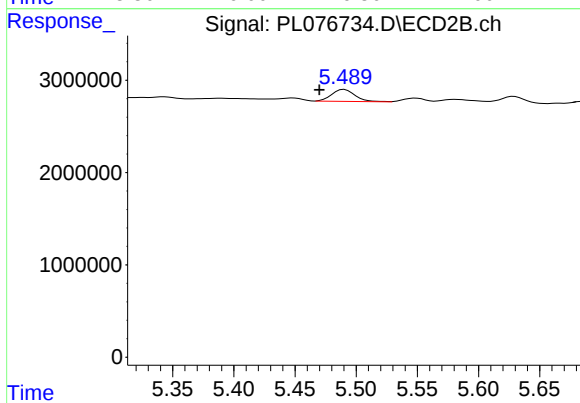

#14 Endrin


R.T.: 5.490 min
Delta R.T.: 0.020 min
Response: 1695804
Conc: 0.68 ng/ml

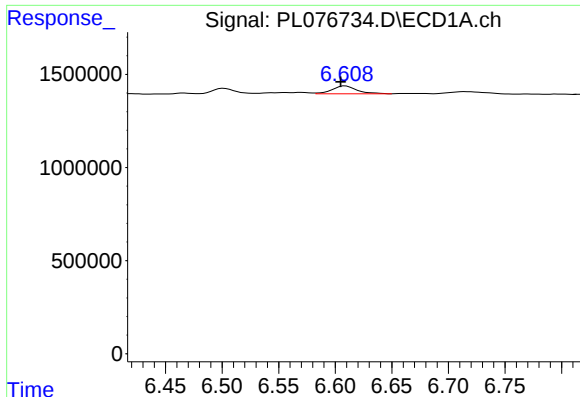

#16 4,4'-DDD


R.T.: 6.609 min
Delta R.T.: 0.004 min
Response: 647536
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

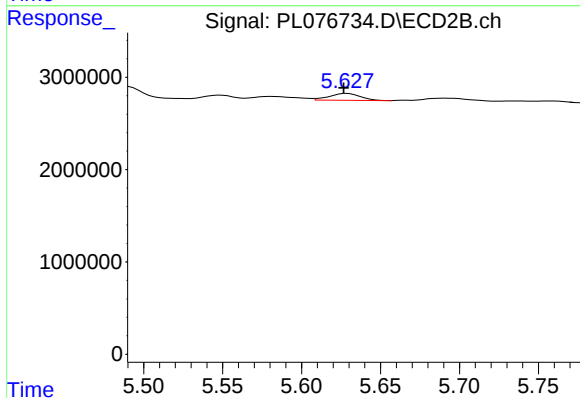


#16 4,4'-DDD

R.T.: 5.629 min
Delta R.T.: 0.002 min
Response: 998005
Conc: 0.42 ng/ml

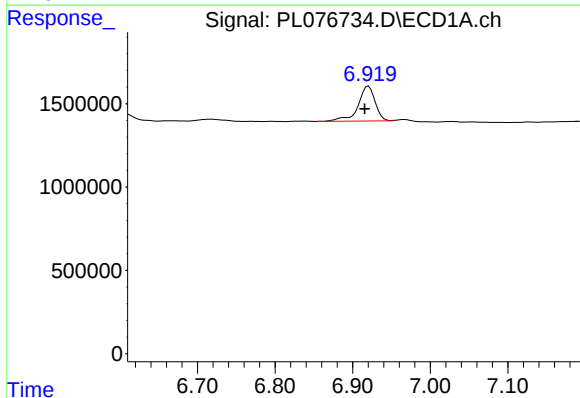


#17 4,4'-DDT

R.T.: 6.920 min
Delta R.T.: 0.005 min
Response: 3204099
Conc: 3.53 ng/ml

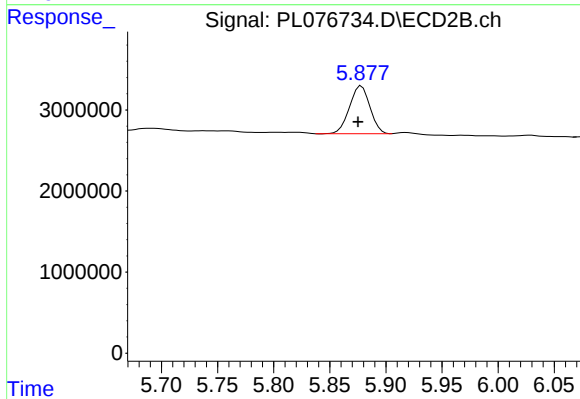

#17 4,4'-DDT


R.T.: 5.878 min
Delta R.T.: 0.003 min
Response: 7449845
Conc: 3.10 ng/ml

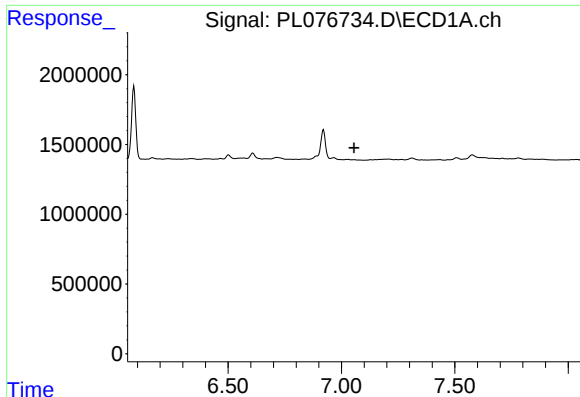

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.055 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

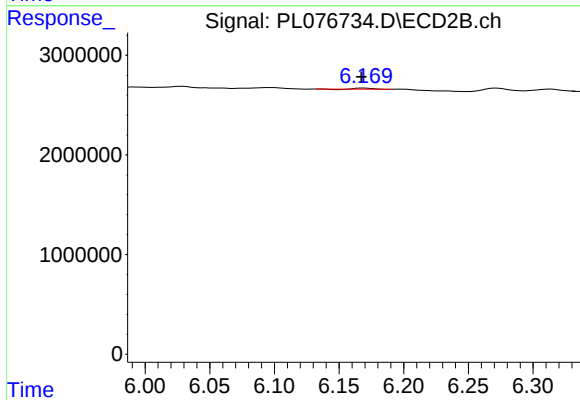


#19 Endosulfan Sulfate

R.T.: 6.170 min
Delta R.T.: 0.003 min
Response: 65985
Conc: 0.03 ng/ml

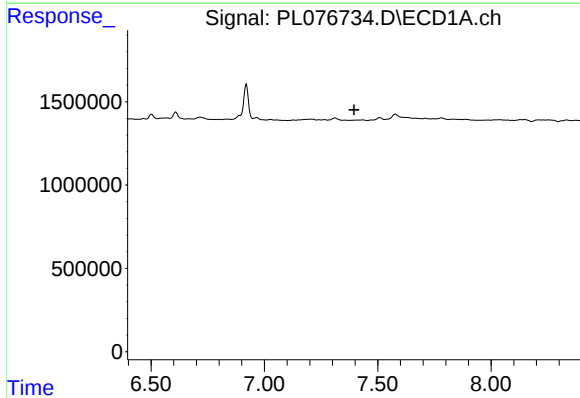


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.396 min
Response: 0
Conc: N.D.

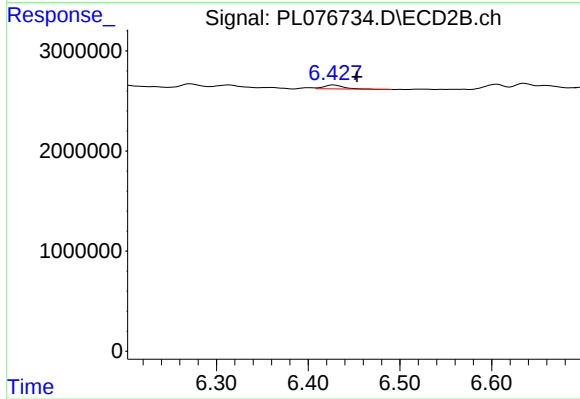

#20 Methoxychlor


R.T.: 6.428 min
Delta R.T.: -0.025 min
Response: 582548
Conc: 0.45 ng/ml

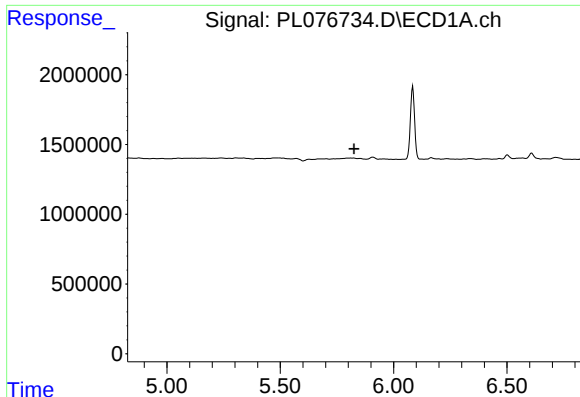

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.825 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

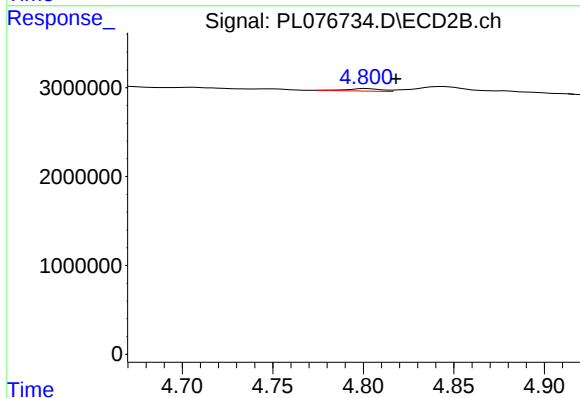


#25 Chlordane-3

R.T.: 4.802 min
Delta R.T.: -0.016 min
Response: 396546
Conc: 1.40 ng/ml

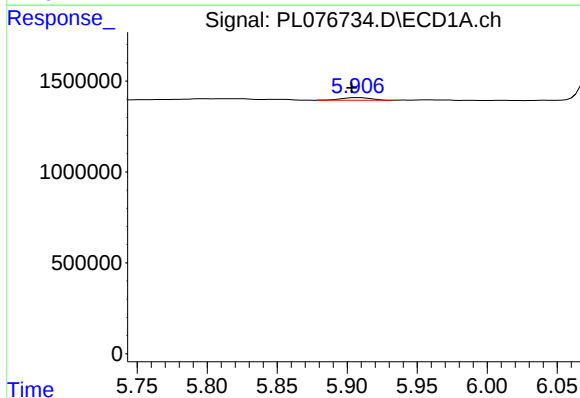


#26 Chlordane-4

R.T.: 5.907 min
Delta R.T.: 0.004 min
Response: 213229
Conc: 1.24 ng/ml

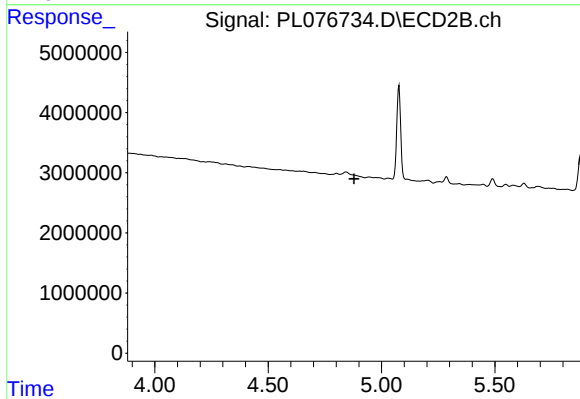

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 4.879 min
Response: 0
Conc: N.D.

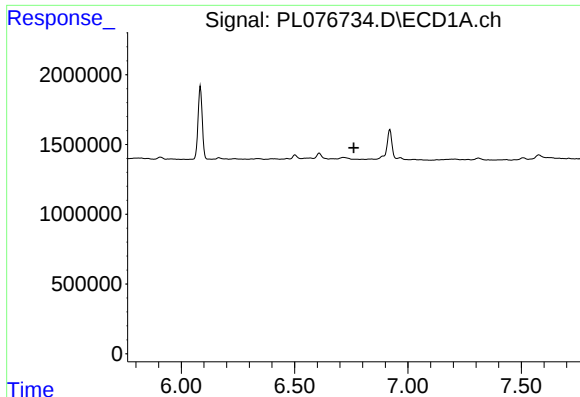

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.761 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

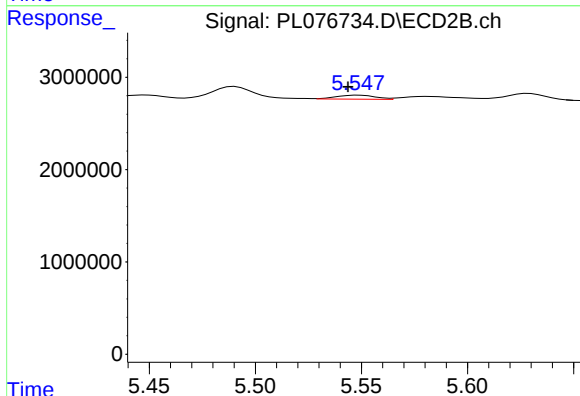


#27 Chlordane-5

R.T.: 5.549 min
Delta R.T.: 0.005 min
Response: 550457
Conc: 6.87 ng/ml

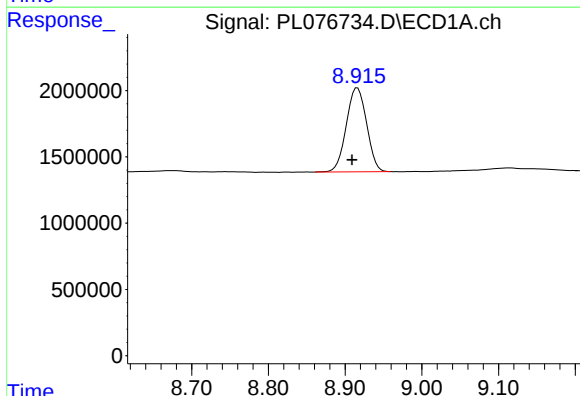

#28 Decachlorobiphenyl

R.T.: 8.916 min
Delta R.T.: 0.007 min
Response: 11742486
Conc: 13.31 ng/ml

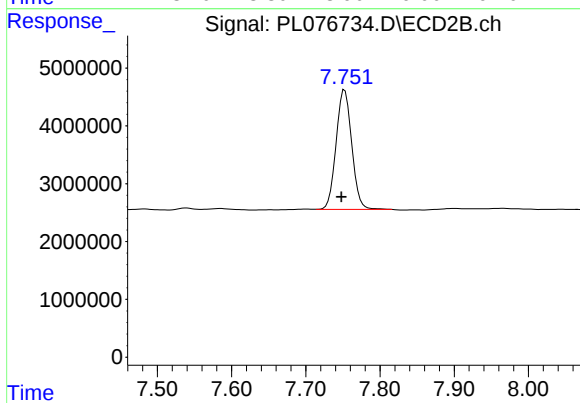

#28 Decachlorobiphenyl

R.T.: 7.753 min
Delta R.T.: 0.004 min
Response: 30383723
Conc: 11.84 ng/ml