

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072922\
 Data File : PL076733.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2022 13:57
 Operator : AR\AJ
 Sample : N3895-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RVE-48

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/29/2022
 Supervised By : Ankita Jodhani 07/29/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 00:05:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 26 05:22:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.642	12413742	31986103	12.028m	10.783m
28)	SA Decachlor...	8.916	7.753	12414891	32493621	14.077	12.659

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072922\
Data File : PL076733.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2022 13:57
Operator : AR\AJ
Sample : N3895-10
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RVE-48


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/29/2022
Supervised By : Ankita Jodhani 07/29/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 00:05:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072622.M
Quant Title : GC Extractables
QLast Update : Tue Jul 26 05:22:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

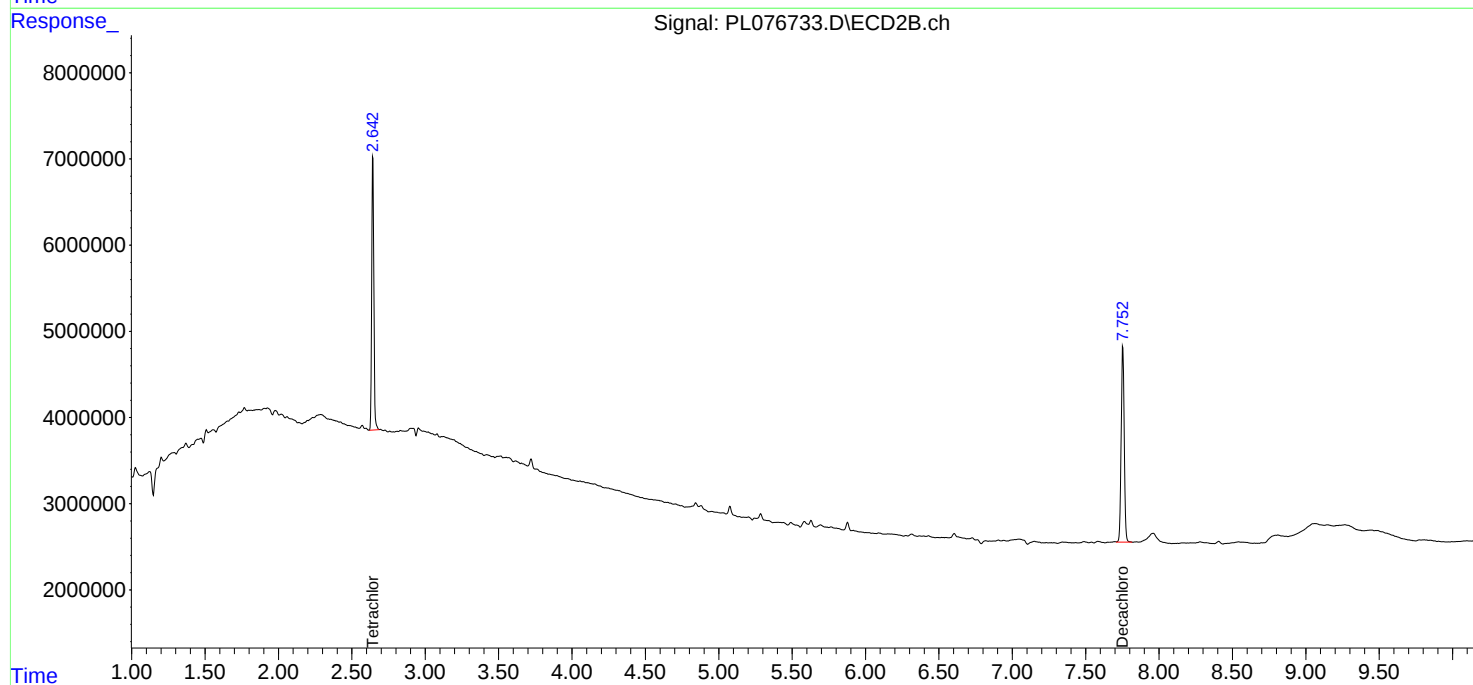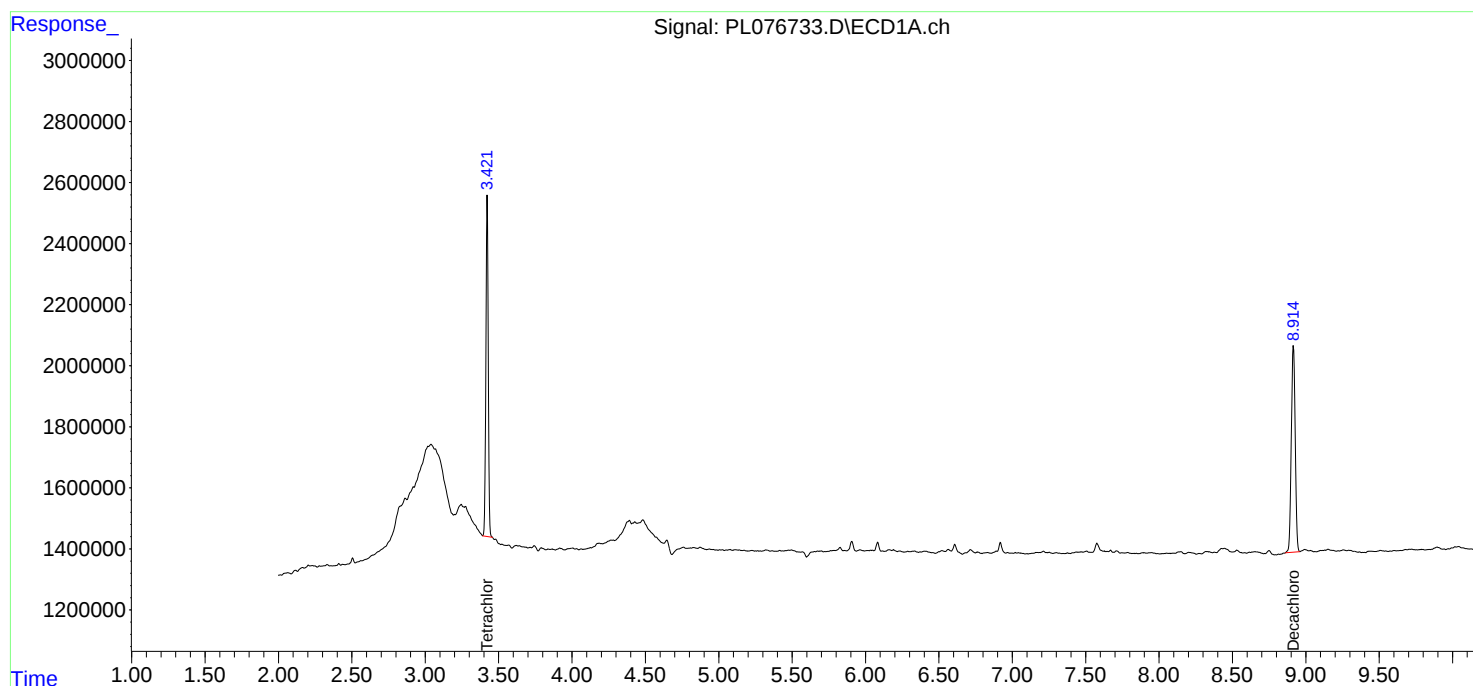

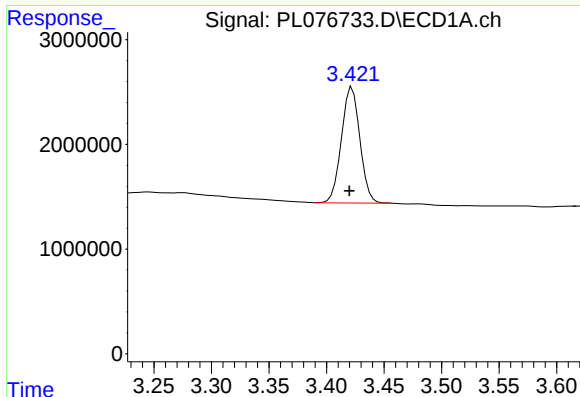


#1 Tetrachloro-m-xylene

R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 12413742
Conc: 12.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
RVE-48


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/29/2022
Supervised By :Ankita Jodhani 07/29/2022

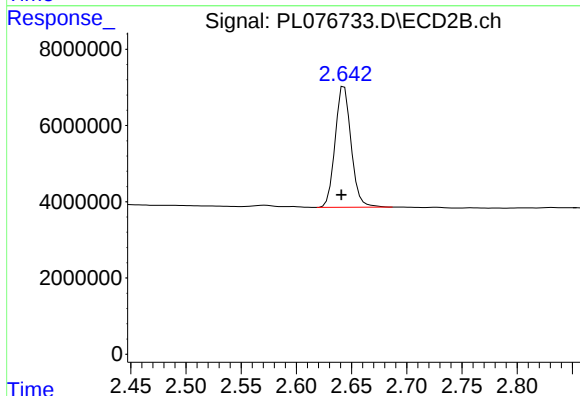


#1 Tetrachloro-m-xylene

R.T.: 2.642 min
Delta R.T.: 0.001 min
Response: 31986103
Conc: 10.78 ng/ml m

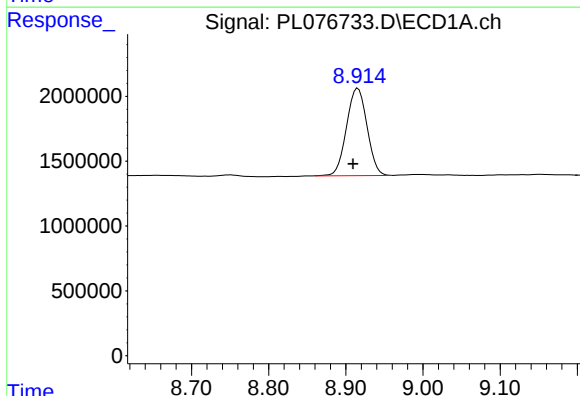

#28 Decachlorobiphenyl

R.T.: 8.916 min
Delta R.T.: 0.006 min
Response: 12414891
Conc: 14.08 ng/ml

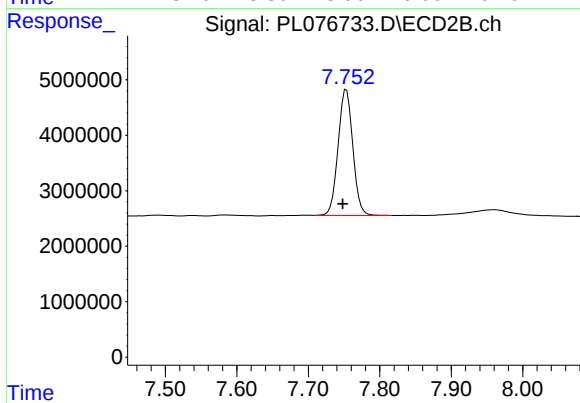

#28 Decachlorobiphenyl

R.T.: 7.753 min
Delta R.T.: 0.005 min
Response: 32493621
Conc: 12.66 ng/ml