

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072925\
 Data File : PL096614.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2025 10:31
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:49:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
8) B	Heptachlo...	5.655	0.000	25701727	0	6.664 N.D. #
13) MA	Dieldrin	0.000	5.425	0 17904132	N.D.	3.031 #
14) MA	Endrin	0.000	5.716	0 37723985	N.D.	6.978 #
24)	Chlordane-2	0.000	4.408	0 32959574	N.D.	135.865 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072925\
Data File : PL096614.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2025 10:31
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:49:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

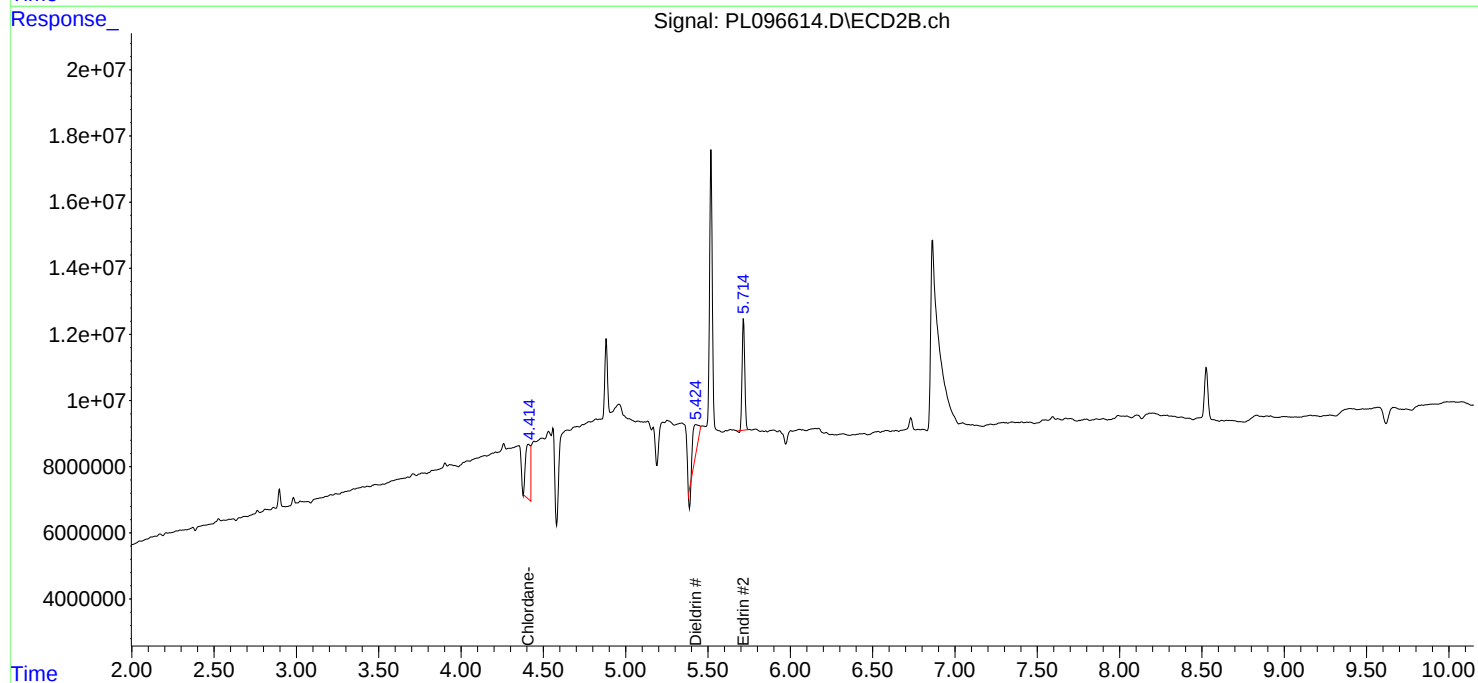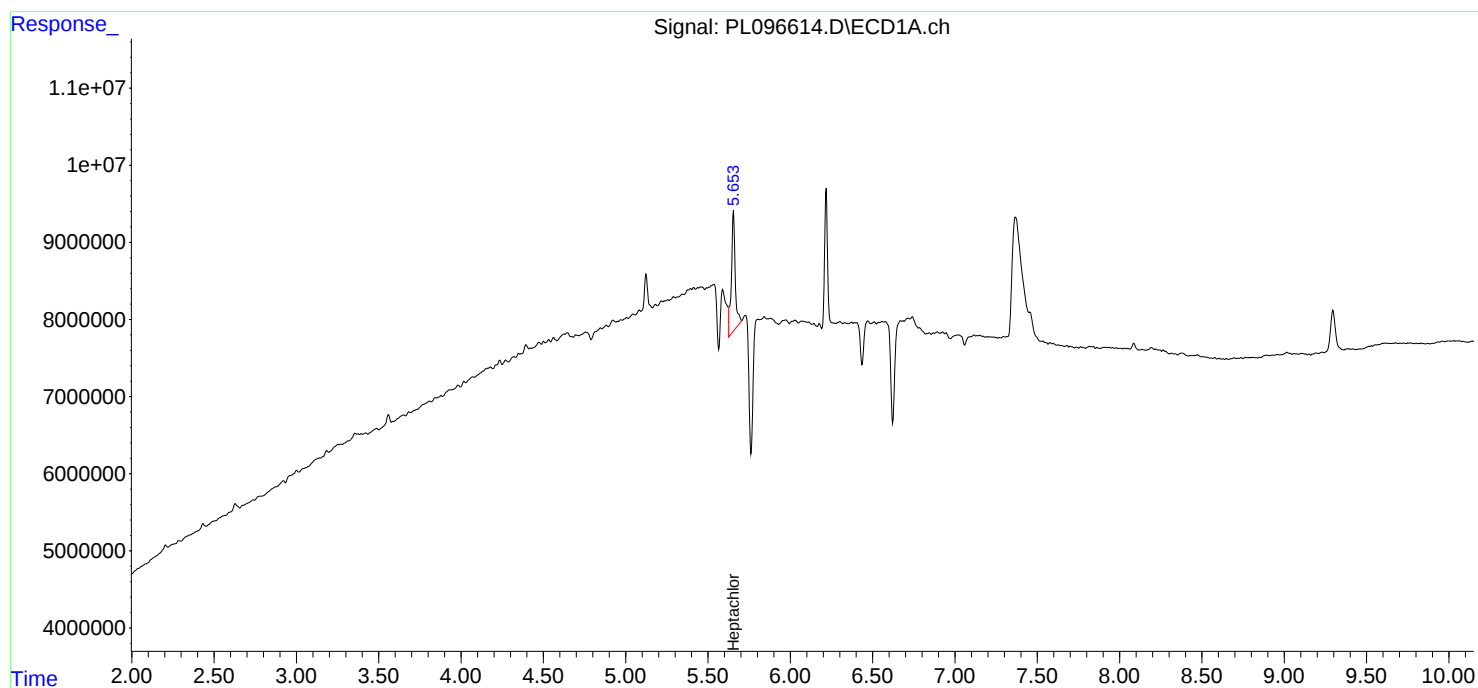


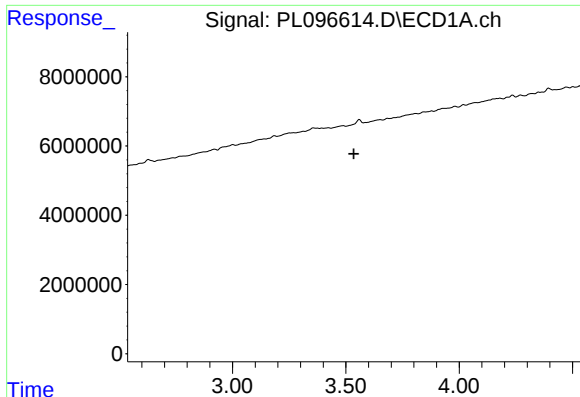

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.535 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

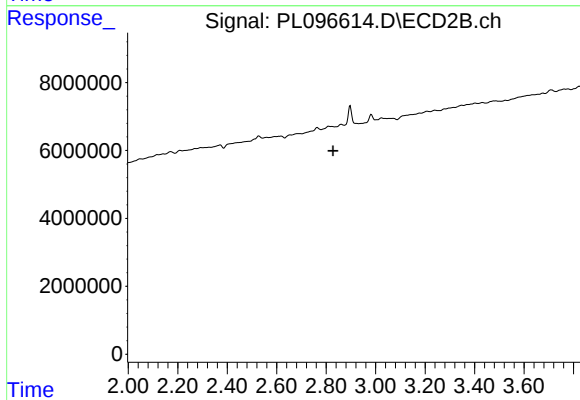


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.828 min
Response: 0
Conc: N.D.

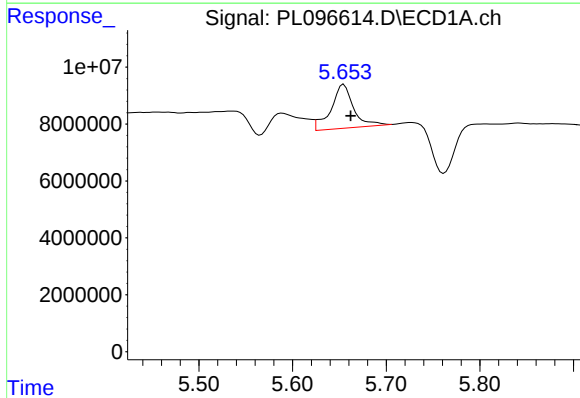


#8 Heptachlor epoxide

R.T.: 5.655 min
Delta R.T.: -0.008 min
Response: 25701727
Conc: 6.66 ng/ml

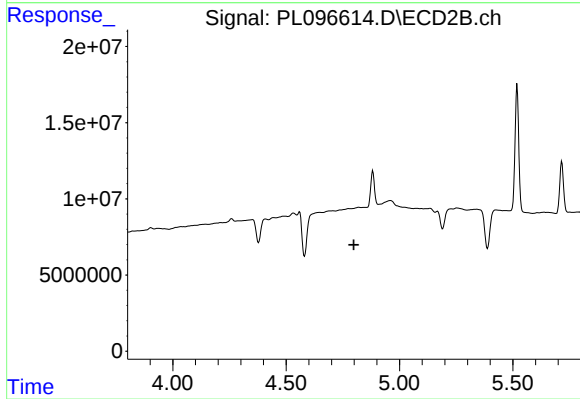

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.799 min
Response: 0
Conc: N.D.

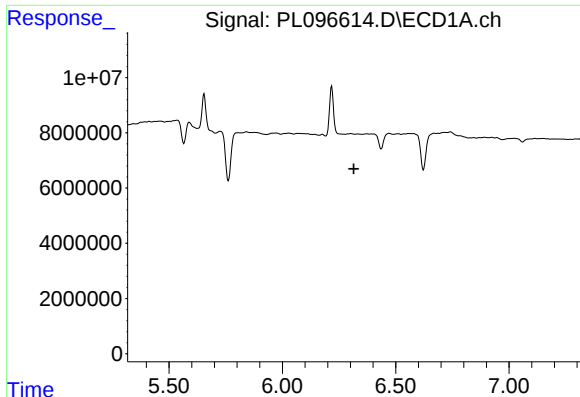

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.316 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

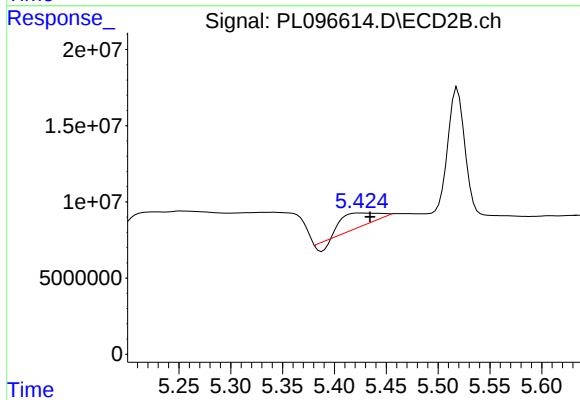


#13 Dieldrin

R.T.: 5.425 min
Delta R.T.: -0.009 min
Response: 17904132
Conc: 3.03 ng/ml

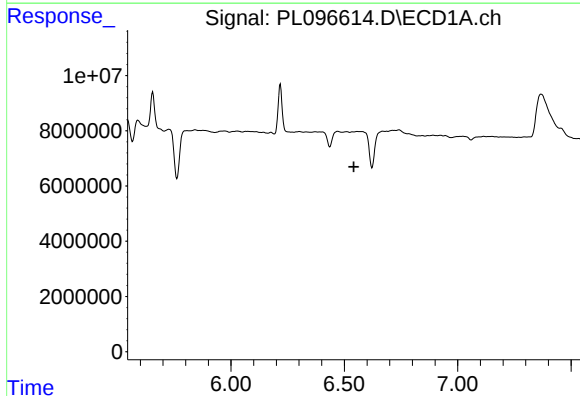


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.542 min
Response: 0
Conc: N.D.

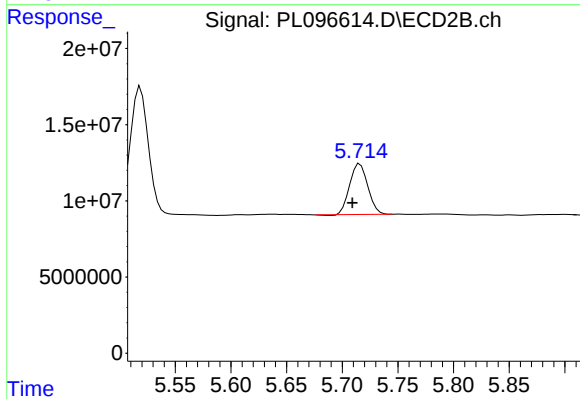

#14 Endrin


R.T.: 5.716 min
Delta R.T.: 0.007 min
Response: 37723985
Conc: 6.98 ng/ml

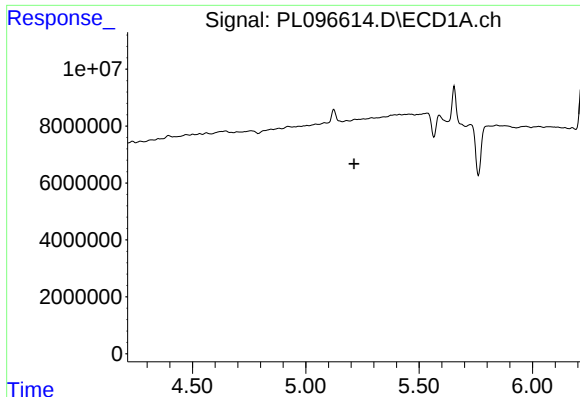

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

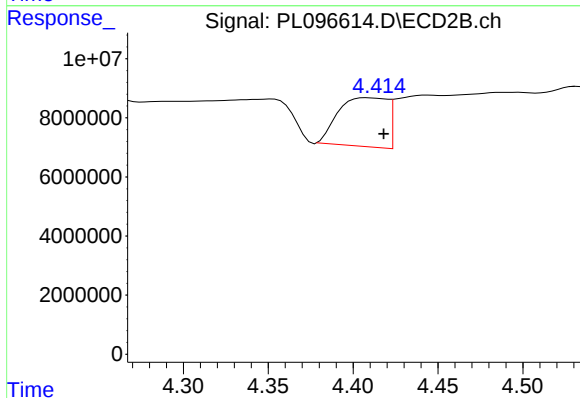


#24 Chlordane-2

R.T.: 4.408 min
Delta R.T.: -0.010 min
Response: 32959574
Conc: 135.86 ng/ml

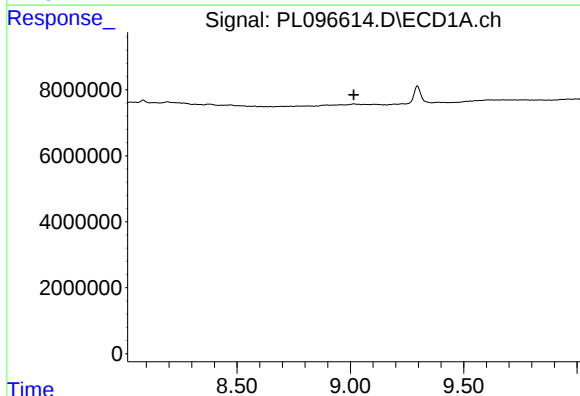

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.016 min
Response: 0
Conc: N.D.

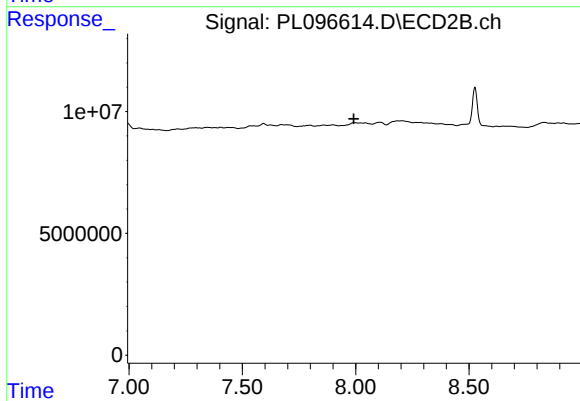

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.