

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072925\
 Data File : PL096622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jul 2025 16:22
 Operator : AR\AJ
 Sample : Q2709-01MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 7211935-295MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 30 01:51:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:58:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.534	2.827	51700368	55422220	16.254	11.600 #
28)	SA Decachlor...	9.017	7.992	32134065	59381298	13.475	13.688
Target Compounds							
2)	A alpha-BHC	3.982	3.332	209.0E6	297.8E6	45.180	42.084
3)	MA gamma-BHC...	4.311	3.664	191.7E6	270.1E6	43.331	40.897
4)	MA Heptachlor	4.903	4.013	181.2E6	265.3E6	43.607	39.822
5)	MB Aldrin	5.243	4.296	180.8E6	244.5E6	42.028	39.390
6)	B beta-BHC	4.497	3.961	79850923	110.5E6	44.240	39.170
7)	B delta-BHC	0.000	4.194	0	257.0E6	N.D.	39.701 #
8)	B Heptachlo...	5.663	4.798	171.0E6	228.4E6	44.349	39.992
9)	A Endosulfan I	6.044	5.169	159.9E6	218.0E6	44.474	39.402
10)	B gamma-Chl...	5.916	5.050	170.6E6	237.9E6	44.833	40.455
11)	B alpha-Chl...	5.997	5.114	170.1E6	232.1E6	44.135	39.340
12)	B 4,4'-DDE	6.167	5.303	138.9E6	224.0E6	43.259	40.623
13)	MA Dieldrin	6.316	5.434	166.8E6	243.1E6	44.952	41.165
14)	MA Endrin	6.543	5.708	142.7E6	233.9E6	47.131	43.274
15)	B Endosulfa...	6.755	6.000	144.7E6	227.1E6	45.183	44.209
16)	A 4,4'-DDD	6.675	5.855	117.2E6	199.2E6	46.339	42.332
17)	MA 4,4'-DDT	6.990	6.108	137.7E6	220.5E6	48.015	43.591
18)	B Endrin al...	6.884	6.179	112.5E6	182.0E6	52.447	48.926
19)	B Endosulfa...	7.118	6.402	137.0E6	235.1E6	47.670	46.214
20)	A Methoxychlor	7.463	6.681	75439028	127.1E6	51.377	46.386
21)	B Endrin ke...	7.598	6.907	146.7E6	262.2E6	48.791	47.077
22)	Mirex	8.077	7.097	126.0E6	206.1E6	50.805	47.269
24)	Chlordane-2	5.243f	0.000	180.8E6	0	1032.889	N.D. #
25)	Chlordane-3	5.916	5.050	170.6E6	237.9E6	255.416	342.125 #
26)	Chlordane-4	5.997	5.114	170.1E6	232.1E6	205.540	372.890 #
27)	Chlordane-5	0.000	6.000	0	227.1E6	N.D.	890.065 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072925\
Data File : PL096622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jul 2025 16:22
Operator : AR\AJ
Sample : Q2709-01MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 30 01:51:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:58:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

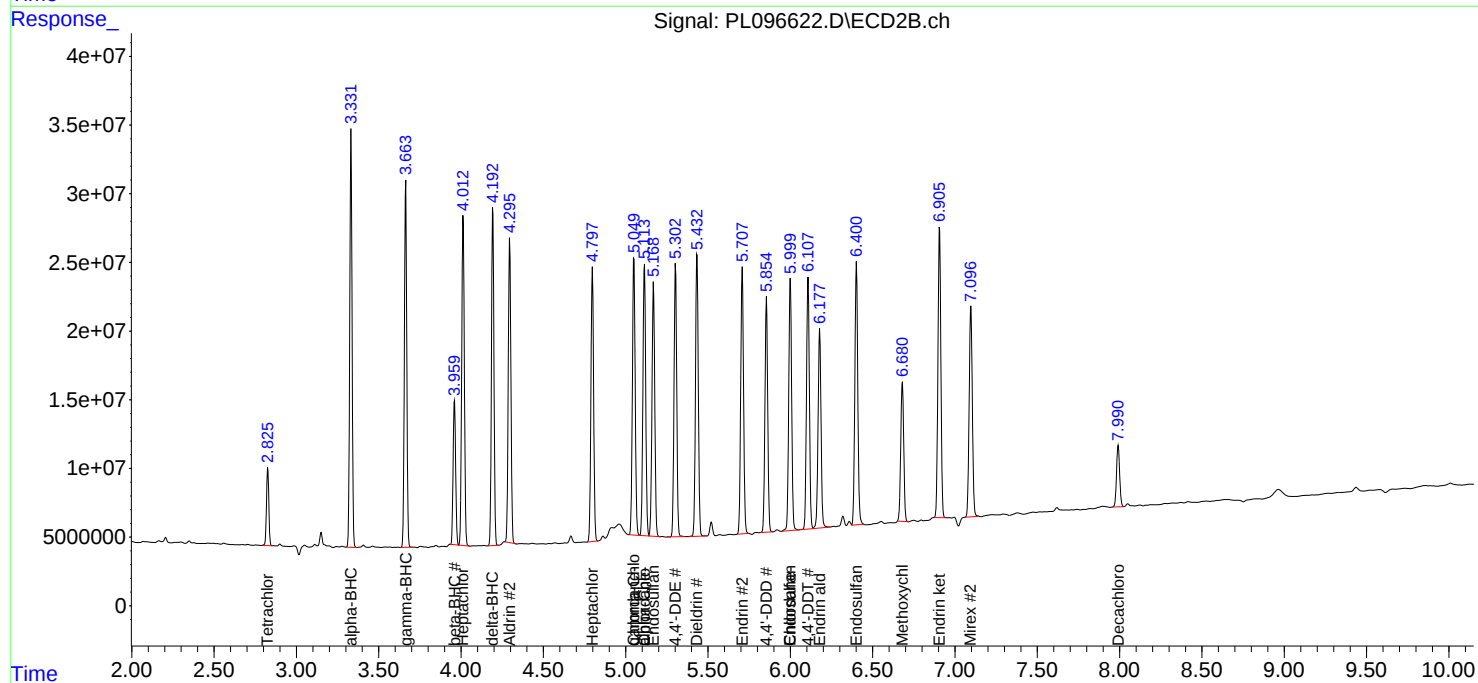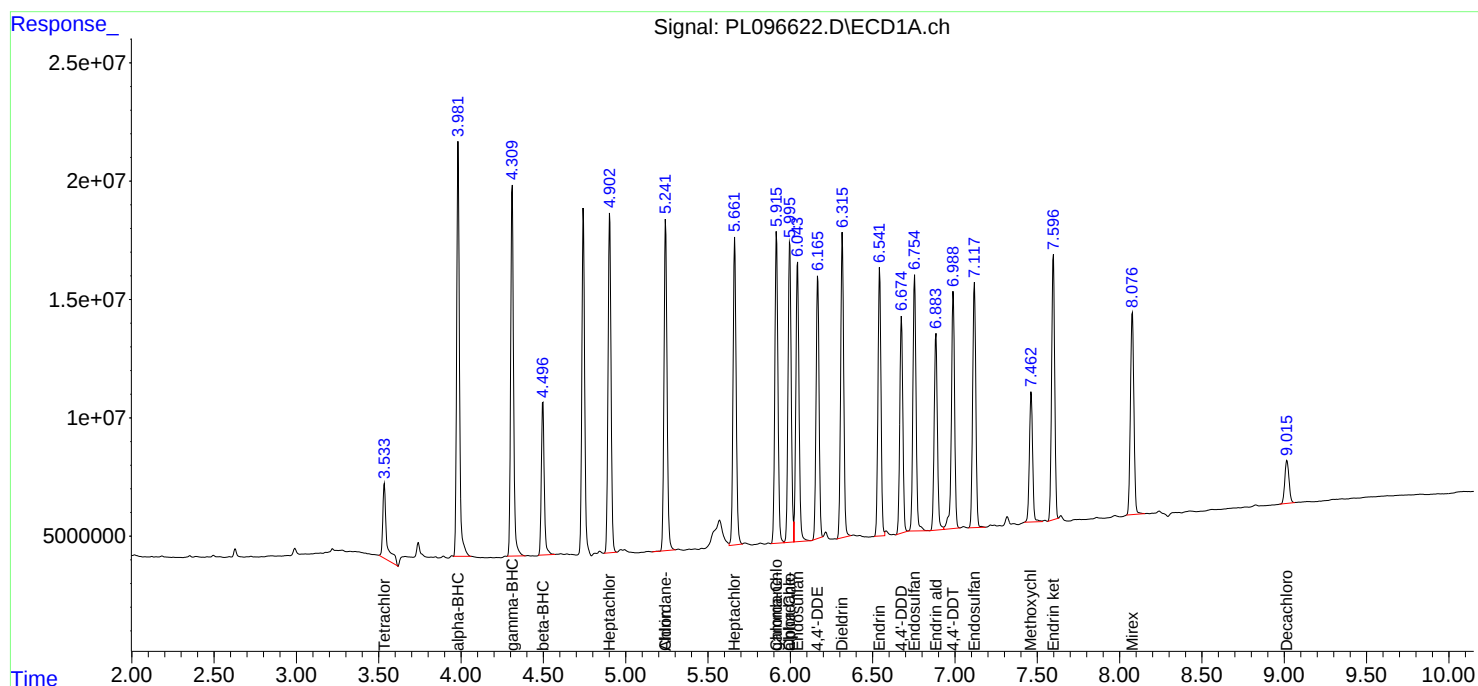


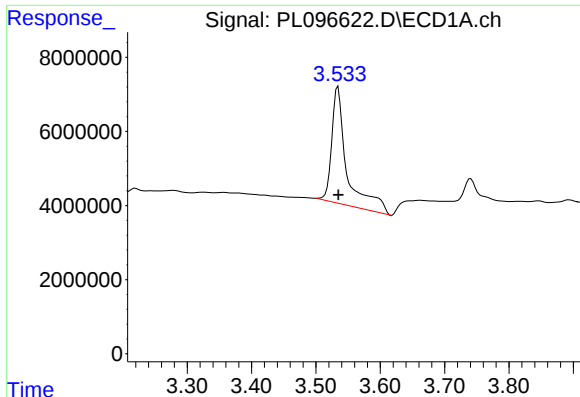

#1 Tetrachloro-m-xylene


R.T.: 3.534 min
Delta R.T.: 0.000 min
Response: 51700368
Conc: 16.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

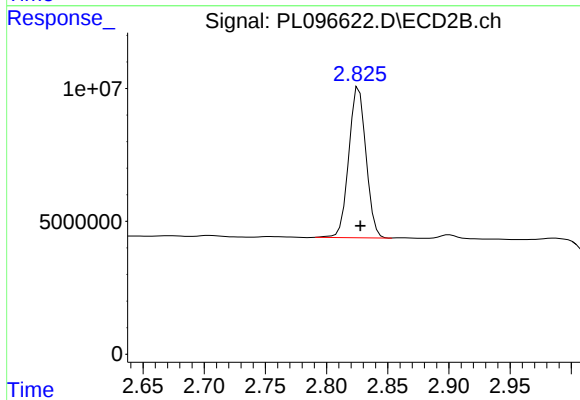


#1 Tetrachloro-m-xylene

R.T.: 2.827 min
Delta R.T.: -0.001 min
Response: 55422220
Conc: 11.60 ng/ml

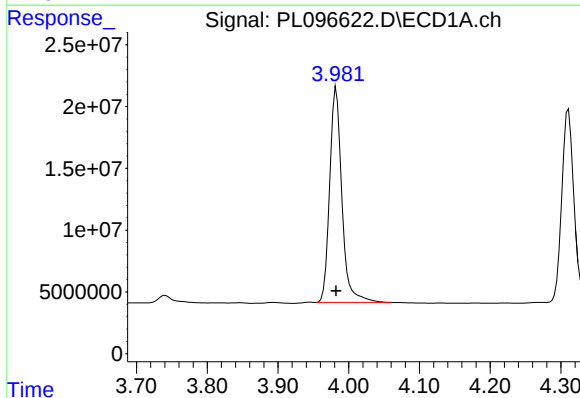


#2 alpha-BHC

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 209018549
Conc: 45.18 ng/ml

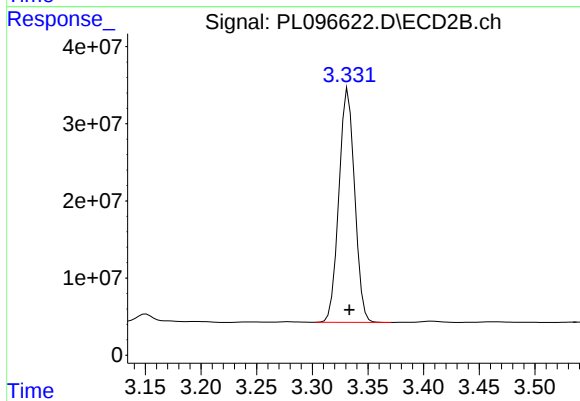

#2 alpha-BHC


R.T.: 3.332 min
Delta R.T.: -0.001 min
Response: 297831741
Conc: 42.08 ng/ml

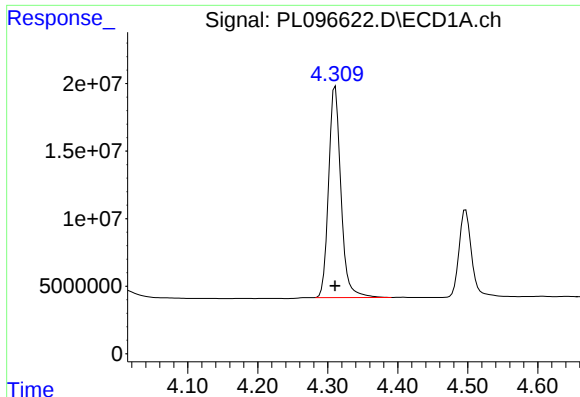

#3 gamma-BHC (Lindane)


R.T.: 4.311 min
Delta R.T.: 0.000 min
Response: 191674424
Conc: 43.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

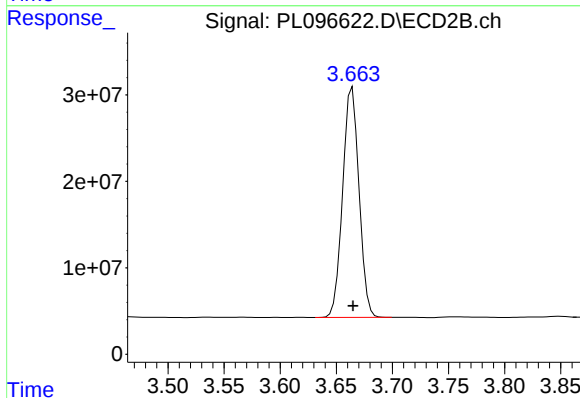


#3 gamma-BHC (Lindane)

R.T.: 3.664 min
Delta R.T.: 0.000 min
Response: 270060538
Conc: 40.90 ng/ml

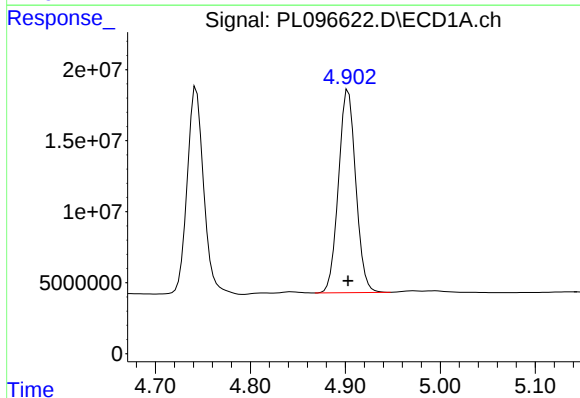


#4 Heptachlor

R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 181215564
Conc: 43.61 ng/ml

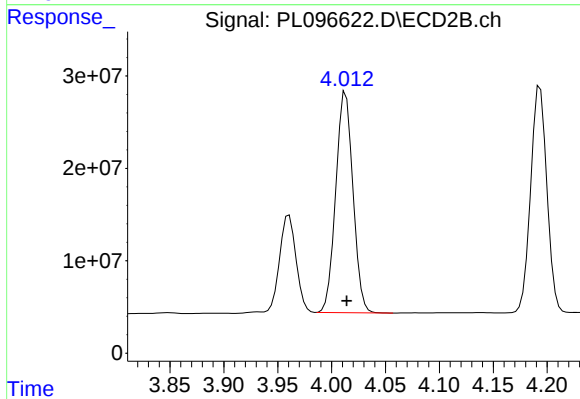

#4 Heptachlor


R.T.: 4.013 min
Delta R.T.: 0.000 min
Response: 265292448
Conc: 39.82 ng/ml

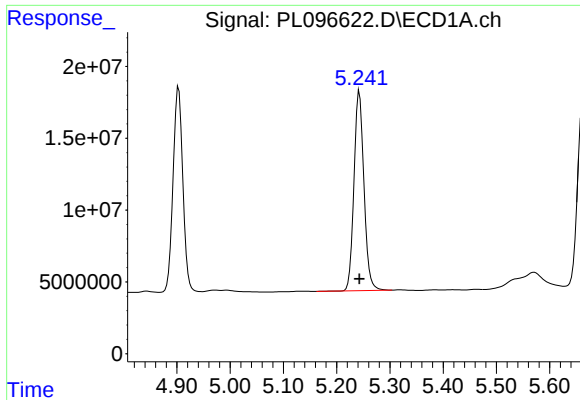

#5 Aldrin


R.T.: 5.243 min
Delta R.T.: 0.000 min
Response: 180762563
Conc: 42.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

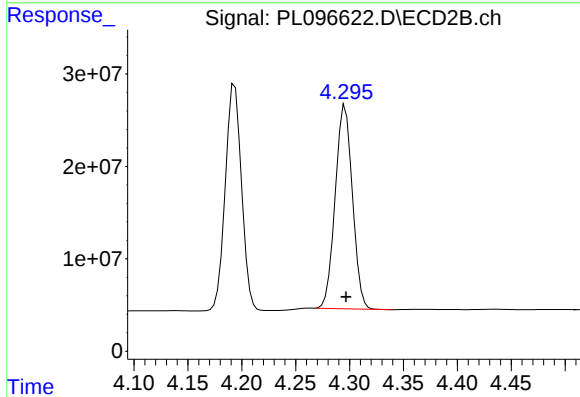


#5 Aldrin

R.T.: 4.296 min
Delta R.T.: 0.000 min
Response: 244495053
Conc: 39.39 ng/ml

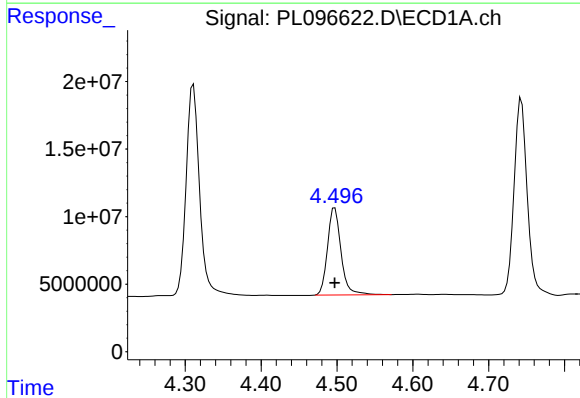


#6 beta-BHC

R.T.: 4.497 min
Delta R.T.: 0.000 min
Response: 79850923
Conc: 44.24 ng/ml

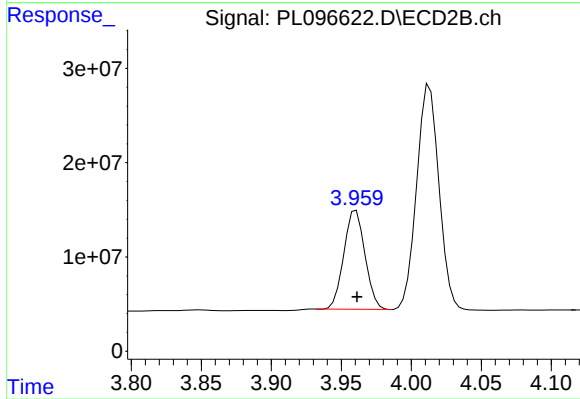

#6 beta-BHC


R.T.: 3.961 min
Delta R.T.: 0.000 min
Response: 110494177
Conc: 39.17 ng/ml

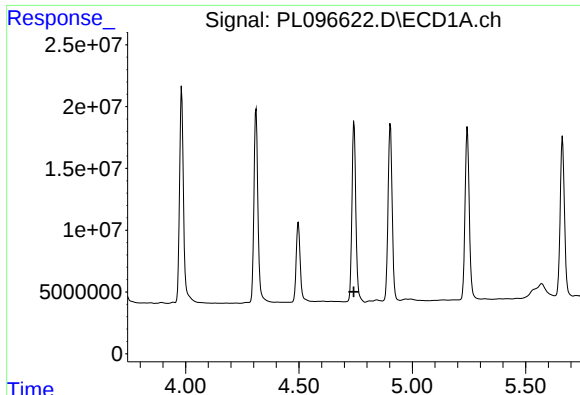

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

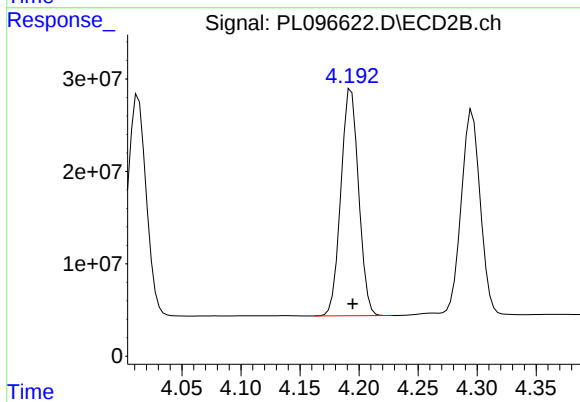


#7 delta-BHC

R.T.: 4.194 min
Delta R.T.: -0.001 min
Response: 257010079
Conc: 39.70 ng/ml

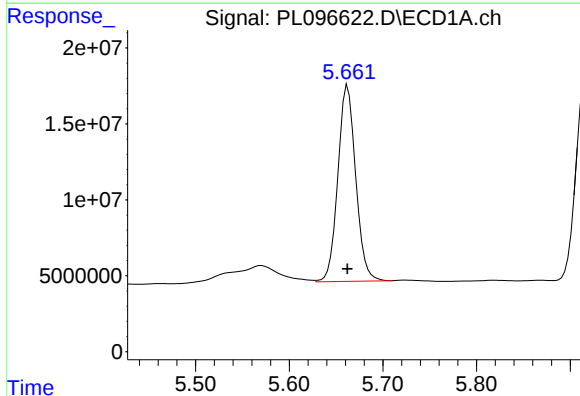


#8 Heptachlor epoxide

R.T.: 5.663 min
Delta R.T.: 0.000 min
Response: 171032212
Conc: 44.35 ng/ml

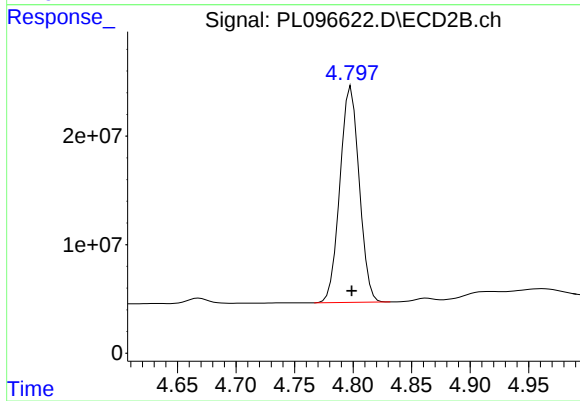

#8 Heptachlor epoxide


R.T.: 4.798 min
Delta R.T.: 0.000 min
Response: 228410074
Conc: 39.99 ng/ml

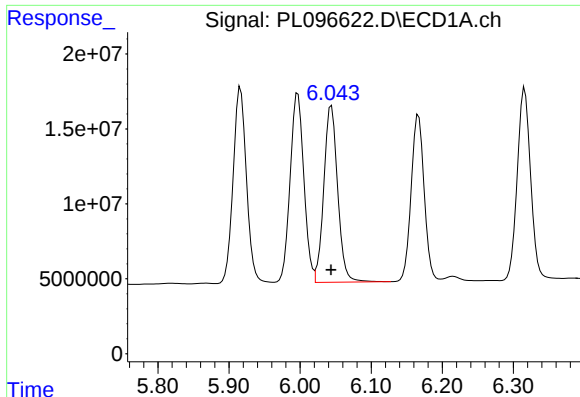

#9 Endosulfan I


R.T.: 6.044 min
Delta R.T.: 0.000 min
Response: 159945995
Conc: 44.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

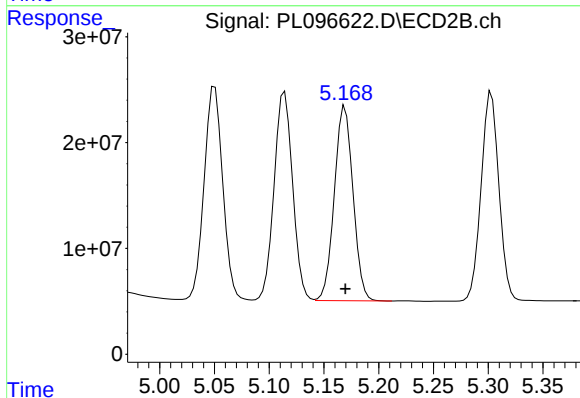


#9 Endosulfan I

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 217950180
Conc: 39.40 ng/ml

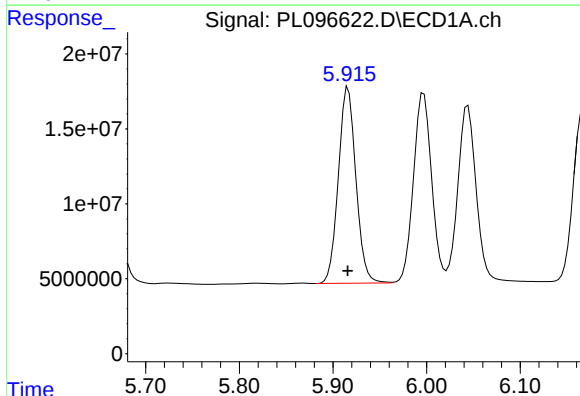


#10 gamma-Chlordane

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 170601720
Conc: 44.83 ng/ml

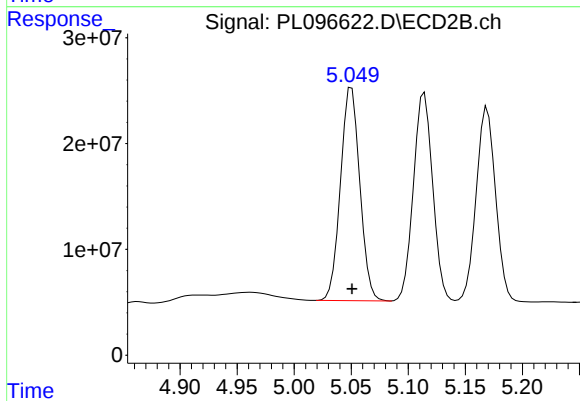

#10 gamma-Chlordane


R.T.: 5.050 min
Delta R.T.: 0.000 min
Response: 237880522
Conc: 40.46 ng/ml

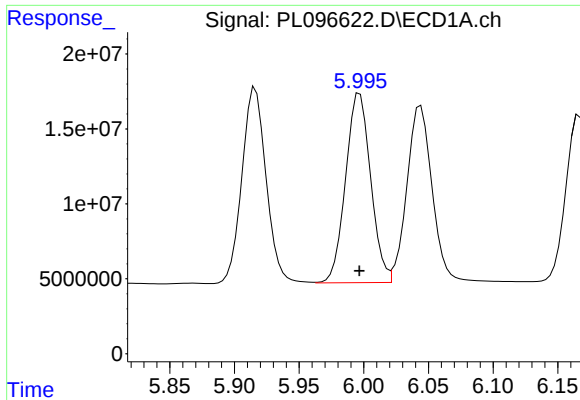

#11 alpha-Chlordane


R.T.: 5.997 min
Delta R.T.: 0.000 min
Response: 170125339
Conc: 44.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

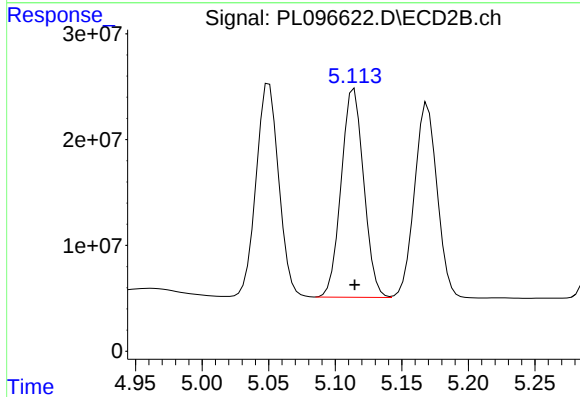


#11 alpha-Chlordane

R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 232061169
Conc: 39.34 ng/ml

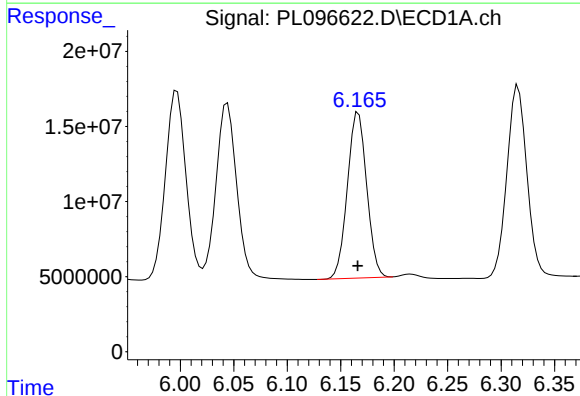


#12 4,4'-DDE

R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 138914417
Conc: 43.26 ng/ml

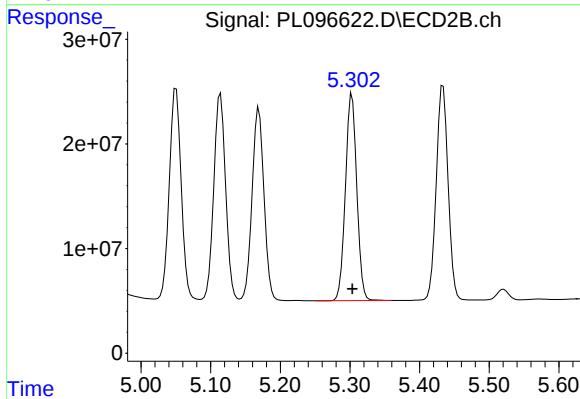

#12 4,4'-DDE


R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 224013386
Conc: 40.62 ng/ml

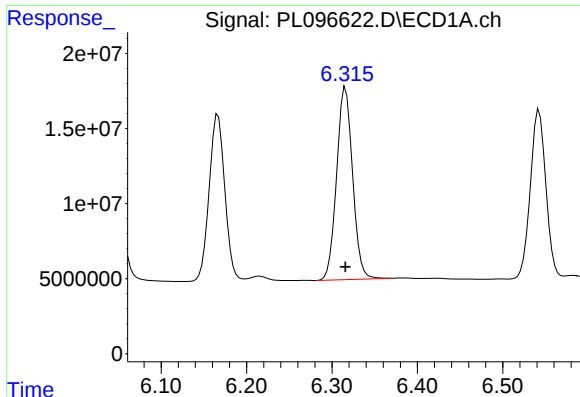

#13 Dieldrin


R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 166824839
Conc: 44.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

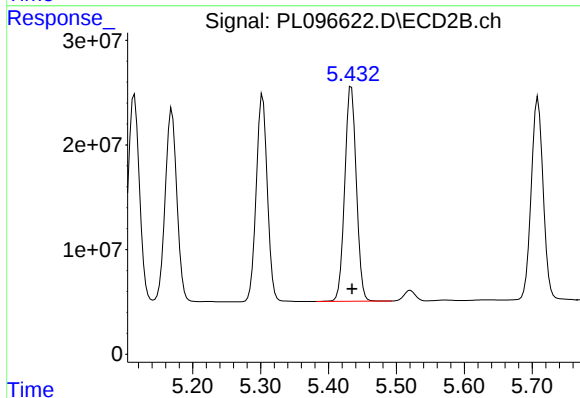


#13 Dieldrin

R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 243140281
Conc: 41.16 ng/ml

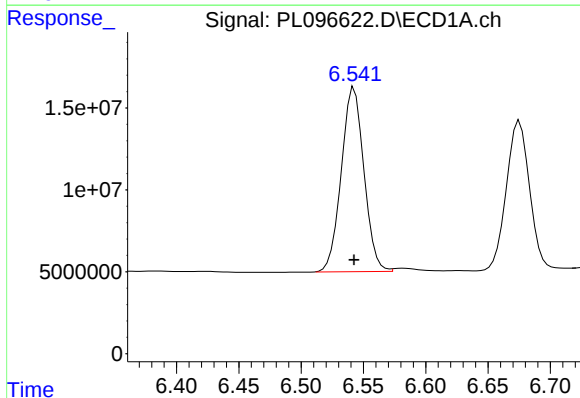


#14 Endrin

R.T.: 6.543 min
Delta R.T.: 0.000 min
Response: 142655932
Conc: 47.13 ng/ml

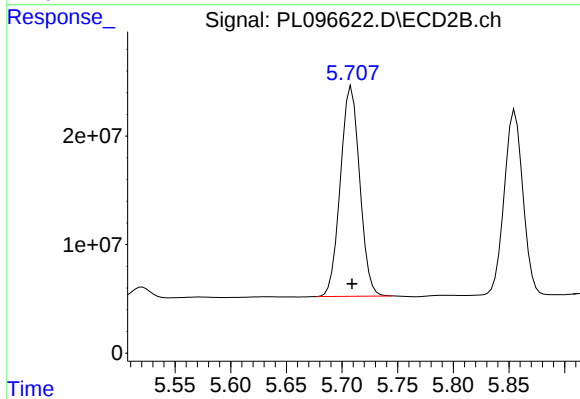

#14 Endrin


R.T.: 5.708 min
Delta R.T.: 0.000 min
Response: 233939865
Conc: 43.27 ng/ml

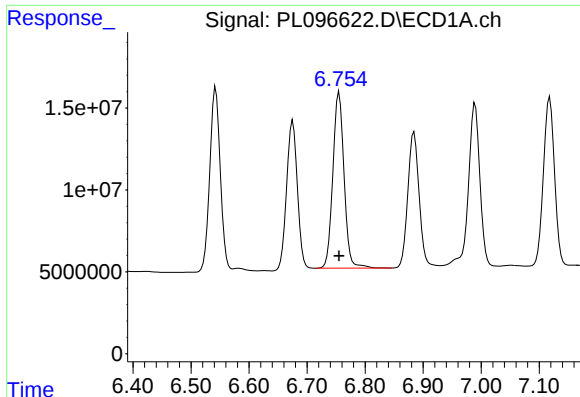

#15 Endosulfan II


R.T.: 6.755 min
Delta R.T.: 0.000 min
Response: 144706070
Conc: 45.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

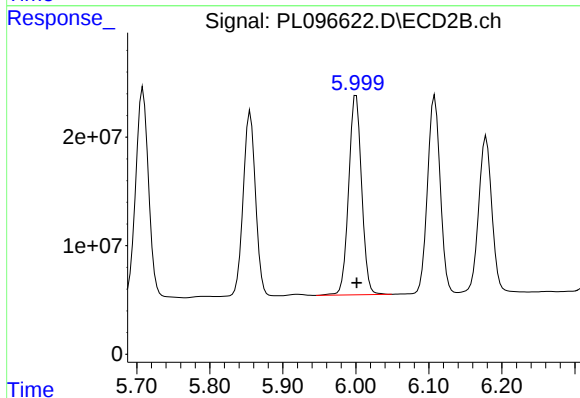


#15 Endosulfan II

R.T.: 6.000 min
Delta R.T.: 0.000 min
Response: 227066135
Conc: 44.21 ng/ml

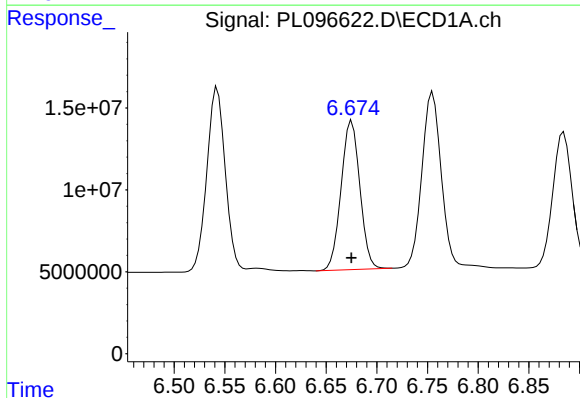


#16 4,4'-DDD

R.T.: 6.675 min
Delta R.T.: 0.000 min
Response: 117162588
Conc: 46.34 ng/ml

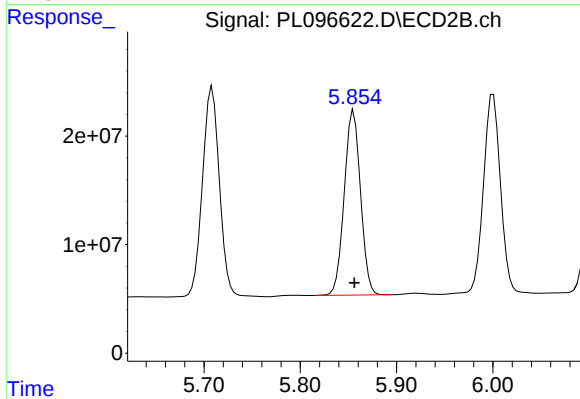

#16 4,4'-DDD


R.T.: 5.855 min
Delta R.T.: 0.000 min
Response: 199183979
Conc: 42.33 ng/ml

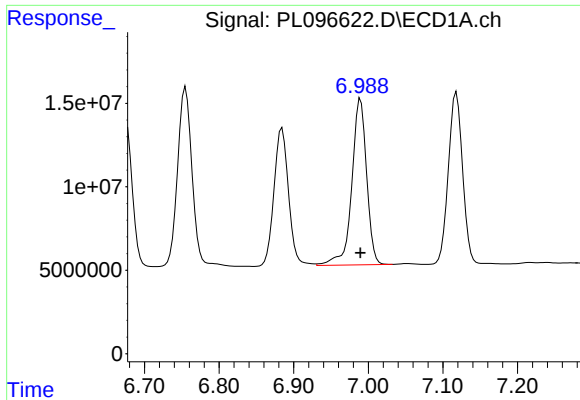

#17 4,4'-DDT


R.T.: 6.990 min
Delta R.T.: 0.000 min
Response: 137690933
Conc: 48.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

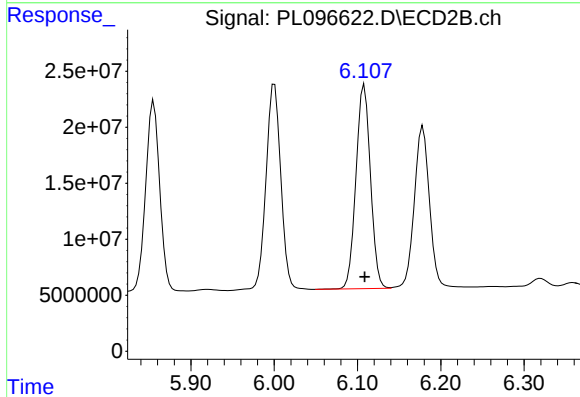


#17 4,4'-DDT

R.T.: 6.108 min
Delta R.T.: 0.000 min
Response: 220494619
Conc: 43.59 ng/ml

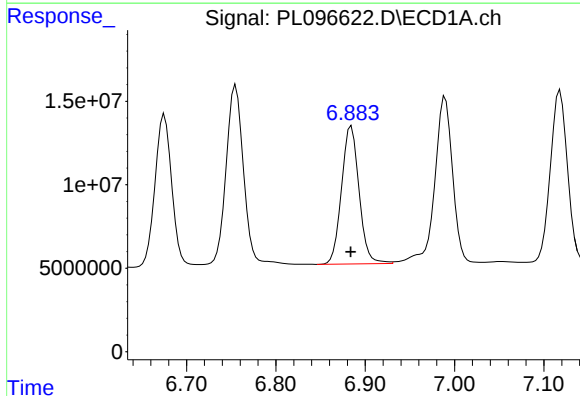


#18 Endrin aldehyde

R.T.: 6.884 min
Delta R.T.: 0.000 min
Response: 112547293
Conc: 52.45 ng/ml

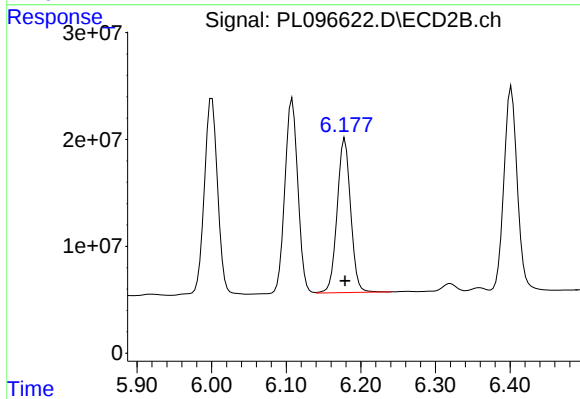

#18 Endrin aldehyde


R.T.: 6.179 min
Delta R.T.: 0.000 min
Response: 181954622
Conc: 48.93 ng/ml

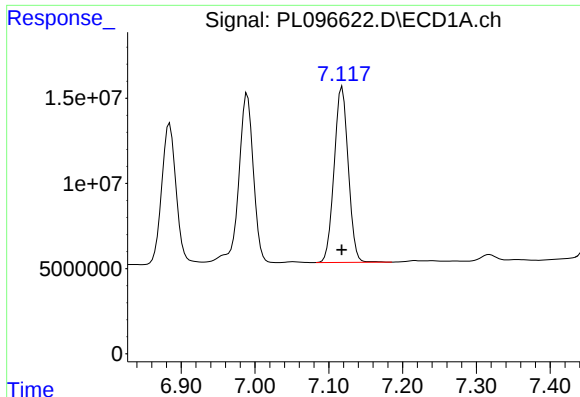

#19 Endosulfan Sulfate


R.T.: 7.118 min
Delta R.T.: 0.000 min
Response: 136989078
Conc: 47.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

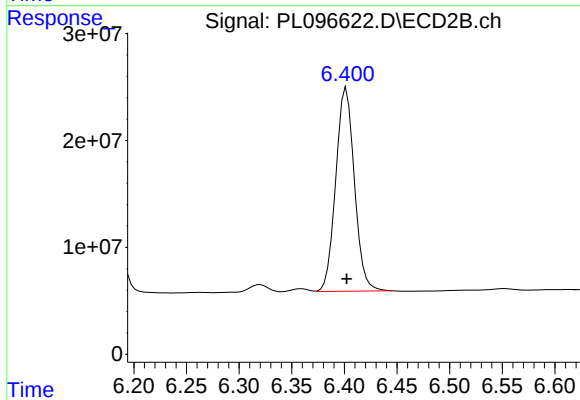


#19 Endosulfan Sulfate

R.T.: 6.402 min
Delta R.T.: 0.000 min
Response: 235053527
Conc: 46.21 ng/ml

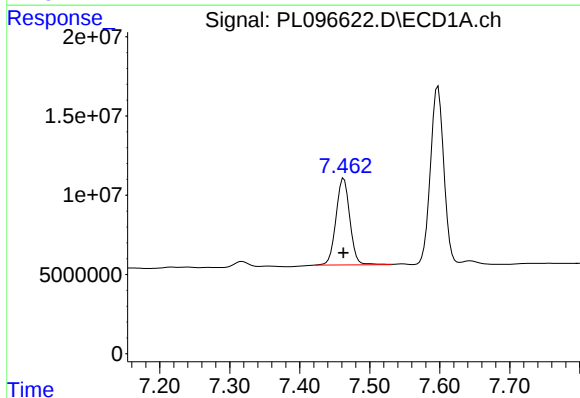


#20 Methoxychlor

R.T.: 7.463 min
Delta R.T.: 0.000 min
Response: 75439028
Conc: 51.38 ng/ml

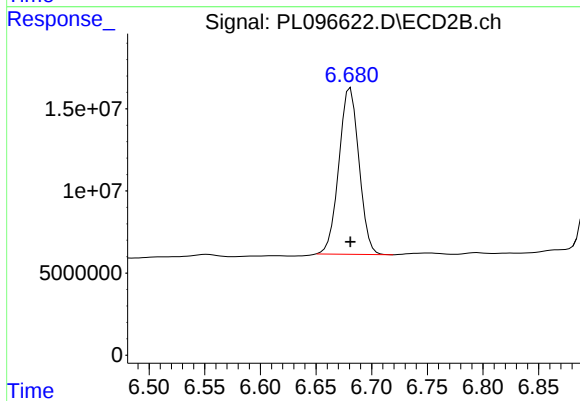

#20 Methoxychlor


R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 127119327
Conc: 46.39 ng/ml

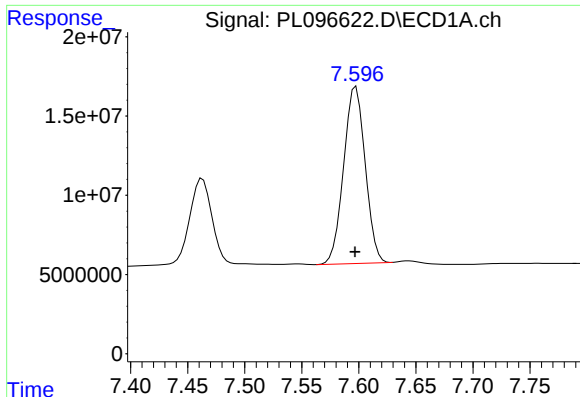

#21 Endrin ketone


R.T.: 7.598 min
Delta R.T.: 0.000 min
Response: 146702527
Conc: 48.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

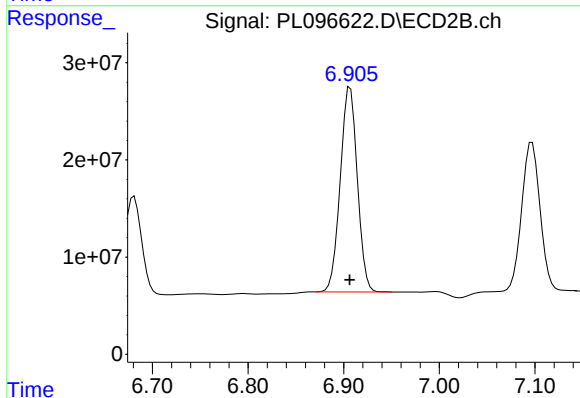


#21 Endrin ketone

R.T.: 6.907 min
Delta R.T.: 0.000 min
Response: 262204438
Conc: 47.08 ng/ml

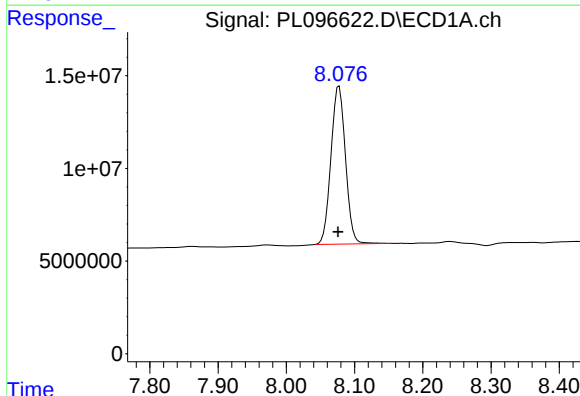


#22 Mirex

R.T.: 8.077 min
Delta R.T.: 0.002 min
Response: 125962549
Conc: 50.80 ng/ml

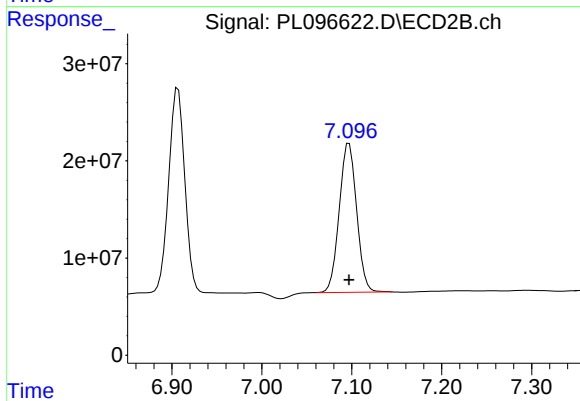

#22 Mirex


R.T.: 7.097 min
Delta R.T.: 0.000 min
Response: 206135827
Conc: 47.27 ng/ml

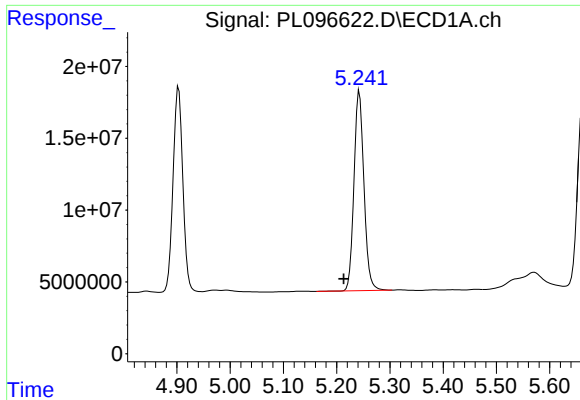

#24 Chlordane-2


R.T.: 5.243 min
Delta R.T.: 0.030 min
Response: 180762563
Conc: 1032.89 ng/m

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

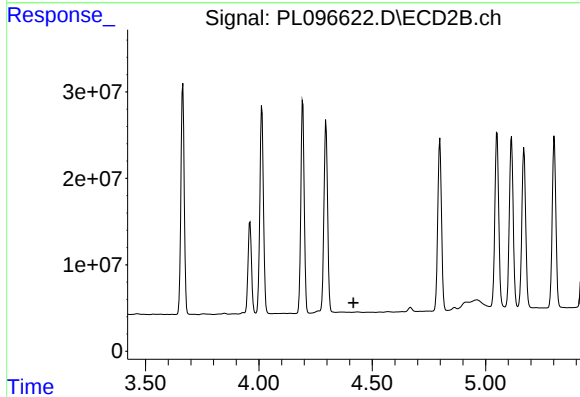


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.418 min
Response: 0
Conc: N.D.

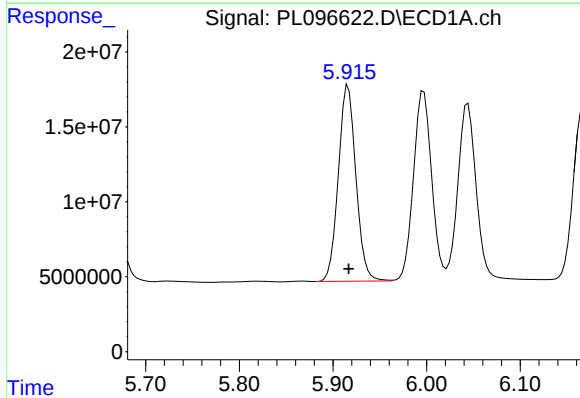


#25 Chlordane-3

R.T.: 5.916 min
Delta R.T.: 0.000 min
Response: 170601720
Conc: 255.42 ng/ml

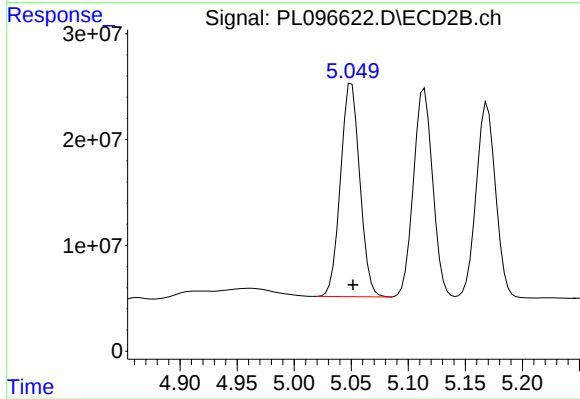

#25 Chlordane-3


R.T.: 5.050 min
Delta R.T.: -0.001 min
Response: 237880522
Conc: 342.13 ng/ml

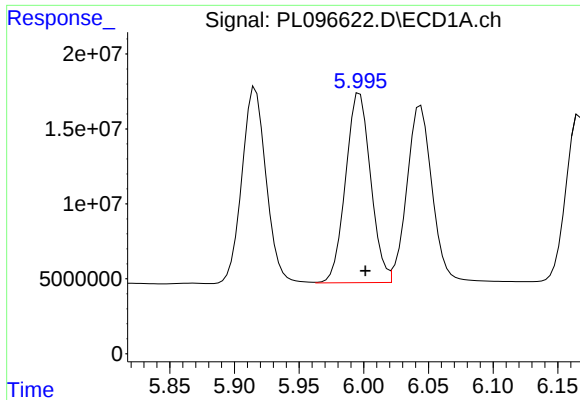

#26 Chlordane-4


R.T.: 5.997 min
Delta R.T.: -0.004 min
Response: 170125339
Conc: 205.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

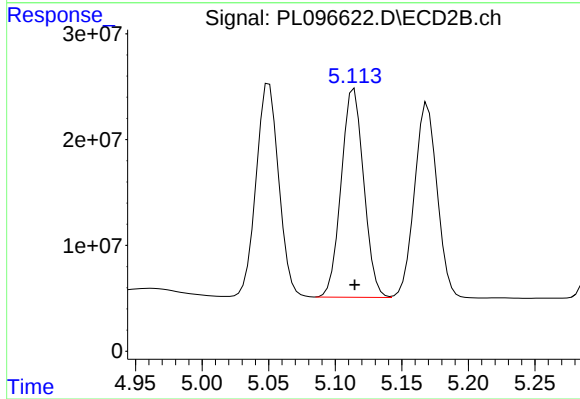


#26 Chlordane-4

R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 232061169
Conc: 372.89 ng/ml

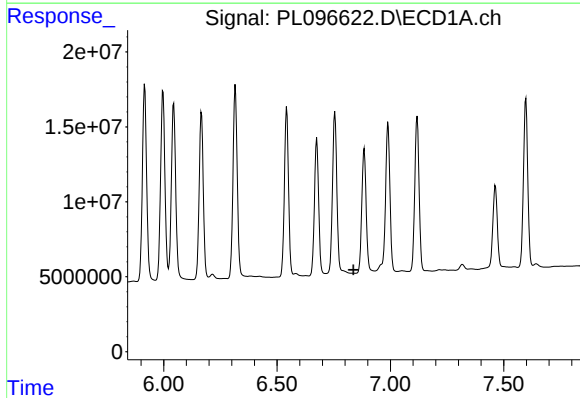


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.838 min
Response: 0
Conc: N.D.

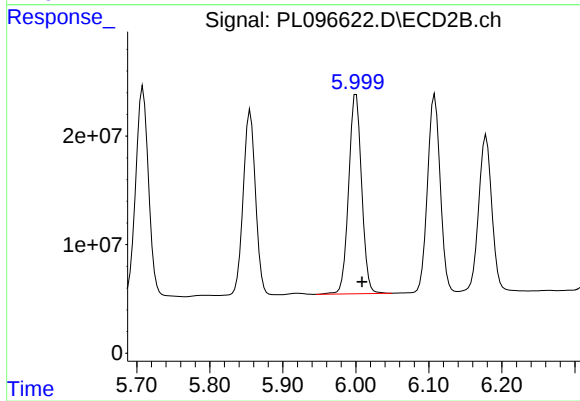

#27 Chlordane-5


R.T.: 6.000 min
Delta R.T.: -0.008 min
Response: 227066135
Conc: 890.06 ng/ml

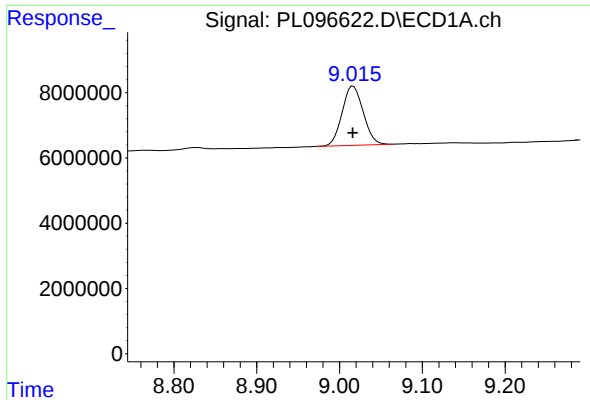

#28 Decachlorobiphenyl

R.T.: 9.017 min
Delta R.T.: 0.000 min
Response: 32134065
Conc: 13.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
7211935-295MS

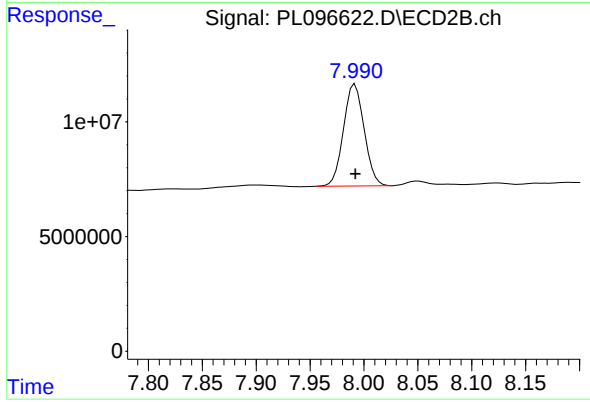

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 59381298
Conc: 13.69 ng/ml