

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073018\
 Data File : PL038714.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2018 16:29
 Operator : AJ\SJ
 Sample : J4218-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-15-D

Manual Integrations
 APPROVED

Sohil
 7/31/2018 1:43:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 01:10:29 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.324	3.927	163.0E6	62875454	21.888	23.953
28)	SA Decachlor...	7.992	8.934	122.2E6	44736859	16.112	18.301
Target Compounds							
16)	A 4,4'-DDD	5.945	6.721	30903495	9488474	4.213m	4.433m
17)	MA 4,4'-DDT	6.179	7.021	191.7E6	56867240	25.809m	26.673

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073018\
Data File : PL038714.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2018 16:29
Operator : AJ\SJ
Sample : J4218-07
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-15-D


Manual Integrations
APPROVED

Sohil
7/31/2018 1:43:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 01:10:29 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

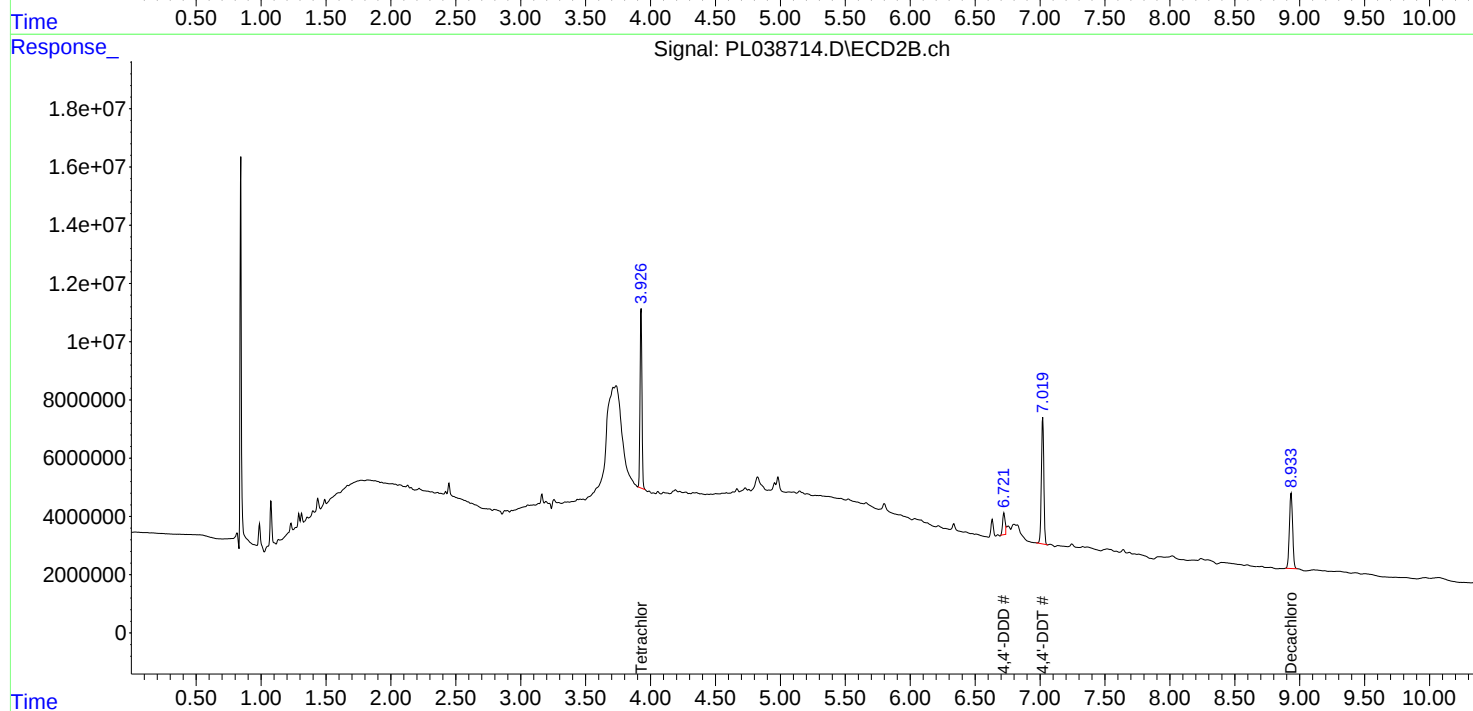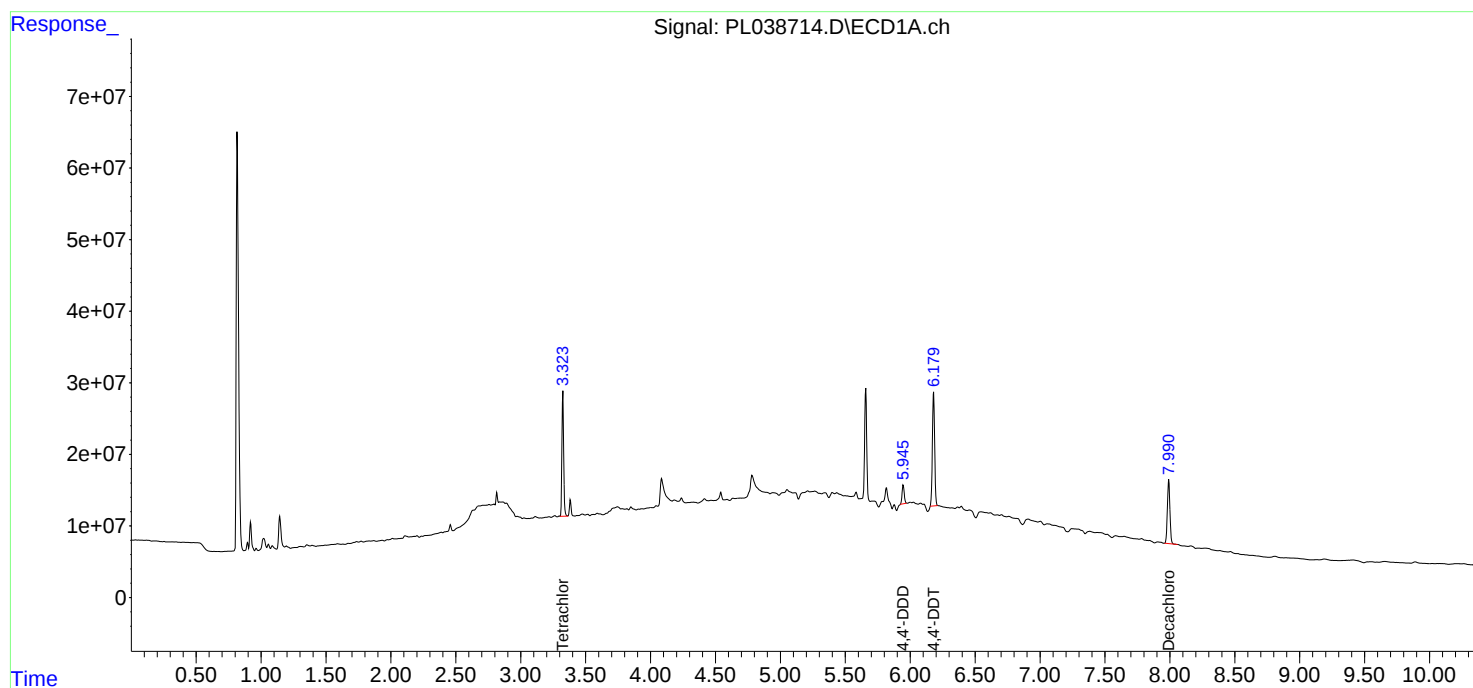

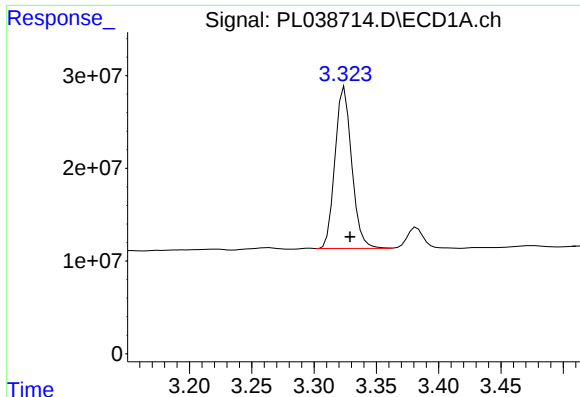


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 162989578
Conc: 21.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15-D


Manual Integrations
APPROVED

Sohil
7/31/2018 1:43:06 PM

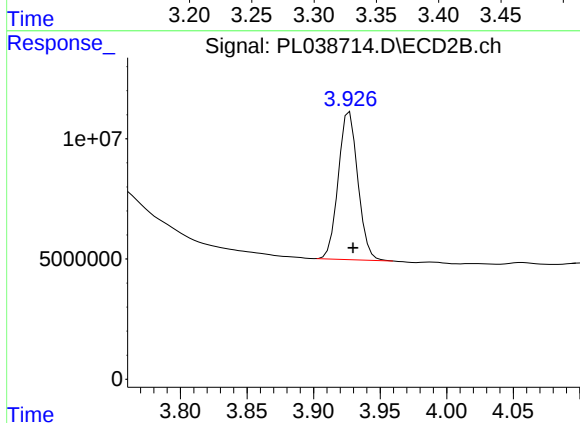


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 62875454
Conc: 23.95 ng/ml

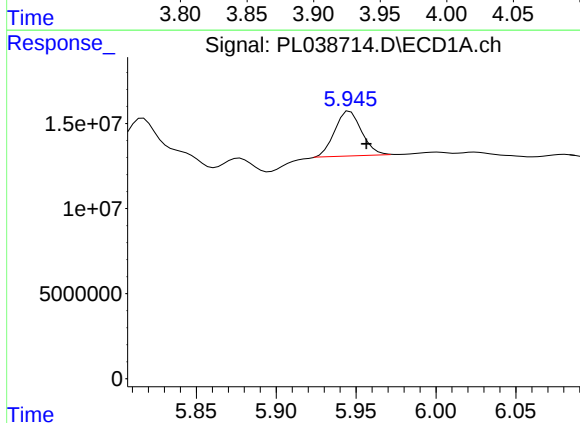


#16 4,4'-DDD

R.T.: 5.945 min
Delta R.T.: -0.012 min
Response: 30903495
Conc: 4.21 ng/ml m

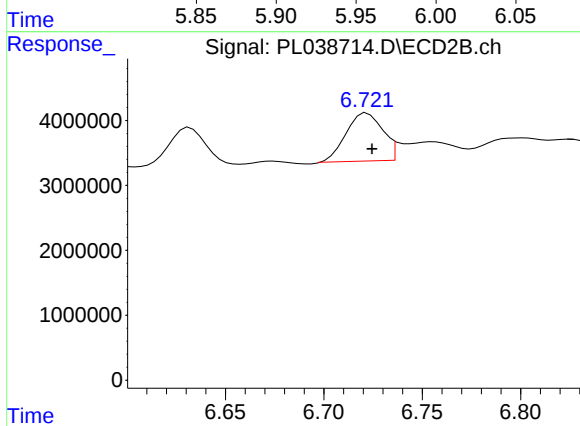

#16 4,4'-DDD

R.T.: 6.721 min
Delta R.T.: -0.004 min
Response: 9488474
Conc: 4.43 ng/ml m

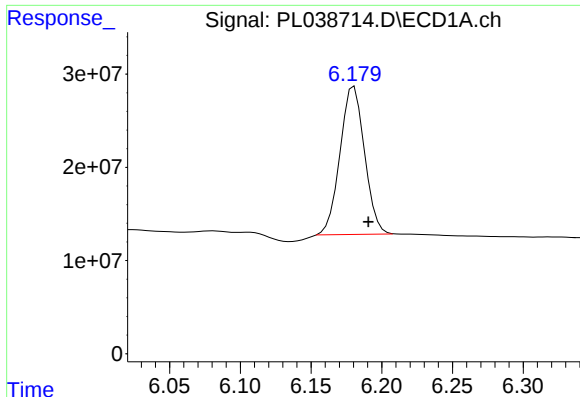


#17 4,4'-DDT

R.T.: 6.179 min
Delta R.T.: -0.011 min
Response: 191728283
Conc: 25.81 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-15-D


Manual Integrations
APPROVED

Sohil
7/31/2018 1:43:06 PM

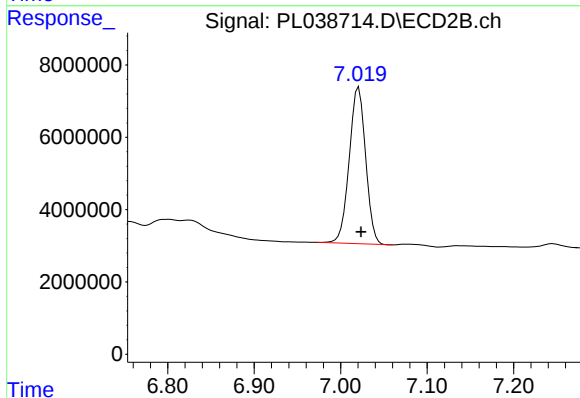


#17 4,4'-DDT

R.T.: 7.021 min
Delta R.T.: -0.003 min
Response: 56867240
Conc: 26.67 ng/ml

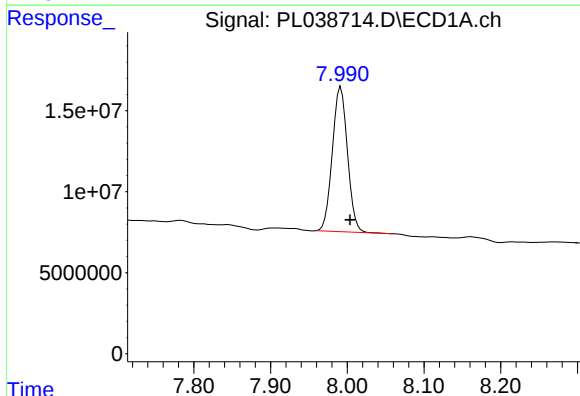

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.012 min
Response: 122226343
Conc: 16.11 ng/ml

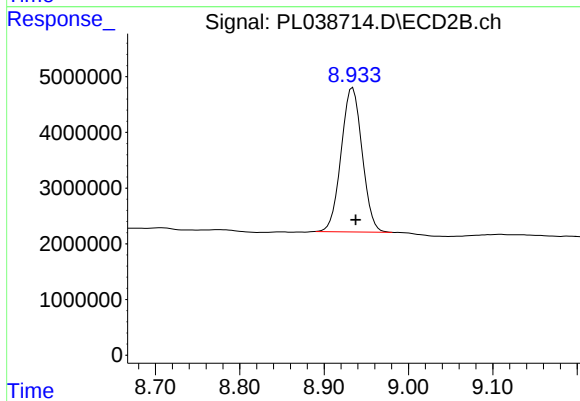

#28 Decachlorobiphenyl

R.T.: 8.934 min
Delta R.T.: -0.003 min
Response: 44736859
Conc: 18.30 ng/ml