

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073018\
 Data File : PL038715.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2018 16:43
 Operator : AJ\SJ
 Sample : J4218-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-15-S

Manual Integrations
 APPROVED

Sohil
 7/31/2018 1:43:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 01:10:57 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
 Quant Title : GC Extractables
 QLast Update : Sat Jul 14 00:12:12 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.324	3.927	154.2E6	59596237	20.702	22.704
28) SA Decachlor...	7.991	8.934	126.0E6	46983958	16.606	19.221
Target Compounds						
17) MA 4,4'-DDT	6.180	7.020	45439179	14246857	6.117	6.682

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073018\
Data File : PL038715.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2018 16:43
Operator : AJ\SJ
Sample : J4218-03
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Sohil
7/31/2018 1:43:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 01:10:57 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL071318.M
Quant Title : GC Extractables
QLast Update : Sat Jul 14 00:12:12 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

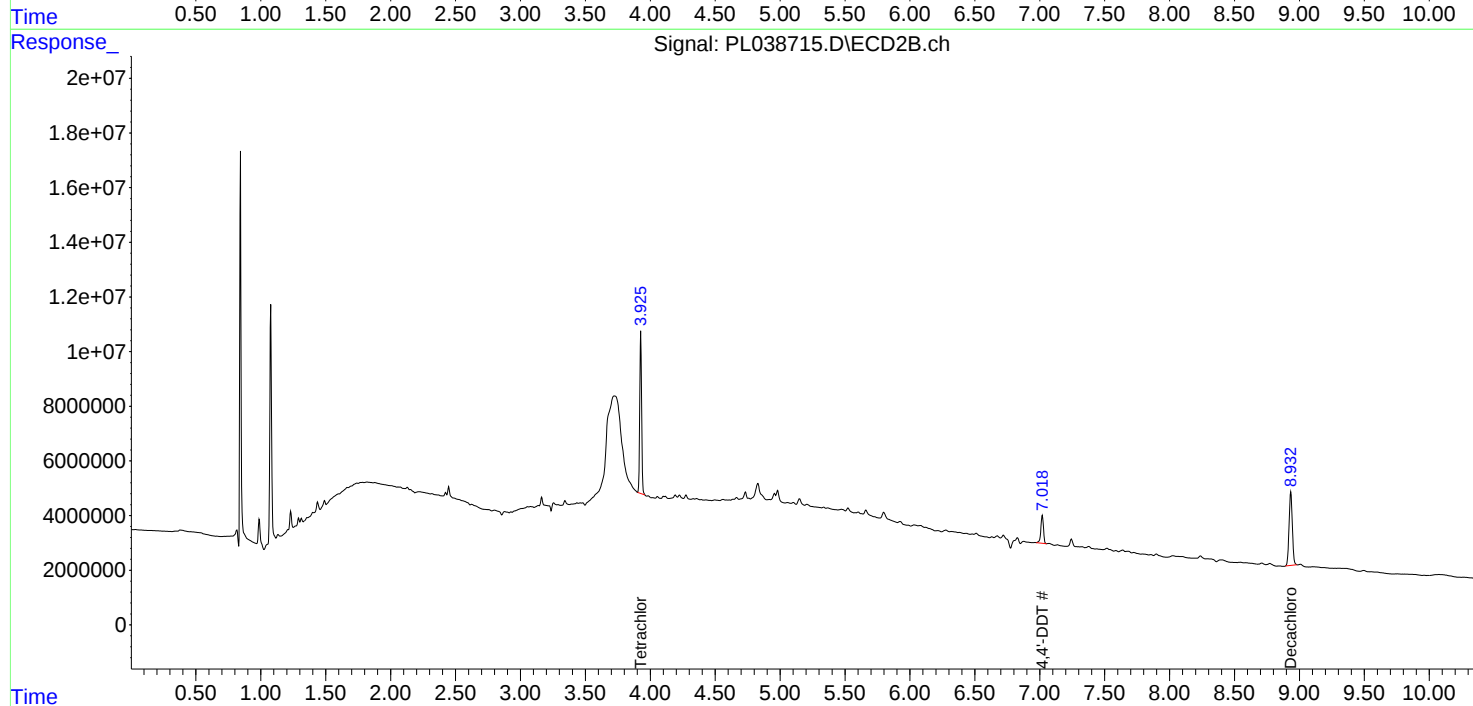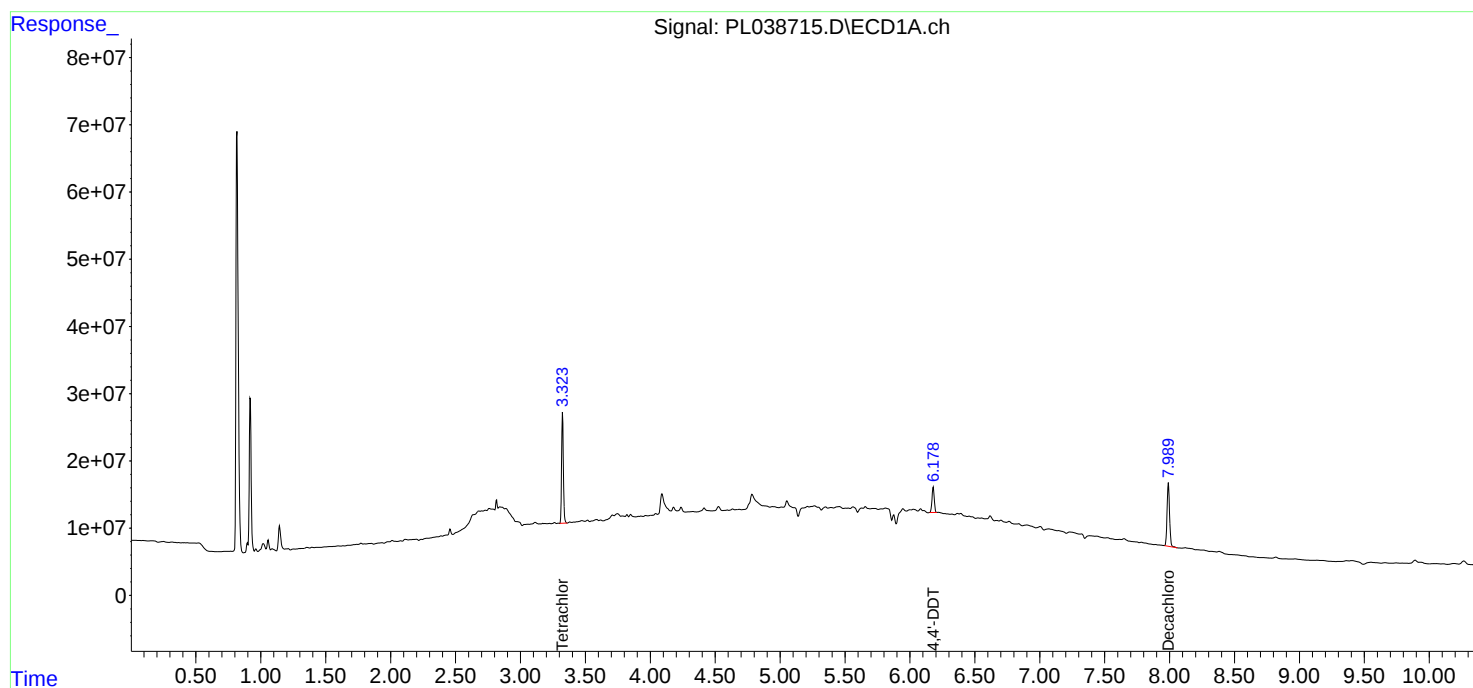

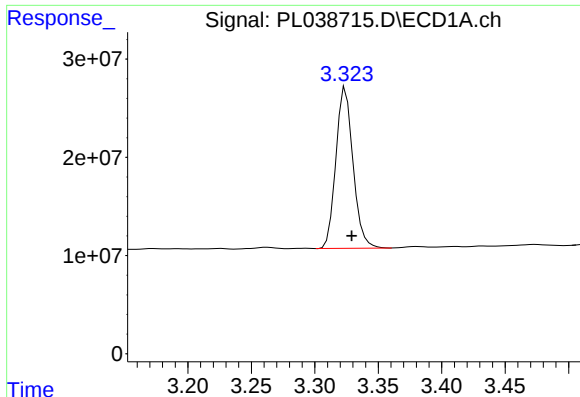


#1 Tetrachloro-m-xylene

R.T.: 3.324 min
Delta R.T.: -0.005 min
Response: 154157000
Conc: 20.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15-S


Manual Integrations
APPROVED

Sohil
7/31/2018 1:43:08 PM

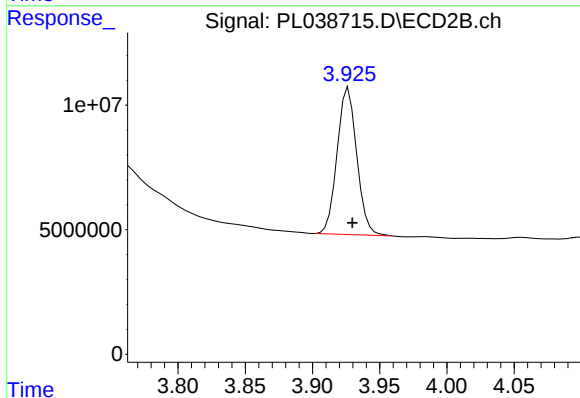


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 59596237
Conc: 22.70 ng/ml

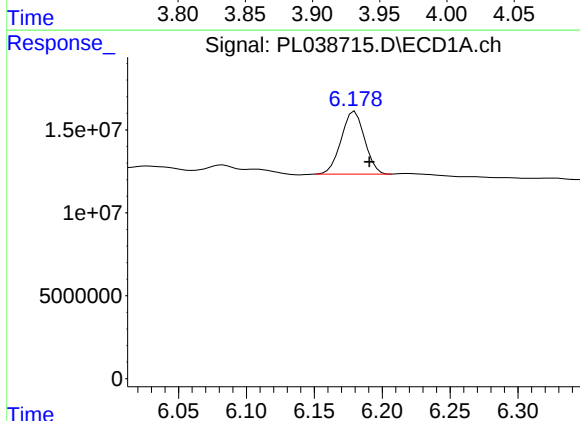


#17 4,4'-DDT

R.T.: 6.180 min
Delta R.T.: -0.011 min
Response: 45439179
Conc: 6.12 ng/ml

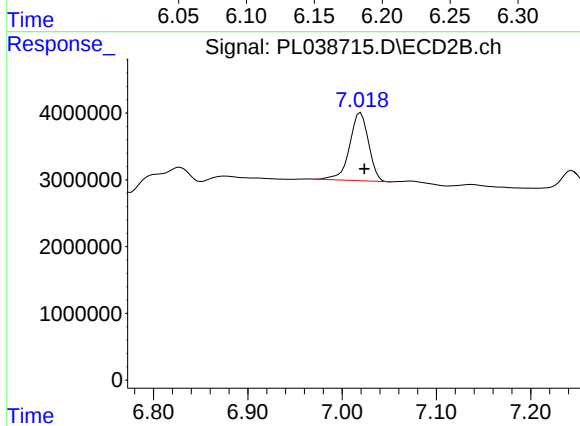

#17 4,4'-DDT

R.T.: 7.020 min
Delta R.T.: -0.004 min
Response: 14246857
Conc: 6.68 ng/ml

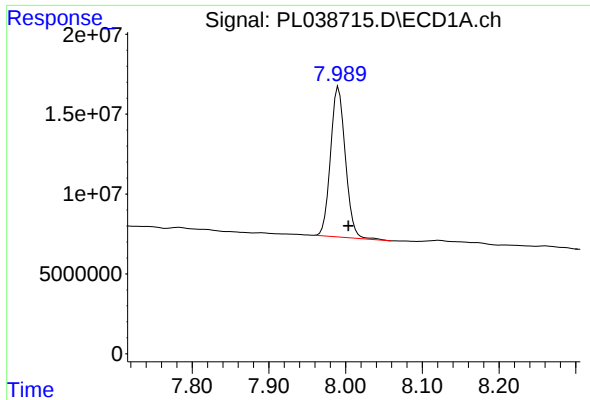

#28 Decachlorobiphenyl

R.T.: 7.991 min

Delta R.T.: -0.013 min


Response: 125968027

Conc: 16.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15-S

Manual Integrations
APPROVED

Sohil
7/31/2018 1:43:08 PM

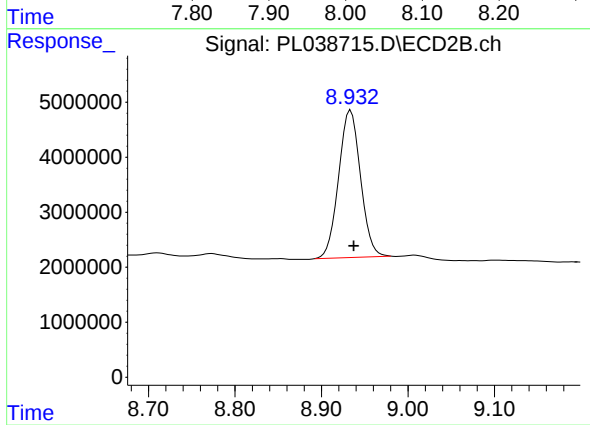

#28 Decachlorobiphenyl

R.T.: 8.934 min

Delta R.T.: -0.004 min

Response: 46983958

Conc: 19.22 ng/ml