

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
 Data File : PL050869.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2019 14:52
 Operator : SM\AJ
 Sample : K3621-07
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-01-072919

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 00:43:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	96058451	26756441	9.560	9.378
28)	SA Decachlor...	7.979	8.958	97912699	31688717	9.670	11.206
Target Compounds							
6)	B beta-BHC	0.000	4.798f	0	1938732	N.D.	1.121 #
8)	B Heptachlo...	0.000	5.806	0	5655995	N.D.	1.479 #
9)	A Endosulfan I	5.303	0.000	10042372	0	0.690	N.D. #
10)	B gamma-Chl...	5.202	0.000	6342684	0	0.402	N.D. #
11)	B alpha-Chl...	0.000	6.097	0	4512782	N.D.	1.231 #
17)	MA 4,4'-DDT	6.166	0.000	3389289	0	0.274	N.D. #
25)	Chlordane-3	5.202	0.000	6342684	0	4.531	N.D. #
26)	Chlordane-4	0.000	6.097	0	4512782	N.D.	7.768 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
Data File : PL050869.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2019 14:52
Operator : SM\AJ
Sample : K3621-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OK-01-072919

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 00:43:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

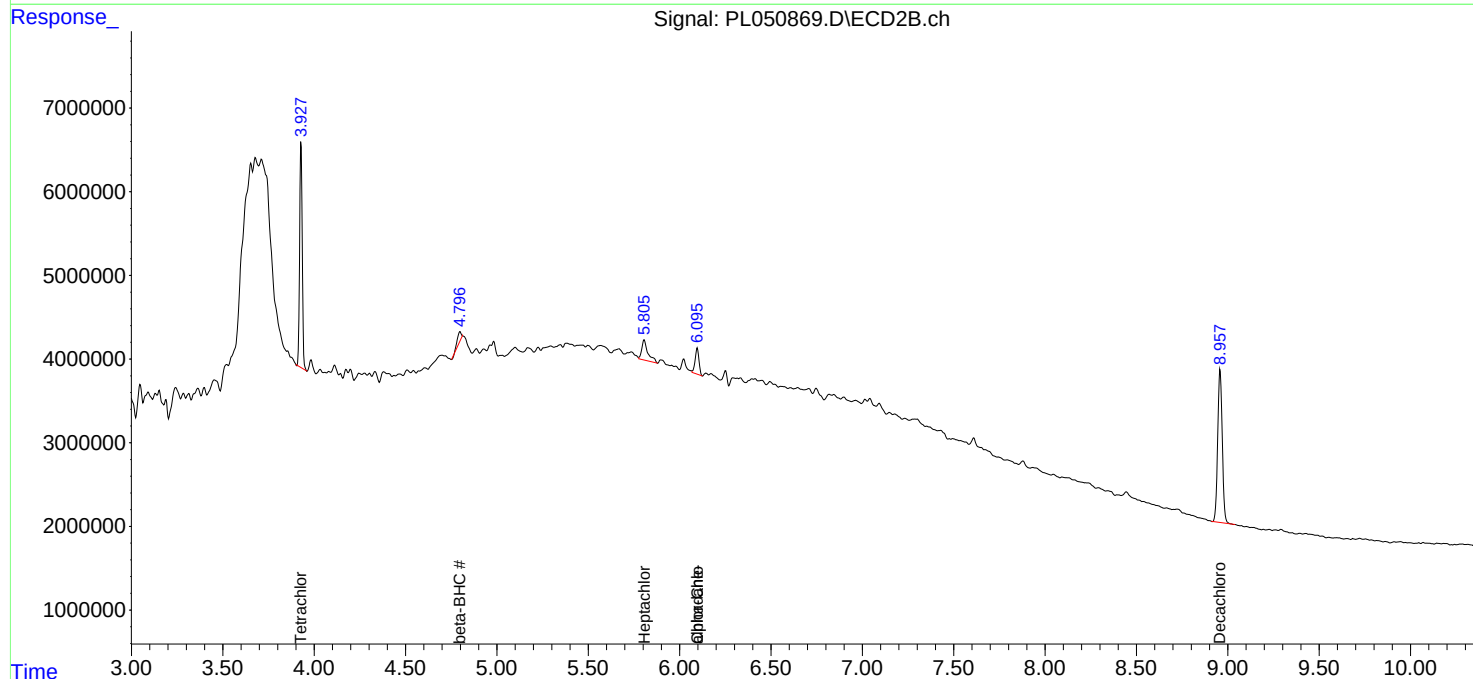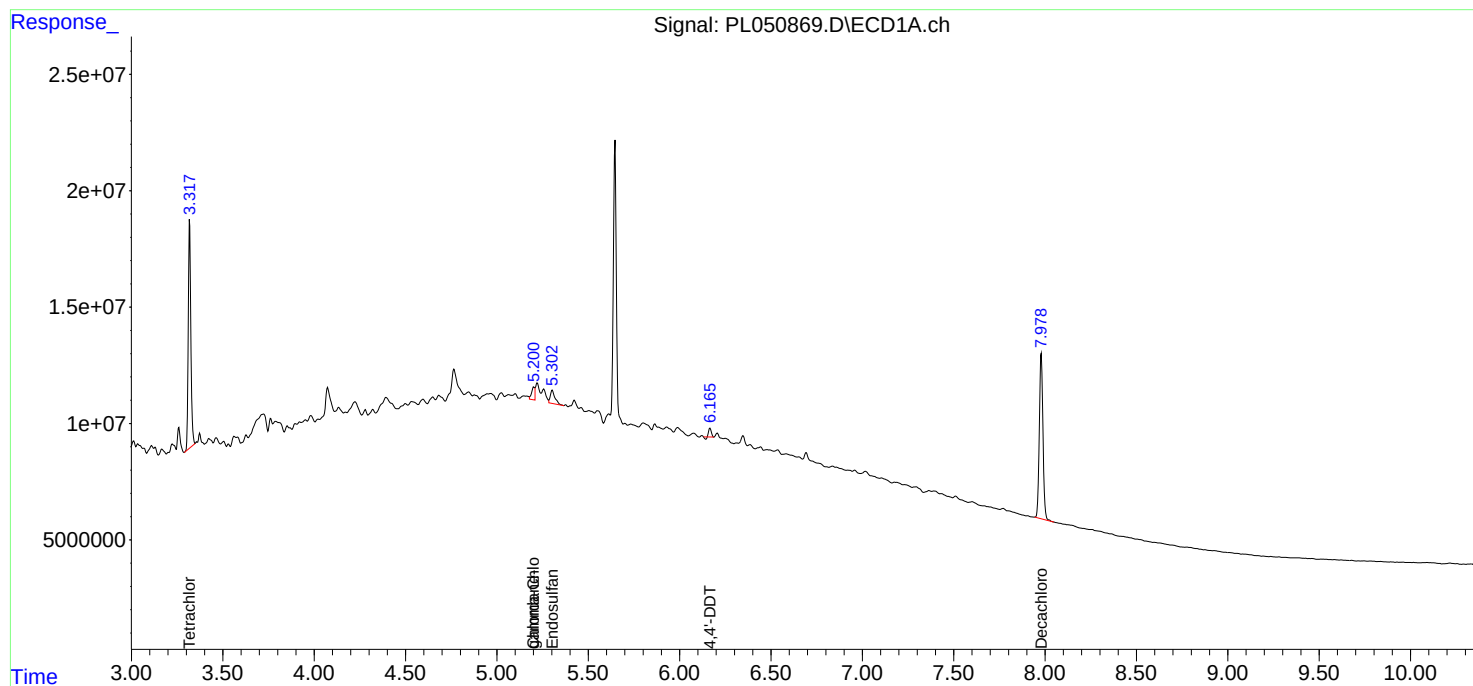


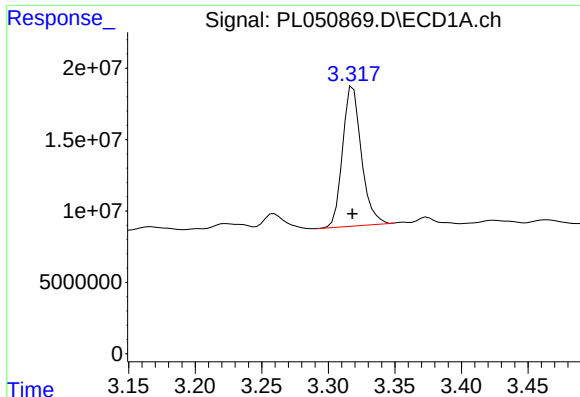

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 96058451
Conc: 9.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-072919

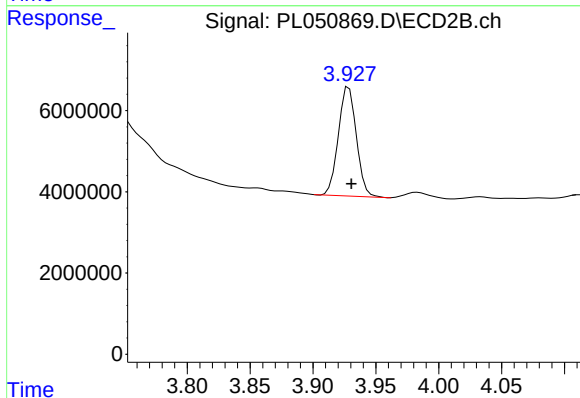


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 26756441
Conc: 9.38 ng/ml

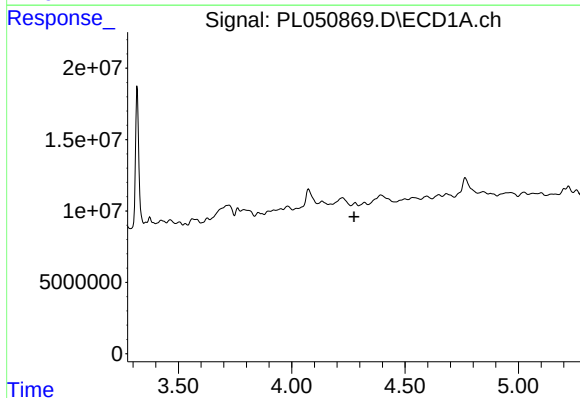


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

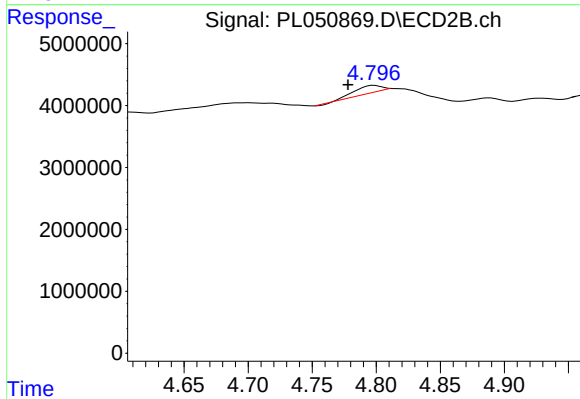

#6 beta-BHC


R.T.: 4.798 min
Delta R.T.: 0.020 min
Response: 1938732
Conc: 1.12 ng/ml

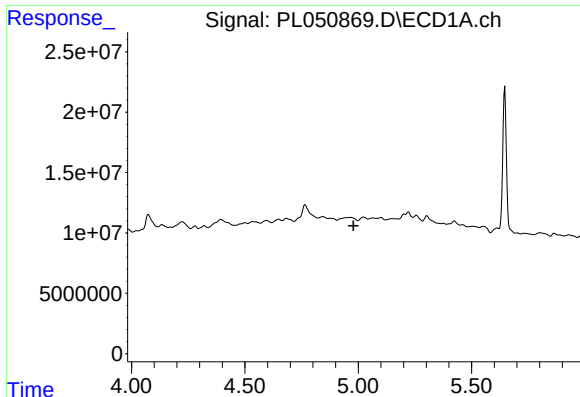

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-01-072919

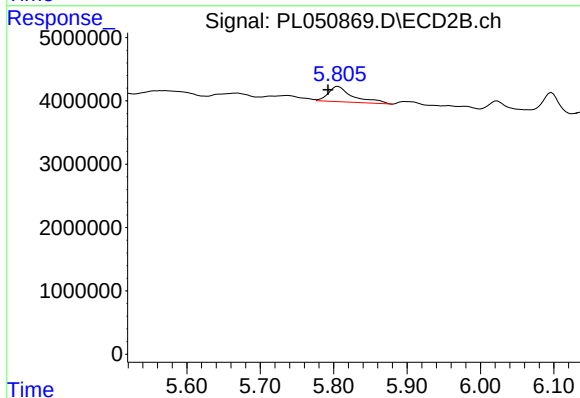


#8 Heptachlor epoxide

R.T.: 5.806 min
Delta R.T.: 0.014 min
Response: 5655995
Conc: 1.48 ng/ml

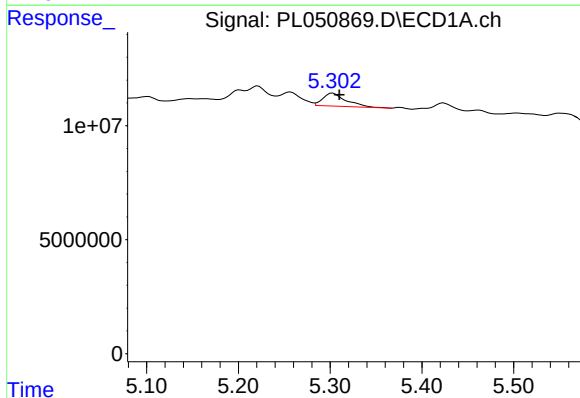


#9 Endosulfan I

R.T.: 5.303 min
Delta R.T.: -0.007 min
Response: 10042372
Conc: 0.69 ng/ml

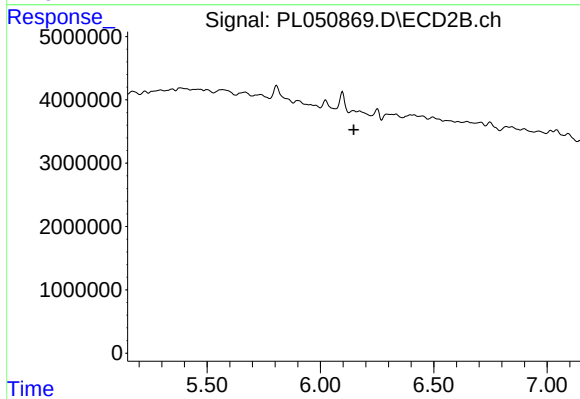

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

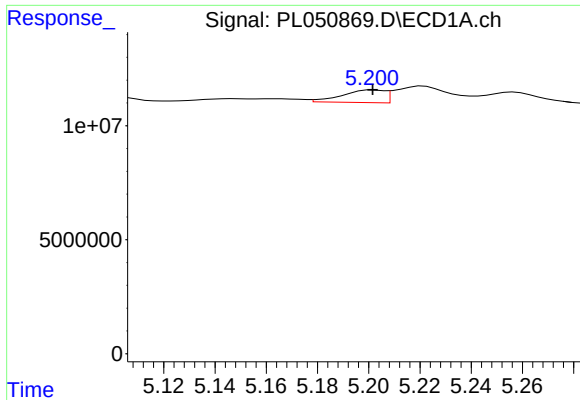

#10 gamma-Chlordane


R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 6342684
Conc: 0.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-072919

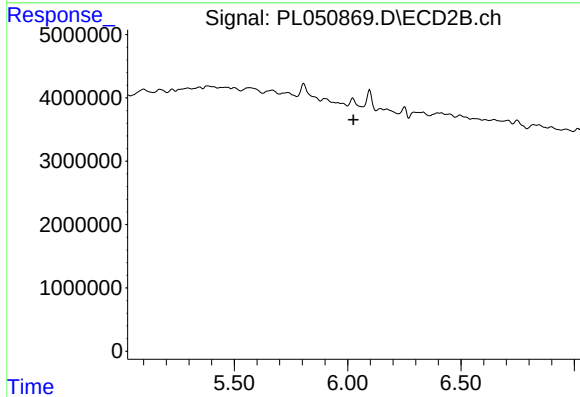


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

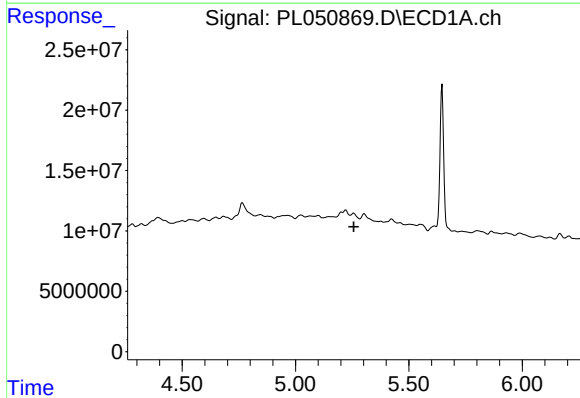


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

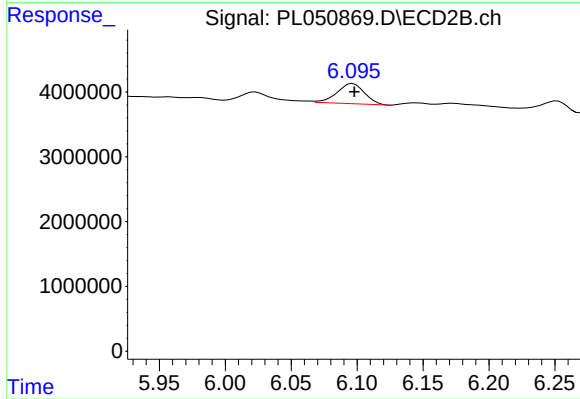

#11 alpha-Chlordane


R.T.: 6.097 min
Delta R.T.: -0.001 min
Response: 4512782
Conc: 1.23 ng/ml

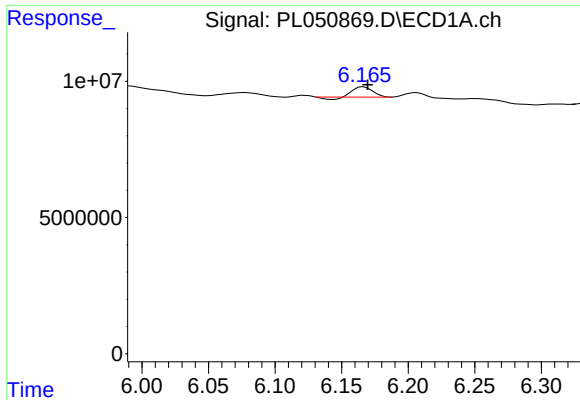

#17 4,4'-DDT


R.T.: 6.166 min
Delta R.T.: -0.003 min
Response: 3389289
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-072919

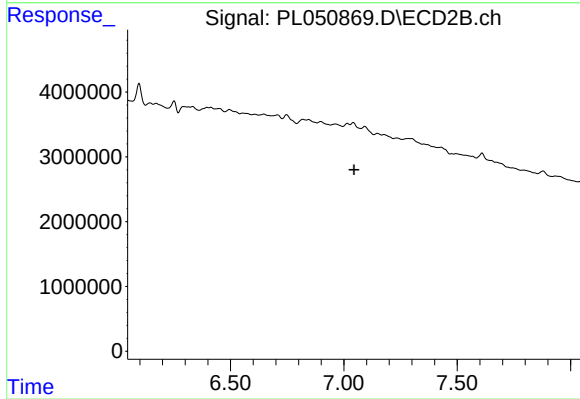


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.046 min
Response: 0
Conc: N.D.

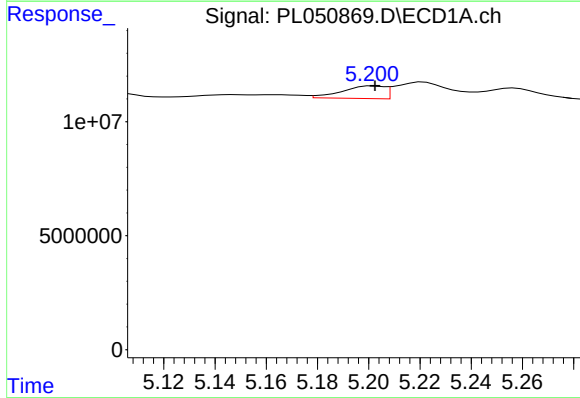


#25 Chlordane-3

R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 6342684
Conc: 4.53 ng/ml

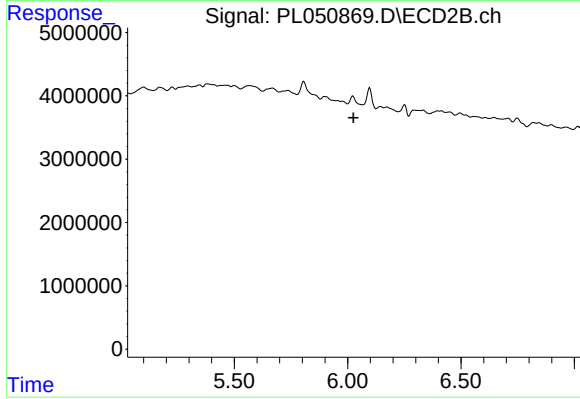

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

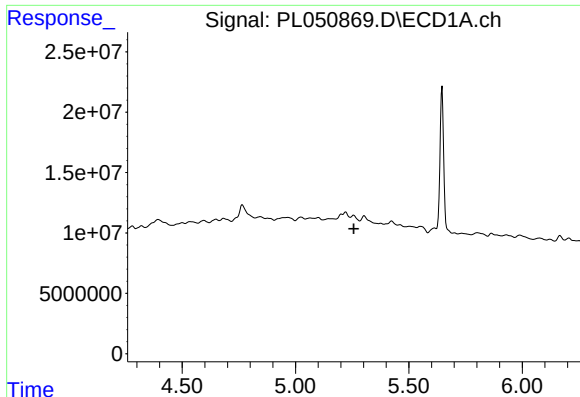

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OK-01-072919

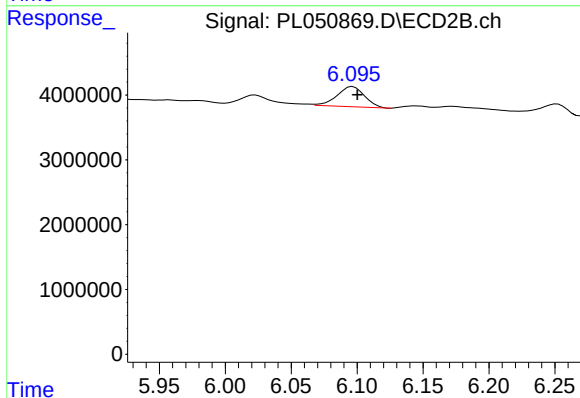


#26 Chlordane-4

R.T.: 6.097 min
Delta R.T.: -0.003 min
Response: 4512782
Conc: 7.77 ng/ml

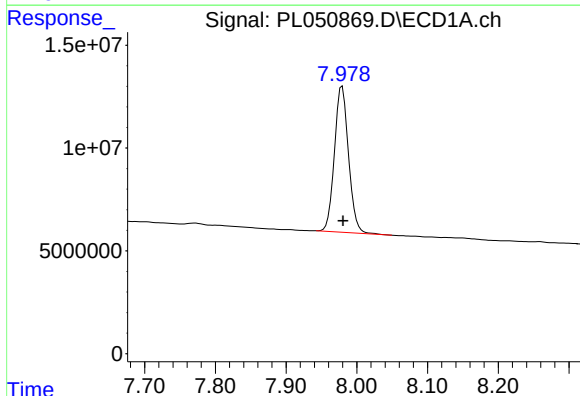

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.001 min
Response: 97912699
Conc: 9.67 ng/ml

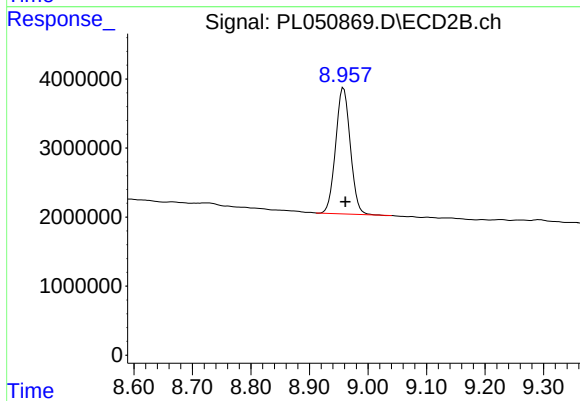

#28 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.003 min
Response: 31688717
Conc: 11.21 ng/ml