

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
 Data File : PL050872.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2019 15:37
 Operator : SM\AJ
 Sample : K4044-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 00:44:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	224.0E6	58316784	22.289	20.439
28)	SA Decachlor...	7.979	8.959	141.2E6	46890760	13.949	16.581
Target Compounds							
6)	B beta-BHC	0.000	4.800f	0	3615111	N.D.	2.091 #
7)	B delta-BHC	0.000	4.983	0	6028774	N.D.	1.559 #
8)	B Heptachlo...	0.000	5.806	0	8814872	N.D.	2.305 #
10)	B gamma-Chl...	5.201	0.000	41038269	0	2.600	N.D. #
11)	B alpha-Chl...	5.269	0.000	19938656	0	1.307	N.D. #
25)	Chlordane-3	5.201	0.000	41038269	0	29.317	N.D. #
26)	Chlordane-4	5.269	0.000	19938656	0	15.117	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
Data File : PL050872.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2019 15:37
Operator : SM\AJ
Sample : K4044-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 00:44:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

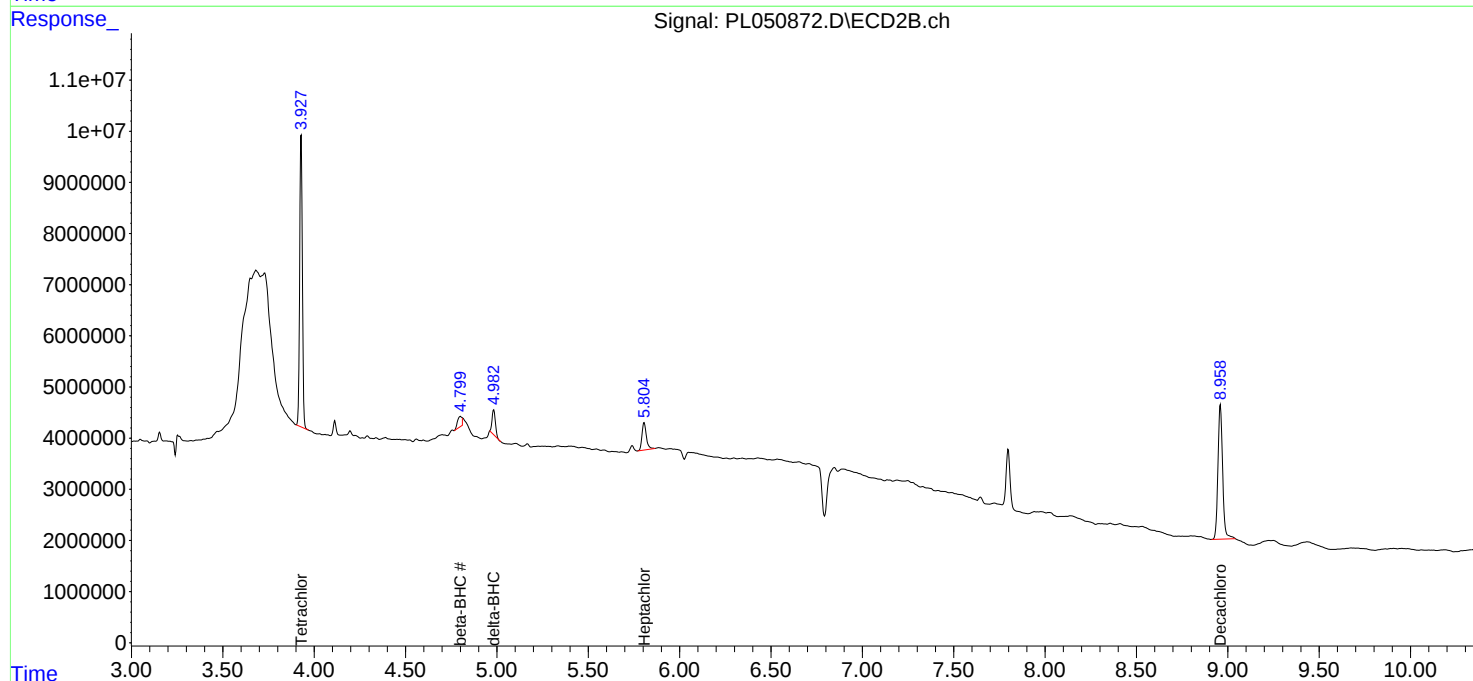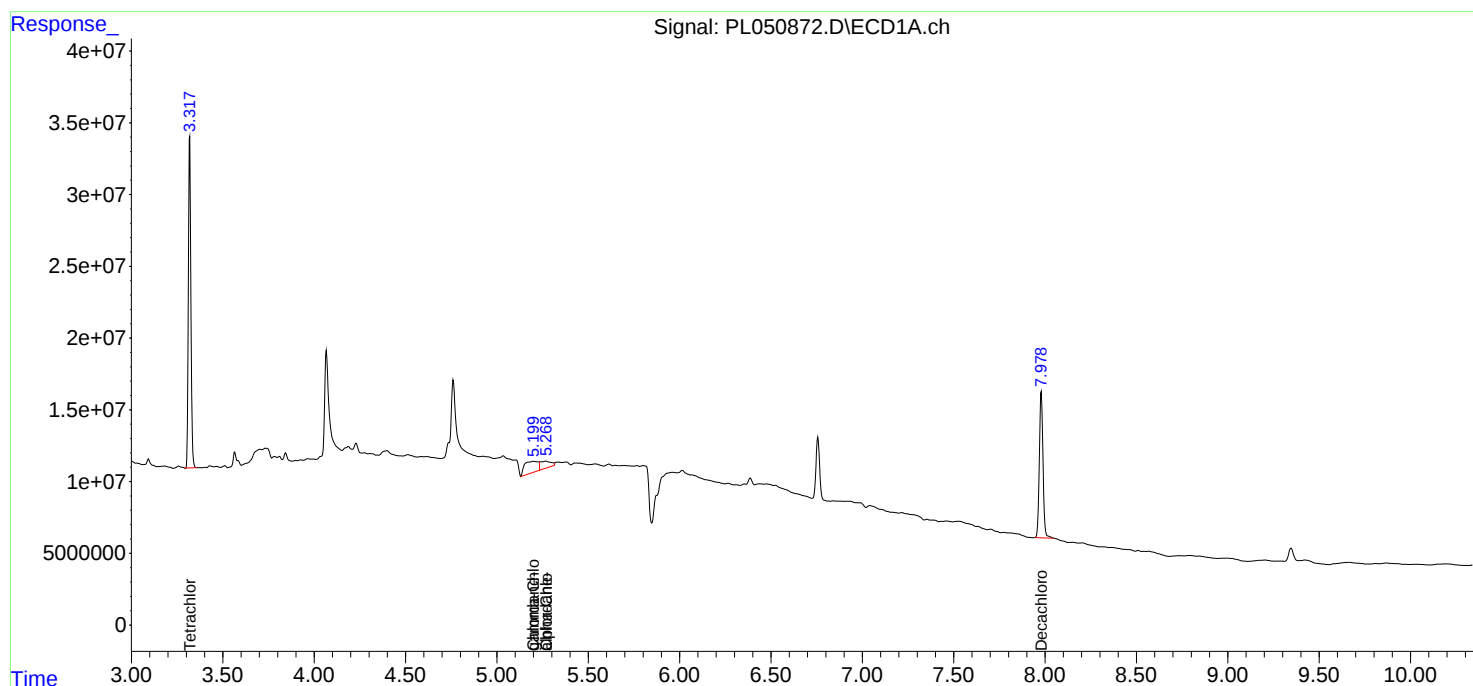


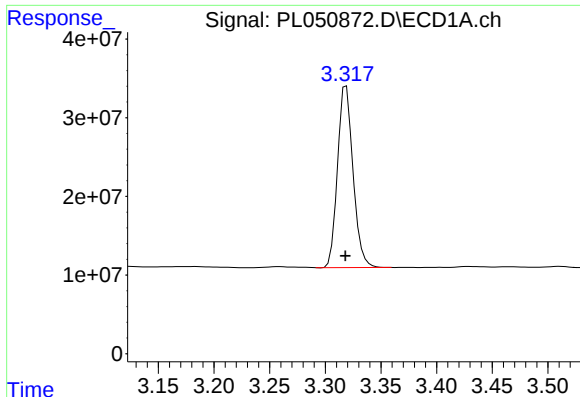

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 223951679
Conc: 22.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

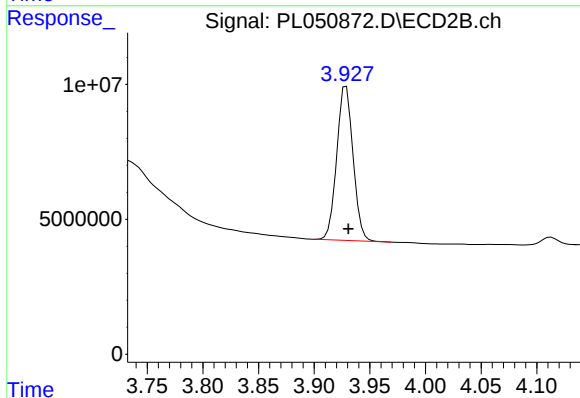


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 58316784
Conc: 20.44 ng/ml

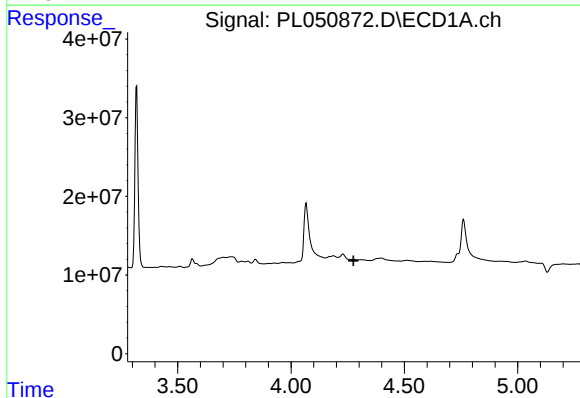


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

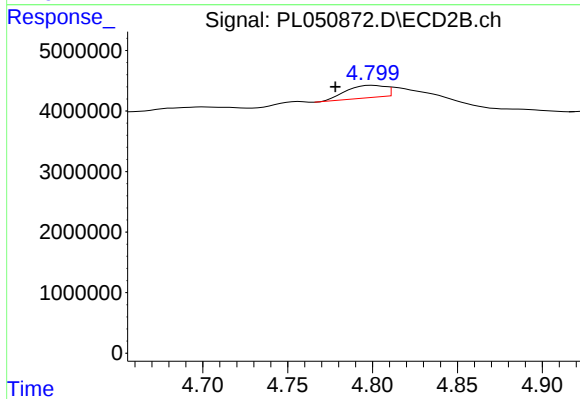

#6 beta-BHC


R.T.: 4.800 min
Delta R.T.: 0.022 min
Response: 3615111
Conc: 2.09 ng/ml

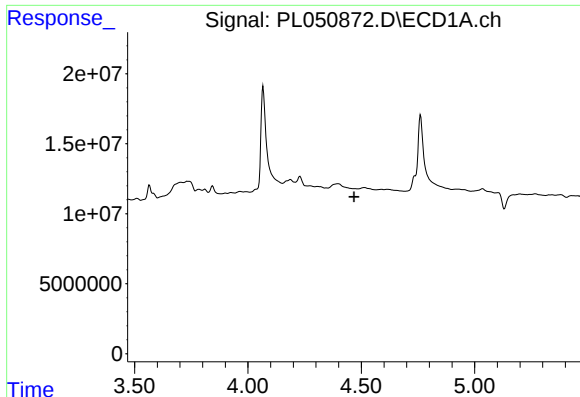

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-6

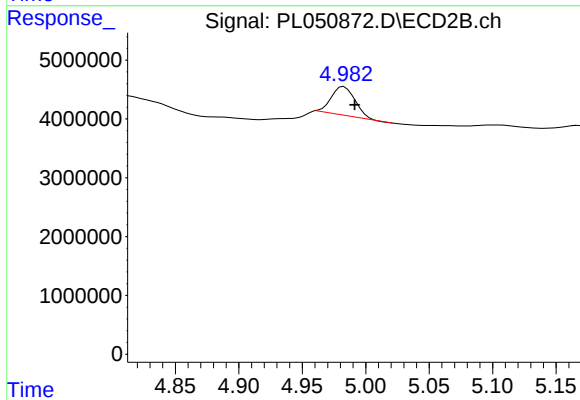


#7 delta-BHC

R.T.: 4.983 min
Delta R.T.: -0.009 min
Response: 6028774
Conc: 1.56 ng/ml

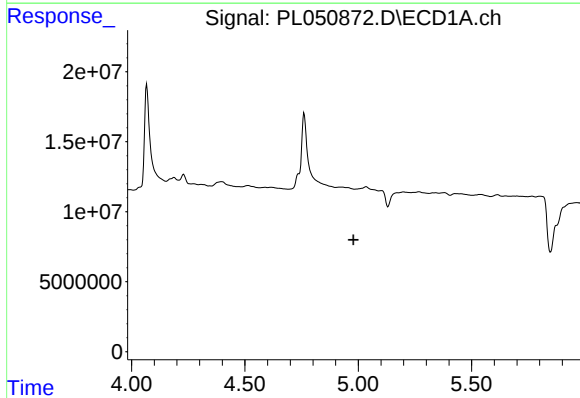


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

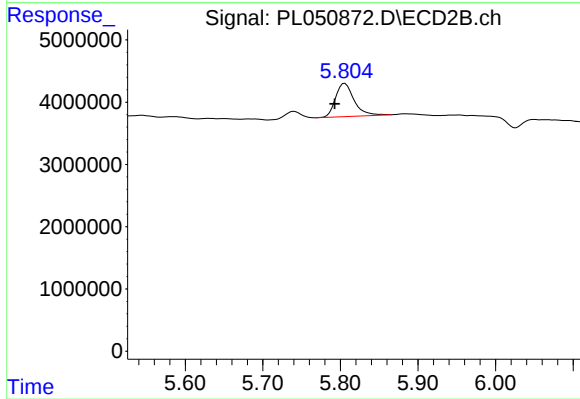

#8 Heptachlor epoxide


R.T.: 5.806 min
Delta R.T.: 0.013 min
Response: 8814872
Conc: 2.30 ng/ml

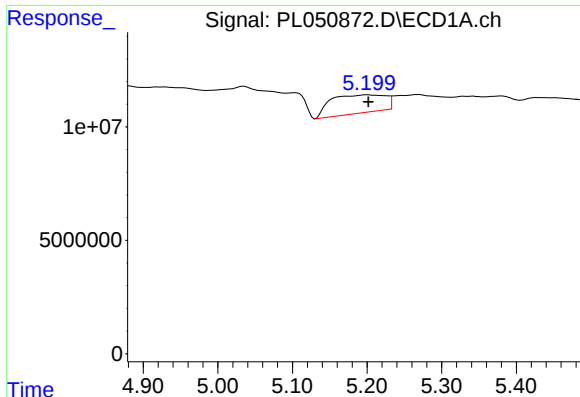

#10 gamma-Chlordane


R.T.: 5.201 min
Delta R.T.: 0.000 min
Response: 41038269
Conc: 2.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

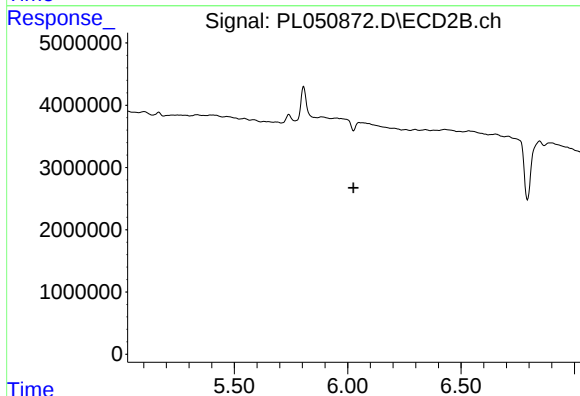


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

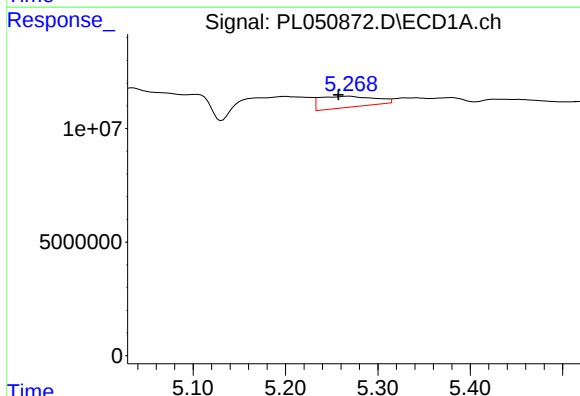


#11 alpha-Chlordane

R.T.: 5.269 min
Delta R.T.: 0.012 min
Response: 19938656
Conc: 1.31 ng/ml

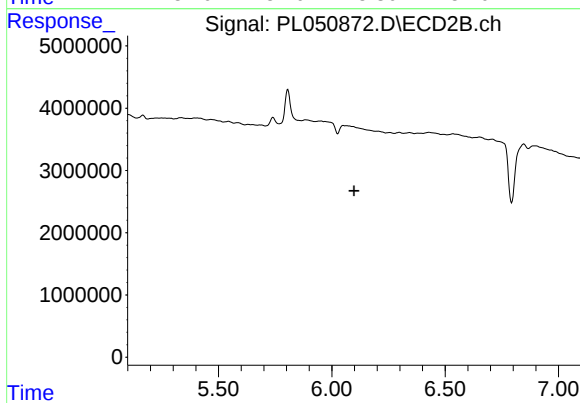

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

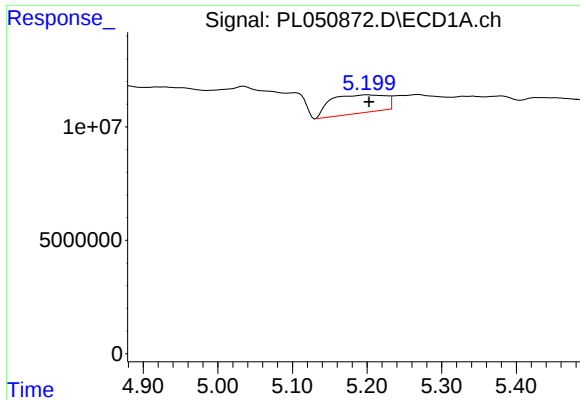

#25 Chlordane-3


R.T.: 5.201 min
Delta R.T.: -0.002 min
Response: 41038269
Conc: 29.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

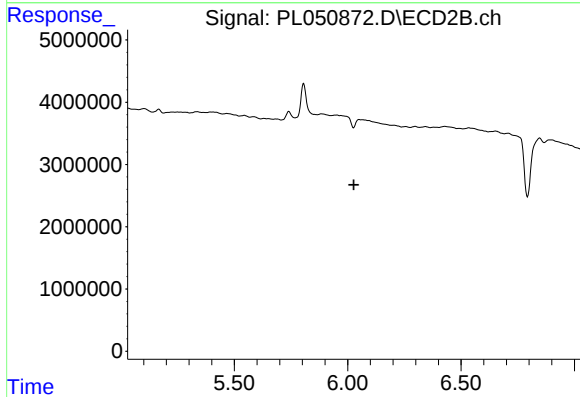


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

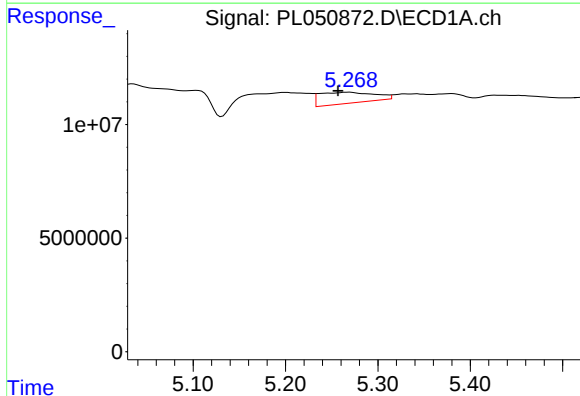


#26 Chlordane-4

R.T.: 5.269 min
Delta R.T.: 0.012 min
Response: 19938656
Conc: 15.12 ng/ml

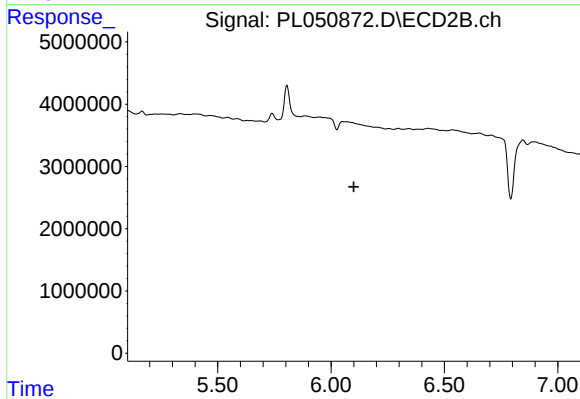

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

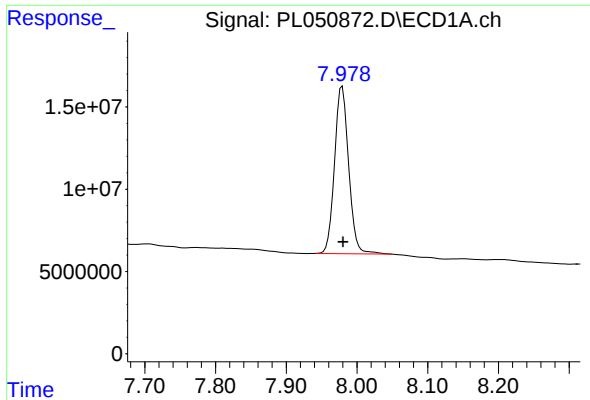

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.001 min
Response: 141237363
Conc: 13.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6

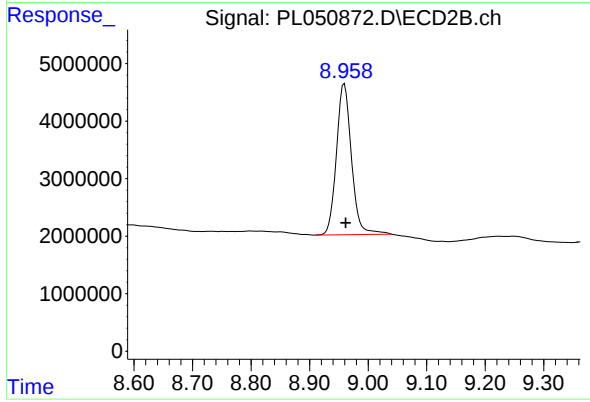

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.002 min
Response: 46890760
Conc: 16.58 ng/ml