

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
 Data File : PL050896.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2019 21:58
 Operator : SM\AJ
 Sample : K4024-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 00:52:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	227.8E6	63321542	22.673	22.193
28)	SA Decachlor...	7.978	8.959	232.6E6	62268656	22.971	22.019
Target Compounds							
4)	MA Heptachlor	4.323f	0.000	5917481	0	0.361	N.D. #
6)	B beta-BHC	4.273	4.805f	-5432082	5559376	N.D.	3.216
10)	B gamma-Chl...	5.187	0.000	3052477	0	0.193	N.D. #
23)	Chlordane-1	4.171	0.000	5617626	0	15.267	N.D. #
25)	Chlordane-3	5.187f	0.000	3052477	0	2.181	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
Data File : PL050896.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2019 21:58
Operator : SM\AJ
Sample : K4024-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 00:52:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

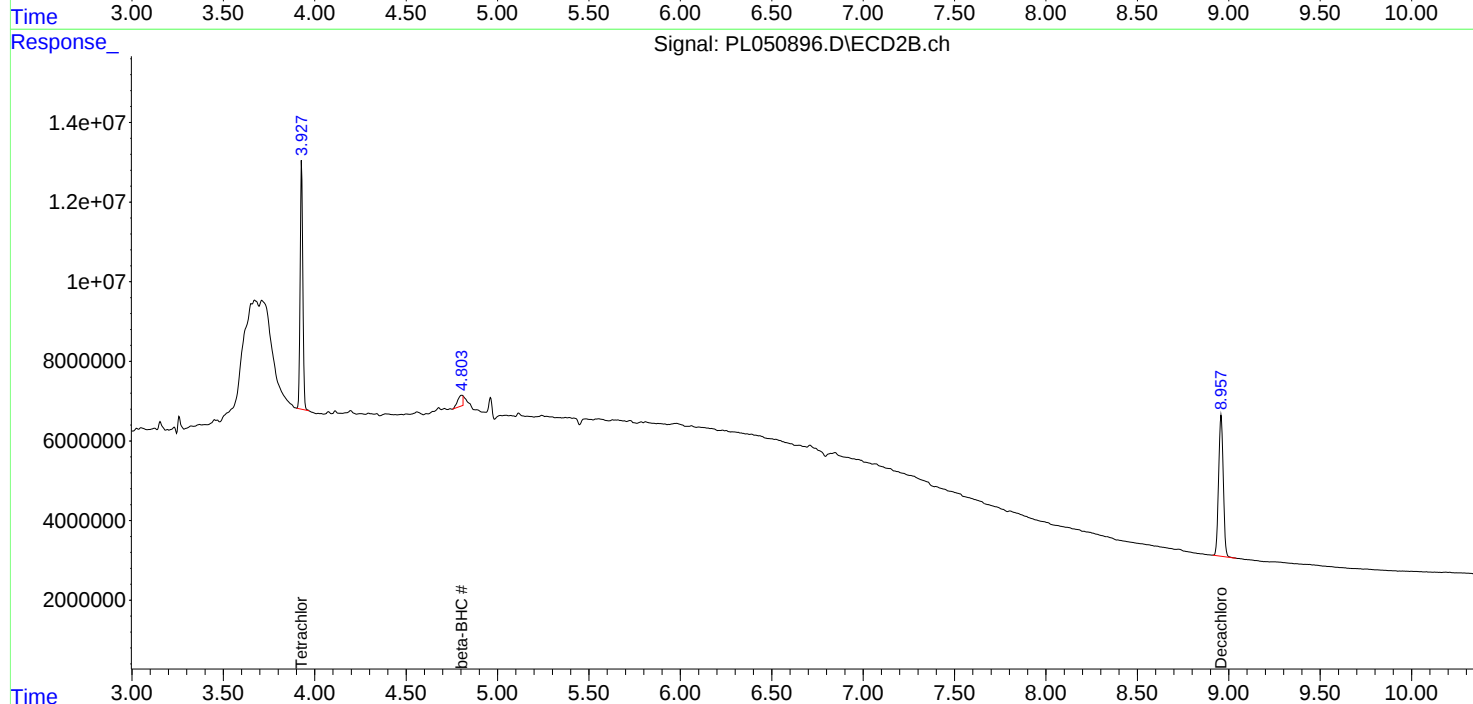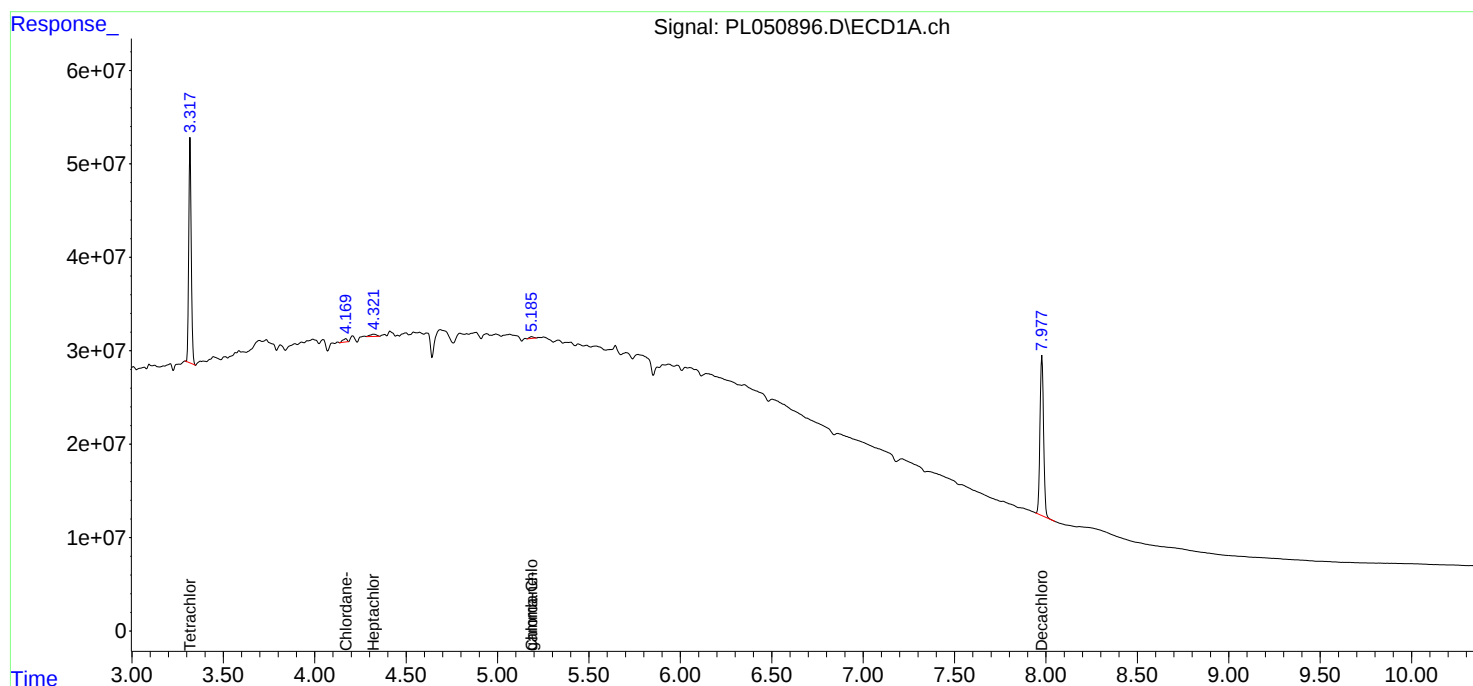


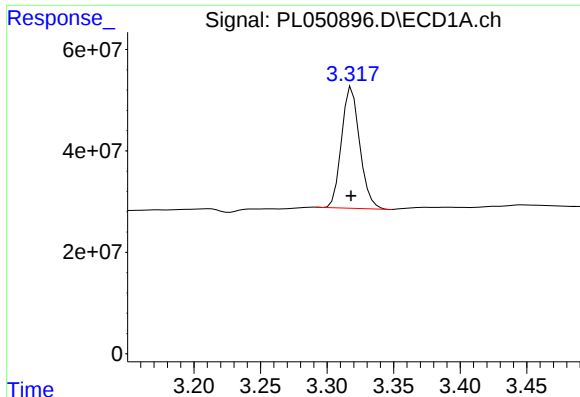

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 227814878
Conc: 22.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8

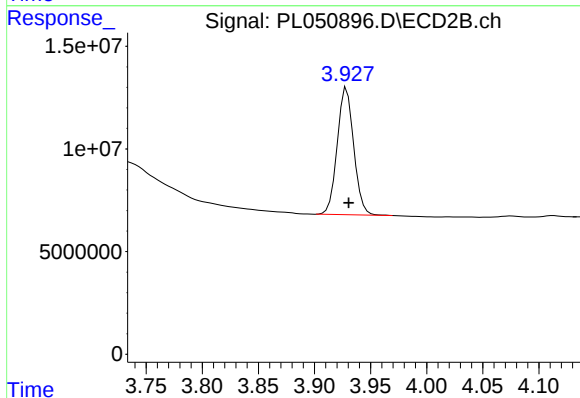


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 63321542
Conc: 22.19 ng/ml

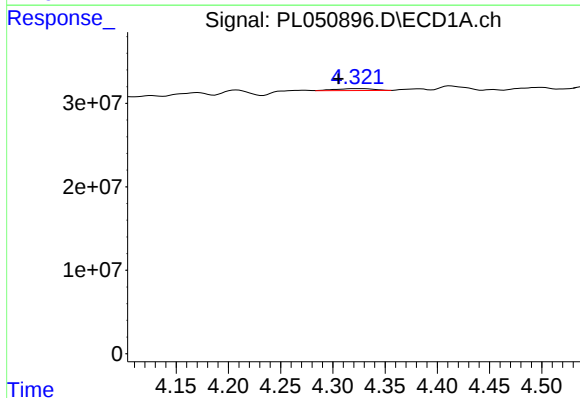


#4 Heptachlor

R.T.: 4.323 min
Delta R.T.: 0.018 min
Response: 5917481
Conc: 0.36 ng/ml

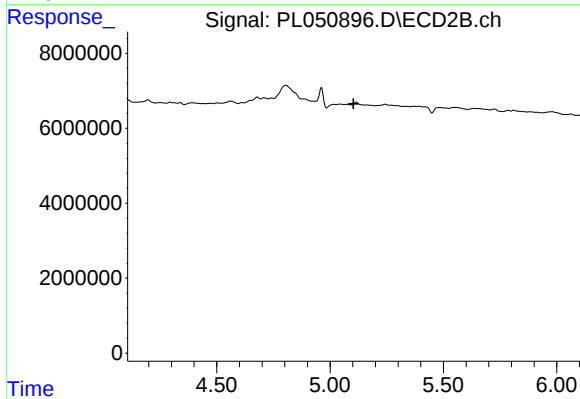

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.104 min
Response: 0
Conc: N.D.

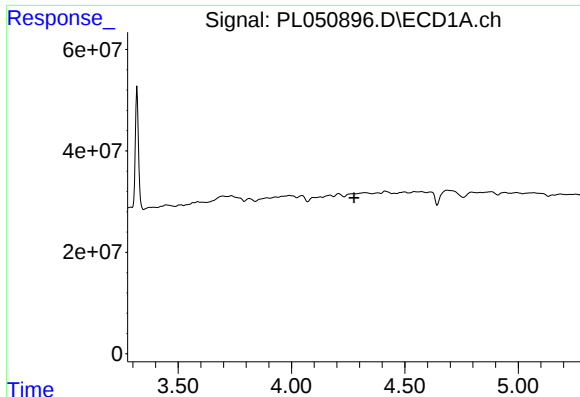

#6 beta-BHC


R.T.: 4.273 min
Delta R.T.: -0.003 min
Response: -5432082
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-8

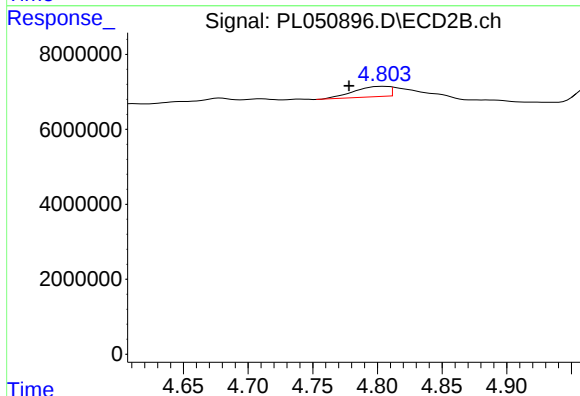


#6 beta-BHC

R.T.: 4.805 min
Delta R.T.: 0.027 min
Response: 5559376
Conc: 3.22 ng/ml

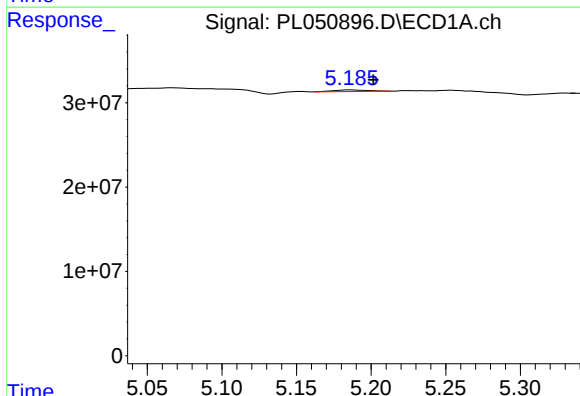


#10 gamma-Chlordane

R.T.: 5.187 min
Delta R.T.: -0.015 min
Response: 3052477
Conc: 0.19 ng/ml

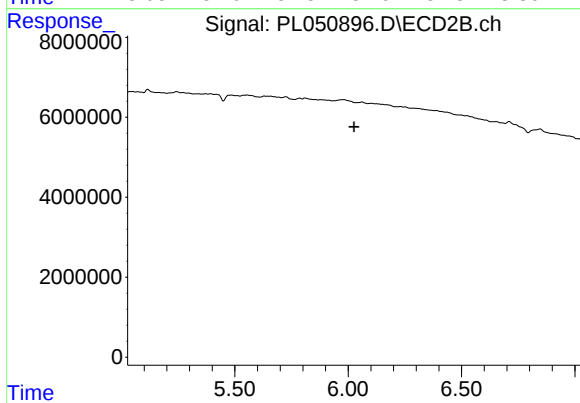

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.026 min
Response: 0
Conc: N.D.

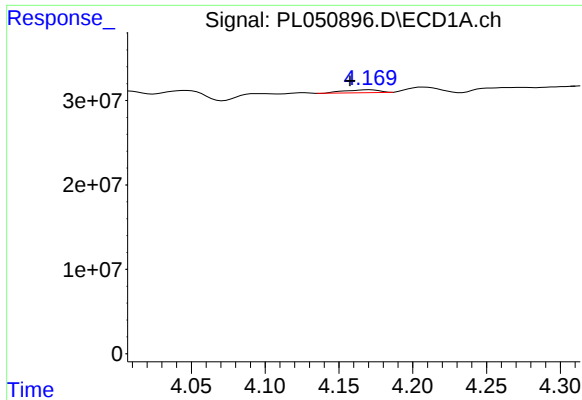

#23 Chlordane-1


R.T.: 4.171 min
Delta R.T.: 0.013 min
Response: 5617626
Conc: 15.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8

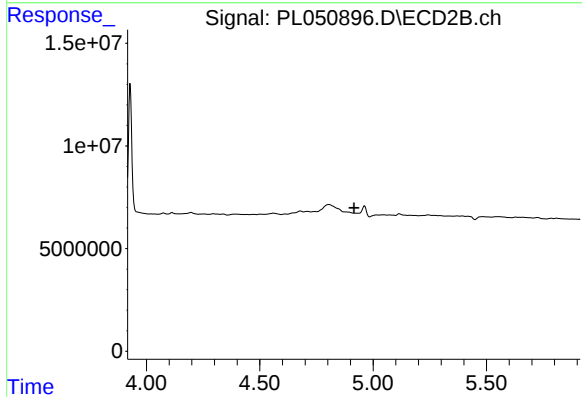


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.916 min
Response: 0
Conc: N.D.

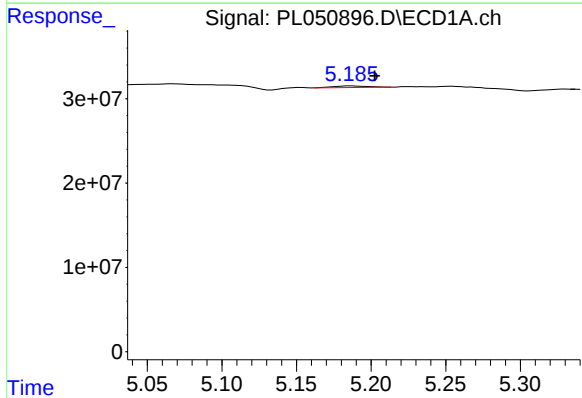


#25 Chlordane-3

R.T.: 5.187 min
Delta R.T.: -0.015 min
Response: 3052477
Conc: 2.18 ng/ml

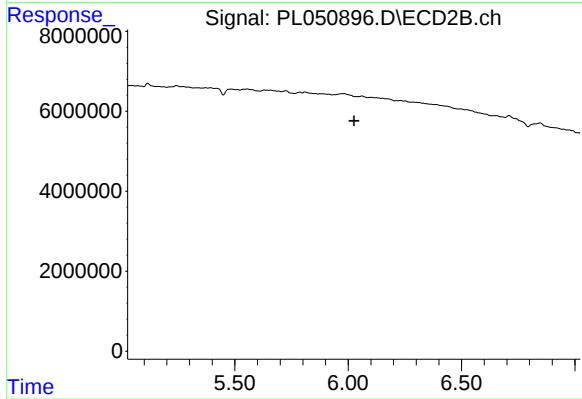

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

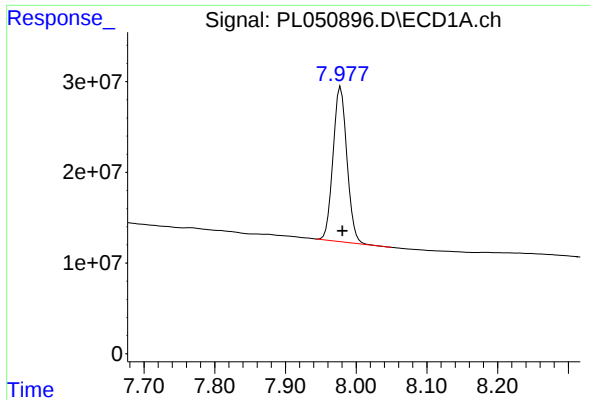

#28 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: -0.002 min
Response: 232584990
Conc: 22.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-8

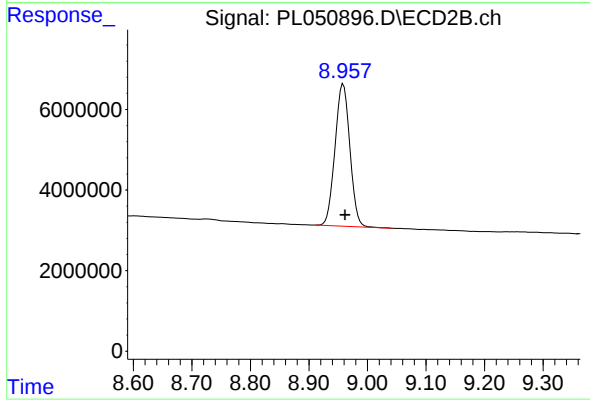

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.003 min
Response: 62268656
Conc: 22.02 ng/ml