

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
 Data File : PL050897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2019 22:13
 Operator : SM\AJ
 Sample : K4024-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 00:52:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	228.0E6	65293017	22.694	22.884
28)	SA Decachlor...	7.979	8.958	250.8E6	66826695	24.767	23.631
Target Compounds							
8)	B Heptachlo...	0.000	5.805	0	5509727	N.D.	1.441 #
10)	B gamma-Chl...	5.198	0.000	3497942	0	0.222	N.D. #
25)	Chlordane-3	5.198	0.000	3497942	0	2.499	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
Data File : PL050897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2019 22:13
Operator : SM\AJ
Sample : K4024-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-6-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 00:52:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

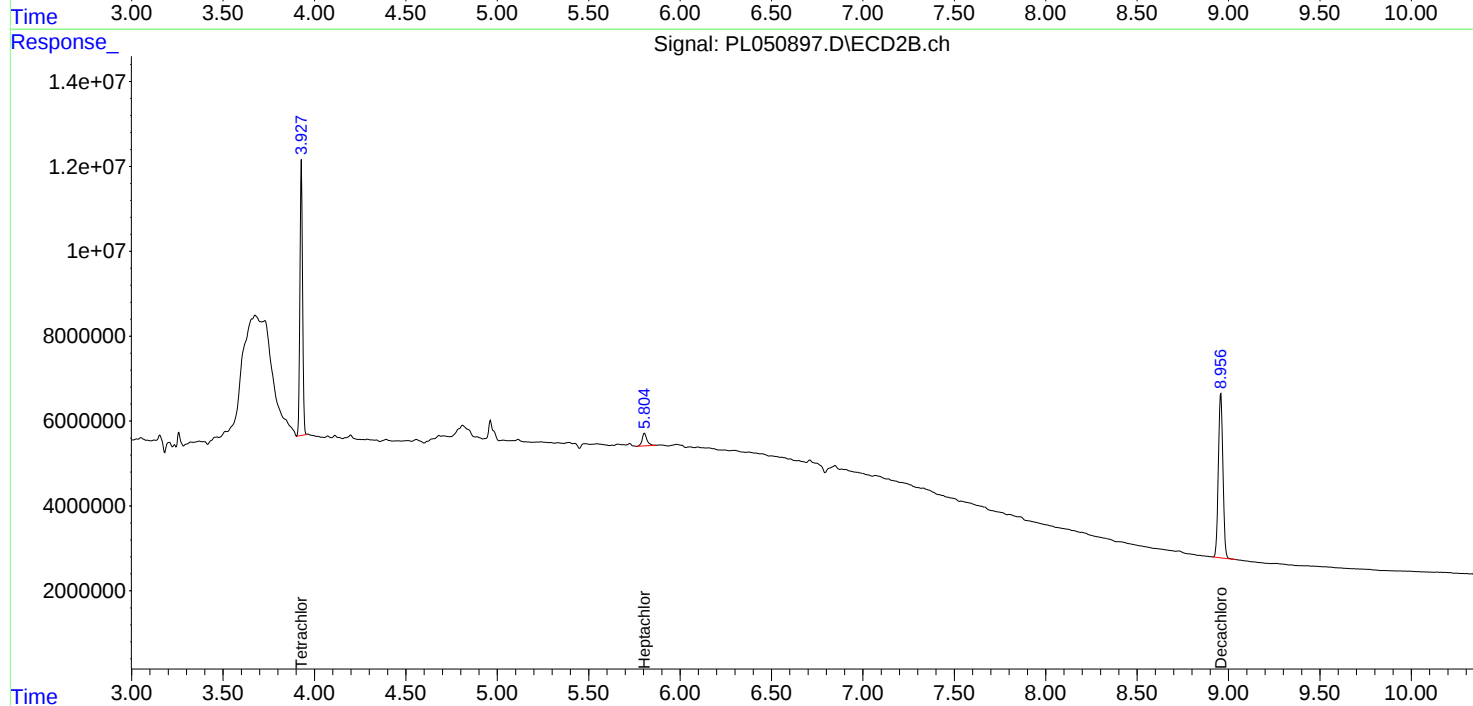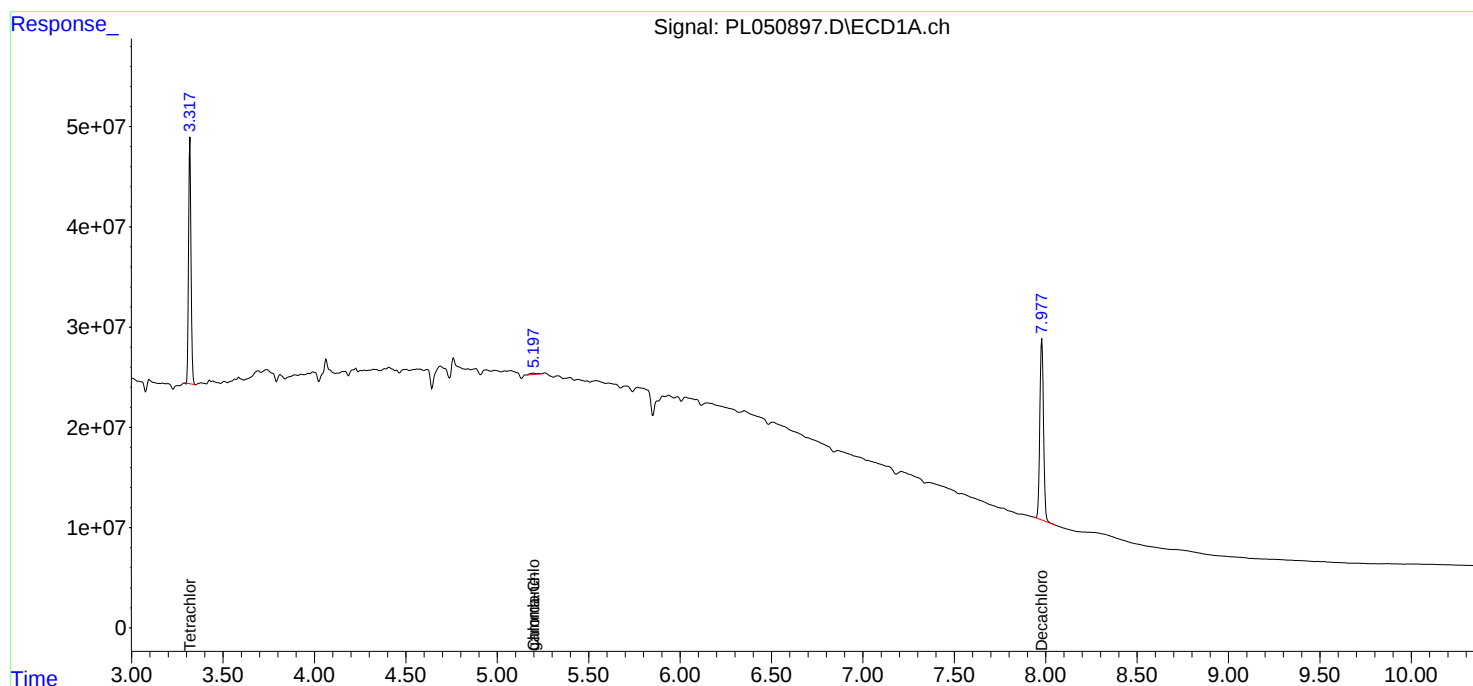


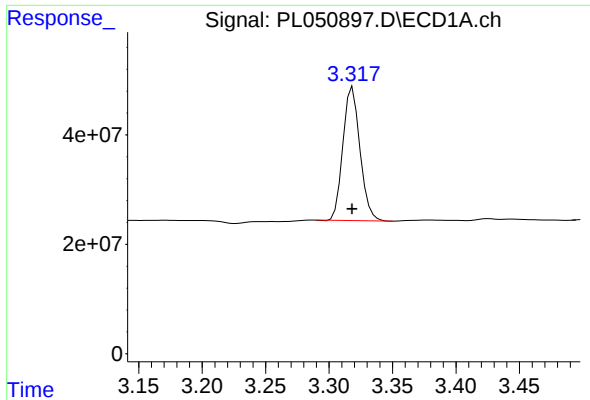

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 228021119
Conc: 22.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-A

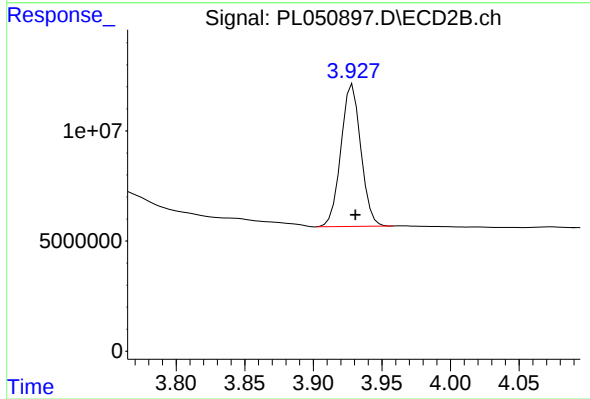


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 65293017
Conc: 22.88 ng/ml

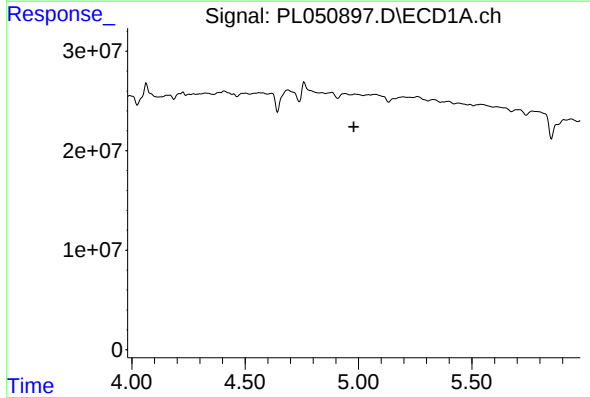


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

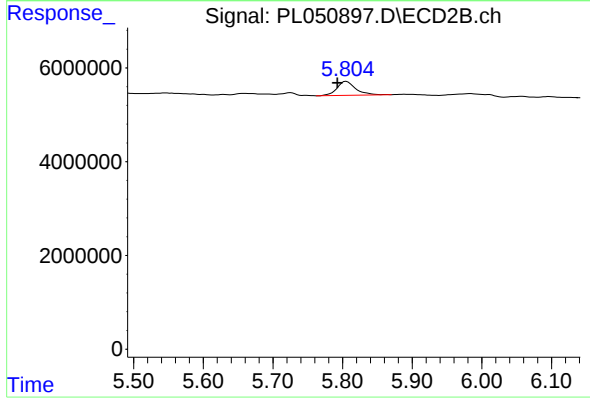

#8 Heptachlor epoxide


R.T.: 5.805 min
Delta R.T.: 0.013 min
Response: 5509727
Conc: 1.44 ng/ml

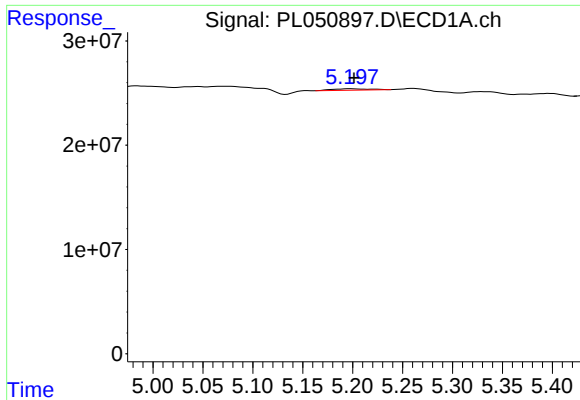

#10 gamma-Chlordane


R.T.: 5.198 min
Delta R.T.: -0.003 min
Response: 3497942
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-A

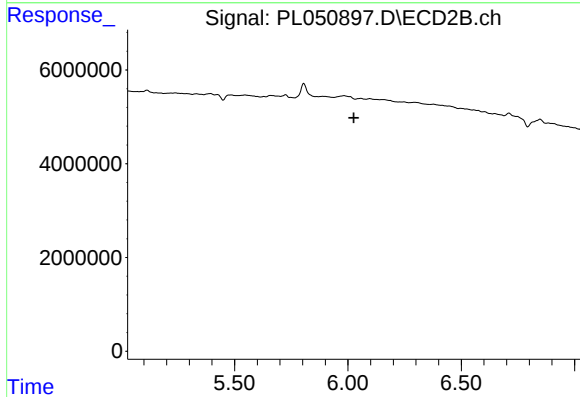


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

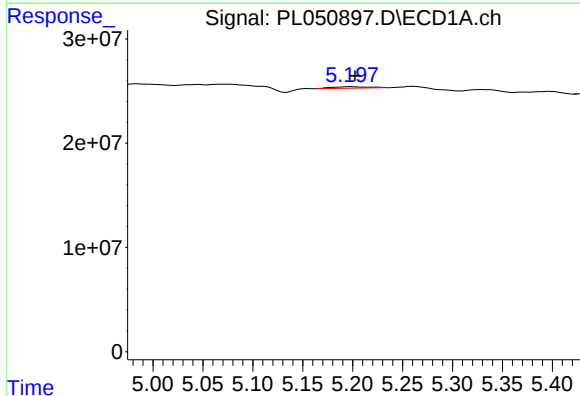


#25 Chlordane-3

R.T.: 5.198 min
Delta R.T.: -0.004 min
Response: 3497942
Conc: 2.50 ng/ml

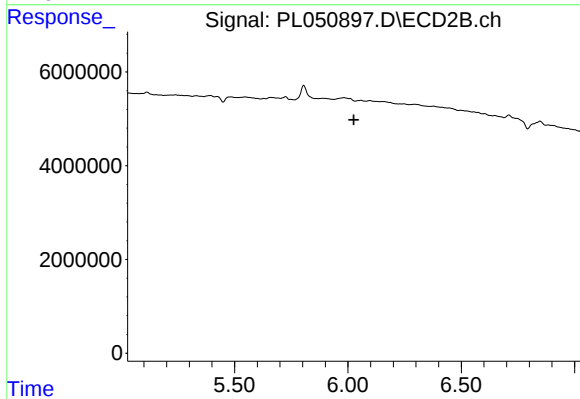

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

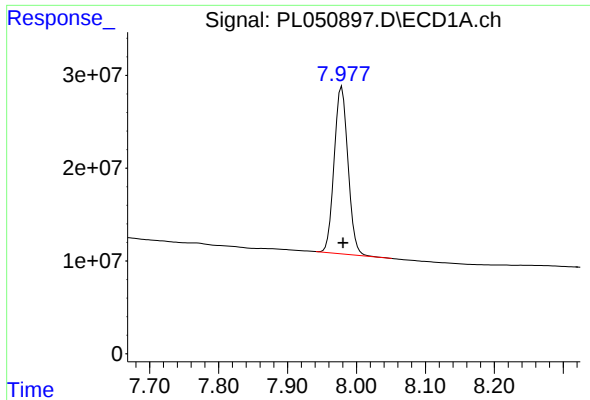

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.002 min
Response: 250777050
Conc: 24.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6-A

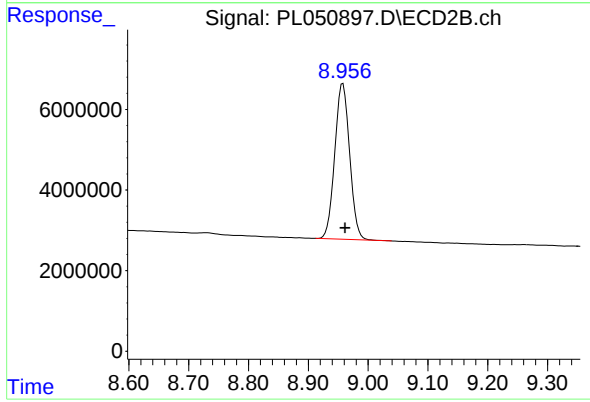

#28 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.004 min
Response: 66826695
Conc: 23.63 ng/ml