

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
 Data File : PL050901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jul 2019 23:14
 Operator : SM\AJ
 Sample : K4044-18
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 00:53:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.319	3.929	215.8E6	61849977	21.479	21.677
28)	SA Decachlor...	7.978	8.958	248.7E6	66207586	24.558	23.412
Target Compounds							
8)	B Heptachlo...	0.000	5.805	0	5723113	N.D.	1.496 #
10)	B gamma-Chl...	5.200	0.000	1091578	0	0.069	N.D. #
25)	Chlordane-3	5.200	0.000	1091578	0	0.780	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
Data File : PL050901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jul 2019 23:14
Operator : SM\AJ
Sample : K4044-18
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 00:53:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

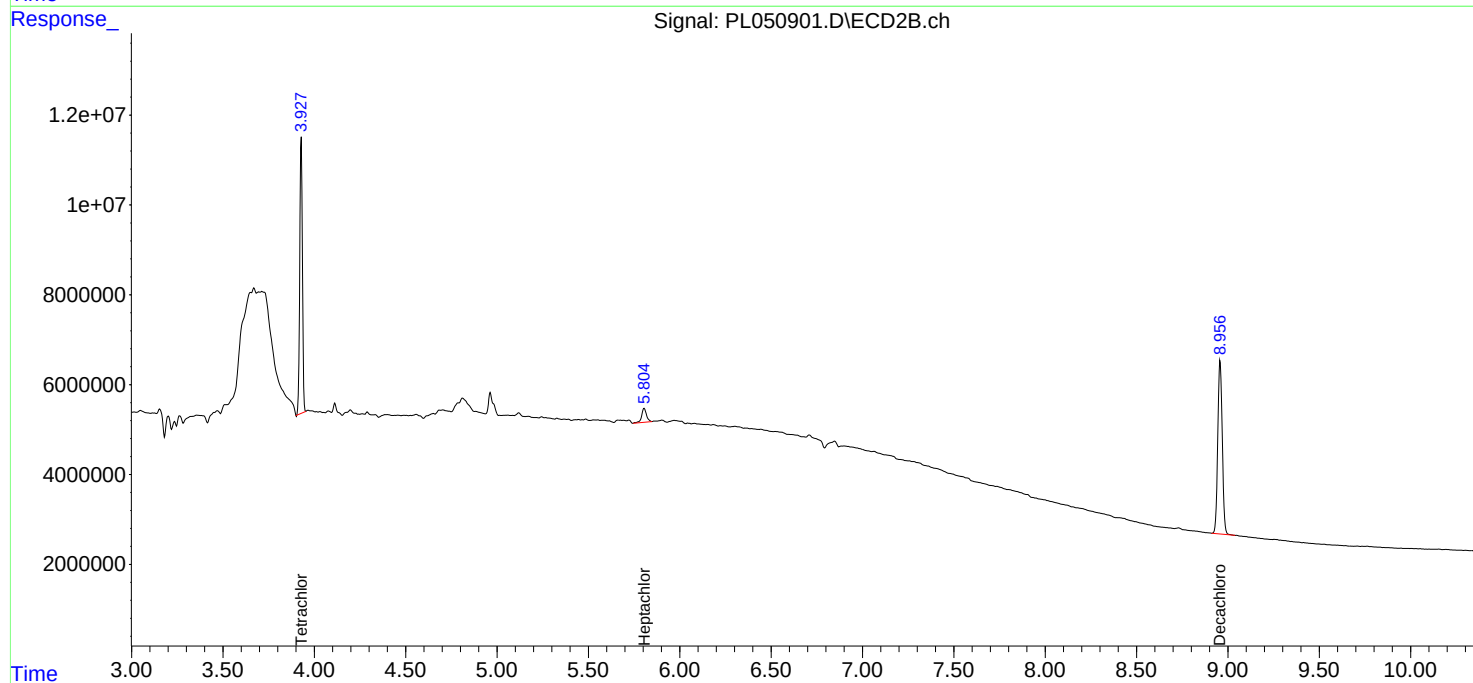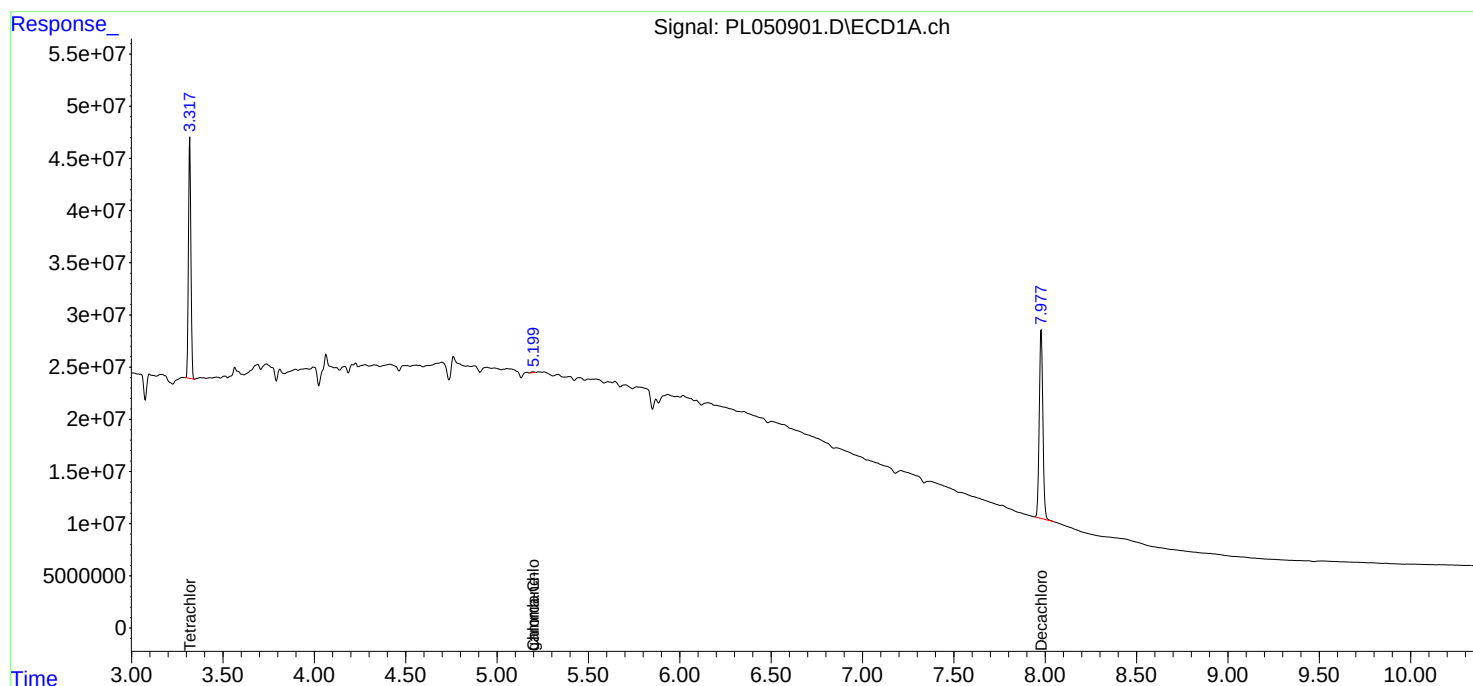


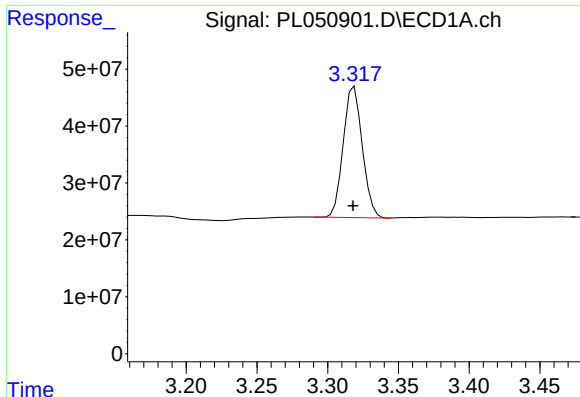

#1 Tetrachloro-m-xylene


R.T.: 3.319 min
Delta R.T.: 0.000 min
Response: 215821876
Conc: 21.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

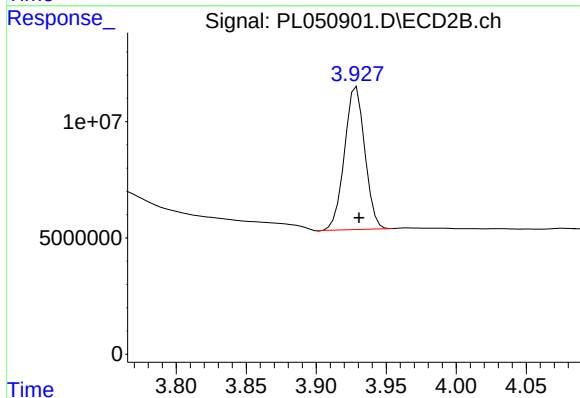


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 61849977
Conc: 21.68 ng/ml

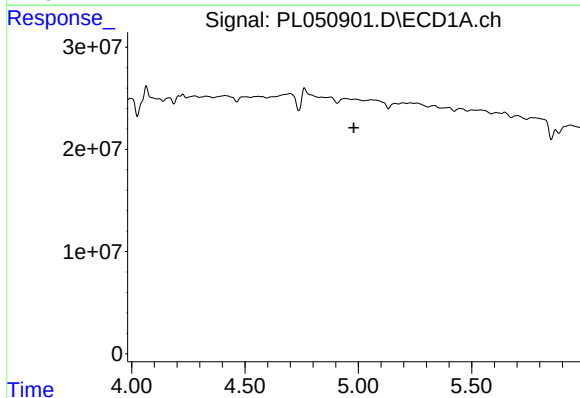


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

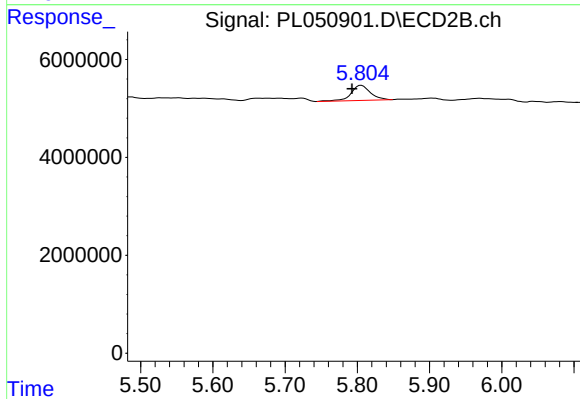

#8 Heptachlor epoxide


R.T.: 5.805 min
Delta R.T.: 0.013 min
Response: 5723113
Conc: 1.50 ng/ml

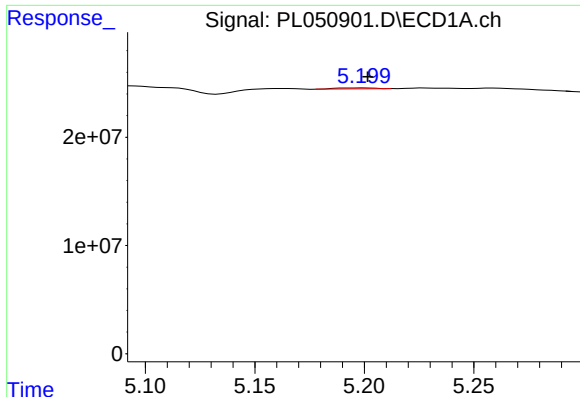

#10 gamma-Chlordane


R.T.: 5.200 min
Delta R.T.: -0.001 min
Response: 1091578
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

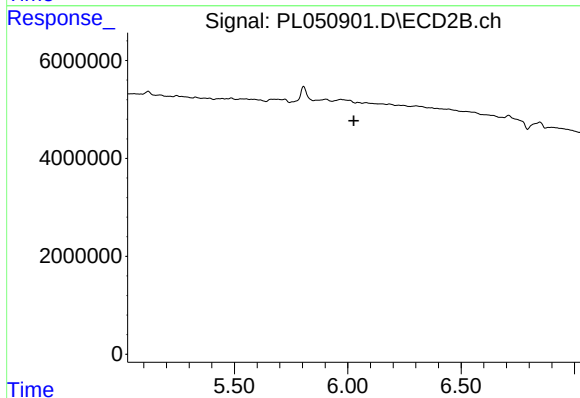


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

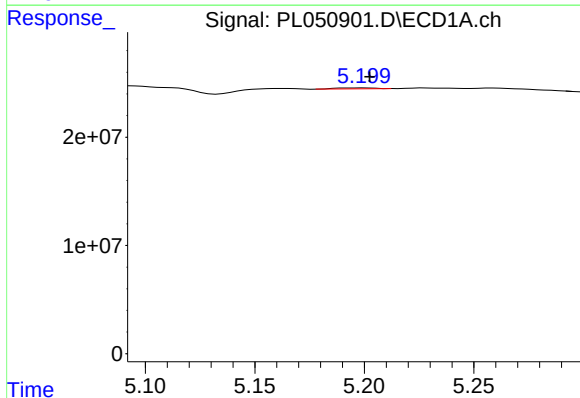


#25 Chlordane-3

R.T.: 5.200 min
Delta R.T.: -0.002 min
Response: 1091578
Conc: 0.78 ng/ml

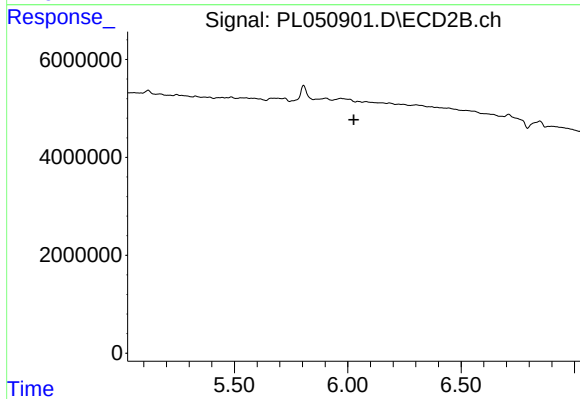

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

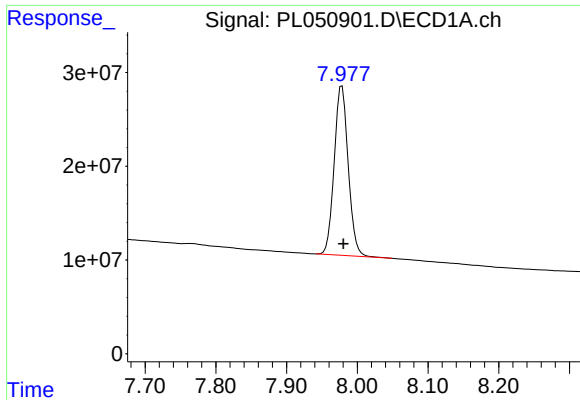

#28 Decachlorobiphenyl

R.T.: 7.978 min
Delta R.T.: -0.002 min
Response: 248655521
Conc: 24.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

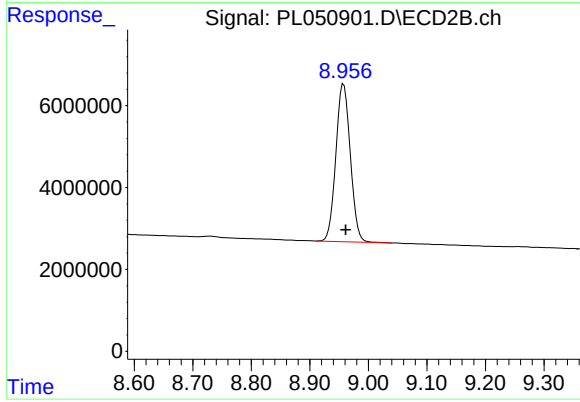

#28 Decachlorobiphenyl

R.T.: 8.958 min
Delta R.T.: -0.004 min
Response: 66207586
Conc: 23.41 ng/ml