

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
 Data File : PL050905.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2019 00:30
 Operator : SM\AJ
 Sample : K4044-17
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 31 03:28:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.318	3.929	123.1E6	33809055	12.255	11.849
28)	SA Decachlor...	7.979	8.959	106.8E6	32482339	10.544	11.486
Target Compounds							
6)	B beta-BHC	0.000	4.801f	0	4766835	N.D.	2.757 #
9)	A Endosulfan I	5.302	0.000	14063309	0	0.967	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073019\
Data File : PL050905.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2019 00:30
Operator : SM\AJ
Sample : K4044-17
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 31 03:28:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

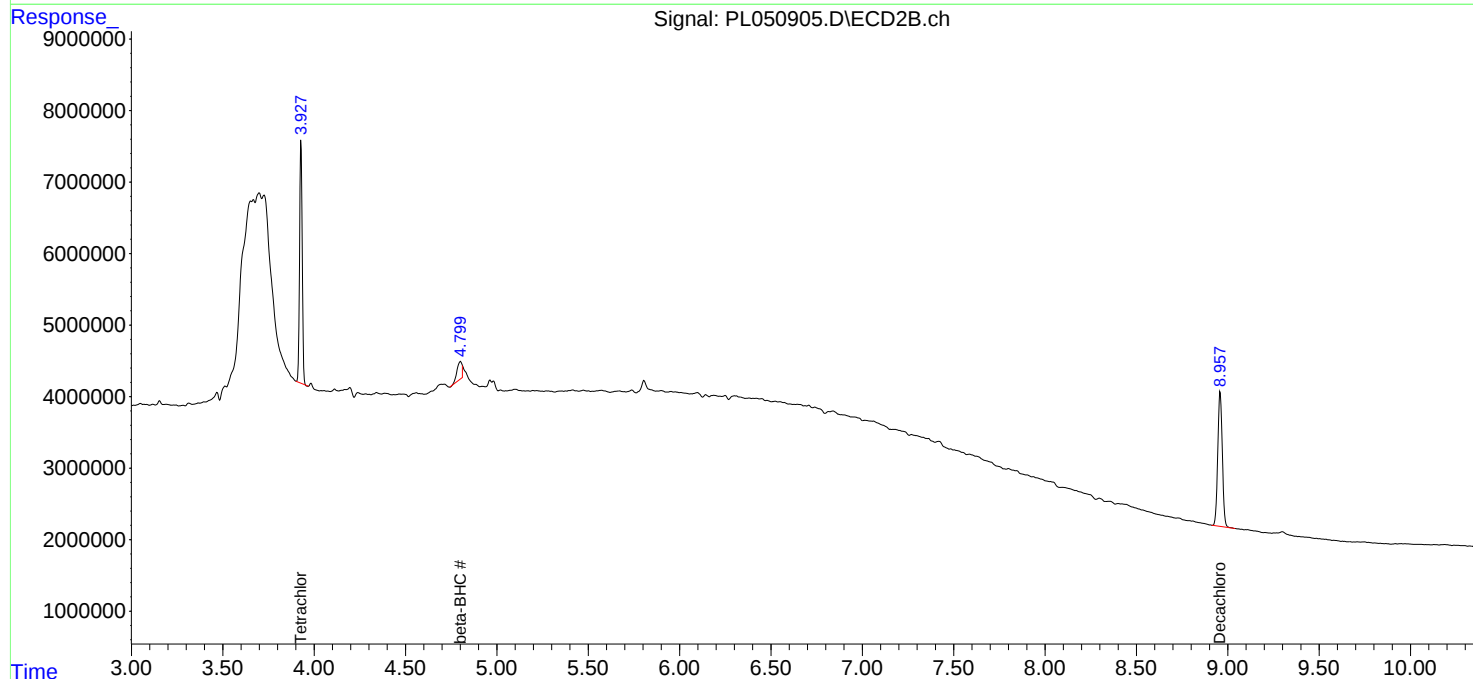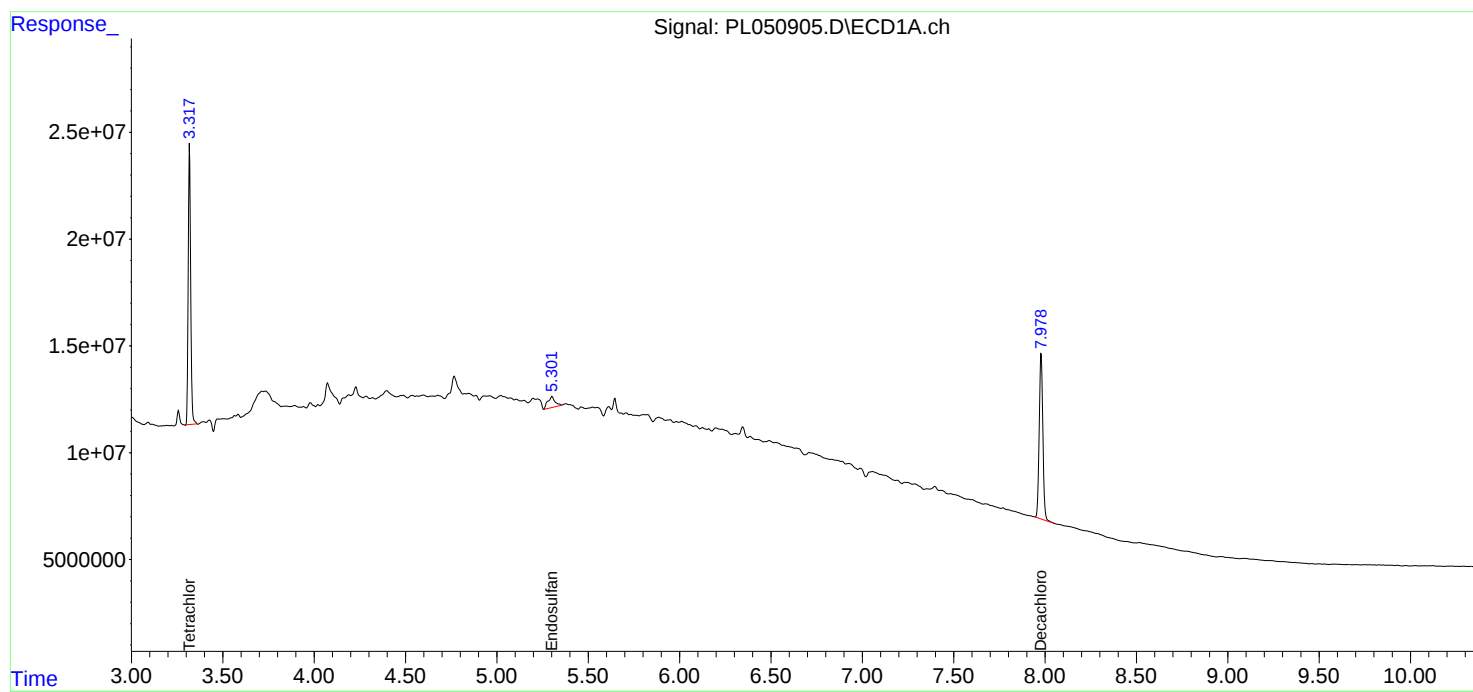


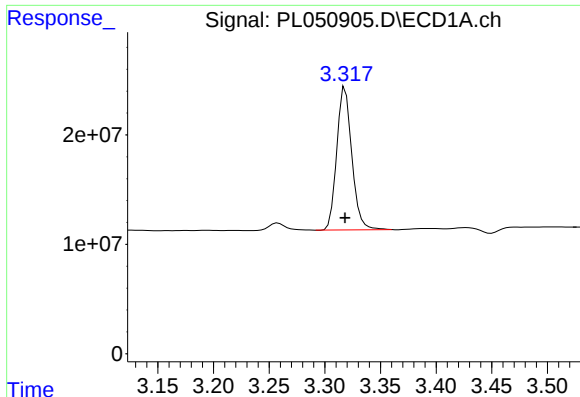

#1 Tetrachloro-m-xylene


R.T.: 3.318 min
Delta R.T.: 0.000 min
Response: 123132701
Conc: 12.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

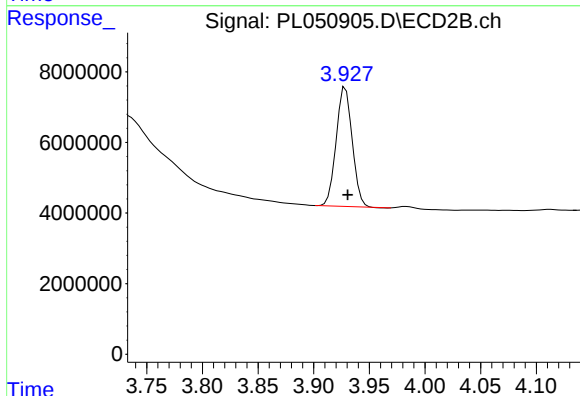


#1 Tetrachloro-m-xylene

R.T.: 3.929 min
Delta R.T.: -0.002 min
Response: 33809055
Conc: 11.85 ng/ml

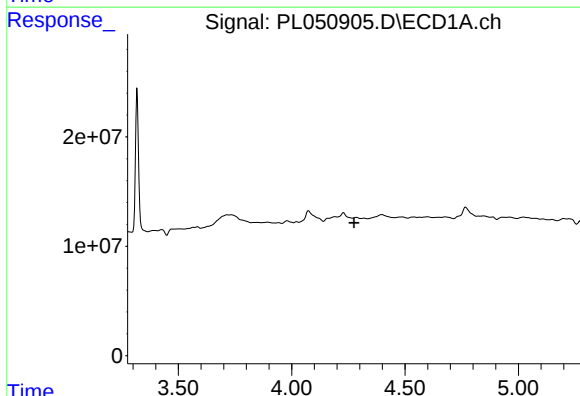


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

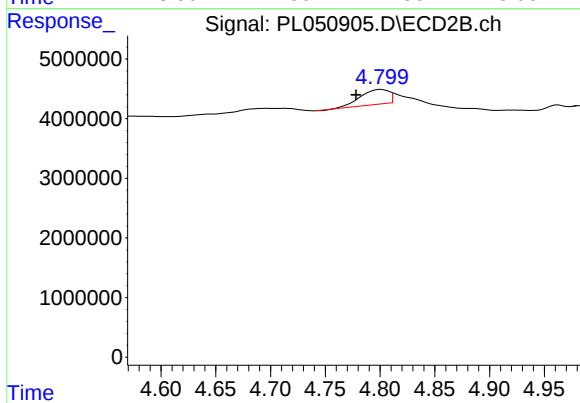

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.023 min
Response: 4766835
Conc: 2.76 ng/ml

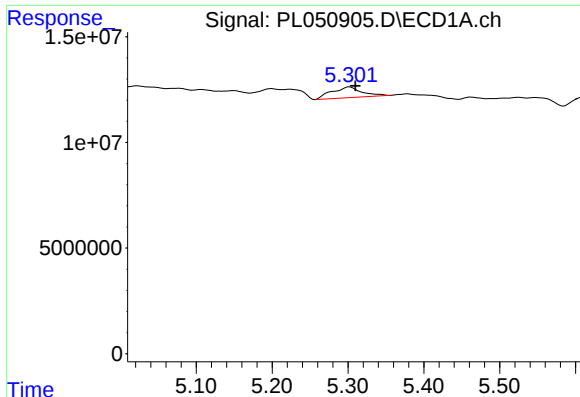

#9 Endosulfan I


R.T.: 5.302 min
Delta R.T.: -0.008 min
Response: 14063309
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

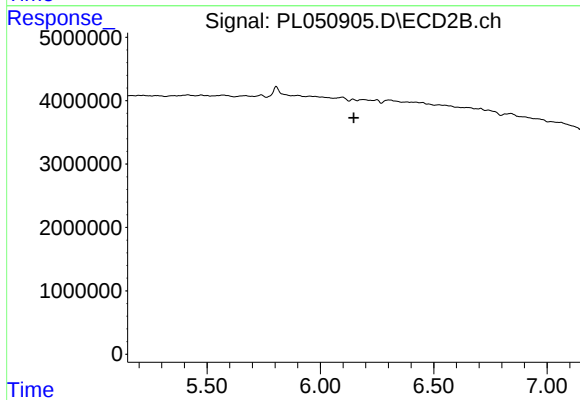


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

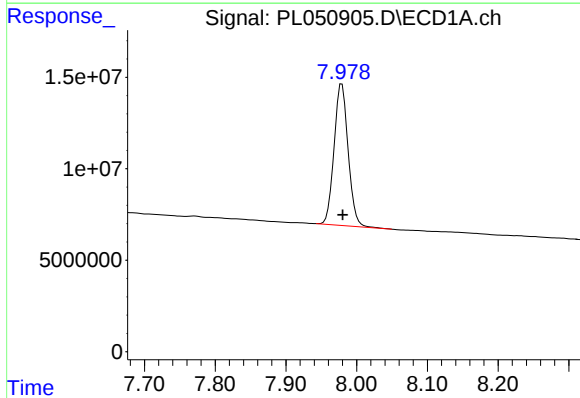

#28 Decachlorobiphenyl

R.T.: 7.979 min
Delta R.T.: -0.001 min
Response: 106761088
Conc: 10.54 ng/ml

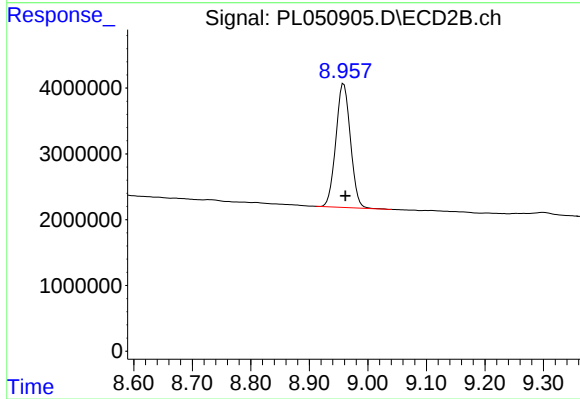

#28 Decachlorobiphenyl

R.T.: 8.959 min
Delta R.T.: -0.003 min
Response: 32482339
Conc: 11.49 ng/ml